
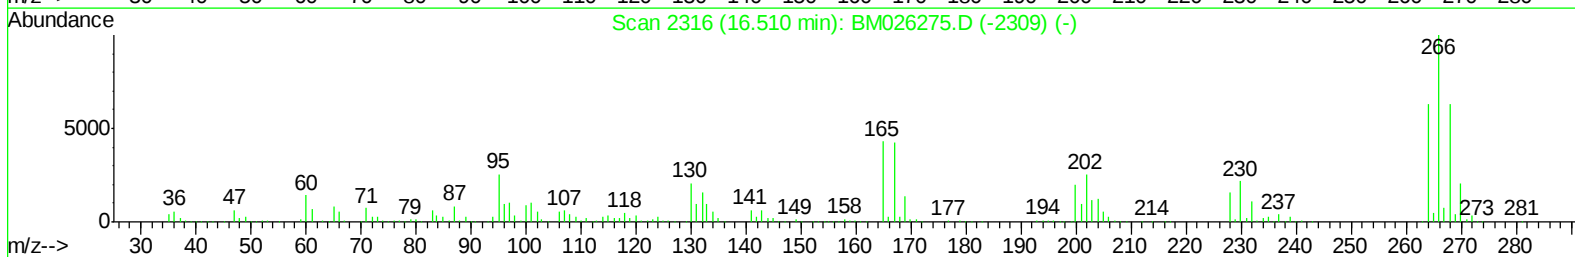
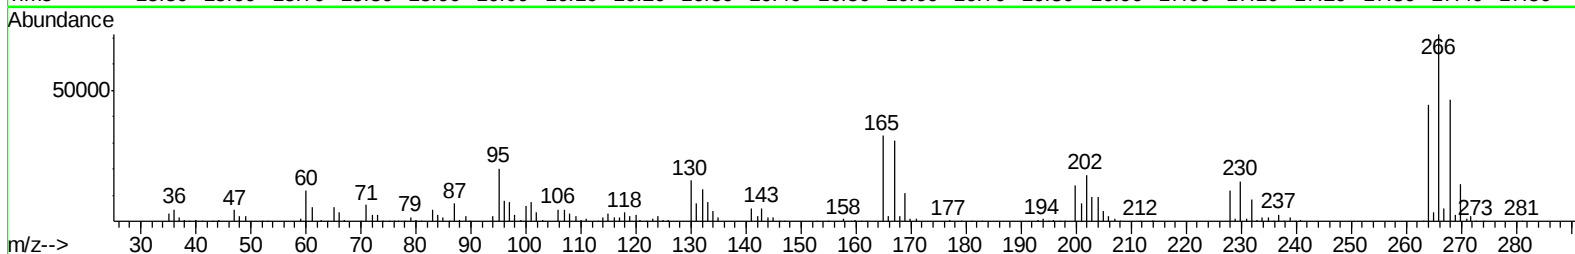


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061520\
Data File : BM026399.D
Acq On : 15 Jun 2020 19:44
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 16 01:32:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 15 12:22:53 2020
Response via : Initial Calibration

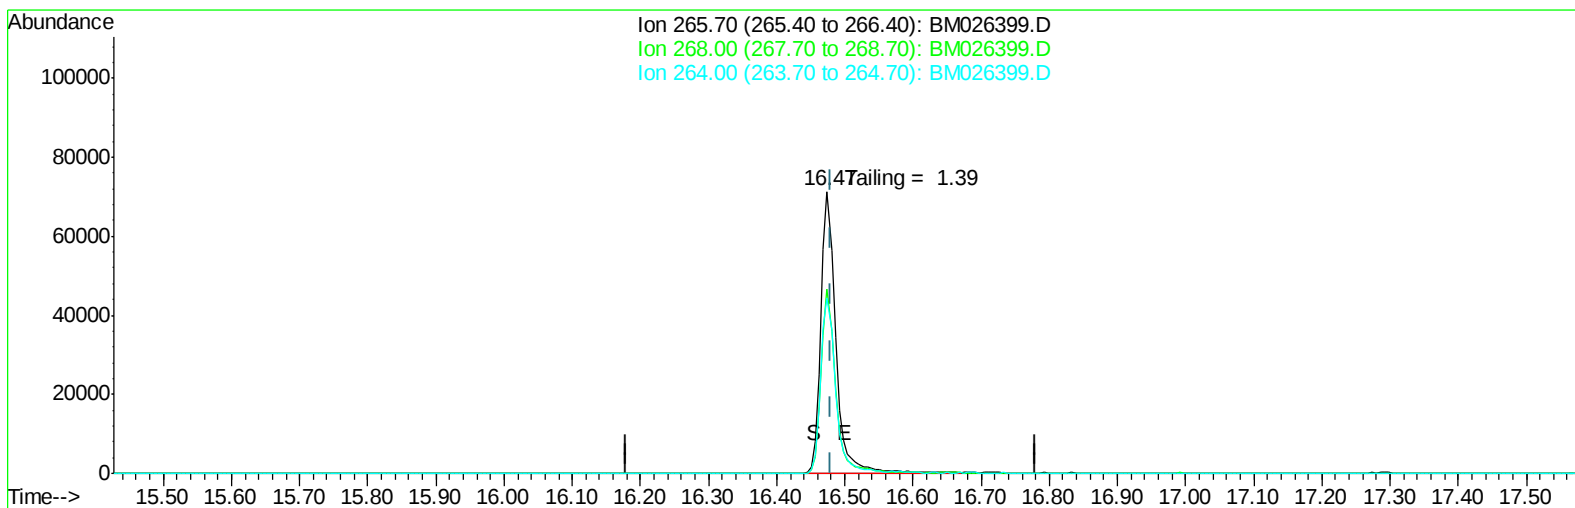

TIC: BM026399.D

(70) Pentachlorophenol (C)




16.474min (-0.006) 229054.72ng

response 106160

Ion	Exp%	Act%
265.70	100	100
268.00	62.80	65.39
264.00	63.20	62.27
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061520\
 Data File : BM026399.D
 Acq On : 15 Jun 2020 19:44
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 16 01:32:34 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM060520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 15 12:22:53 2020
 Response via : Initial Calibration

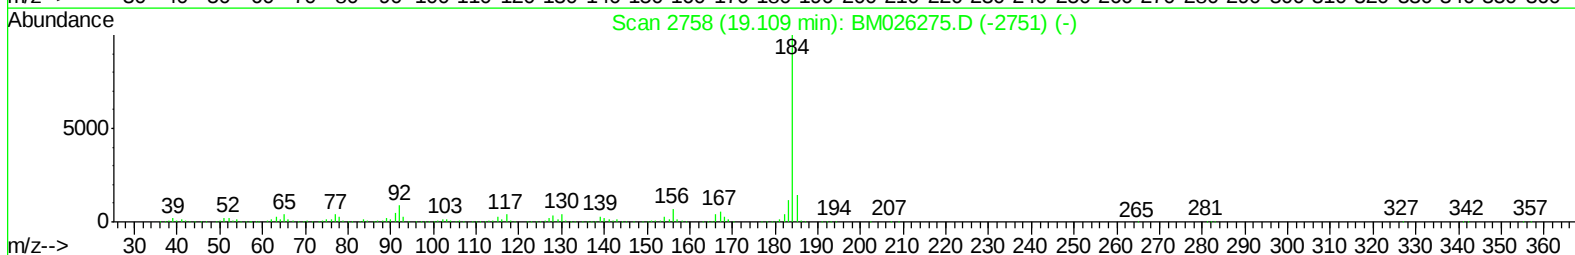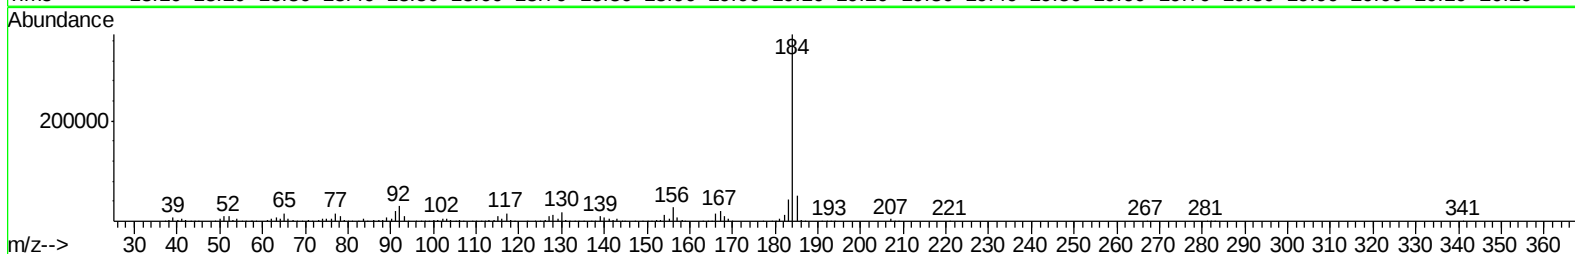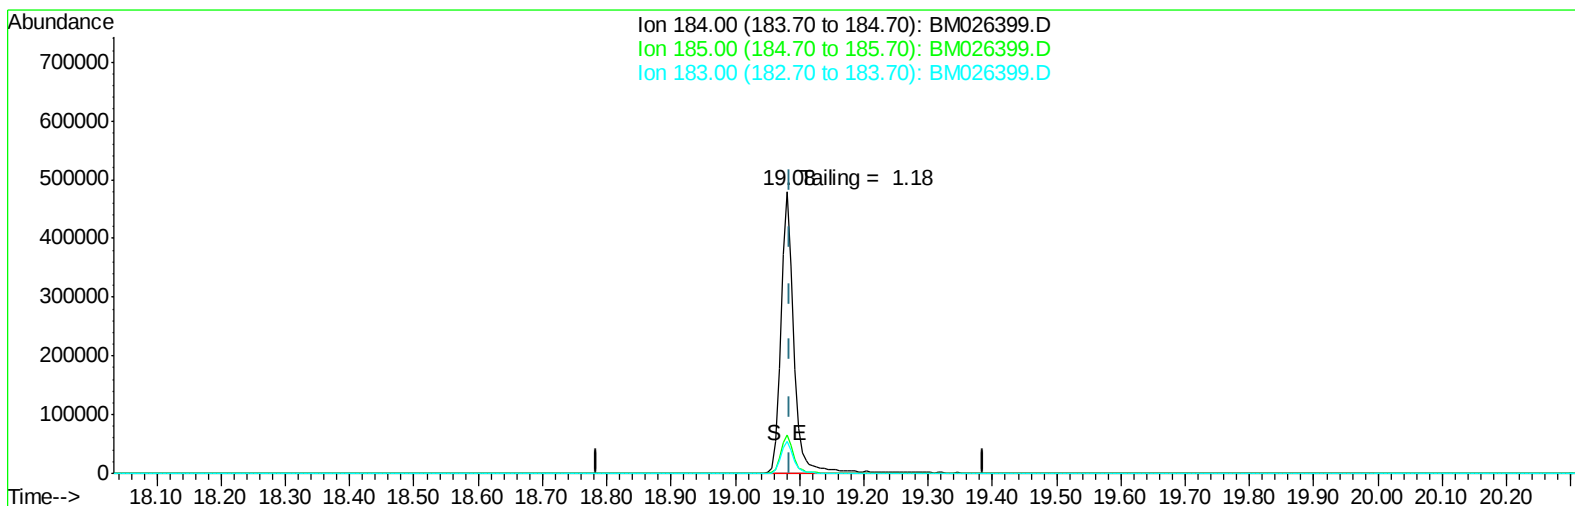

TIC: BM026399.D

(77) Benzidine

19.080min (-0.006) 68752.61ng

response 668350

Ion	Exp%	Act%
184.00	100	100
185.00	14.00	13.83
183.00	11.80	11.46
0.00	0.00	0.00