


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM061520\
 Data File : BM026384.D
 Acq On : 15 Jun 2020 09:44
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM060520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 15 12:22:53 2020

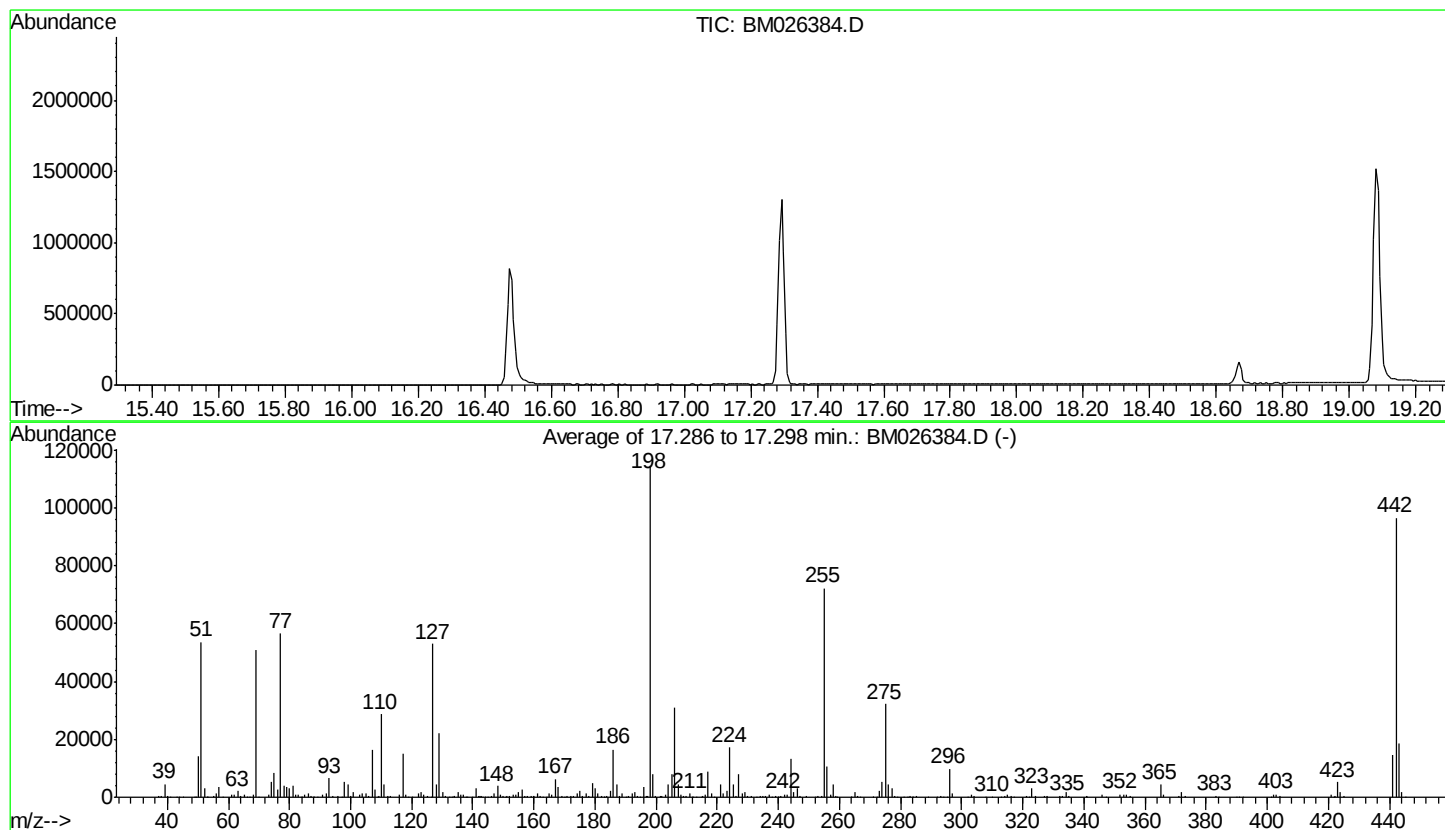

AutoFind: Scans 2448, 2449, 2450; Background Corrected with Scan 2442

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.8	53656	PASS
68	69	0.00	2	1.9	956	PASS
69	198	0.00	100	44.3	50720	PASS
70	69	0.00	2	0.5	229	PASS
127	198	10	80	46.3	53029	PASS
197	198	0.00	2	0.5	606	PASS
198	198	100	100	100.0	114584	PASS
199	198	5	9	6.8	7805	PASS
275	198	10	60	28.0	32133	PASS
365	198	1	100	3.7	4270	PASS
441	198	0.01	100	12.9	14749	PASS
442	198	50	100	84.2	96440	PASS
443	442	15	24	19.3	18599	PASS