


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM061520\
 Data File : BM026399.D
 Acq On : 15 Jun 2020 19:44
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM060520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 15 12:22:53 2020

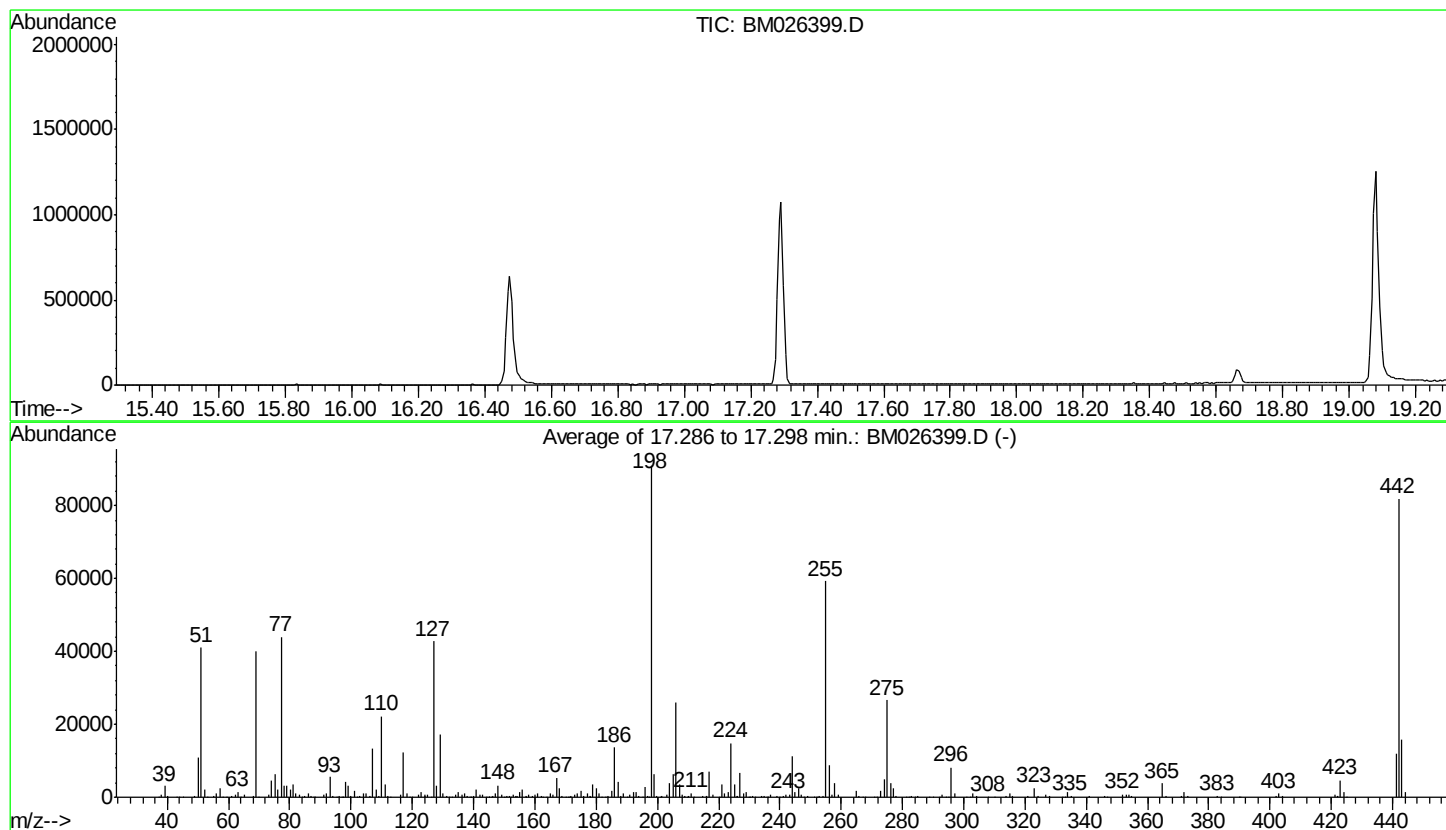

AutoFind: Scans 2448, 2449, 2450; Background Corrected with Scan 2441

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.1	41024	PASS
68	69	0.00	2	1.3	531	PASS
69	198	0.00	100	44.1	40058	PASS
70	69	0.00	2	0.4	161	PASS
127	198	10	80	47.0	42693	PASS
197	198	0.00	2	0.5	431	PASS
198	198	100	100	100.0	90930	PASS
199	198	5	9	6.8	6156	PASS
275	198	10	60	29.3	26650	PASS
365	198	1	100	4.1	3703	PASS
441	198	0.01	100	13.2	12015	PASS
442	198	50	100	90.0	81842	PASS
443	442	15	24	19.3	15781	PASS