


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM061521\
Data File : BM030460.D
Acq On : 15 Jun 2021 23:58
Operator : CG/JU
Sample : M2662-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDM1

Manual Integrations
APPROVED

mohammad
6/16/2021 8:32:21 AM

Quant Time: Jun 16 01:52:53 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM060121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 15 20:50:06 2021
Response via : Initial Calibration

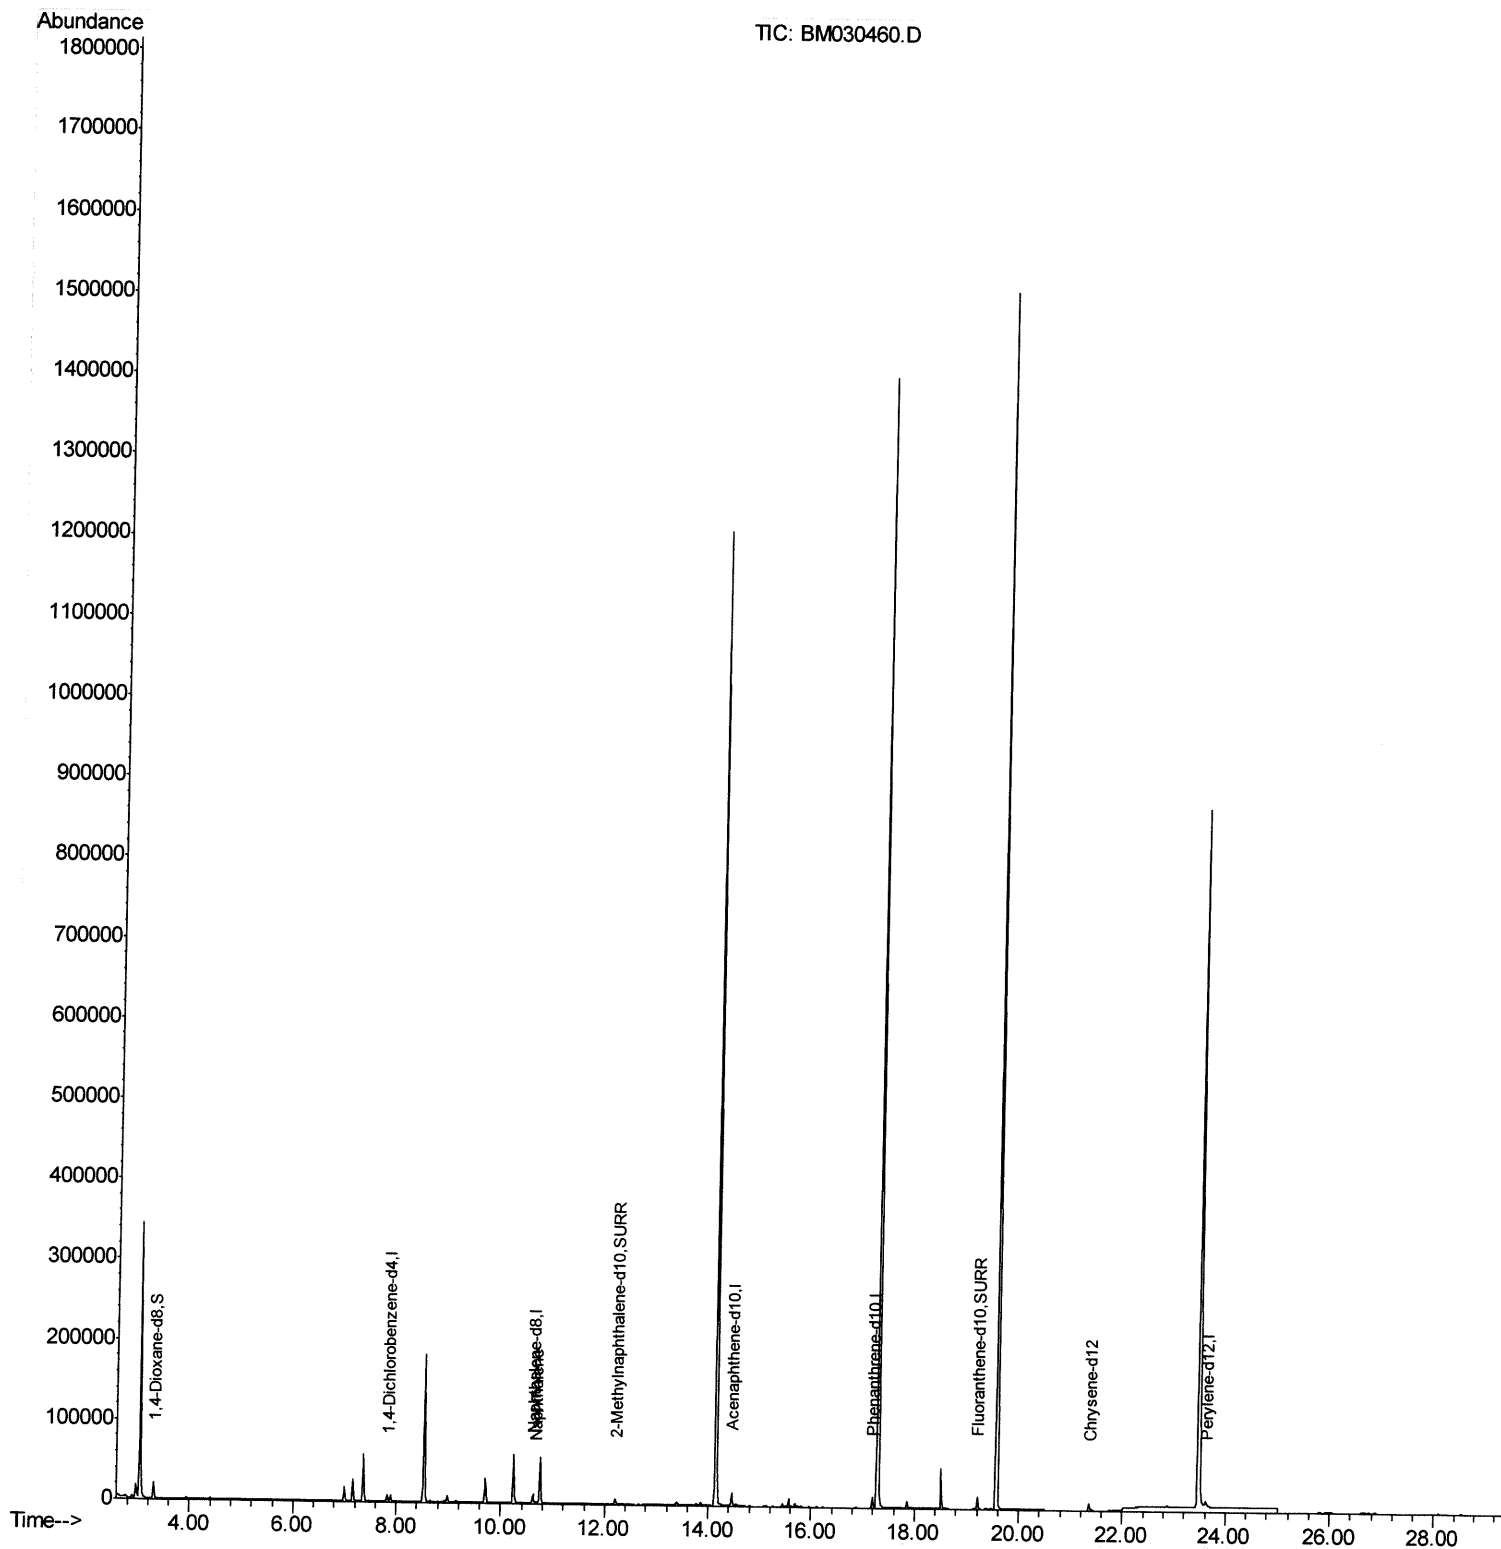


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM061521\
Data File : BM030460.D
Acq On : 15 Jun 2021 23:58
Operator : CG/JU
Sample : M2662-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDM1

Manual Integrations
APPROVED

mohammad
6/16/2021 8:32:21 AM

Quant Time: Jun 16 01:49:54 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM060121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 15 20:50:06 2021
Response via : Initial Calibration

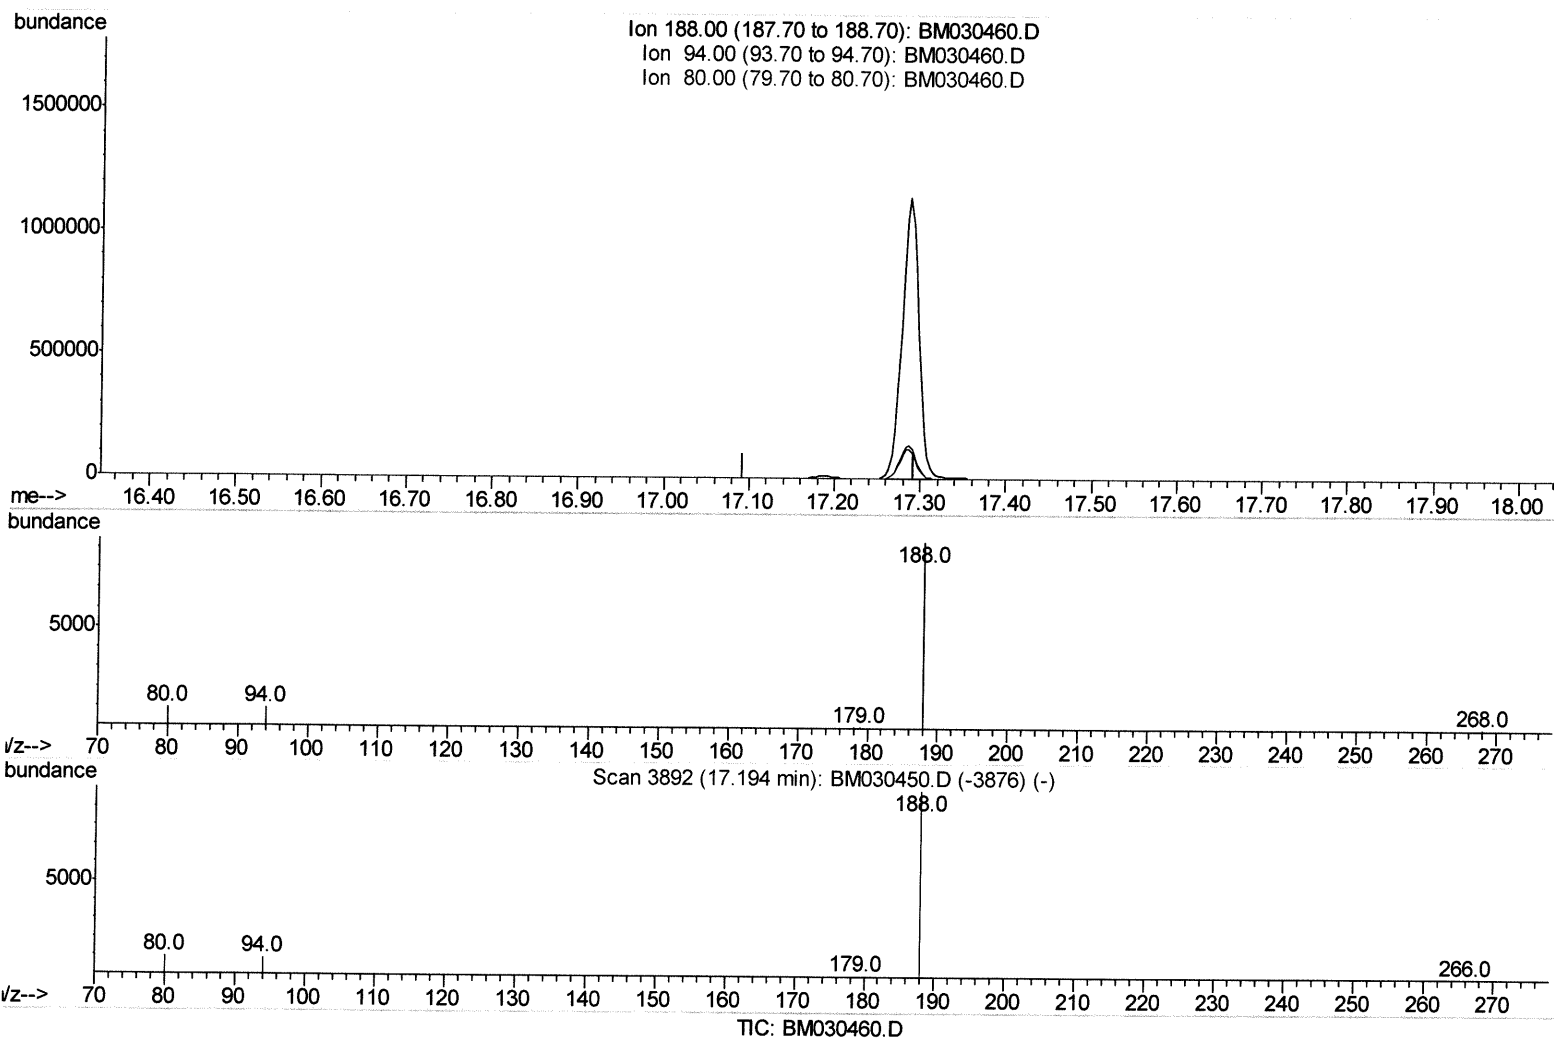

(13) Phenanthrene-d10 (I)

17.194min (-17.194) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.80	0.00#
80.00	12.90	0.00#
0.00	0.00	0.00


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM061521\
 Data File : BM030460.D
 Acq On : 15 Jun 2021 23:58
 Operator : CG/JU
 Sample : M2662-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDM1

Manual Integrations
 APPROVED

mohammad
 6/16/2021 8:32:21 AM

Quant Time: Jun 16 01:49:54 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM060121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 15 20:50:06 2021
 Response via : Initial Calibration

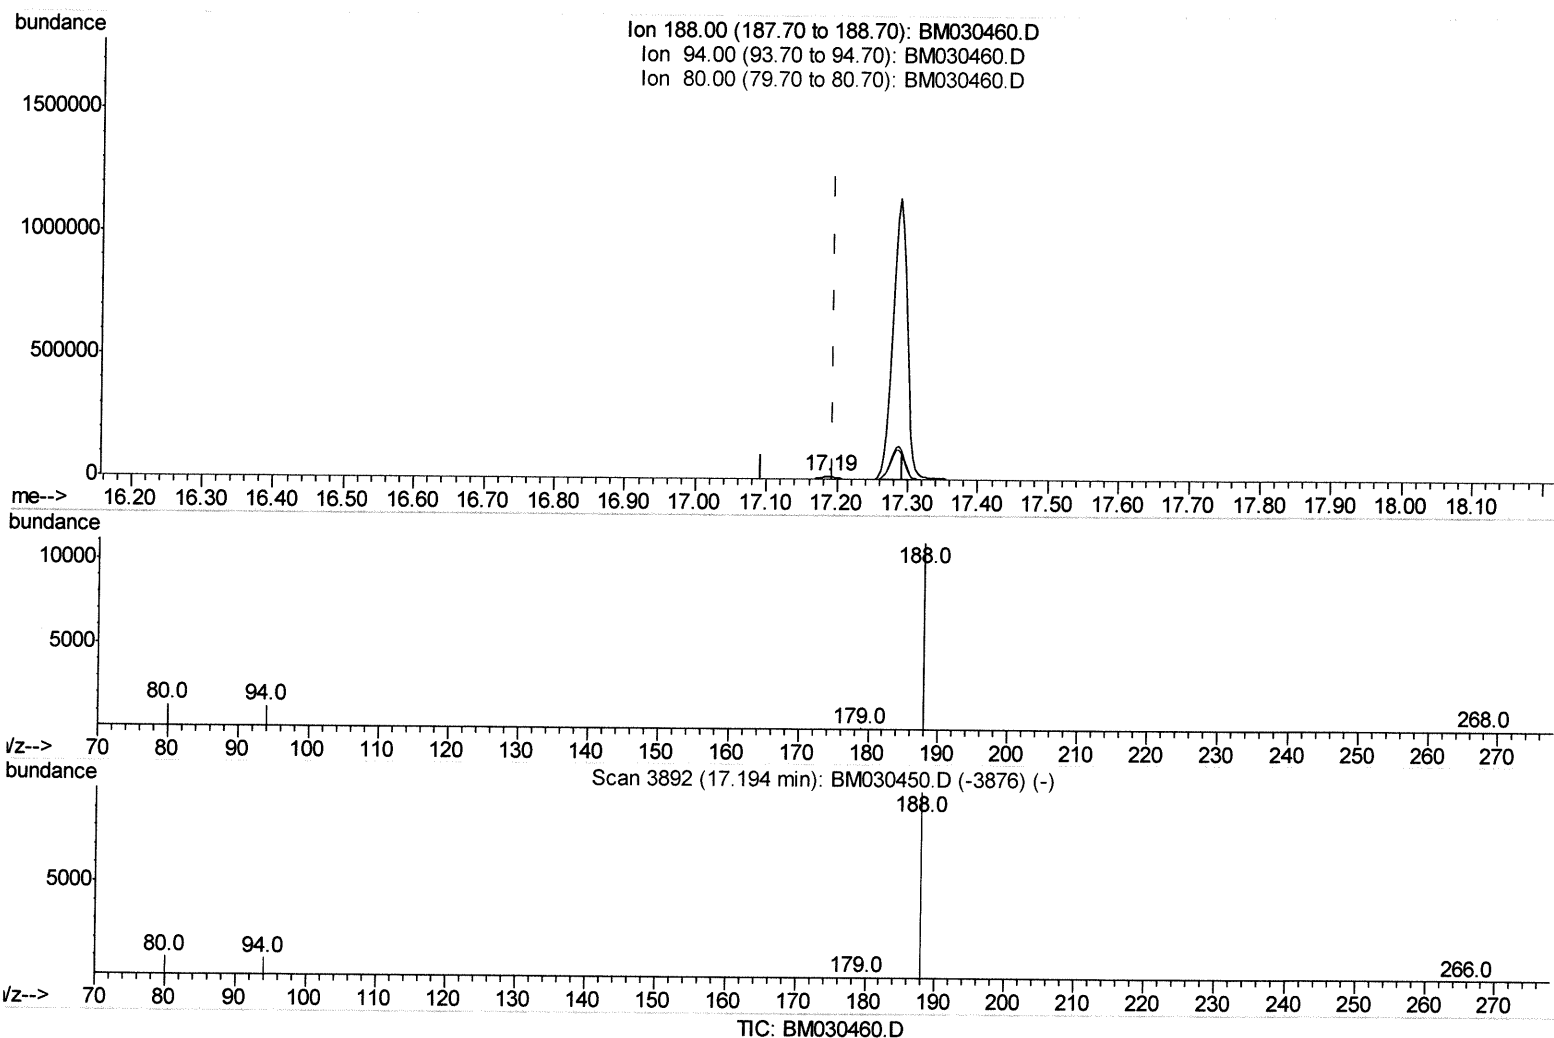

(13) Phenanthrene-d10 (I)

17.186min (-0.007) 0.40ng/ul m

JU 6/20/21

response 15978

Ion	Exp%	Act%
188.00	100	100
94.00	11.80	10.72
80.00	12.90	11.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM061521\
 Data File : BM030460.D
 Acq On : 15 Jun 2021 23:58
 Operator : CG/JU
 Sample : M2662-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDM1

Manual Integrations
 APPROVED

mohammad
 6/16/2021 8:32:21 AM

Quant Time: Jun 16 01:52:53 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM060121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 15 20:50:06 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	4063	0.40	ng/ul	0.00
4) Naphthalene-d8	10.62	136	15162	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.45	164	9641	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.19	188	15978m	0.40	ng/ul	0.00
17) Chrysene-d12	21.35	240	10007	0.40	ng/ul	0.00
23) Perylene-d12	23.62	264	11691	0.40	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.30	96	12961	3.25	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.20	152	10039	0.46	ng/ul	0.00
18) Fluoranthene-d10	19.21	212	17273	0.51	ng/ul	0.00
Target Compounds						
5) Naphthalene	10.66	128	952	0.021	ng/ul#	Ovalue 78

(#) = qualifier out of range (m) = manual integration (+) = signals summed

201 6/30/21