
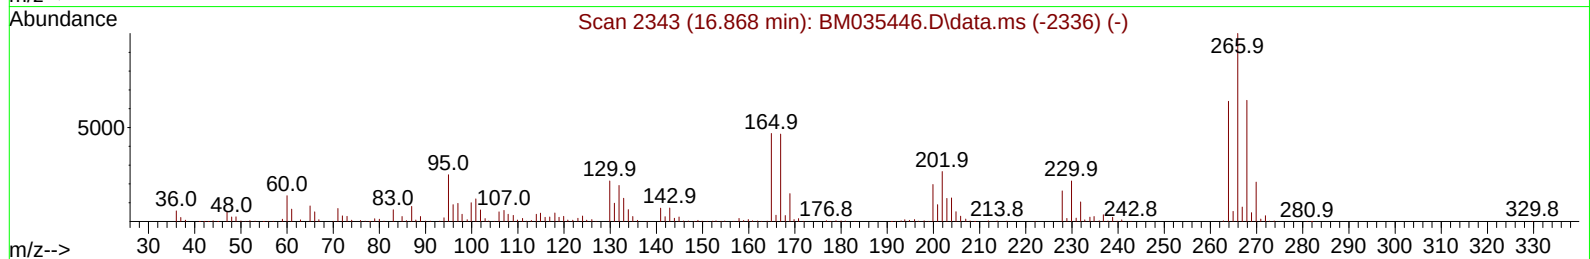
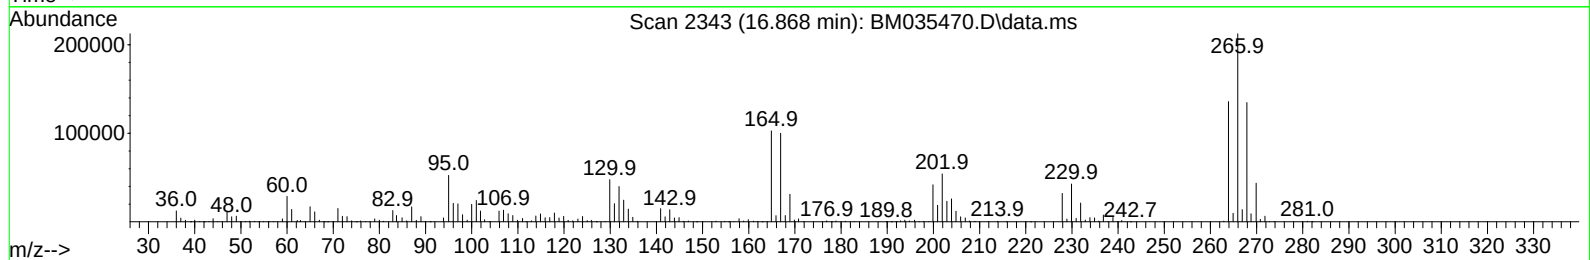


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM061522\  
 Data File : BM035470.D  
 Acq On : 15 Jun 2022 10:01  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 16 00:31:51 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM061022.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jun 10 16:05:33 2022  
 Response via : Initial Calibration

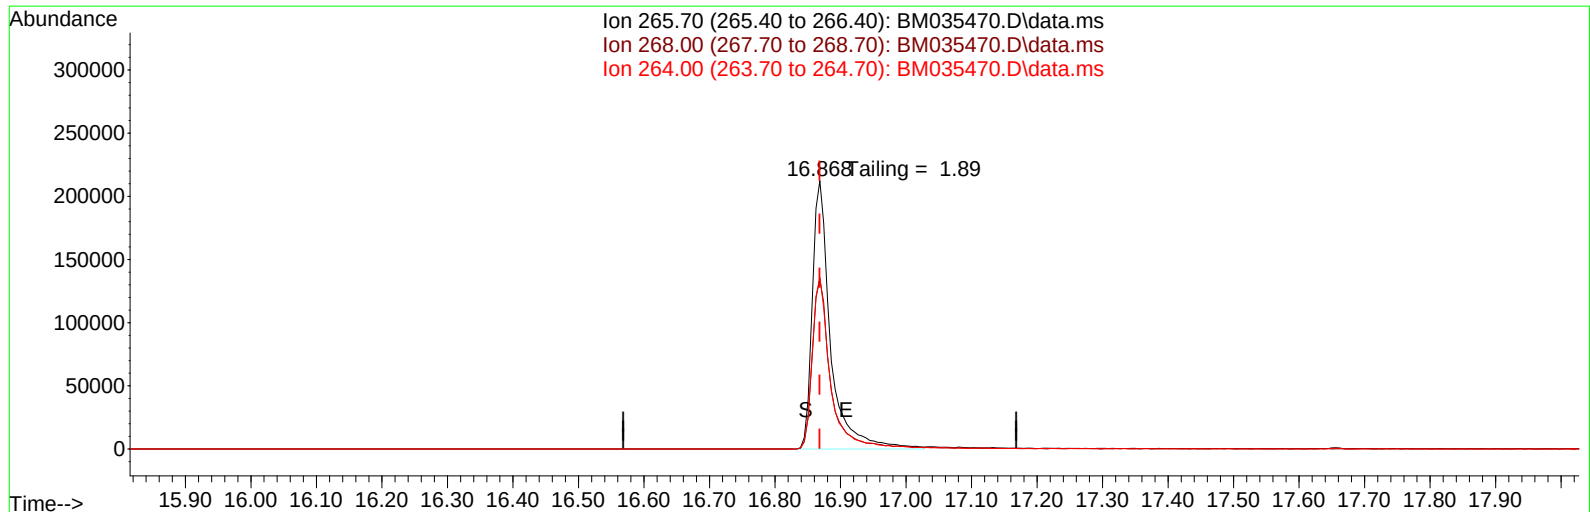

TIC: BM035470.D\data.ms

**(70) Pentachlorophenol (C)**




16.868min (+ 0.000) 0.00 ng

response 413599

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 64.90  | 63.39  |
| 264.00 | 63.30  | 63.93  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM061522\  
Data File : BM035470.D  
Acq On : 15 Jun 2022 10:01  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 16 00:31:51 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM061022.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Jun 10 16:05:33 2022  
Response via : Initial Calibration

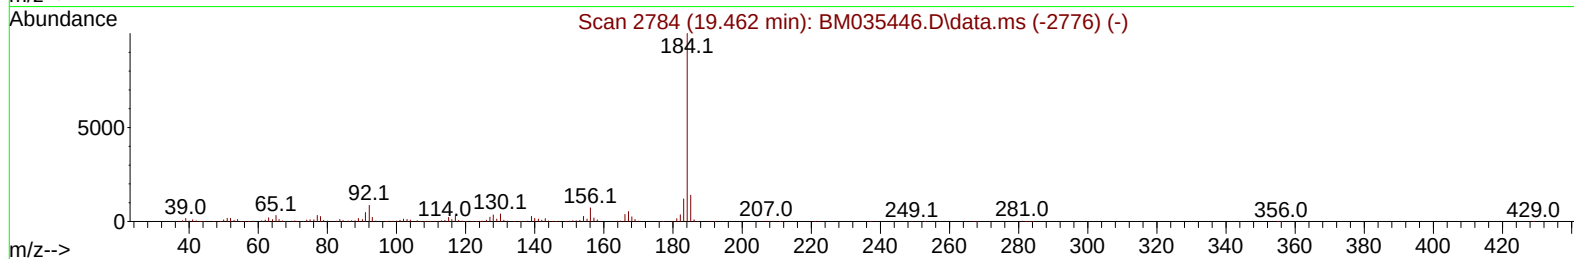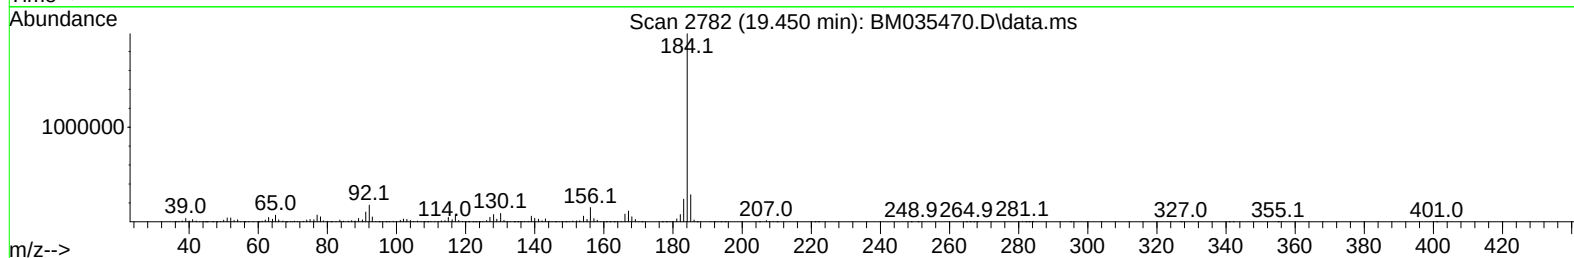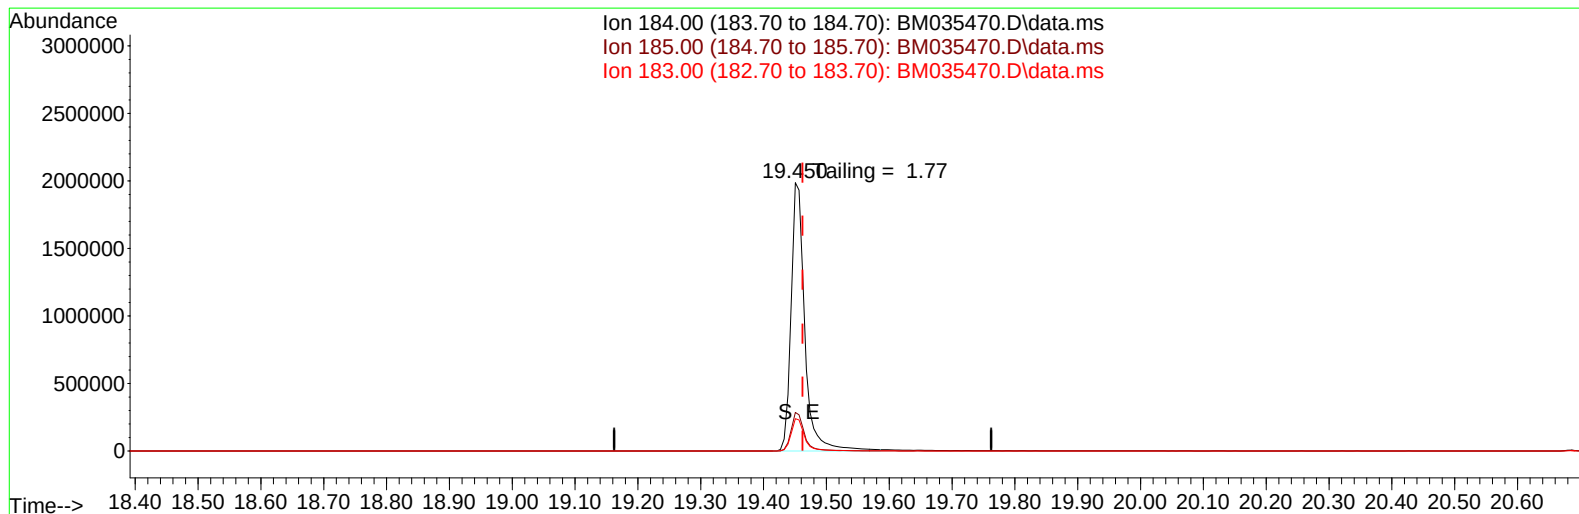

TIC: BM035470.D\data.ms

**(77) Benzidine****19.450min (-0.012) 2169512.31 ng****response 3070896**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.10  | 14.38  |
| 183.00 | 11.90  | 12.04  |
| 0.00   | 0.00   | 0.00   |