

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061522\
 Data File : BM035472.D
 Acq On : 15 Jun 2022 11:14
 Operator : CG/JU
 Sample : PB145531BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB145531BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035472.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.946	311	316	328	rBV	141651	210628	1.19%	0.242%
2	5.405	388	394	420	rBV	6355284	9527805	53.92%	10.933%
3	7.005	658	666	700	rBV	5853600	10042251	56.83%	11.523%
4	7.816	797	804	815	rBV	1079452	1772683	10.03%	2.034%
5	8.981	994	1002	1024	rBV	3600094	6311798	35.72%	7.243%
6	10.616	1272	1280	1302	rBV	1387737	2683945	15.19%	3.080%
7	13.081	1692	1699	1716	rBV	9330280	14342733	81.17%	16.458%
8	14.457	1926	1933	1959	rBV	2246364	3590127	20.32%	4.120%
9	15.951	2180	2187	2220	rBV	6066842	9897724	56.01%	11.357%
10	17.204	2394	2400	2418	rBV	2554825	3989128	22.57%	4.577%
11	19.833	2841	2847	2861	rBV	13902944	17670964	100.00%	20.277%
12	21.392	3107	3112	3125	rBV	2616996	3855567	21.82%	4.424%
13	23.739	3504	3511	3525	rVB2	1416446	3252633	18.41%	3.732%




Sum of corrected areas: 87147986

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061522\
Data File : BM035472.D
Acq On : 15 Jun 2022 11:14
Operator : CG/JU
Sample : PB145531BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145531BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

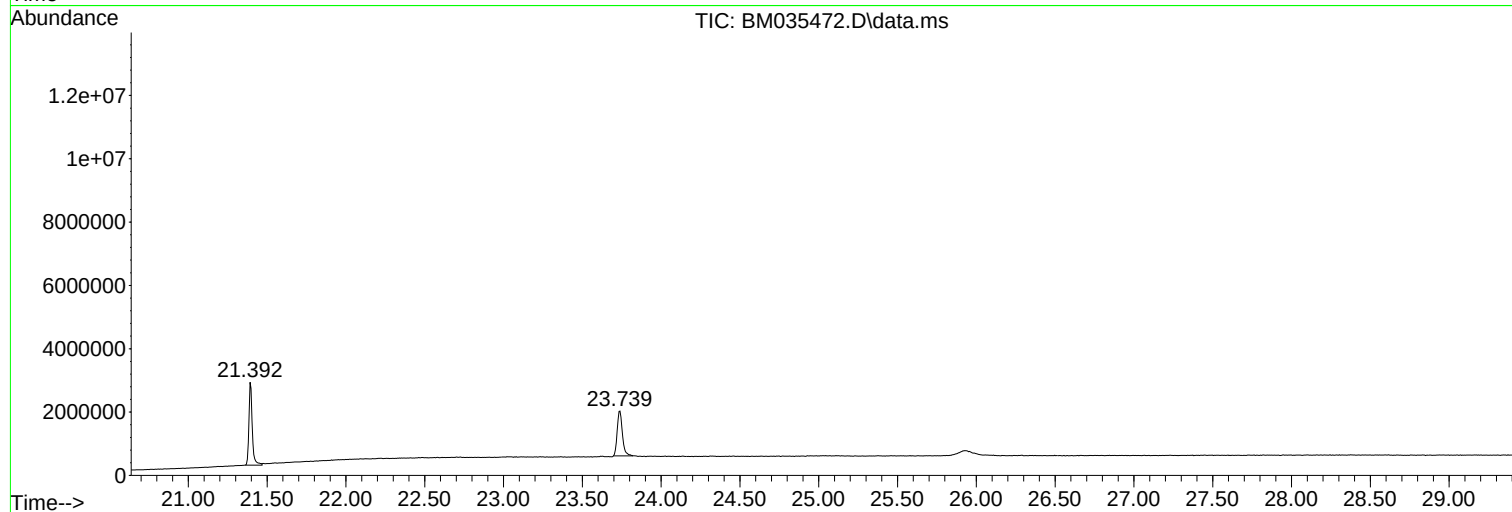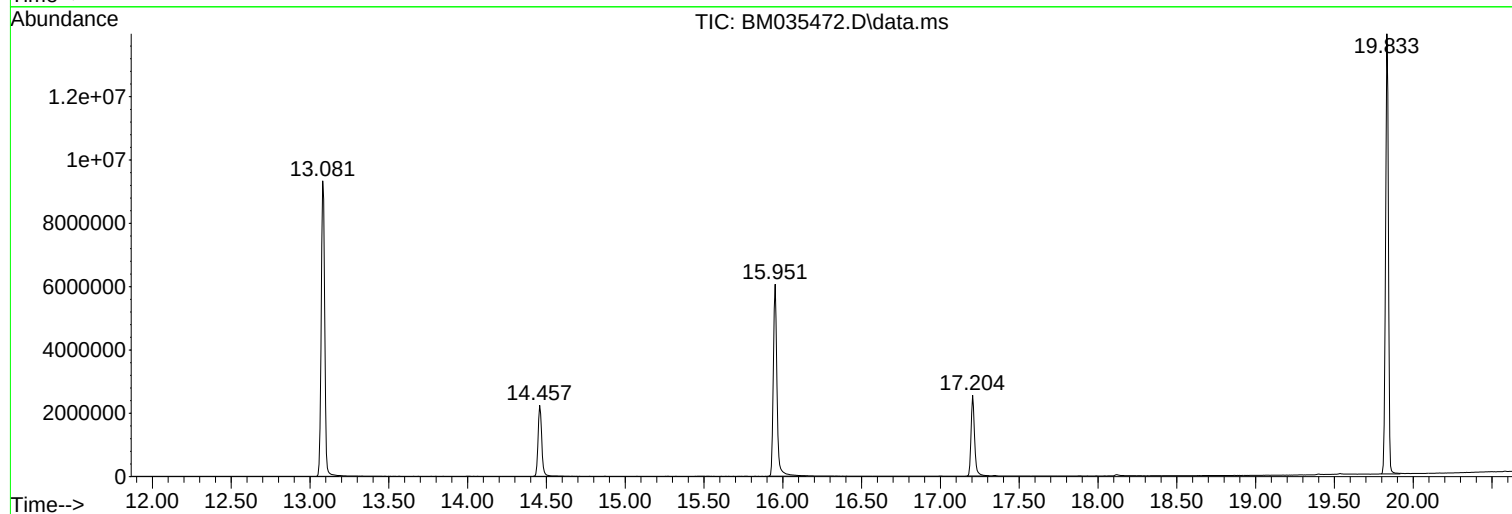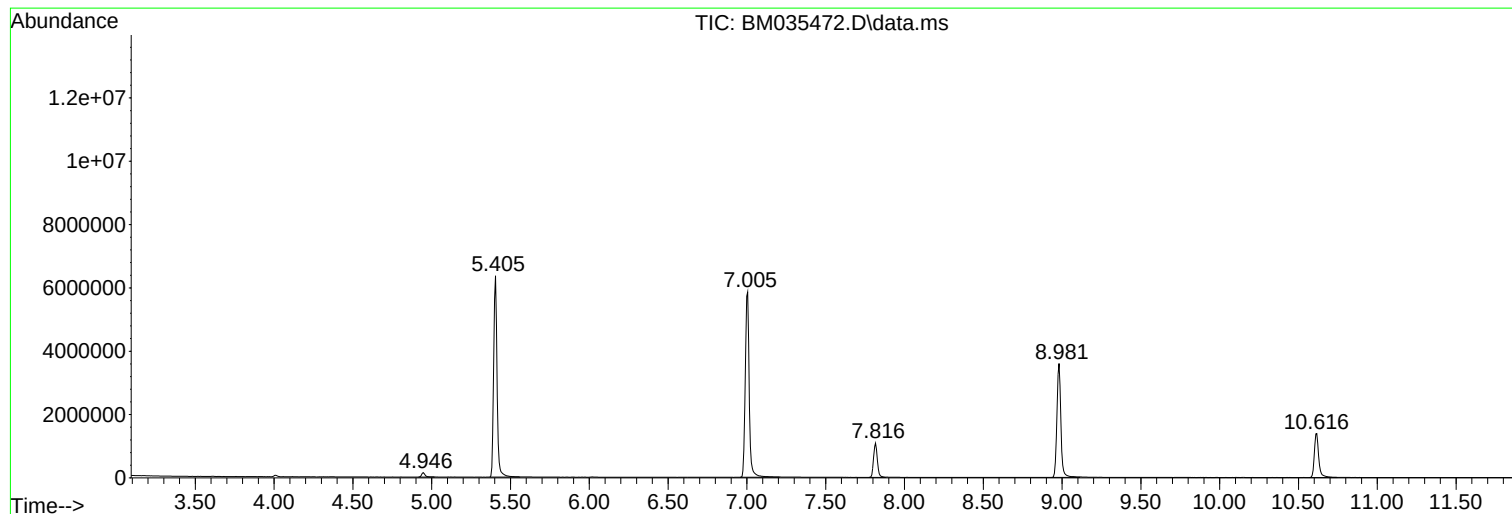

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061522\
Data File : BM035472.D
Acq On : 15 Jun 2022 11:14
Operator : CG/JU
Sample : PB145531BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145531BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.946	2.38 ng	210628	1,4-Dichlorobenzene-d4	7.816

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64		
2	3-Hydroxy-3-methyl-2-butanone	102	C5H10O2	000115-22-0	23		
3	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	12		
4	5-Hexen-2-one	98	C6H10O	000109-49-9	9		
5	Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	9		

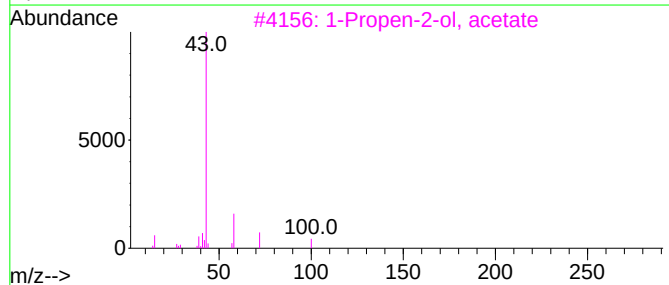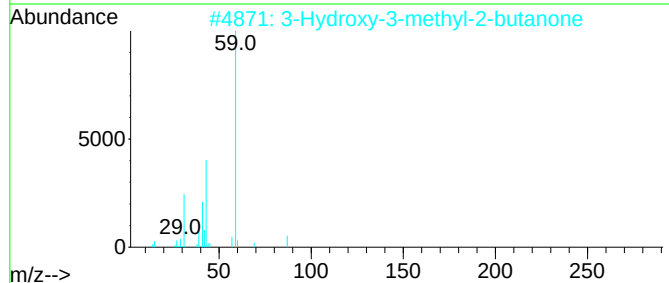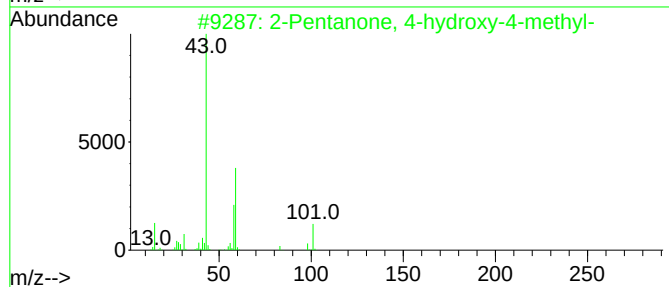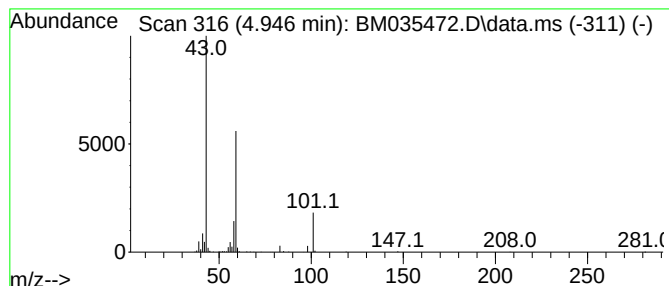

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061522\
Data File : BM035472.D
Acq On : 15 Jun 2022 11:14
Operator : CG/JU
Sample : PB145531BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145531BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.946	2.4	ng	210628	1	7.816	1772680	20.0