

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061522\
 Data File : BM035476.D
 Acq On : 15 Jun 2022 16:58
 Operator : CG/JU
 Sample : PB145557BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB145557BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035476.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.404	388	394	414	rBV	4796244	7310276	42.78%	9.653%
2	7.004	658	666	694	rBV	4335964	7603557	44.50%	10.040%
3	7.816	797	804	819	rBV	850647	1425800	8.34%	1.883%
4	8.981	994	1002	1021	rBV	2733161	4810923	28.16%	6.353%
5	10.616	1273	1280	1304	rBV	1121003	2145263	12.55%	2.833%
6	13.080	1692	1699	1715	rBV	7658793	11675491	68.33%	15.417%
7	14.457	1925	1933	1949	rBV	1856576	2980441	17.44%	3.936%
8	15.951	2180	2187	2218	rBV	5375716	8578622	50.20%	11.328%
9	17.204	2394	2400	2420	rBV	2201653	3645273	21.33%	4.813%
10	18.115	2550	2555	2565	rBV	115799	248304	1.45%	0.328%
11	19.392	2768	2772	2784	rBV	79358	178109	1.04%	0.235%
12	19.833	2841	2847	2860	rBV	13712927	17087214	100.00%	22.563%
13	21.391	3107	3112	3123	rBV	2950929	4108818	24.05%	5.426%
14	23.738	3504	3511	3524	rVB2	1845422	3933333	23.02%	5.194%




Sum of corrected areas: 75731424

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061522\
Data File : BM035476.D
Acq On : 15 Jun 2022 16:58
Operator : CG/JU
Sample : PB145557BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145557BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

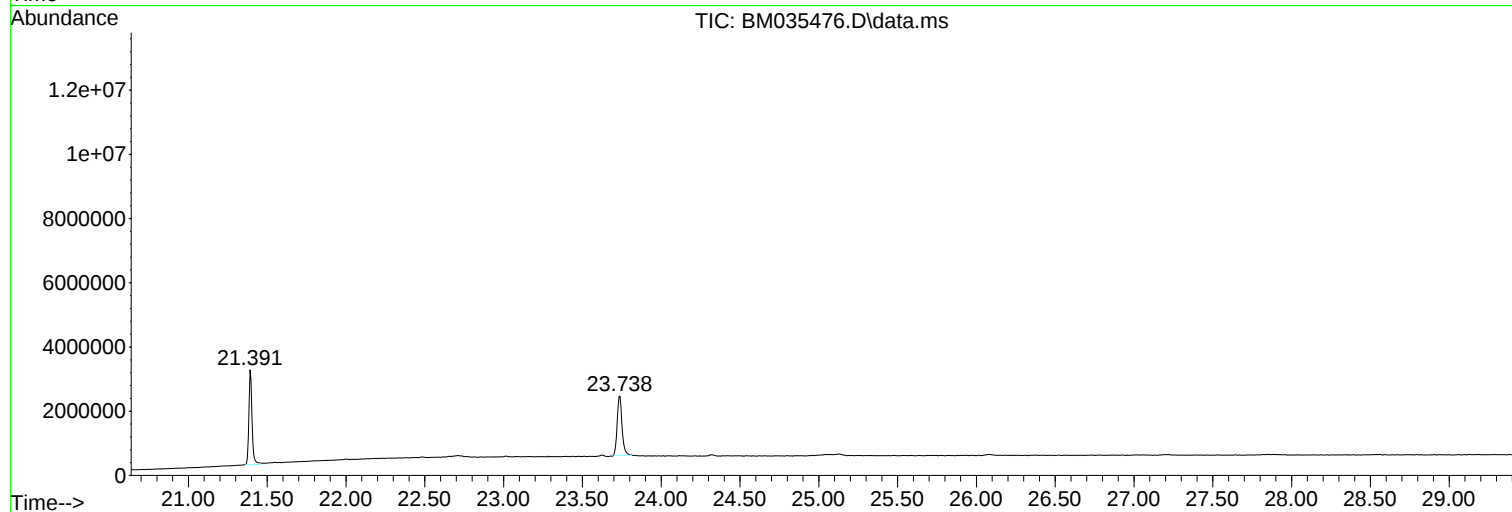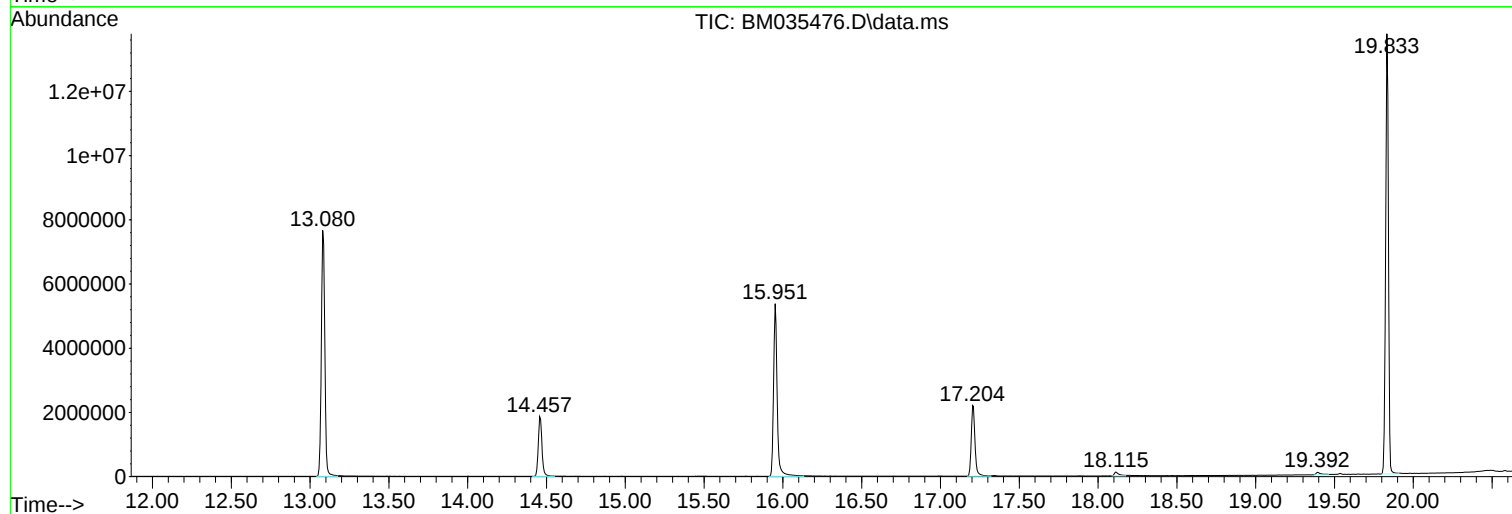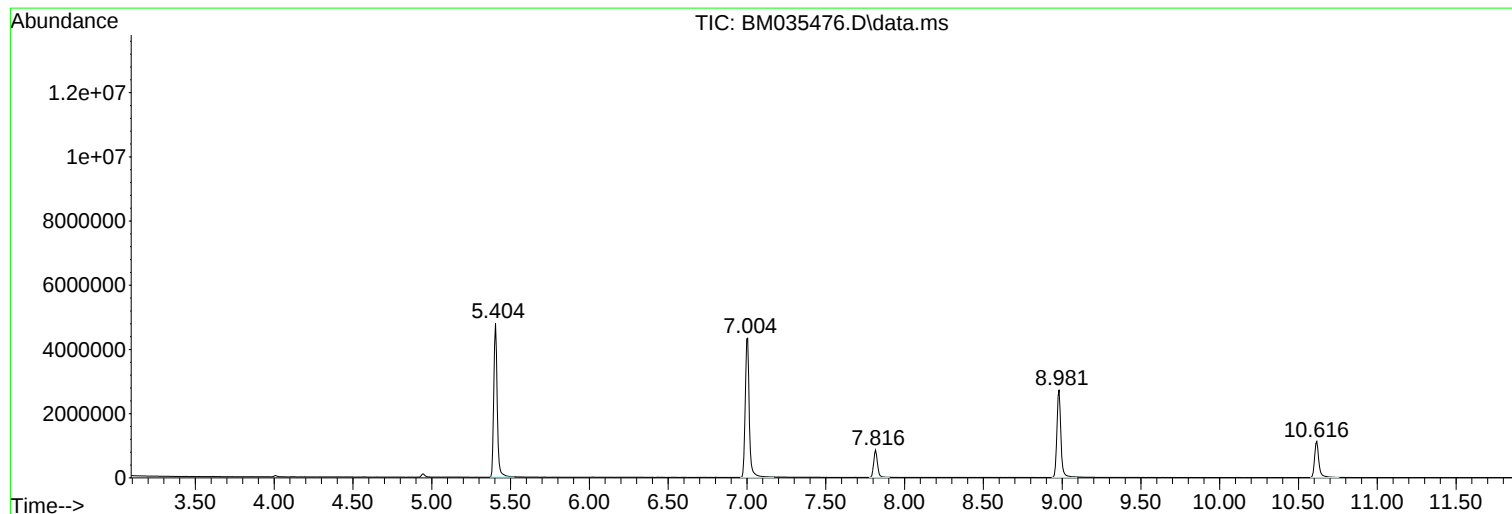

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061522\
Data File : BM035476.D
Acq On : 15 Jun 2022 16:58
Operator : CG/JU
Sample : PB145557BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145557BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061522\
Data File : BM035476.D
Acq On : 15 Jun 2022 16:58
Operator : CG/JU
Sample : PB145557BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145557BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------