


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061522\
 Data File : BM035470.D
 Acq On : 15 Jun 2022 10:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 10 16:05:33 2022

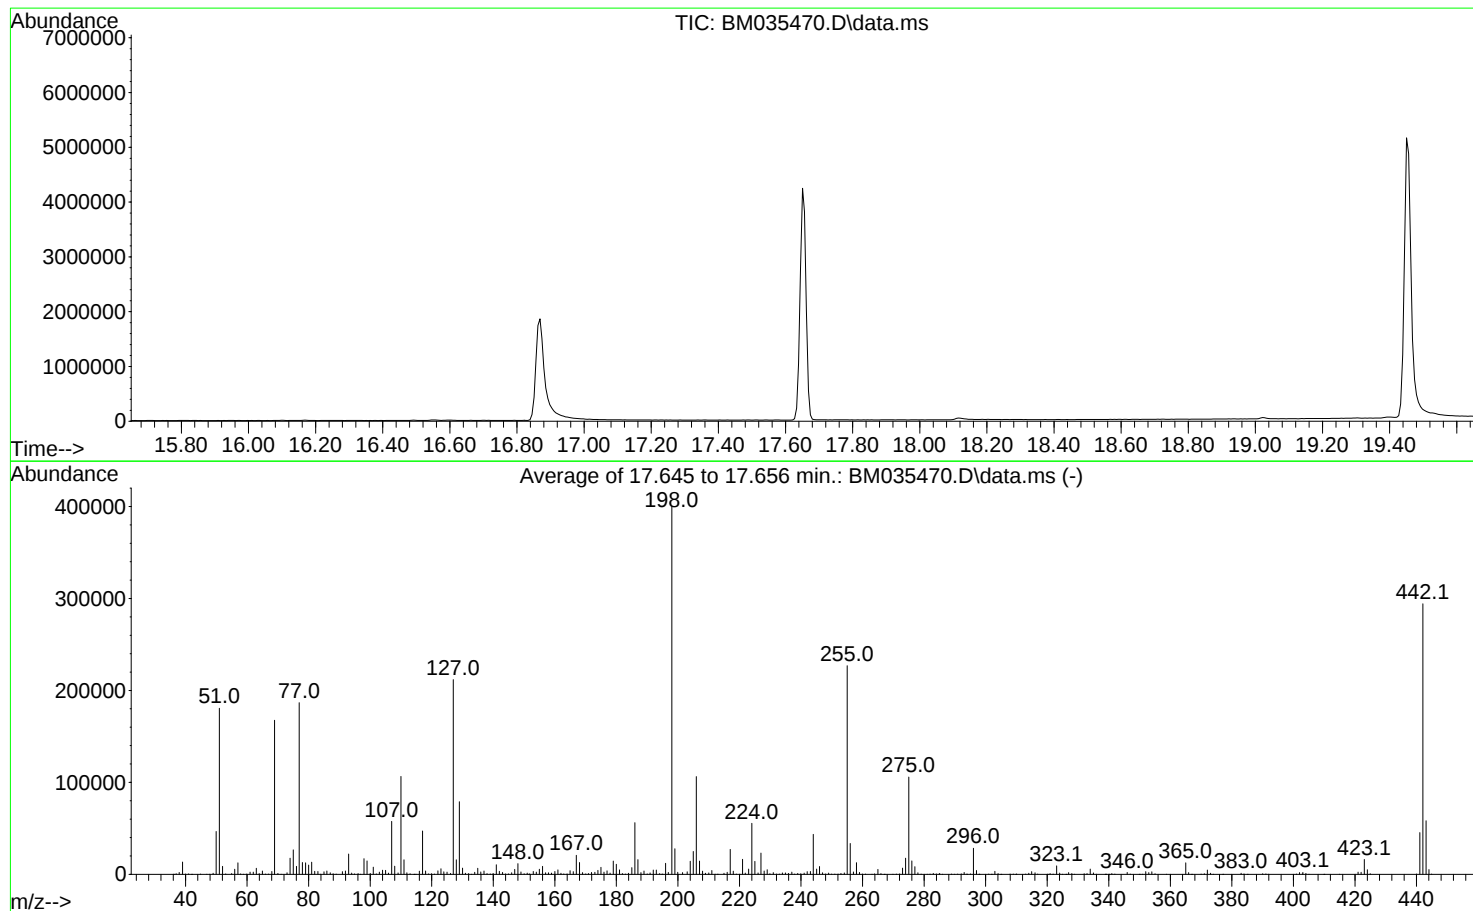

AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.2	180633	PASS
68	69	0.00	2	1.8	3064	PASS
69	198	0.00	100	41.9	167492	PASS
70	69	0.00	2	0.6	1001	PASS
127	198	10	80	52.9	211755	PASS
197	198	0.00	2	0.5	2133	PASS
198	198	100	100	100.0	400021	PASS
199	198	5	9	7.0	27888	PASS
275	198	10	60	26.5	105819	PASS
365	198	1	100	3.1	12478	PASS
441	198	0.01	100	11.4	45491	PASS
442	442	50	100	100.0	294208	PASS
443	442	15	24	19.8	58336	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/15/2022	BNA_M	<u>BM035470.D</u>
Compound Name	Response	Retention Time
DDT	1479909	20.686
DDD	15157	20.25
DDE	4627	19.745
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19784	1499693	1.32

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061522\
 Data File : BM035470.D
 Acq On : 15 Jun 2022 10:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jun 16 00:31:51 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 10 16:05:33 2022
 Response via : Initial Calibration

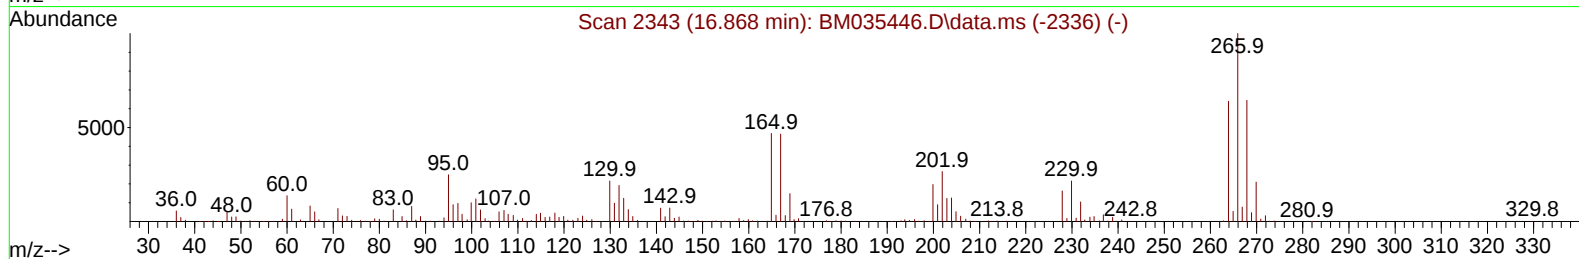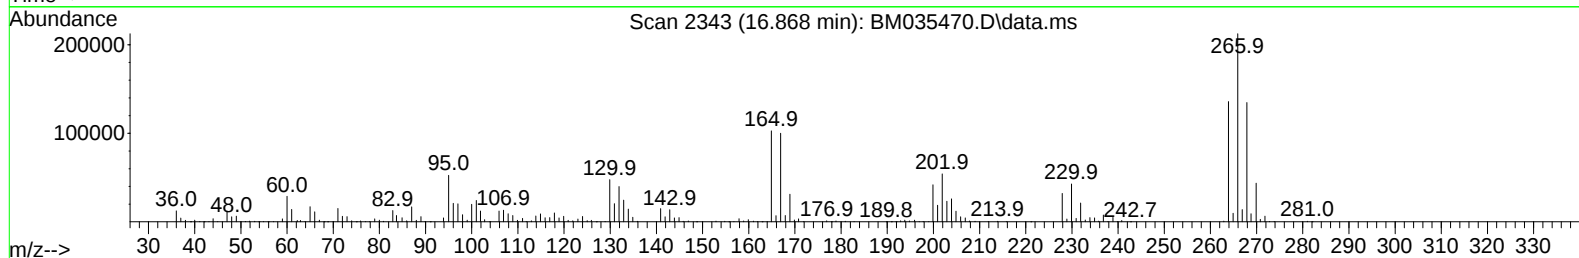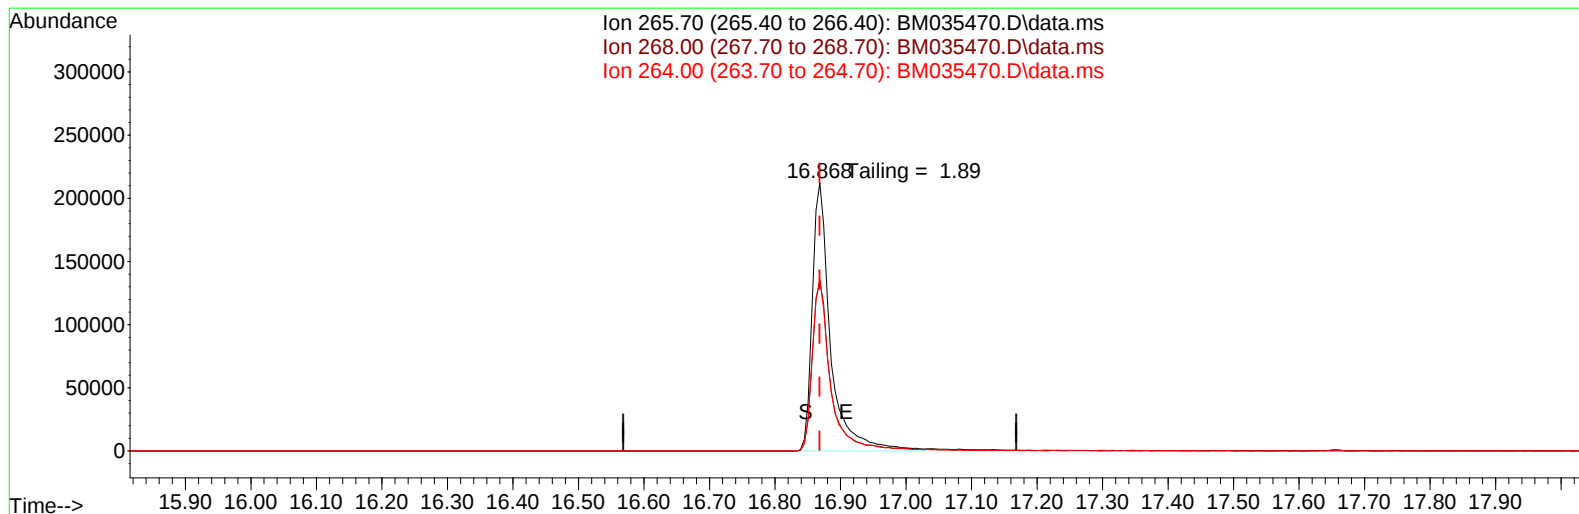

TIC: BM035470.D\data.ms

(70) Pentachlorophenol (C)

16.868min (+ 0.000) 0.00 ng




response 413599

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.39
264.00	63.30	63.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061522\
Data File : BM035470.D
Acq On : 15 Jun 2022 10:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 16 00:31:51 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM061022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 10 16:05:33 2022
Response via : Initial Calibration

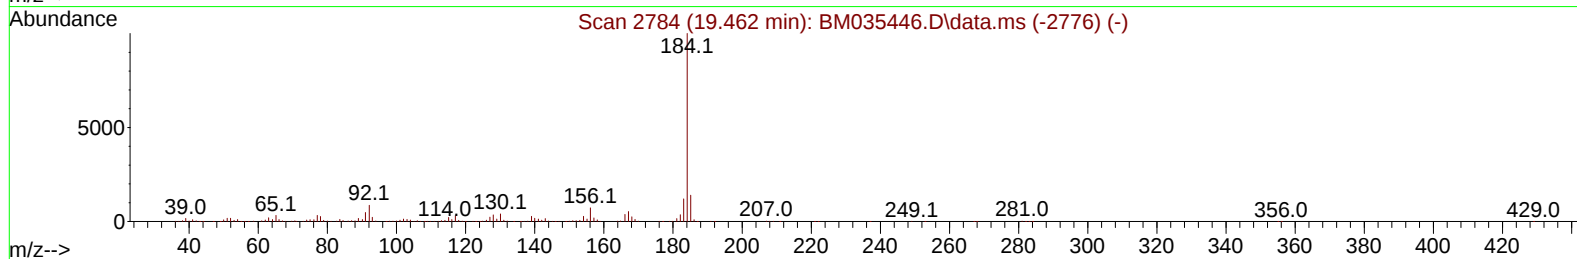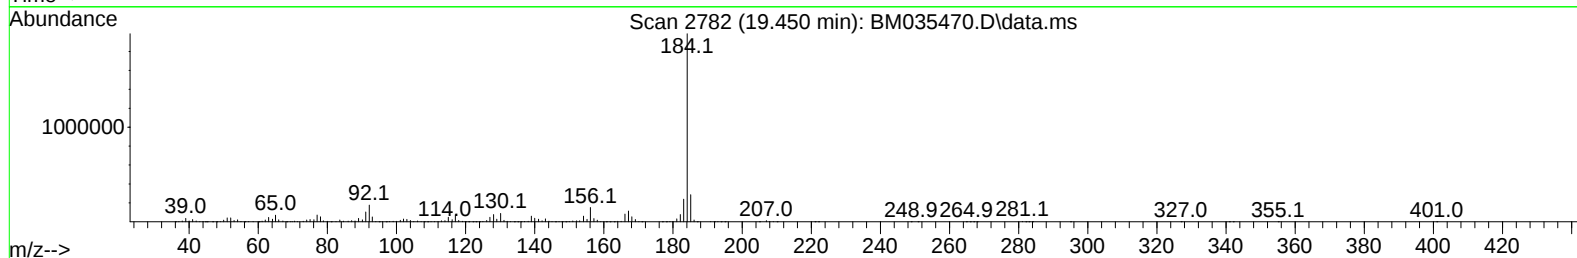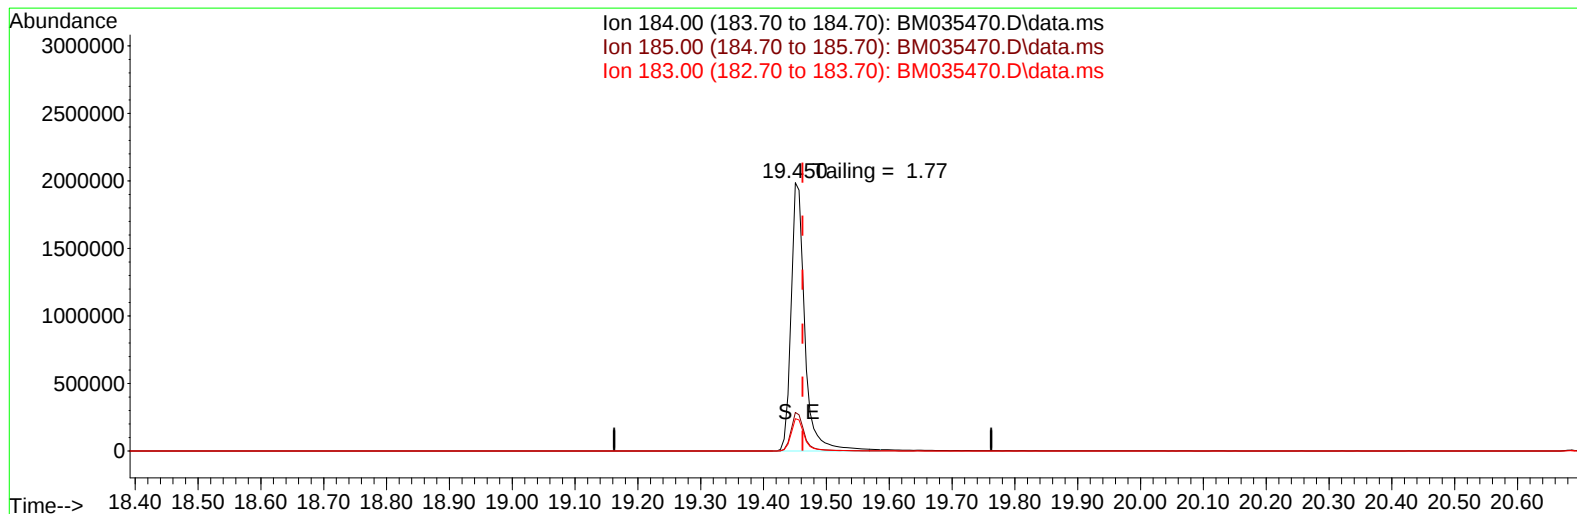

TIC: BM035470.D\data.ms

(77) Benzidine

19.450min (-0.012) 2169512.31 ng

response 3070896

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.38
183.00	11.90	12.04
0.00	0.00	0.00