

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061615\
 Data File : BM001707.D
 Acq On : 16 Jun 2015 10:51
 Operator : TP/IZ
 Sample : PB84015BL
 Misc : SBLK71
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK71

Quant Time: Jun 17 05:23:34 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061515.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 17 05:22:36 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	67862	20.00	ng/ul	0.00
18) Naphthalene-d8	10.46	136	261939	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	152668	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	340530	20.00	ng/ul	0.00
77) Chrysene-d12	21.26	240	402838	20.00	ng/ul	0.00
85) Perylene-d12	23.48	264	432652	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.14	96	7947	5.58	ng/uL	0.00
5) Phenol-d5	6.83	99	156263	29.98	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	91603	31.37	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	127117	30.84	ng/ul	0.00
13) 4-Methylphenol-d8	8.37	113	131638	31.46	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	58479	32.25	ng/ul	0.00
22) 2-Nitrophenol-d4	9.55	143	67026	33.81	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.07	165	129986	30.63	ng/ul	0.00
29) 4-Chloroaniline-d4	10.59	131	178037	41.23	ng/ul	0.00
43) Dimethylphthalate-d6	13.73	166	382322	33.77	ng/ul	0.00
46) Acenaphthylene-d8	14.01	160	478074	32.21	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	61399	29.40	ng/ul	0.00
57) Fluorene-d10	15.32	176	351657	33.48	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	61551	29.59	ng/ul	0.00
70) Anthracene-d10	17.16	188	538260	33.93	ng/ul	0.00
78) Pyrene-d10	19.46	212	611257	35.82	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.34	264	669621	35.11	ng/ul	0.00


Target Compounds					Qvalue
15) N-Nitroso-di-n-propylamine	8.37	70	3513	1.08 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061615\
Data File : BM001707.D
Acq On : 16 Jun 2015 10:51
Operator : TP/IZ
Sample : PB84015BL
Misc : SBLK71
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK71

Quant Time: Jun 17 05:23:34 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061515.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 17 05:22:36 2015
Response via : Initial Calibration

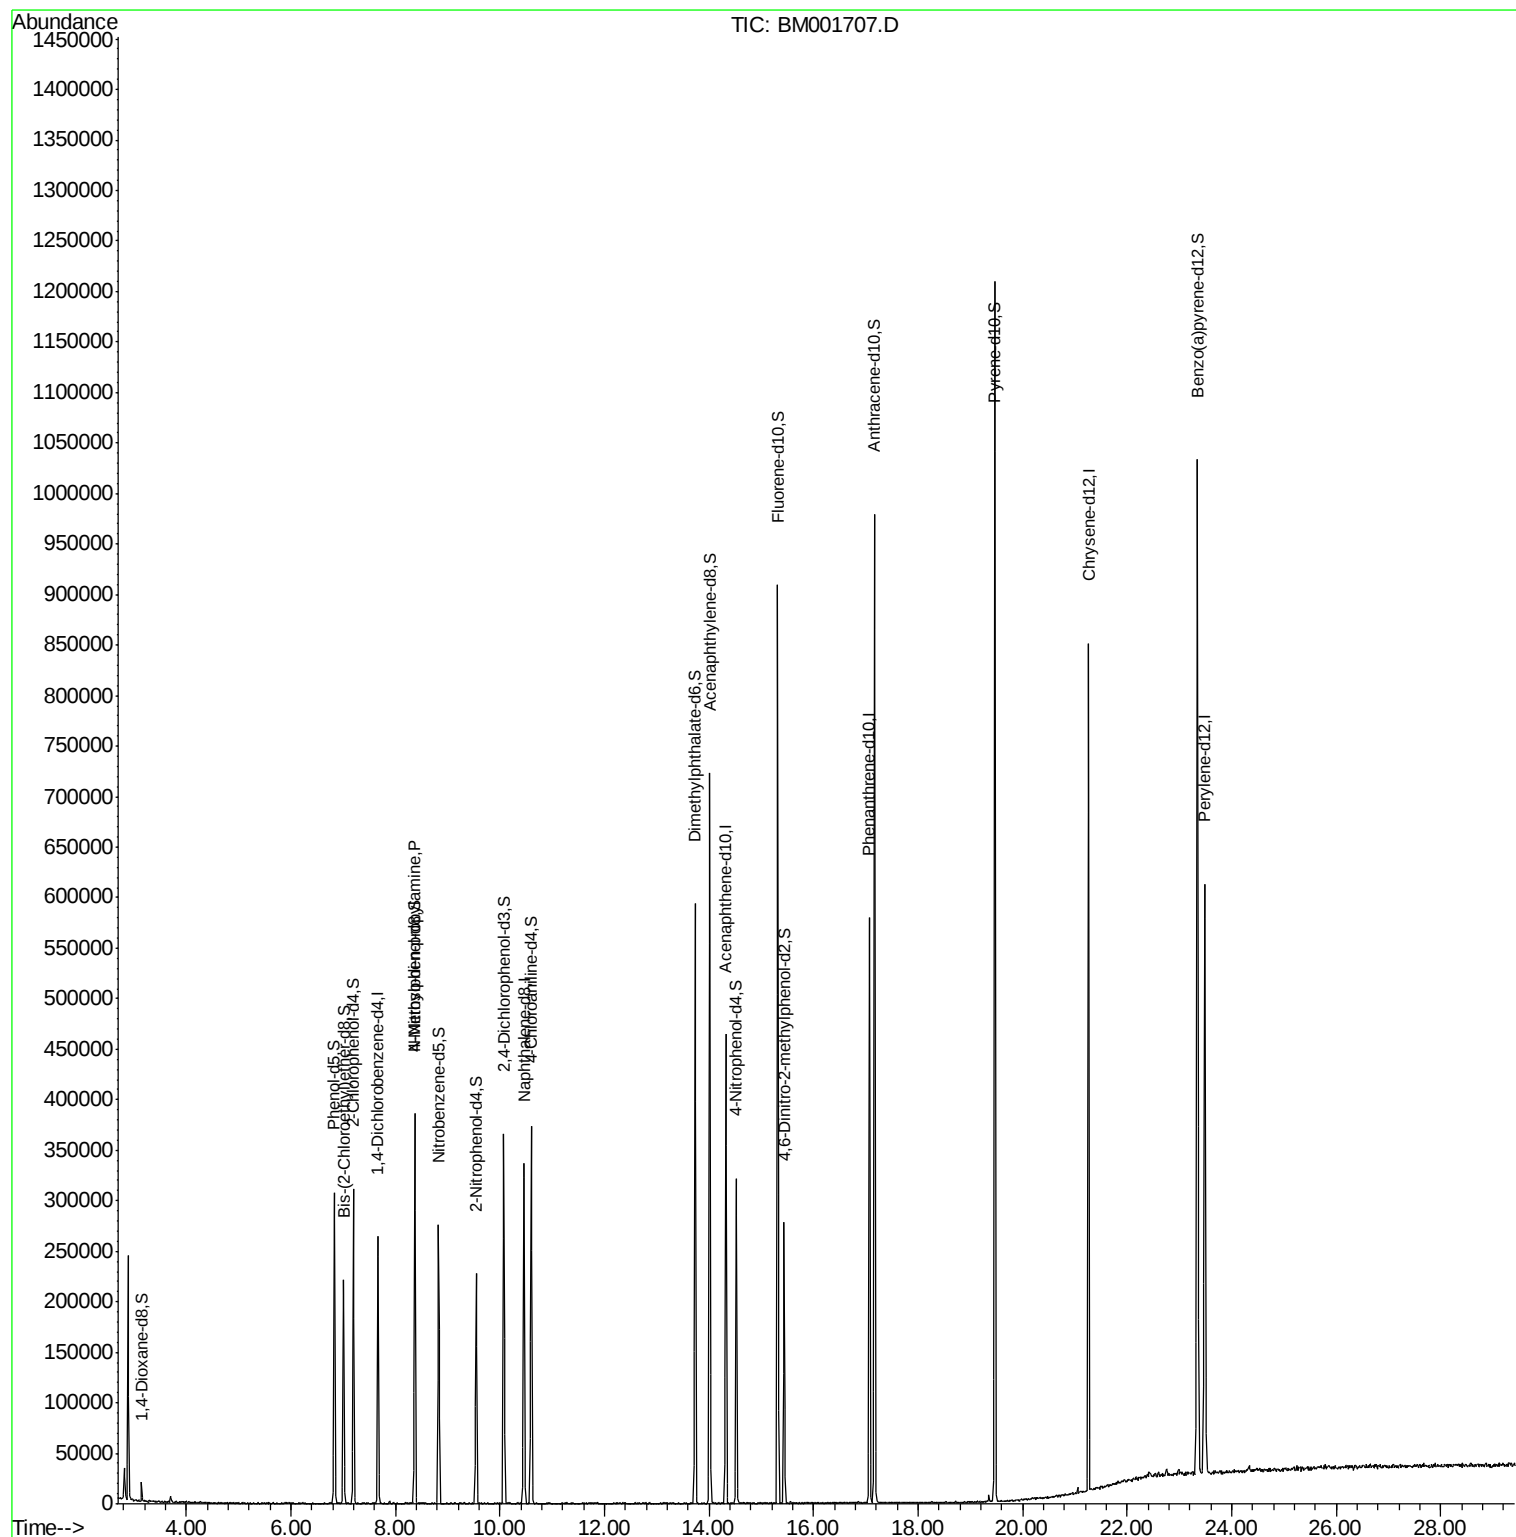

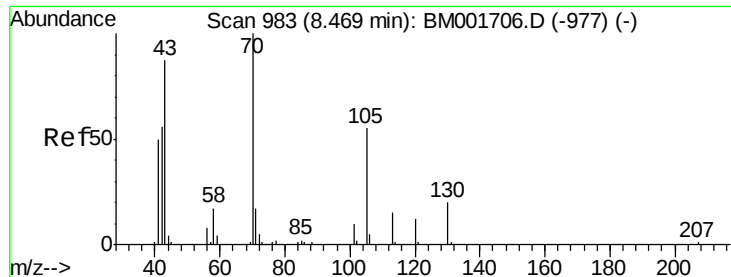

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.08 ng/ul
 RT: 8.37 min Scan# 966
 Delta R.T. -0.10 min
 Lab File: BM001707.D
 Acq: 16 Jun 2015 10:51

Instrument :
 BNA_M
 ClientSampleId :
 SBLK71

Tgt Ion: 70 Resp: 3513
 Ion Ratio Lower Upper
 70 100
 42 351.1 45.2 67.8#
 101 0.0 7.8 11.6#
 130 0.0 15.5 23.3#

