

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061615\
 Data File : BM001710.D
 Acq On : 16 Jun 2015 12:38
 Operator : TP/IZ
 Sample : PB84014BL
 Misc : SBLK72
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK72

Quant Time: Jun 17 05:24:09 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061515.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 17 05:22:36 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	66857	20.00	ng/ul	0.00
18) Naphthalene-d8	10.46	136	265001	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	159382	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	360874	20.00	ng/ul	0.00
77) Chrysene-d12	21.26	240	450197	20.00	ng/ul	0.00
85) Perylene-d12	23.48	264	474912	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.14	96	8266	5.89	ng/uL	0.00
5) Phenol-d5	6.83	99	157101	30.60	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	91625	31.85	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	126900	31.25	ng/ul	0.00
13) 4-Methylphenol-d8	8.37	113	131216	31.83	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	57950	31.59	ng/ul	0.00
22) 2-Nitrophenol-d4	9.54	143	66148	32.98	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.07	165	130693	30.44	ng/ul	0.00
29) 4-Chloroaniline-d4	10.59	131	180004	41.21	ng/ul	0.00
43) Dimethylphthalate-d6	13.73	166	401433	33.97	ng/ul	0.00
46) Acenaphthylene-d8	14.01	160	497857	32.13	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	67784	31.09	ng/ul	0.00
57) Fluorene-d10	15.32	176	366877	33.45	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	65038	29.50	ng/ul	0.00
70) Anthracene-d10	17.16	188	571426	33.99	ng/ul	0.00
78) Pyrene-d10	19.46	212	659752	34.60	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.34	264	743637	35.52	ng/ul	0.00


Target Compounds					Qvalue
15) N-Nitroso-di-n-propylamine	8.37	70	3403	1.06 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061615\
Data File : BM001710.D
Acq On : 16 Jun 2015 12:38
Operator : TP/IZ
Sample : PB84014BL
Misc : SBLK72
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK72

Quant Time: Jun 17 05:24:09 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061515.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 17 05:22:36 2015
Response via : Initial Calibration

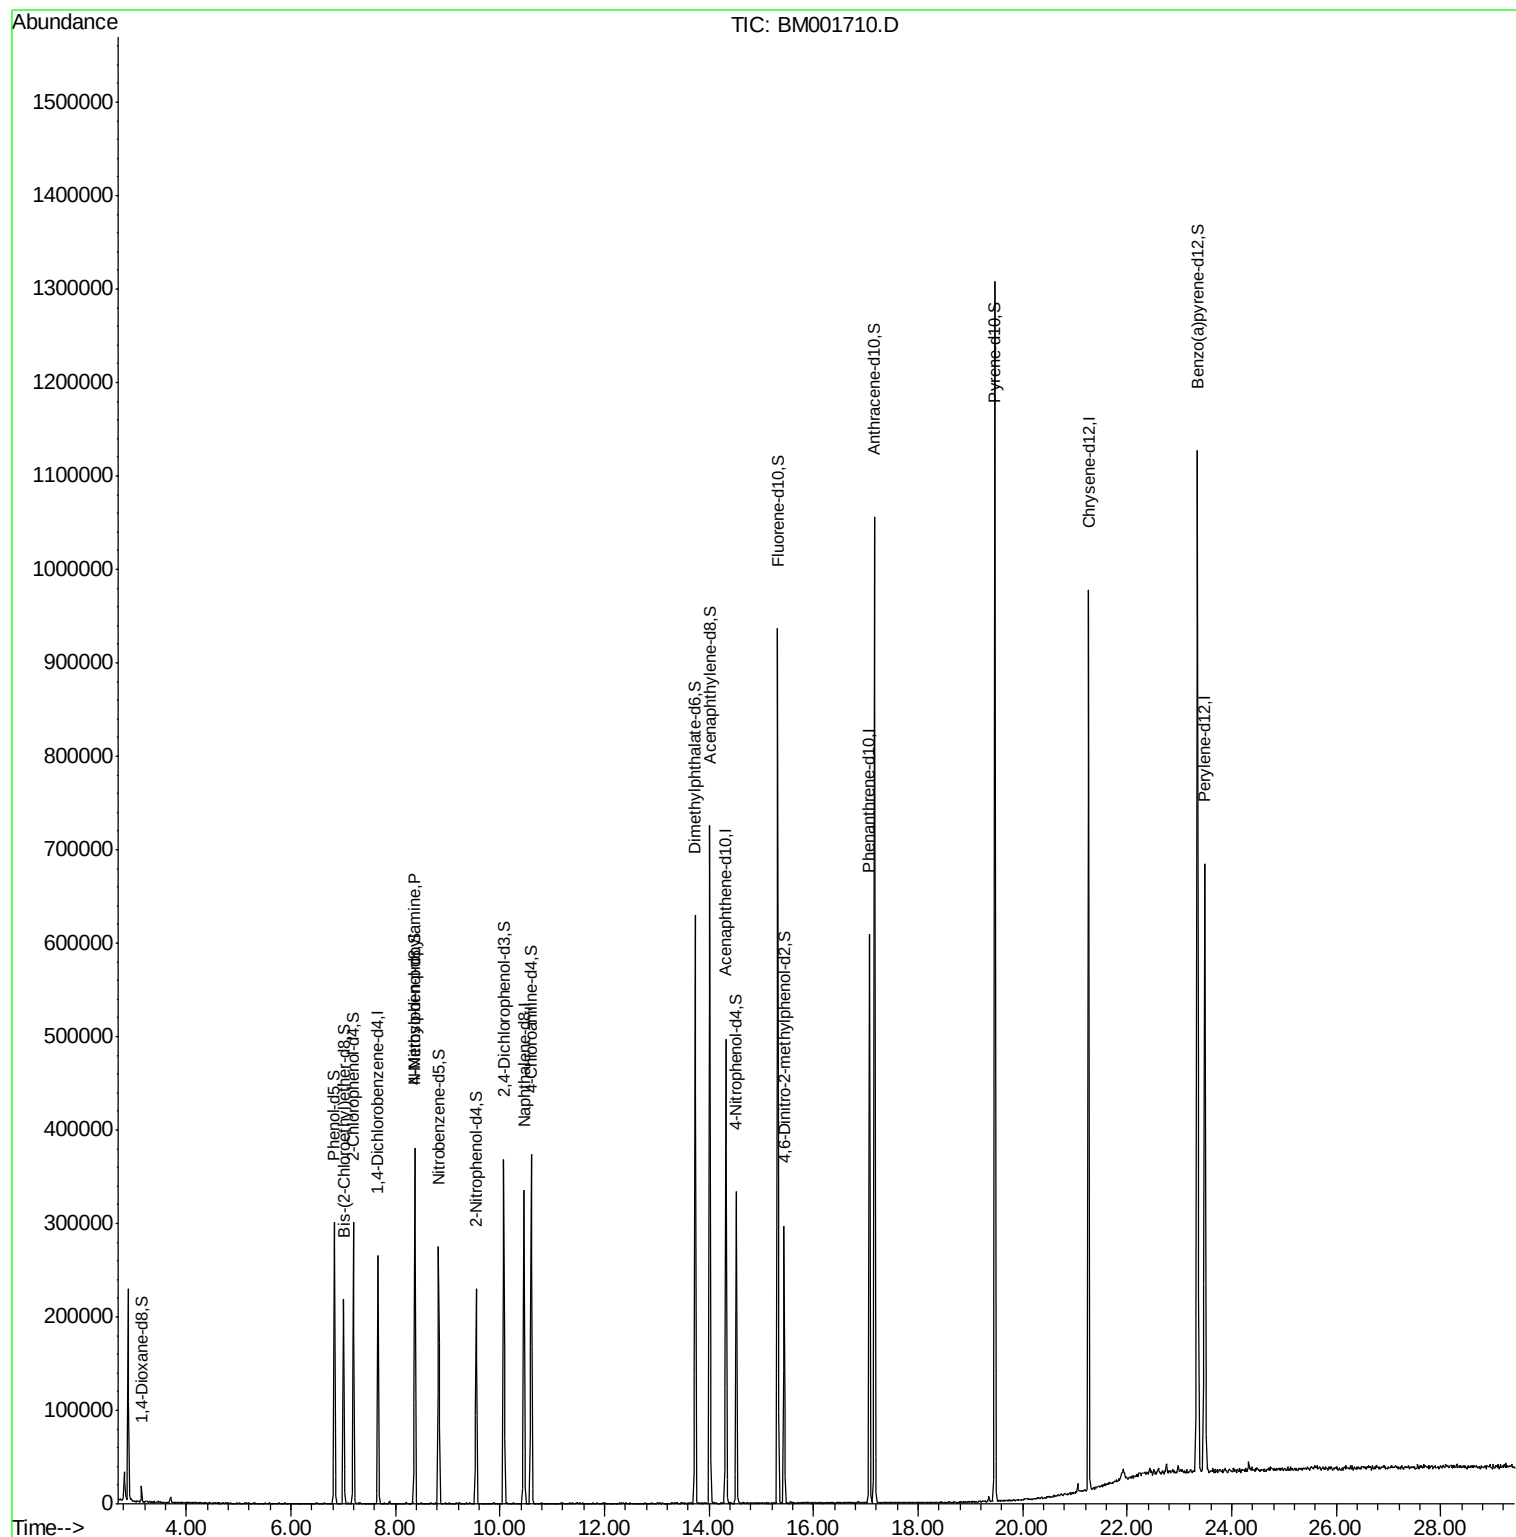

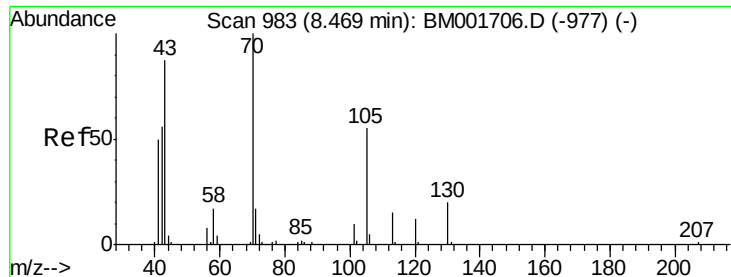

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.06 ng/ul
 RT: 8.37 min Scan# 966
 Delta R.T. -0.10 min
 Lab File: BM001710.D
 Acq: 16 Jun 2015 12:38

Instrument :
 BNA_M
 ClientSampleId :
 SBLK72

Tgt Ion:	70	Resp:	3403
Ion	Ratio	Lower	Upper
70	100		
42	276.8	45.2	67.8#
101	0.0	7.8	11.6#
130	0.0	15.5	23.3#

