


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061615\
Data File : BM001705.D
Acq On : 16 Jun 2015 09:39
Operator : TP/IZ
Sample : DFTPP60
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP60

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061515.M
Title : SVOA CALIBRATION
Last Update : Wed Jun 17 05:39:06 2015

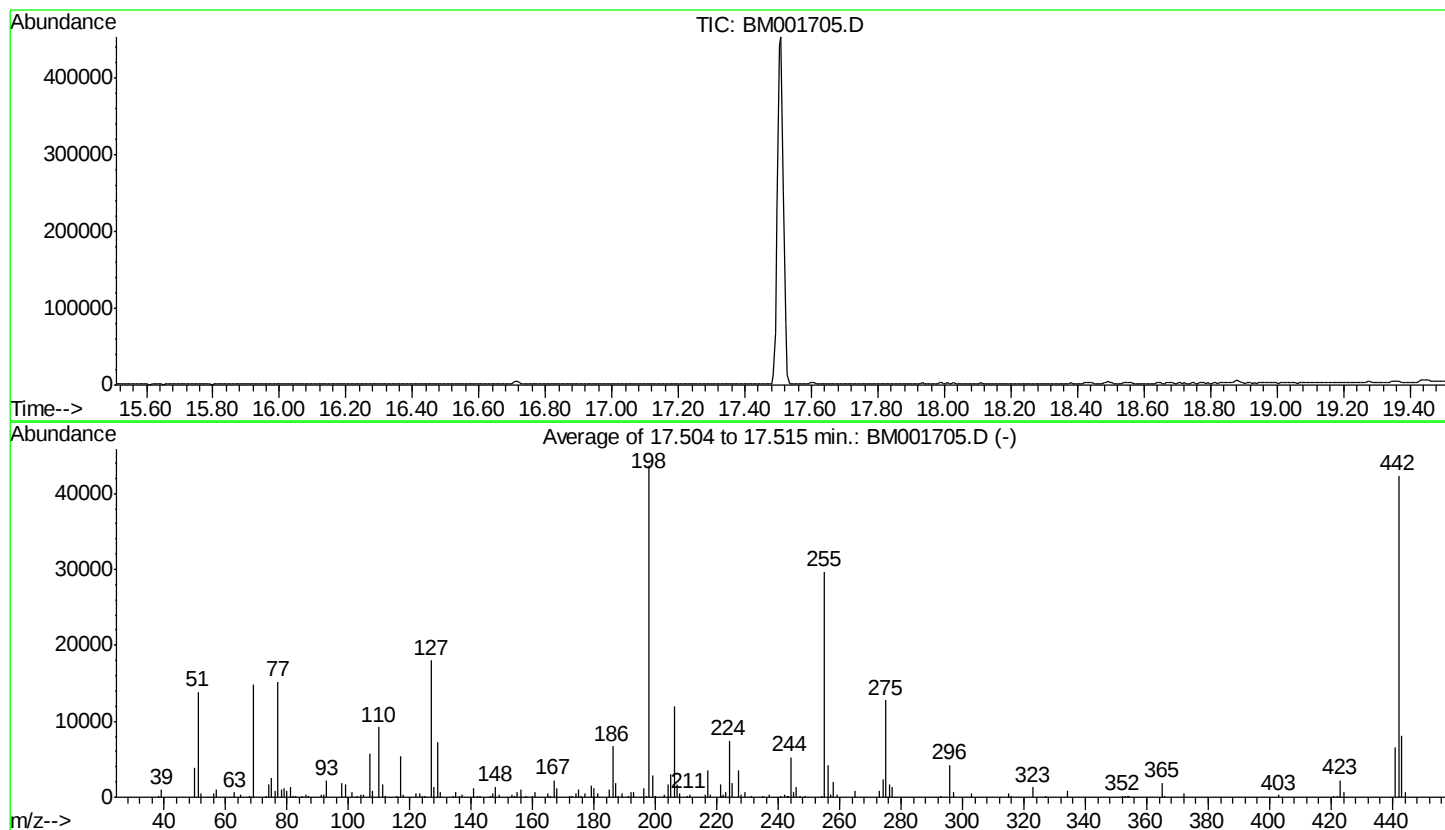

AutoFind: Scans 2519, 2520, 2521; Background Corrected with Scan 2514

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.8	13883	PASS
68	69	0.00	2	1.6	236	PASS
69	198	0.00	100	33.9	14807	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.3	18010	PASS
197	198	0.00	2	0.3	131	PASS
198	198	100	100	100.0	43656	PASS
199	198	5	9	6.6	2896	PASS
275	198	10	60	29.3	12772	PASS
365	198	1	100	4.3	1863	PASS
441	442	0.01	24	15.4	6524	PASS
442	198	50	100	97.1	42386	PASS
443	442	15	24	19.1	8087	PASS

m/z	Abundance
38.00	312.0
39.10	1307.0
40.00	473.0
43.90	895.0
50.10	5077.0
51.10	18592.0
52.00	616.0
56.00	527.0
57.00	1213.0
63.00	789.0
65.10	488.0
67.90	385.0
69.00	18640.0
73.10	376.0
74.00	2236.0
75.00	3565.0
76.10	878.0
77.10	19912.0
78.10	1339.0
79.00	1570.0
80.00	1139.0
81.00	1797.0
82.00	375.0
83.00	384.0
86.00	504.0
86.90	338.0
91.00	476.0
91.90	532.0
93.00	2497.0
98.00	2334.0
99.00	2127.0
101.00	888.0
102.90	316.0
103.90	593.0
105.00	580.0
107.00	7140.0
108.00	1017.0
110.00	11275.0
110.90	2178.0
112.00	305.0
115.90	439.0
117.00	6653.0
118.00	670.0
121.90	472.0
123.00	704.0
124.10	368.0
125.00	427.0
127.00	22760.0
128.00	1633.0
129.00	8991.0
129.90	672.0
133.90	325.0
134.90	736.0
136.00	356.0
137.00	445.0
140.90	1516.0
142.00	515.0
142.90	338.0
146.00	375.0
147.00	674.0
148.00	1695.0
148.90	455.0
153.00	478.0
153.90	391.0
155.00	820.0
156.00	1100.0
157.90	356.0
160.10	359.0
160.90	812.0
165.10	551.0
165.90	439.0
167.00	2713.0
168.00	1435.0
171.90	465.0
173.00	329.0
174.00	676.0
174.90	1264.0
175.90	306.0
176.80	445.0
179.00	2093.0
180.00	1242.0
181.10	612.0
185.00	1149.0
186.00	8113.0
187.00	2159.0
188.90	601.0
192.10	693.0
193.10	861.0
196.10	1303.0
197.00	394.0
198.00	51096.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60

199.00	3496.0
199.90	308.0
202.90	431.0
204.00	2076.0
205.10	3271.0
206.10	13424.0
207.00	2486.0
207.90	678.0
210.20	438.0
211.10	616.0
216.00	416.0
217.00	4408.0
218.00	423.0
221.10	1704.0
222.00	556.0
223.00	824.0
224.00	8579.0
225.00	2057.0
227.00	3764.0
227.90	303.0
229.00	815.0
231.10	356.0
237.00	578.0
242.00	449.0
243.10	403.0
244.00	5650.0
245.00	766.0
246.00	1631.0
247.00	306.0
255.00	32248.0
256.00	4678.0
257.00	380.0
258.00	2026.0
259.00	420.0
265.10	917.0
273.00	933.0
274.00	2706.0
275.00	13613.0
276.10	1790.0
276.90	1328.0
296.00	4507.0
297.00	678.0
302.90	492.0
315.00	525.0
316.00	323.0
323.10	1327.0
334.00	889.0
353.00	305.0
353.90	383.0
365.10	1744.0
372.00	578.0
403.00	527.0
423.00	2068.0
424.10	617.0
441.00	5818.0
442.10	39200.0
443.10	7338.0
444.00	668.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60

m/z	Abundance
39.00	1126.0
40.00	512.0
44.00	981.0
50.00	4389.0
51.10	15451.0
52.00	716.0
56.00	562.0
57.00	1004.0
62.90	755.0
65.00	464.0
68.00	324.0
69.00	17160.0
74.00	1859.0
75.00	2584.0
76.10	1034.0
77.10	16944.0
78.10	1232.0
79.00	1614.0
80.00	966.0
81.00	1498.0
82.00	351.0
85.00	301.0
85.90	379.0
90.90	338.0
92.00	513.0
93.00	2624.0
98.00	1818.0
99.00	1823.0
101.00	793.0
103.00	324.0
104.00	510.0
104.90	639.0
107.00	6685.0
108.00	942.0
110.00	11113.0
111.00	1742.0
117.00	6252.0
117.90	487.0
122.00	653.0
123.10	672.0
124.00	301.0
127.00	20328.0
128.00	1349.0
129.00	8518.0
130.00	1029.0
135.00	646.0
135.90	307.0
136.90	361.0
140.90	1564.0
142.70	312.0
147.00	674.0
147.90	1694.0
148.90	488.0
153.10	461.0
155.10	772.0
156.00	1243.0
160.00	388.0
160.90	714.0
165.00	659.0
167.00	2736.0
168.00	1313.0
173.00	409.0
174.00	623.0
175.00	1328.0
175.90	378.0
176.90	605.0
179.00	1796.0
179.90	1440.0
181.00	772.0
185.00	1003.0
186.00	7833.0
187.00	2272.0
188.00	368.0
189.00	595.0
191.00	300.0
191.90	752.0
193.00	891.0
196.00	1732.0
198.00	51528.0
199.00	3445.0
203.00	455.0
204.00	1935.0
205.00	3778.0
206.00	14327.0
207.00	2453.0
207.90	725.0
211.10	496.0
216.00	369.0
216.90	3982.0
218.00	469.0
221.00	2224.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60

221.70	579.0
223.10	694.0
224.00	8747.0
225.00	2387.0
227.00	4094.0
227.90	672.0
229.00	877.0
235.00	372.0
237.10	327.0
240.90	322.0
241.90	563.0
242.80	361.0
244.00	5897.0
245.00	977.0
245.90	1631.0
247.00	327.0
248.90	458.0
254.10	328.0
255.00	35472.0
256.00	5130.0
257.00	421.0
258.00	2606.0
258.90	511.0
264.90	1041.0
272.90	1062.0
274.00	2698.0
275.00	15827.0
276.00	2009.0
277.00	1804.0
293.00	388.0
296.00	5277.0
297.00	806.0
303.00	531.0
314.90	633.0
316.00	365.0
323.10	1490.0
327.00	311.0
334.00	1162.0
352.10	559.0
354.10	482.0
365.00	2176.0
366.00	347.0
372.10	771.0
402.90	414.0
421.00	437.0
422.00	361.0
423.10	2583.0
424.10	892.0
441.10	8211.0
442.10	50560.0
443.10	9912.0
444.10	872.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60

m/z	Abundance
39.00	504.0
39.90	532.0
44.00	991.0
50.10	2216.0
51.10	7607.0
52.00	353.0
56.00	330.0
57.00	590.0
63.00	389.0
69.00	8621.0
73.00	326.0
74.00	940.0
75.00	1508.0
76.00	629.0
77.10	8868.0
78.10	554.0
78.90	611.0
79.90	473.0
80.90	814.0
85.90	371.0
93.00	1353.0
97.90	1194.0
99.00	934.0
101.00	374.0
107.00	3350.0
108.00	502.0
110.00	5190.0
111.00	920.0
117.00	3135.0
122.10	353.0
123.00	375.0
127.00	10943.0
128.00	866.0
129.00	4361.0
130.00	455.0
135.00	466.0
141.00	560.0
146.90	379.0
147.90	852.0
155.00	333.0
156.10	727.0
161.00	509.0
164.90	315.0
167.00	1337.0
168.00	847.0
174.00	318.0
175.00	411.0
176.90	352.0
179.00	911.0
180.00	763.0
181.10	329.0
185.00	828.0
186.00	4142.0
187.00	1118.0
188.80	329.0
191.90	377.0
192.90	417.0
196.00	660.0
197.90	28344.0
198.90	1747.0
204.00	1066.0
205.00	2105.0
206.10	8206.0
207.10	1607.0
208.00	371.0
217.00	2287.0
218.00	356.0
221.00	1272.0
221.90	367.0
222.90	644.0
224.00	5052.0
225.00	1212.0
227.00	2537.0
228.90	390.0
244.10	4137.0
245.10	457.0
246.00	782.0
255.00	21360.0
256.00	2767.0
257.90	1346.0
265.10	415.0
272.80	453.0
274.00	1657.0
275.00	8877.0
276.00	1045.0
277.00	970.0
296.00	2965.0
296.90	377.0
302.90	462.0
315.00	444.0
323.10	1052.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60

334.00	666.0
365.00	1670.0
372.10	431.0
423.00	1956.0
424.10	581.0
441.00	5545.0
442.10	37400.0
443.10	7013.0
444.00	696.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60

Scan 2514 (17.474 min): BM001705.D
DFTPP60

m/z	Abundance
39.90	537.0
44.00	1032.0
207.10	460.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60