

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061616\
 Data File : BM005827.D
 Acq On : 16 Jun 2016 05:15
 Operator : UM/SJ
 Sample : H3535-13MSD
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Quant Time: Jun 16 06:59:13 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 16 01:45:55 2016
 Response via : Initial Calibration

Instrument :
 BNA M
 ClientSampleId :
 D9XX1MSD

Manual Integrations
 APPROVED

umangi
 6/16/2016 6:48:32 PM

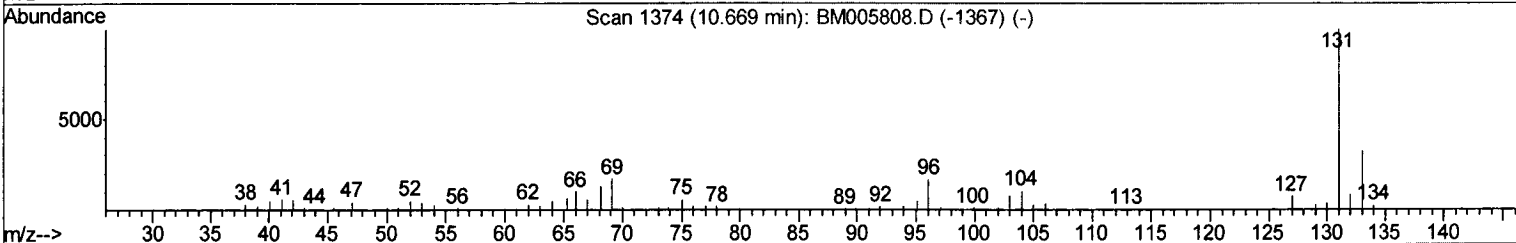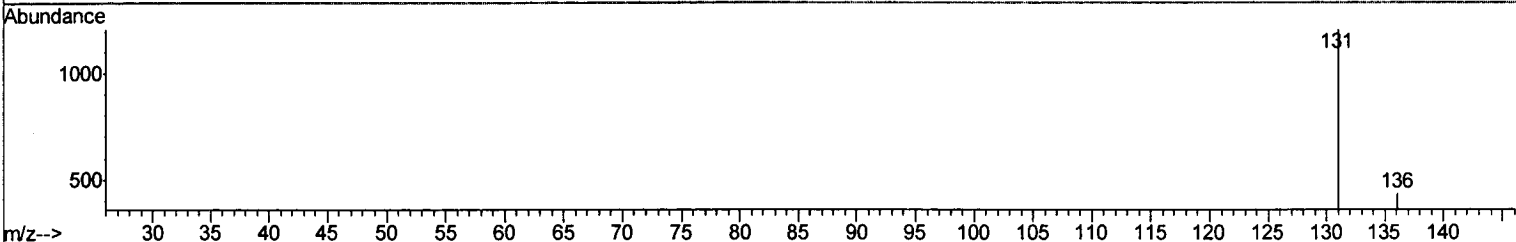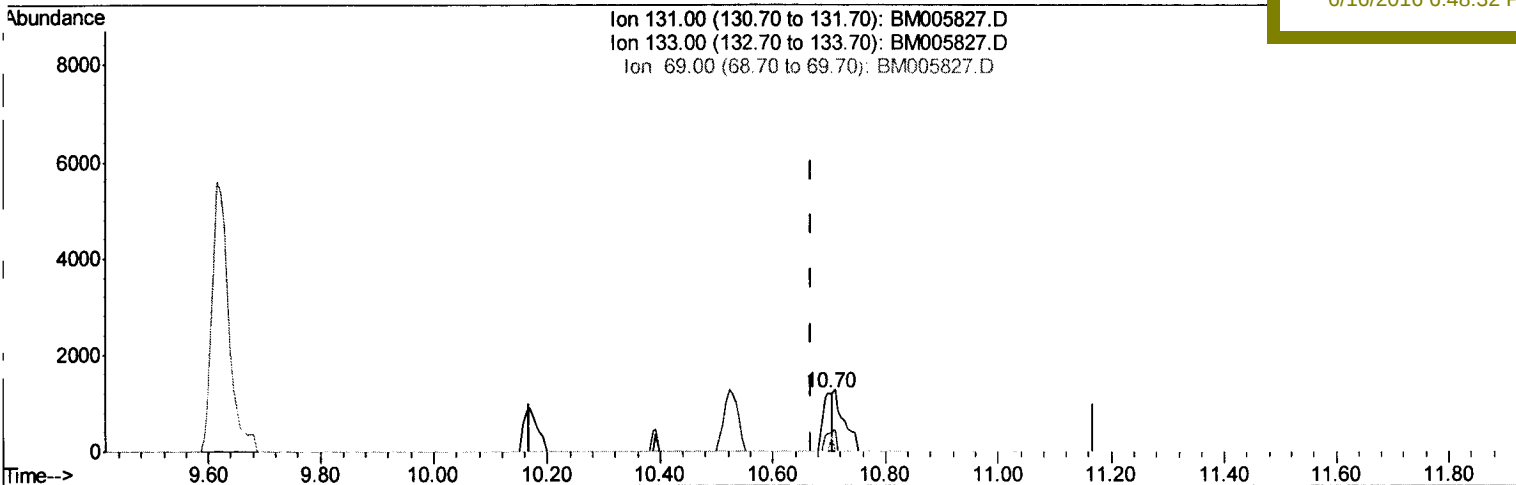

TIC: BM005827.D

(12) 4-Chloroaniline-d4 (S)

10.698min (+0.030) 0.27ng/ul

response 1426

Ion	Exp%	Act%
131.00	100	100
133.00	32.40	29.69
69.00	17.50	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061616\
 Data File : BM005827.D
 Acq On : 16 Jun 2016 05:15
 Operator : UM/SJ
 Sample : H3535-13MSD
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9XX1MSD

Manual Integrations
 APPROVED

umangi
 6/16/2016 6:48:32 PM

Quant Time: Jun 16 06:59:13 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 16 01:45:55 2016
 Response via : Initial Calibration

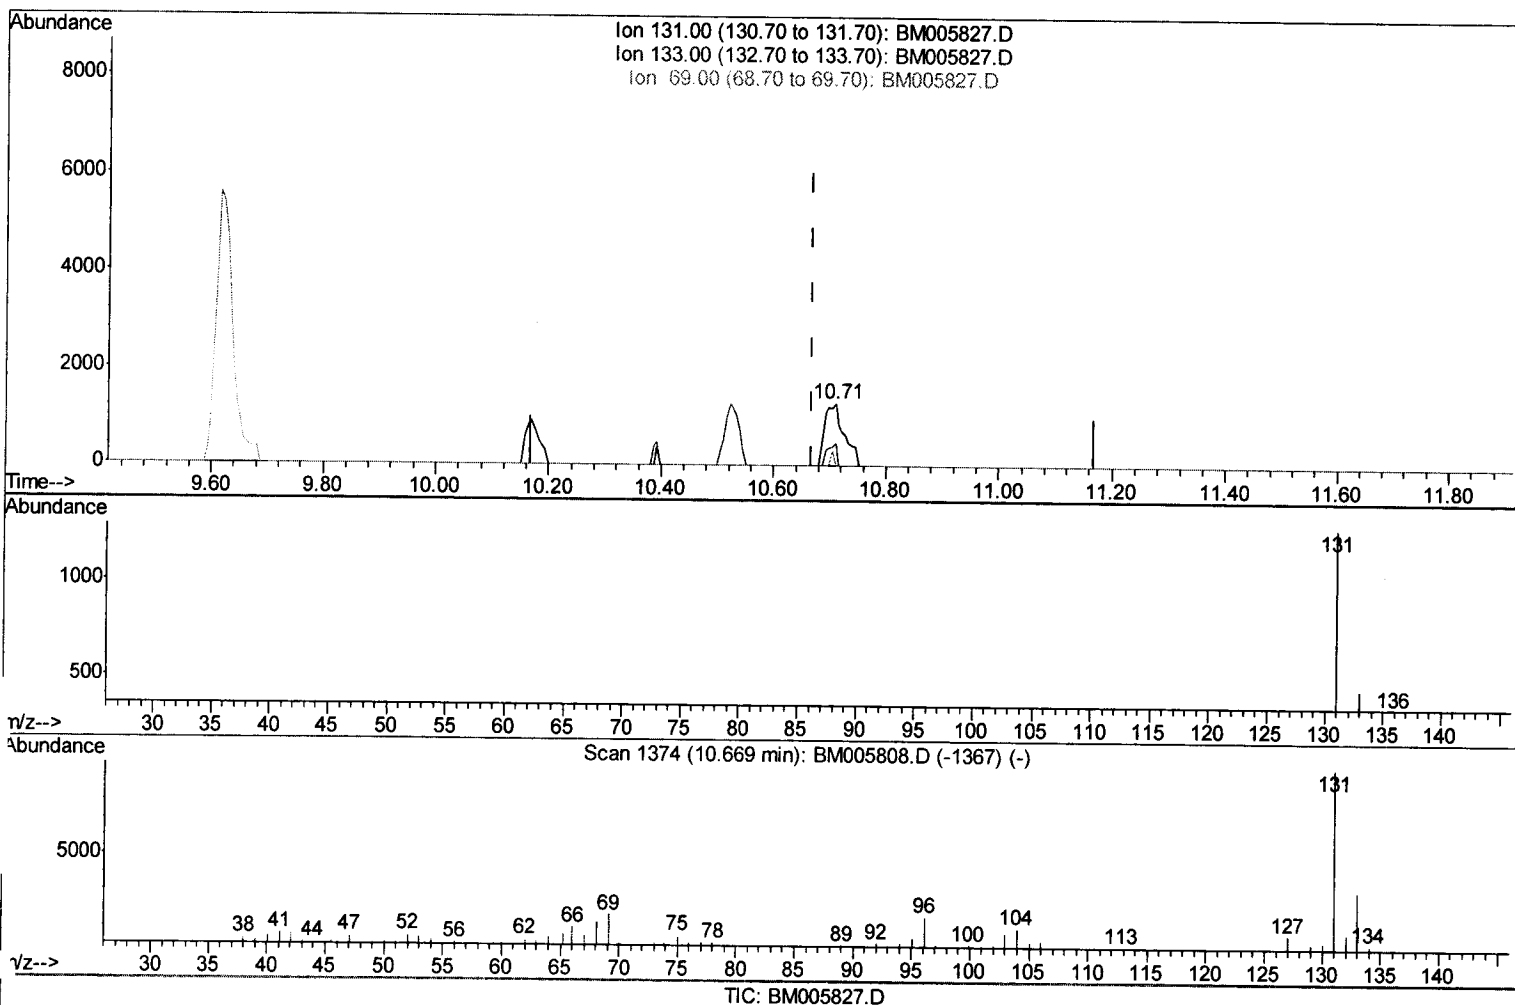

(12) 4-Chloroaniline-d4 (S)

10.710min (+0.041) 0.59ng/ul m

response 3083

Ion	Exp%	Act%
131.00	100	100
133.00	32.40	34.97
69.00	17.50	0.00#
0.00	0.00	0.00

> U.M
 06/20/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061616\
Data File : BM005827.D
Acq On : 16 Jun 2016 05:15
Operator : UM/SJ
Sample : H3535-13MSD
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9XX1MSD

Quant Time: Jun 16 06:59:13 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061516.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 16 01:45:55 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

umangi
6/16/2016 6:48:32 PM

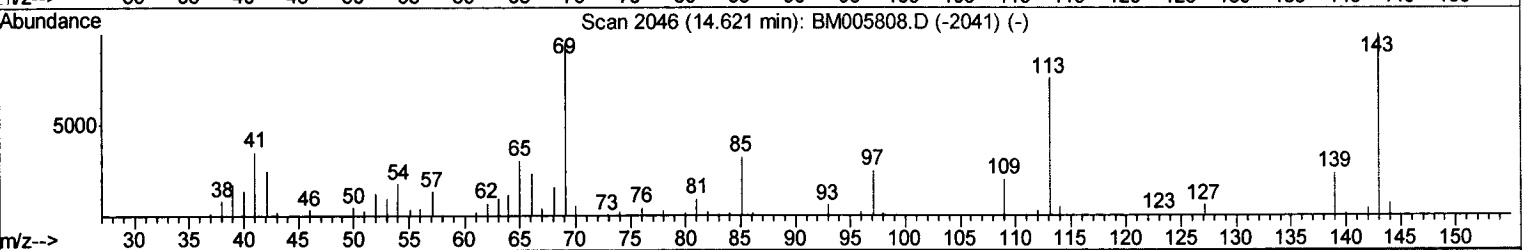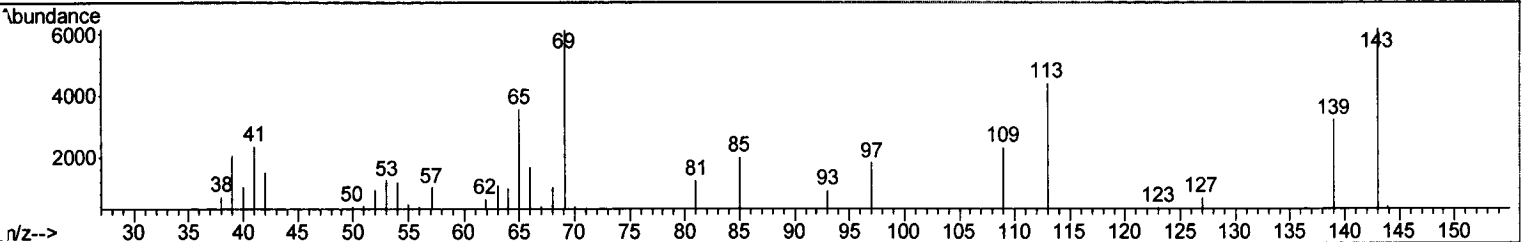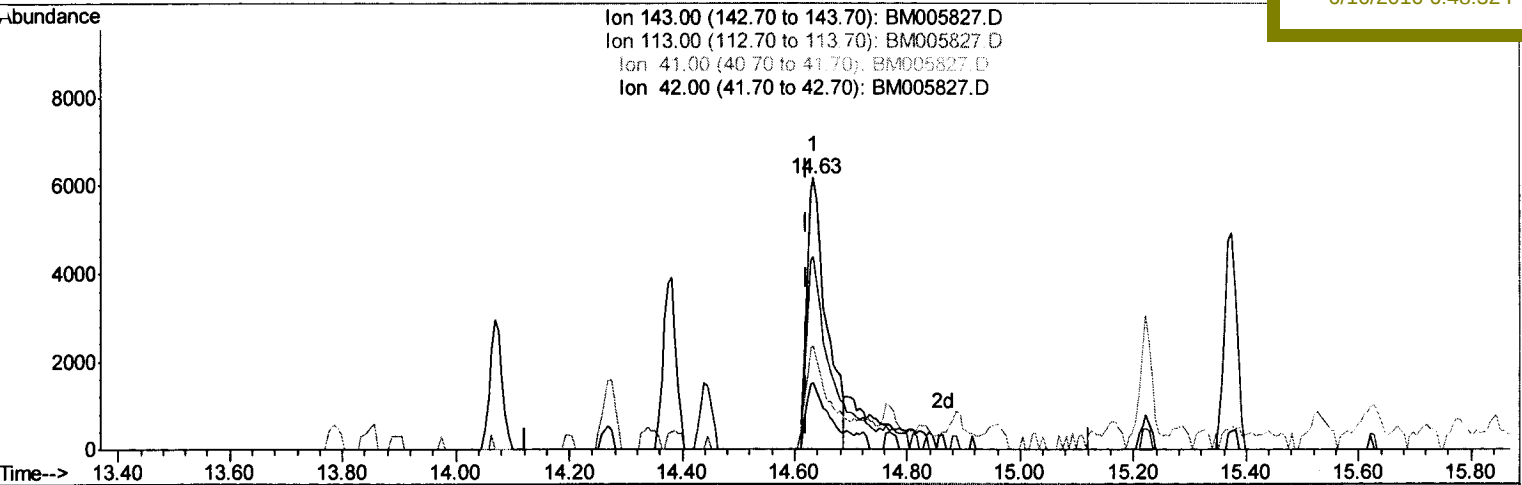

TIC: BM005827.D

(20) 4-Nitrophenol-d4 (S)

14.633min (+0.012) 7.59ng/ul

response 15114

Ion	Exp%	Act%
143.00	100	100
113.00	74.90	71.44
41.00	39.60	38.18
42.00	23.50	24.47

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061616\
 Data File : BM005827.D
 Acq On : 16 Jun 2016 05:15
 Operator : UM/SJ
 Sample : H3535-13MSD
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9XX1MSD

Manual Integrations
 APPROVED

umangi
 6/16/2016 6:48:32 PM

Quant Time: Jun 16 06:59:13 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 16 01:45:55 2016
 Response via : Initial Calibration

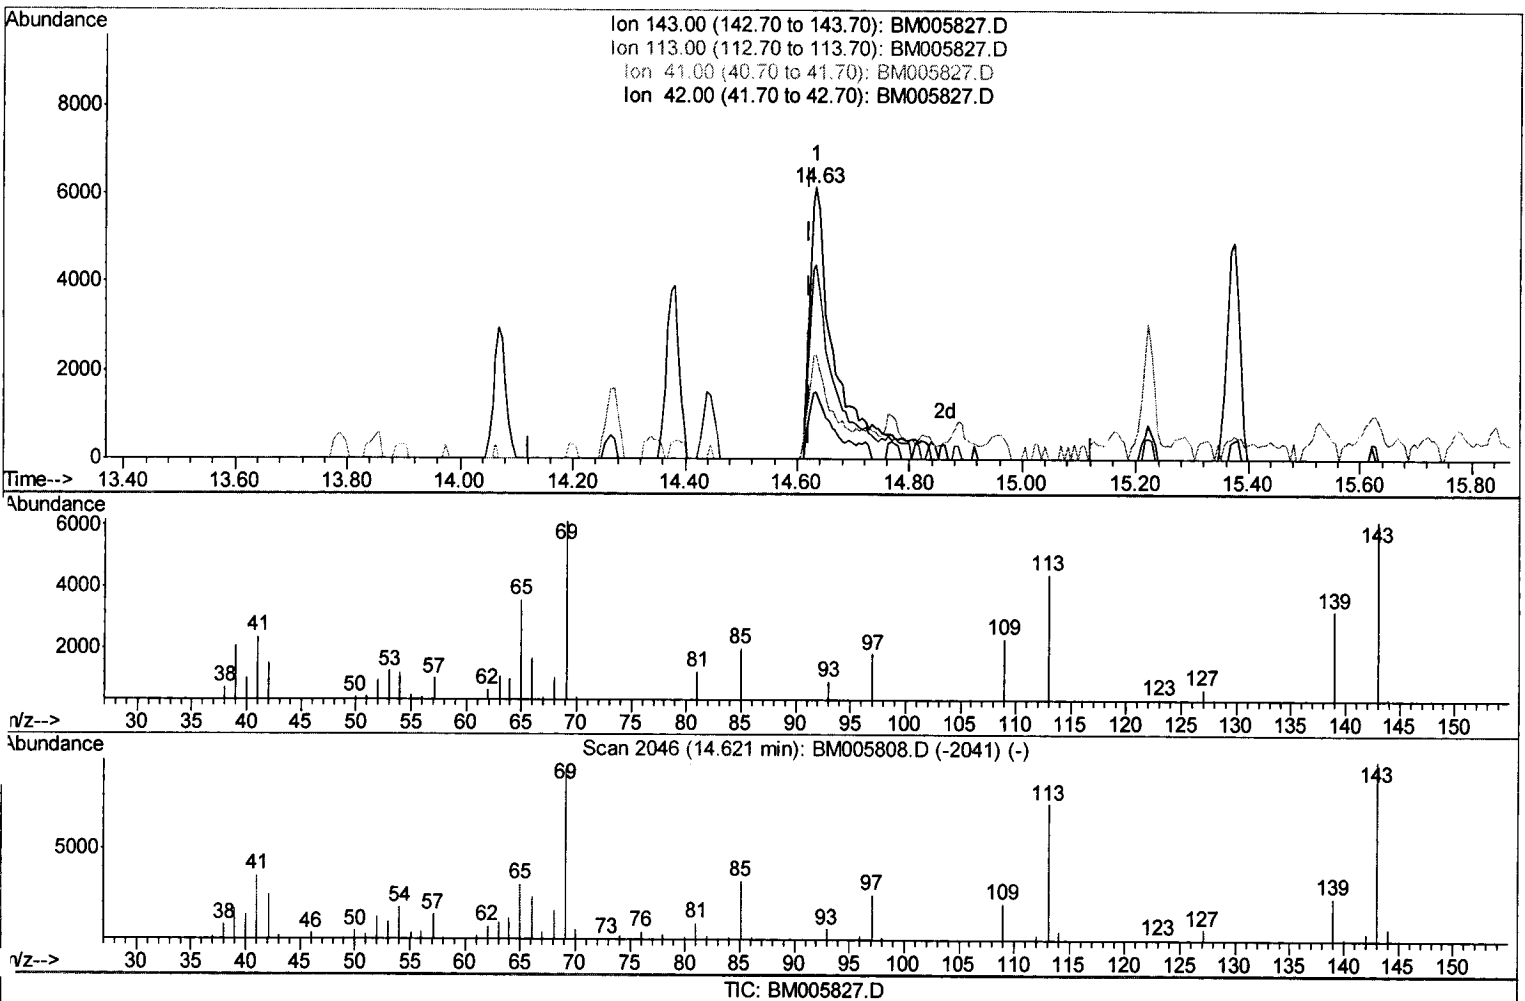

(20) 4-Nitrophenol-d4 (S)

14.633min (+0.012) 10.54ng/ul m

response 20990

Ion	Exp%	Act%
143.00	100	100
113.00	74.90	71.44
41.00	39.60	38.18
42.00	23.50	24.47

> U.M
 06/20/16

ta Path : Z:\HPCHEM1\BNA_M\DATA\BM061616\
 ta File : BM005827.D
 g On : 16 Jun 2016 05:15
 erator : UM/SJ
 mple : H3535-13MSD
 .sc :
 S Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9XX1MSD

Manual Integrations
 APPROVED

umangi
 6/16/2016 6:48:32 PM

ant Time: Jun 16 07:02:18 2016
 ant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061516.M
 uant Title : SVOA CALIBRATION
 Last Update : Thu Jun 16 01:45:55 2016
 esponse via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	62739	20.00	ng/ul	0.00
7) Naphthalene-d8	10.52	136	315348	20.00	ng/ul	0.00
15) Acenaphthene-d10	14.38	164	218124	20.00	ng/ul	0.00
23) Phenanthrene-d10	17.13	188	545228	20.00	ng/ul	0.00
29) Chrysene-d12	21.31	240	650318	20.00	ng/ul	0.00
34) Perylene-d12	23.56	264	608694	20.00	ng/ul	0.00

System Monitoring Compounds

2) 1,4-Dioxane-d8	3.19	96	1342	0.99	ng/uL	0.00
3) Phenol-d5	6.92	99	67464	13.09	ng/ul	0.00
4) Bis-(2-Chloroethyl)ether-d	7.07	67	61378	20.01	ng/ul	0.00
5) 2-Chlorophenol-d4	7.27	132	65468	15.25	ng/ul	0.00
6) 4-Methylphenol-d8	8.46	113	32895	7.56	ng/ul	0.00
8) Nitrobenzene-d5	8.90	128	40090	17.95	ng/ul	0.00
9) 2-Nitrophenol-d4	9.62	143	23103	9.31	ng/ul	0.00
10) 2,4-Dichlorophenol-d3	10.16	165	62244	13.11	ng/ul	0.00
12) 4-Chloroaniline-d4	10.71	131	3083m	0.59	ng/ul	0.04
16) Dimethylphthalate-d6	13.79	166	170777	9.86	ng/ul	0.00
17) Acenaphthylene-d8	14.07	160	445994	20.27	ng/ul	0.00
20) 4-Nitrophenol-d4	14.63	143	20990m	10.54	ng/ul	0.01
21) Fluorene-d10	15.37	176	347132	24.07	ng/ul	0.00
24) 4,6-Dinitro-2-methylphenol	15.53	200	11196	4.59	ng/ul	0.00
26) Anthracene-d10	17.22	188	560038	22.14	ng/ul	0.00
30) Pyrene-d10	19.52	212	690542	21.82	ng/ul	0.00
37) Benzo(a)pyrene-d12	23.42	264	535295	19.04	ng/ul	0.00

Target Compounds						Qvalue
19) Acenaphthene	14.45	153	313381	21.57	ng/ul	100
31) Pyrene	19.55	202	900142	22.54	ng/ul	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

} U.M
 06/20/16

Quantitation Report (QT Reviewed)

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061616\
 Data File : BM005827.D
 Acq On : 16 Jun 2016 05:15
 Operator : UM/SJ
 Sample : H3535-13MSD
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9XX1MSD

Manual Integration
 APPROVED

umangi
 6/16/2016 6:48:32 PM

Quant Time: Jun 16 07:02:18 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 16 01:45:55 2016
 Response via : Initial Calibration

