

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061621\
 Data File : BM030464.D
 Acq On : 16 Jun 2021 10:52
 Operator : CG/JU
 Sample : PB137067BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK067

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM060621.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030464.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.299	32	36	46	rVB	55151	83455	1.52%	0.175%
2	3.716	103	107	129	rBV	486093	987414	18.03%	2.068%
3	4.034	158	161	170	rVB3	9998	16320	0.30%	0.034%
4	6.992	656	664	678	rBV	769962	1238150	22.60%	2.593%
5	7.157	685	692	703	rBV	594181	967709	17.67%	2.027%
6	7.357	719	726	735	rBV	799362	1277431	23.32%	2.675%
7	7.822	798	805	814	rBV	598164	939233	17.15%	1.967%
8	8.528	917	925	939	rBV	896482	1479006	27.00%	3.097%
9	8.975	993	1001	1018	rBV	696042	1174562	21.44%	2.460%
10	9.698	1117	1124	1135	rBV	543845	921534	16.82%	1.930%
11	10.233	1207	1215	1240	rBV	822892	1493673	27.27%	3.128%
12	10.610	1271	1279	1288	rBV	792209	1320056	24.10%	2.765%
13	10.745	1294	1302	1322	rBV	818072	1558913	28.46%	3.265%
14	11.886	1482	1496	1499	rBV8	5822	17545	0.32%	0.037%
15	12.204	1545	1550	1558	rBV2	13348	25313	0.46%	0.053%
16	13.857	1824	1831	1844	rBV	1617817	2322438	42.40%	4.864%
17	14.139	1872	1879	1892	rBV	1895767	2724324	49.74%	5.705%
18	14.445	1924	1931	1943	rBV	1194846	1790210	32.68%	3.749%
19	14.645	1958	1965	1985	rBV	550842	1009890	18.44%	2.115%
20	15.439	2093	2100	2108	rBV	2568770	3526524	64.38%	7.386%
21	15.557	2114	2120	2135	rBV	590214	913715	16.68%	1.914%
22	15.680	2136	2141	2148	rVB2	29140	47882	0.87%	0.100%
23	16.221	2229	2233	2237	rBV3	6862	10693	0.20%	0.022%
24	16.974	2357	2361	2366	rVB	6748	9423	0.17%	0.020%
25	17.180	2389	2396	2406	rBV	1487724	2146435	39.19%	4.495%
26	17.280	2406	2413	2429	rVV2	2732342	3897236	71.15%	8.162%
27	19.203	2736	2740	2746	rBV	28181	38075	0.70%	0.080%
28	19.456	2779	2783	2787	rBV	24625	32602	0.60%	0.068%
29	19.568	2795	2802	2810	rBV	3530338	4730410	86.36%	9.907%
30	21.344	3099	3104	3111	rBV	2049035	2588393	47.25%	5.421%
31	23.474	3459	3466	3475	rBV2	2916538	5477517	100.00%	11.471%
32	23.615	3484	3490	3501	rVB2	1531297	2983039	54.46%	6.247%




Sum of corrected areas: 47749120

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061621\
Data File : BM030464.D
Acq On : 16 Jun 2021 10:52
Operator : CG/JU
Sample : PB137067BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK067

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM060621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

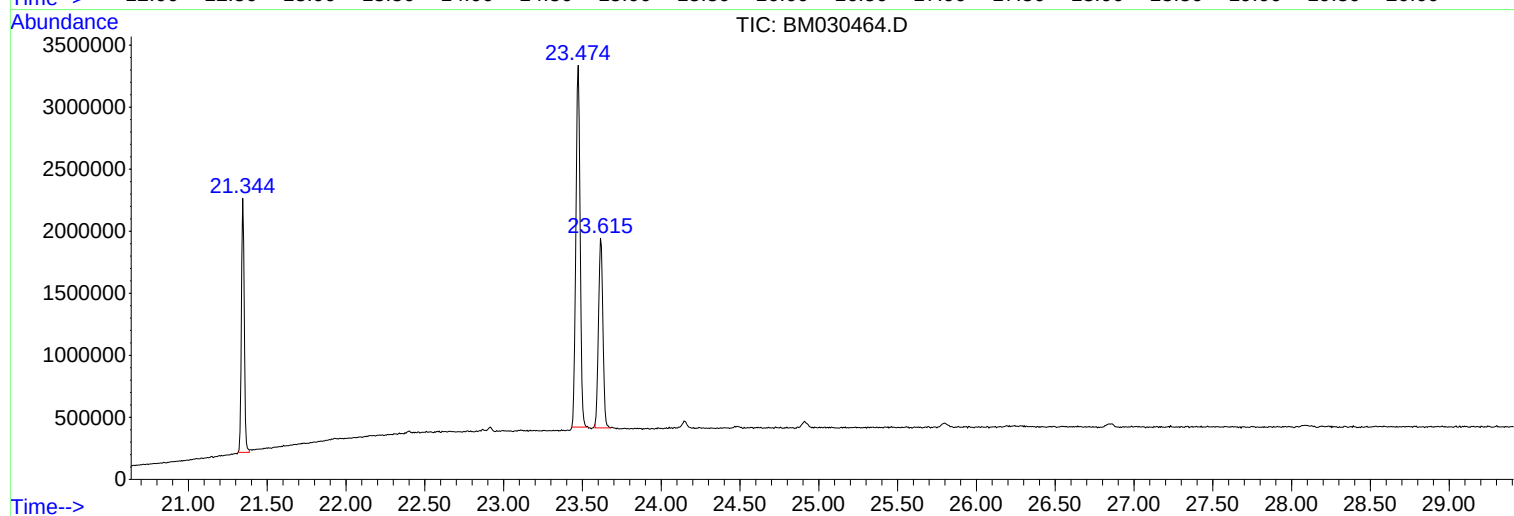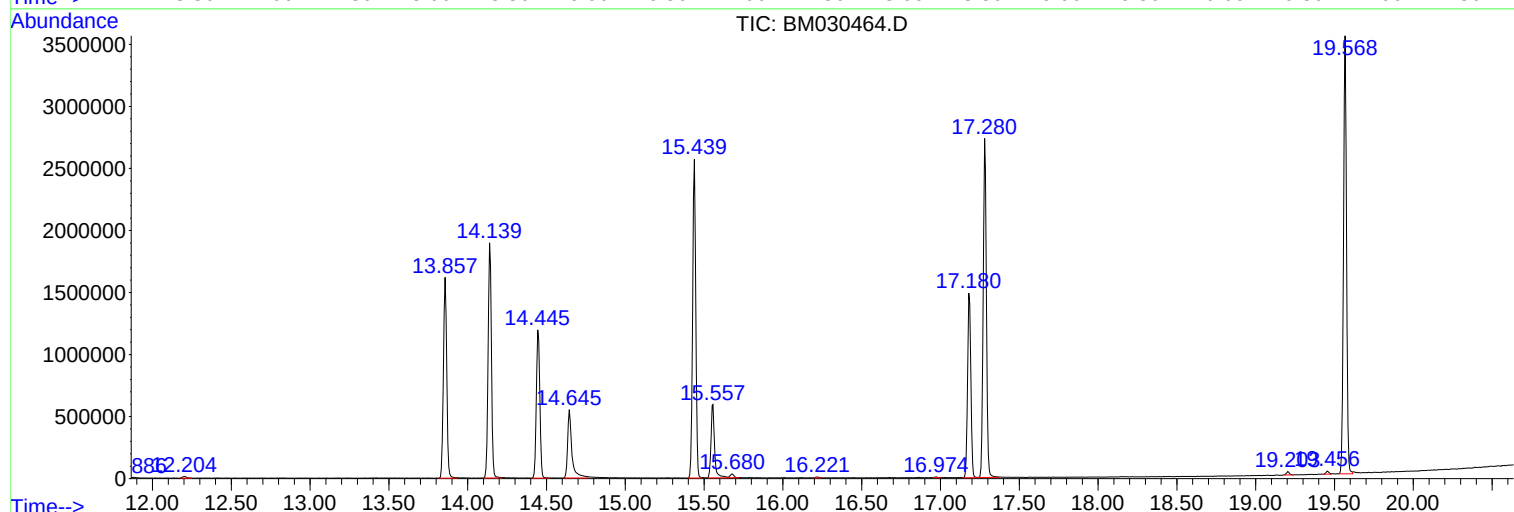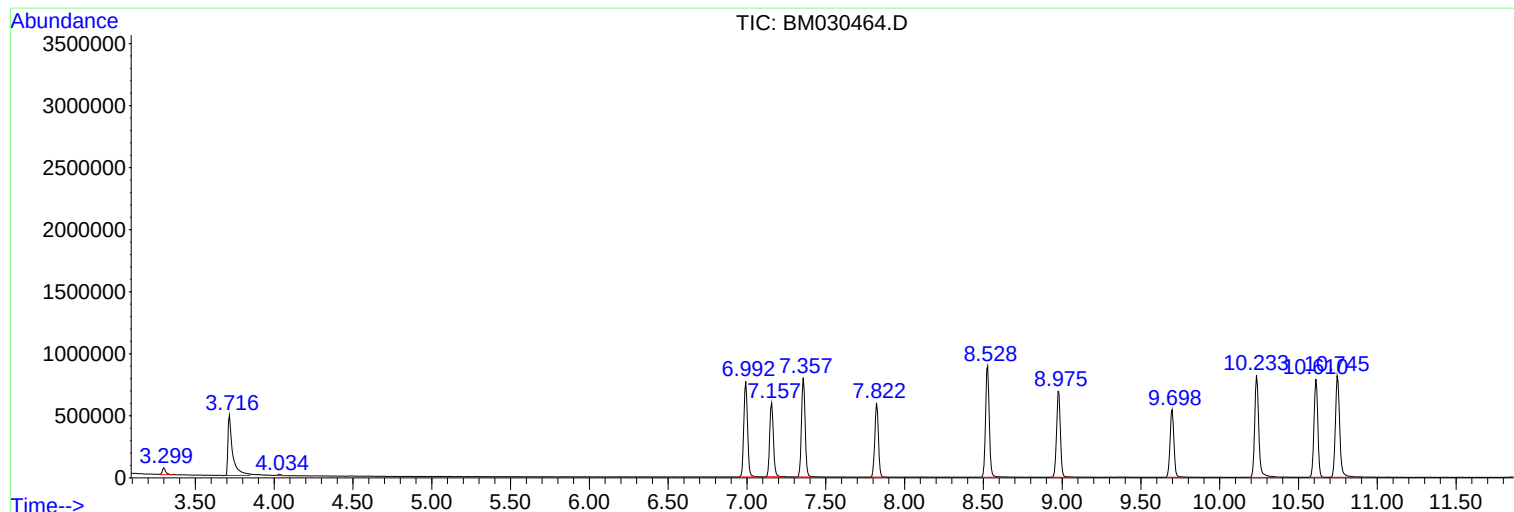

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061621\
Data File : BM030464.D
Acq On : 16 Jun 2021 10:52
Operator : CG/JU
Sample : PB137067BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK067

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM060621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061621\
Data File : BM030464.D
Acq On : 16 Jun 2021 10:52
Operator : CG/JU
Sample : PB137067BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK067

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM060621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------