

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061621\
 Data File : BM030479.D
 Acq On : 16 Jun 2021 22:59
 Operator : CG/JU
 Sample : M2596-06DL 5X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG5Q2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM060621.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030479.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	38	43	55	rBV2	31220	115337	3.76%	0.730%
2	3.822	121	125	133	rVB	49704	72480	2.36%	0.459%
3	3.887	134	136	140	rVV4	6745	9233	0.30%	0.058%
4	3.946	143	146	152	rVB2	11882	16761	0.55%	0.106%
5	4.040	158	162	166	rVB	18352	26230	0.85%	0.166%
6	4.410	222	225	229	rVB6	5570	8429	0.27%	0.053%
7	4.475	234	236	240	rBV5	2914	3675	0.12%	0.023%
8	4.587	250	255	263	rVB	12854	21643	0.71%	0.137%
9	4.952	313	317	324	rVB2	12551	22172	0.72%	0.140%
10	5.057	331	335	345	rVB10	7452	18477	0.60%	0.117%
11	5.352	381	385	389	rVB3	7608	10361	0.34%	0.066%
12	5.481	403	407	416	rVB3	16013	35751	1.17%	0.226%
13	5.846	464	469	475	rBV5	7880	13652	0.44%	0.086%
14	5.893	475	477	480	rVB4	3711	3756	0.12%	0.024%
15	6.222	531	533	538	rVB5	3448	5139	0.17%	0.033%
16	6.640	600	604	605	rBV5	2450	3073	0.10%	0.019%
17	6.998	656	665	672	rBV2	61612	110893	3.61%	0.702%
18	7.157	687	692	698	rBV	46173	77175	2.52%	0.489%
19	7.363	721	727	736	rBV	67495	113020	3.68%	0.716%
20	7.828	798	806	814	rBV	652711	1048213	34.16%	6.637%
21	8.057	840	845	850	rVB7	3138	5229	0.17%	0.033%
22	8.534	920	926	939	rVB	57732	108677	3.54%	0.688%
23	8.922	988	992	993	rBV3	4294	4109	0.13%	0.026%
24	8.981	996	1002	1013	rVB	54937	103932	3.39%	0.658%
25	9.392	1070	1072	1077	rVB5	2617	3700	0.12%	0.023%
26	9.522	1088	1094	1096	rBV6	2176	3810	0.12%	0.024%
27	9.704	1118	1125	1132	rBV	39360	73512	2.40%	0.465%
28	10.245	1210	1217	1228	rBV	61159	128322	4.18%	0.813%
29	10.616	1272	1280	1293	rBV	802088	1420158	46.28%	8.992%
30	10.757	1297	1304	1313	rBV	39671	92436	3.01%	0.585%
31	11.110	1361	1364	1366	rBV4	2145	3073	0.10%	0.019%
32	11.886	1494	1496	1503	rVB6	4481	4917	0.16%	0.031%
33	12.810	1649	1653	1654	rBV4	2790	3693	0.12%	0.023%
34	13.180	1713	1716	1719	rVB4	2552	3123	0.10%	0.020%
35	13.222	1722	1723	1728	rBV5	1782	3095	0.10%	0.020%
36	13.275	1728	1732	1738	rVB6	3760	7013	0.23%	0.044%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061621\
 Data File : BM030479.D
 Acq On : 16 Jun 2021 22:59
 Operator : CG/JU
 Sample : M2596-06DL 5X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG5Q2DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM060621.M
 Title : SVOA CALIBRATION

37	13.857	1825	1831	1838	rBV	123270	194672	6.34%	1.233%
38	14.145	1870	1880	1889	rBV	156177	251956	8.21%	1.595%
39	14.345	1907	1914	1919	rBV7	7019	15666	0.51%	0.099%
40	14.451	1924	1932	1940	rBV	1232645	1854648	60.44%	11.743%
41	14.674	1964	1970	1978	rBV3	19895	54887	1.79%	0.348%
42	14.851	1992	2000	2001	rBV8	5563	10935	0.36%	0.069%
43	14.957	2016	2018	2024	rVB7	2013	3308	0.11%	0.021%
44	15.245	2064	2067	2068	rBV3	2921	3916	0.13%	0.025%
45	15.298	2074	2076	2080	rBV4	2856	3155	0.10%	0.020%
46	15.439	2094	2100	2106	rBV	220960	326236	10.63%	2.066%
47	15.492	2107	2109	2114	rVV5	5929	7367	0.24%	0.047%
48	15.563	2118	2121	2128	rBV7	5396	12938	0.42%	0.082%
49	15.857	2166	2171	2177	rBV2	21354	29021	0.95%	0.184%
50	16.157	2217	2222	2223	rBV5	4979	6196	0.20%	0.039%
51	16.380	2256	2260	2261	rBV4	3089	4604	0.15%	0.029%
52	16.727	2317	2319	2323	rBV5	3932	4677	0.15%	0.030%
53	16.839	2333	2338	2340	rBV6	9915	16892	0.55%	0.107%
54	16.951	2352	2357	2360	rBV5	21419	35204	1.15%	0.223%
55	17.186	2390	2397	2402	rBV	1525419	2191181	71.41%	13.874%
56	17.227	2402	2404	2408	rVV	49098	63063	2.06%	0.399%
57	17.286	2408	2414	2424	rVB2	234063	383526	12.50%	2.428%
58	18.074	2545	2548	2552	rBV5	26267	35800	1.17%	0.227%
59	19.239	2743	2746	2752	rVB	93914	116393	3.79%	0.737%
60	19.568	2798	2802	2815	rBV2	311956	590507	19.24%	3.739%
61	21.350	3100	3105	3110	rBV	2106534	2803885	91.37%	17.753%
62	23.621	3486	3491	3501	rVB2	1554732	3068551	100.00%	19.429%


Sum of corrected areas: 15793453

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061621\
Data File : BM030479.D
Acq On : 16 Jun 2021 22:59
Operator : CG/JU
Sample : M2596-06DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG5Q2DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM060621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

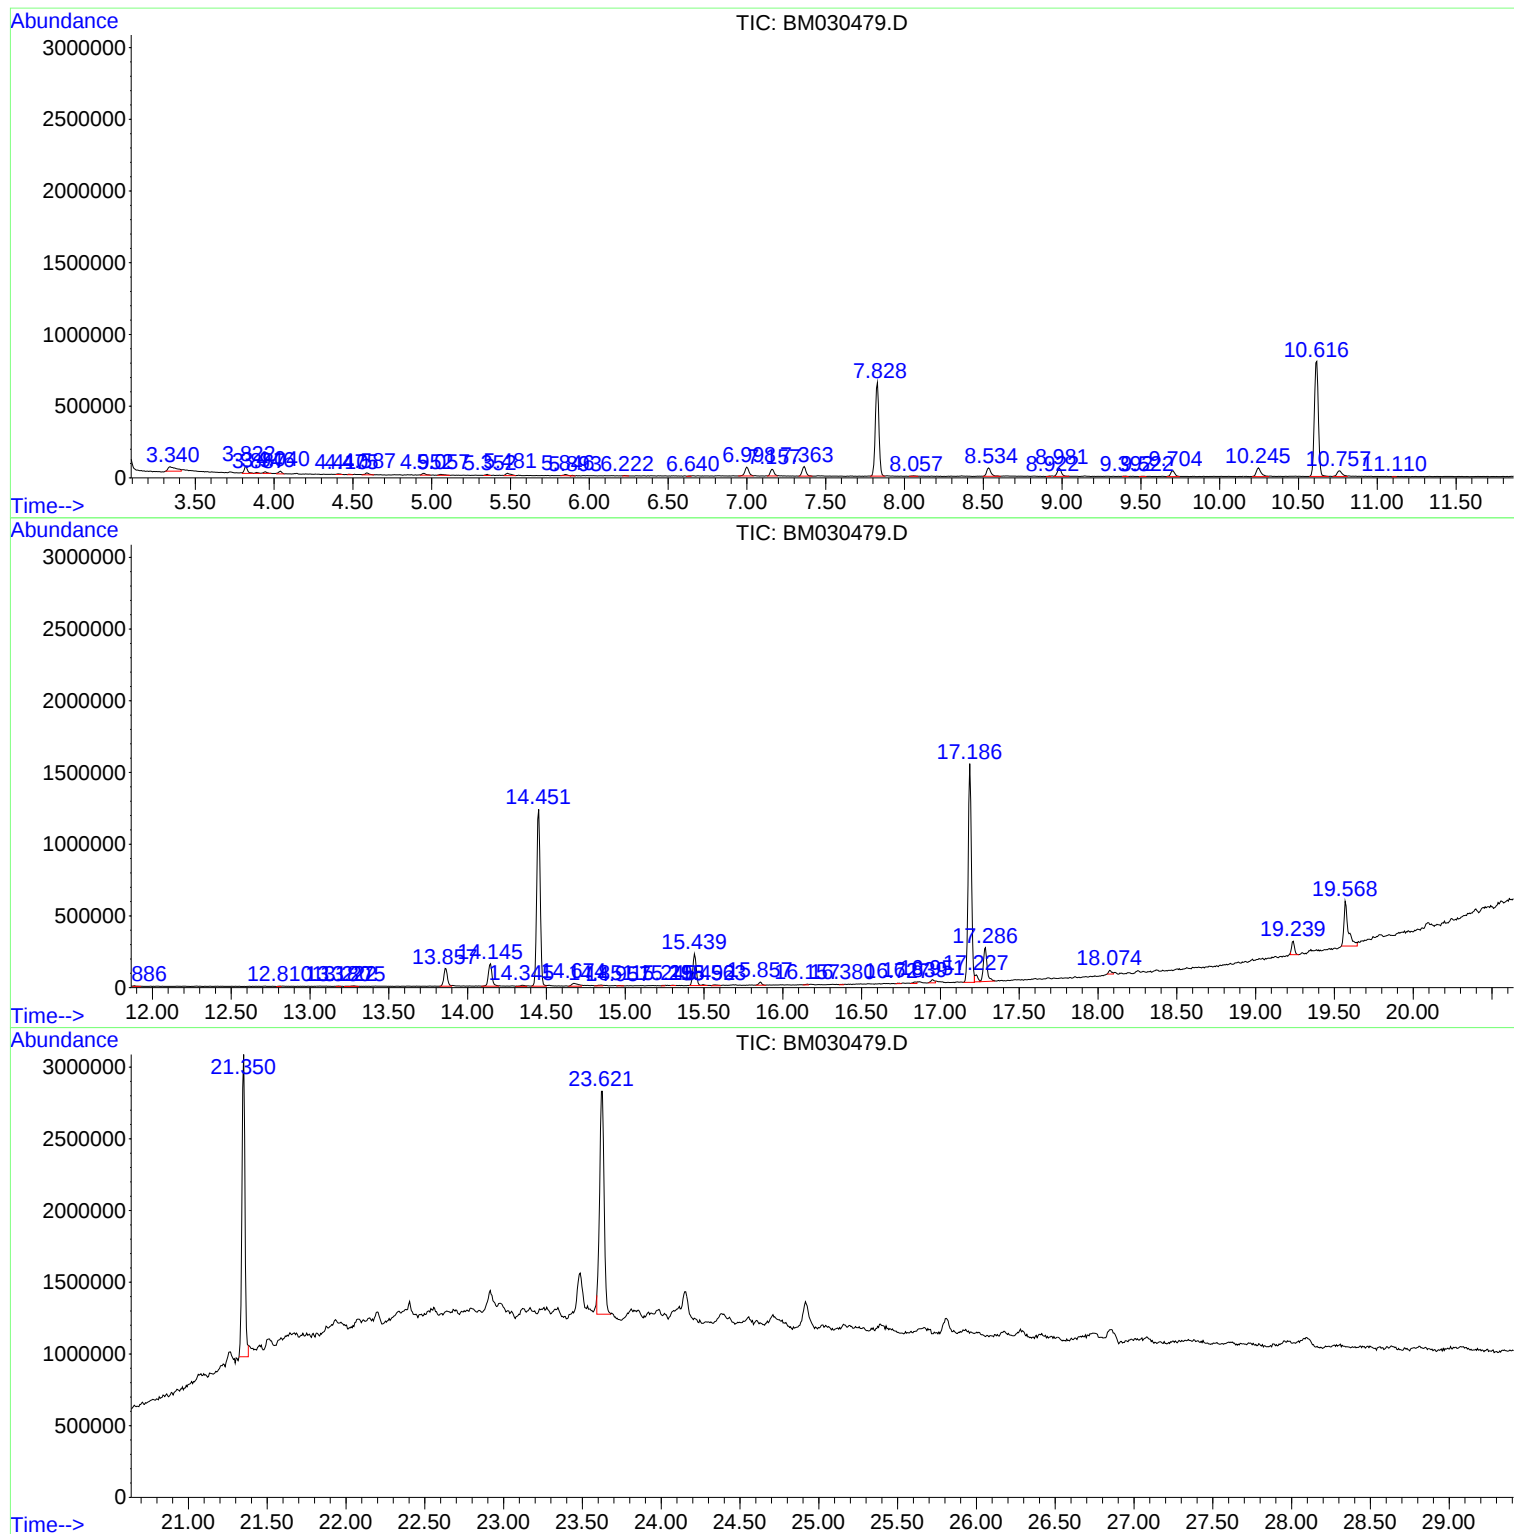

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061621\
Data File : BM030479.D
Acq On : 16 Jun 2021 22:59
Operator : CG/JU
Sample : M2596-06DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG5Q2DL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM060621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Butenoic acid, methyl est... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.340	2.20 ng/ul	115337	1,4-Dichlorobenzene-d4	7.828

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Butenoic acid, methyl ester, (Z)-	100	C5H8O2	004358-59-2	59
2			2-Propenoic acid, 2-methyl-, 2-h...	144	C7H12O3	000923-26-2	56
3			Methyl methacrylate	100	C5H8O2	000080-62-6	53
4			Methyl 3-butenate	100	C5H8O2	003724-55-8	53
5			Methyl methacrylate	100	C5H8O2	000080-62-6	50

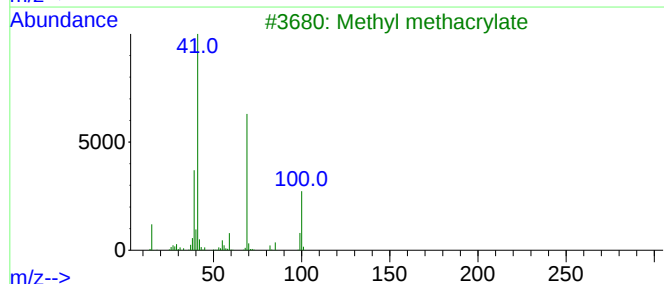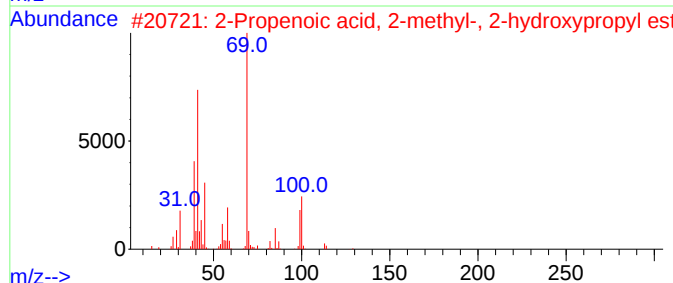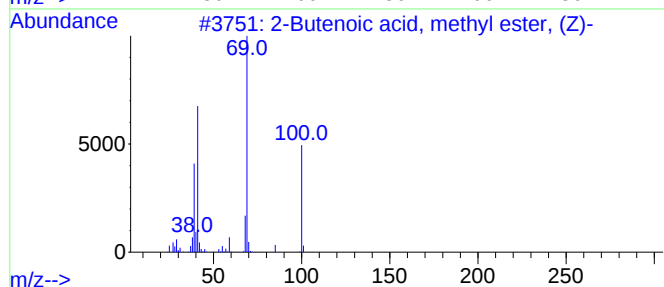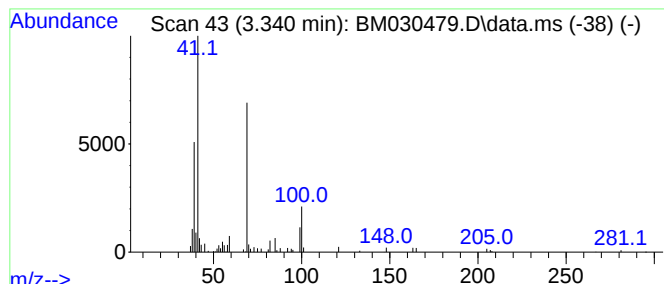

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061621\
Data File : BM030479.D
Acq On : 16 Jun 2021 22:59
Operator : CG/JU
Sample : M2596-06DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG5Q2DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM060621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Butenoic acid...	3.340	2.2	ng/ul	115337	1	7.828	1048210	20.0