

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061715\
 Data File : BM001717.D
 Acq On : 17 Jun 2015 11:12
 Operator : TP/IZ
 Sample : PB84051BL
 Misc : SBLK74
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK74

Quant Time: Jun 18 03:28:43 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061515.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 18 03:27:43 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	56248	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	214090	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	127667	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	300264	20.00	ng/ul	0.00
77) Chrysene-d12	21.26	240	362867	20.00	ng/ul	0.00
85) Perylene-d12	23.48	264	383226	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.14	96	7367	6.24	ng/uL	0.00
5) Phenol-d5	6.83	99	128230	29.68	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	78142	32.29	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	105070	30.75	ng/ul	0.00
13) 4-Methylphenol-d8	8.37	113	103730	29.91	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	47131	31.80	ng/ul	0.00
22) 2-Nitrophenol-d4	9.55	143	50797	31.35	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.07	165	104040	29.99	ng/ul	0.00
29) 4-Chloroaniline-d4	10.59	131	141932	40.22	ng/ul	0.00
43) Dimethylphthalate-d6	13.73	166	320727	33.88	ng/ul	0.00
46) Acenaphthylene-d8	14.01	160	397645	32.04	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	50384	28.85	ng/ul	0.00
57) Fluorene-d10	15.32	176	294555	33.53	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	46454	25.33	ng/ul	0.00
70) Anthracene-d10	17.16	188	473229	33.83	ng/ul	0.00
78) Pyrene-d10	19.46	212	540901	35.19	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.34	264	586601	34.73	ng/ul	0.00


Target Compounds					Qvalue
45) 2,6-Dinitrotoluene	13.73	165	2515	1.29 ng/ul#	34


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061715\
Data File : BM001717.D
Acq On : 17 Jun 2015 11:12
Operator : TP/IZ
Sample : PB84051BL
Misc : SBLK74
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK74

Quant Time: Jun 18 03:28:43 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061515.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 18 03:27:43 2015
Response via : Initial Calibration

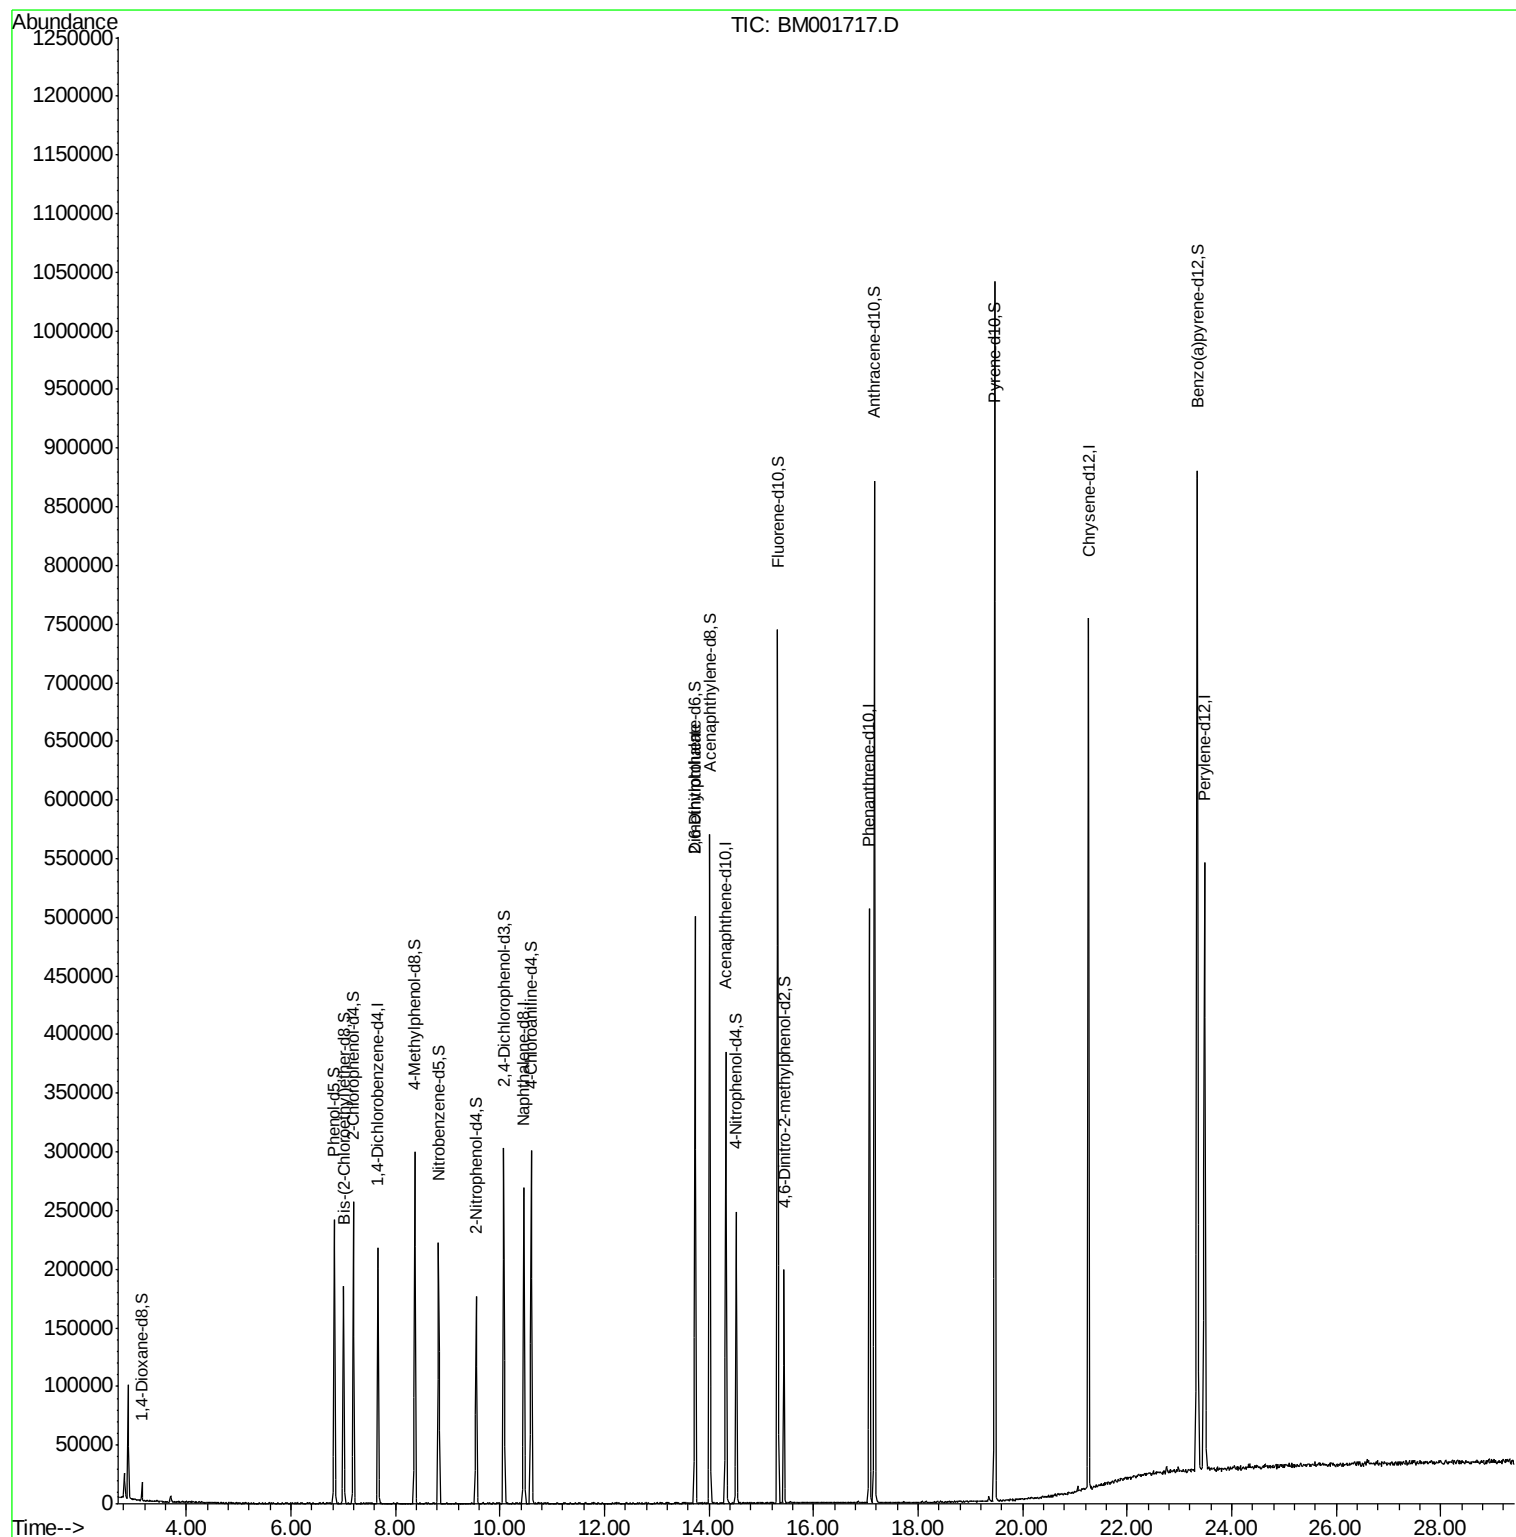

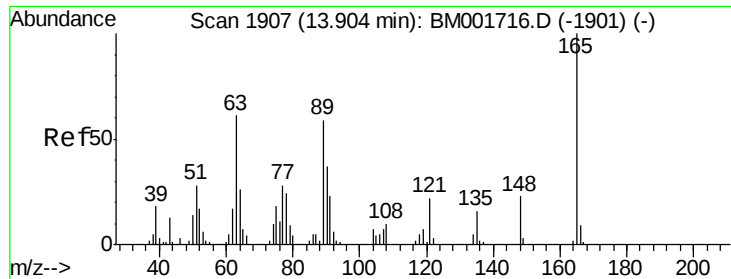

#45

2,6-Dinitrotoluene

Concen: 1.29 ng/ul

RT: 13.73 min Scan# 1877

Delta R.T. -0.18 min

Lab File: BM001717.D


Acq: 17 Jun 2015 11:12

Instrument :

BNA_M

ClientSampleId :

SBLK74

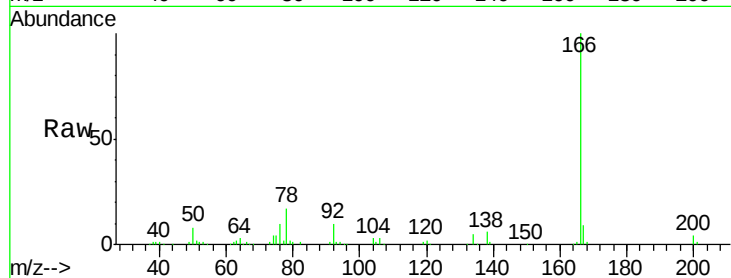

Tgt Ion:	165	Resp:	2515
Ion Ratio	Lower	Upper	
165	100		
89	0.0	49.1	73.7#
121	34.5	17.4	26.2#

