


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061715\
 Data File : BM001715.D
 Acq On : 17 Jun 2015 09:56
 Operator : TP/IZ
 Sample : DFTPP61
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP61

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061515.M
 Title : SVOA CALIBRATION
 Last Update : Thu Jun 18 03:27:43 2015

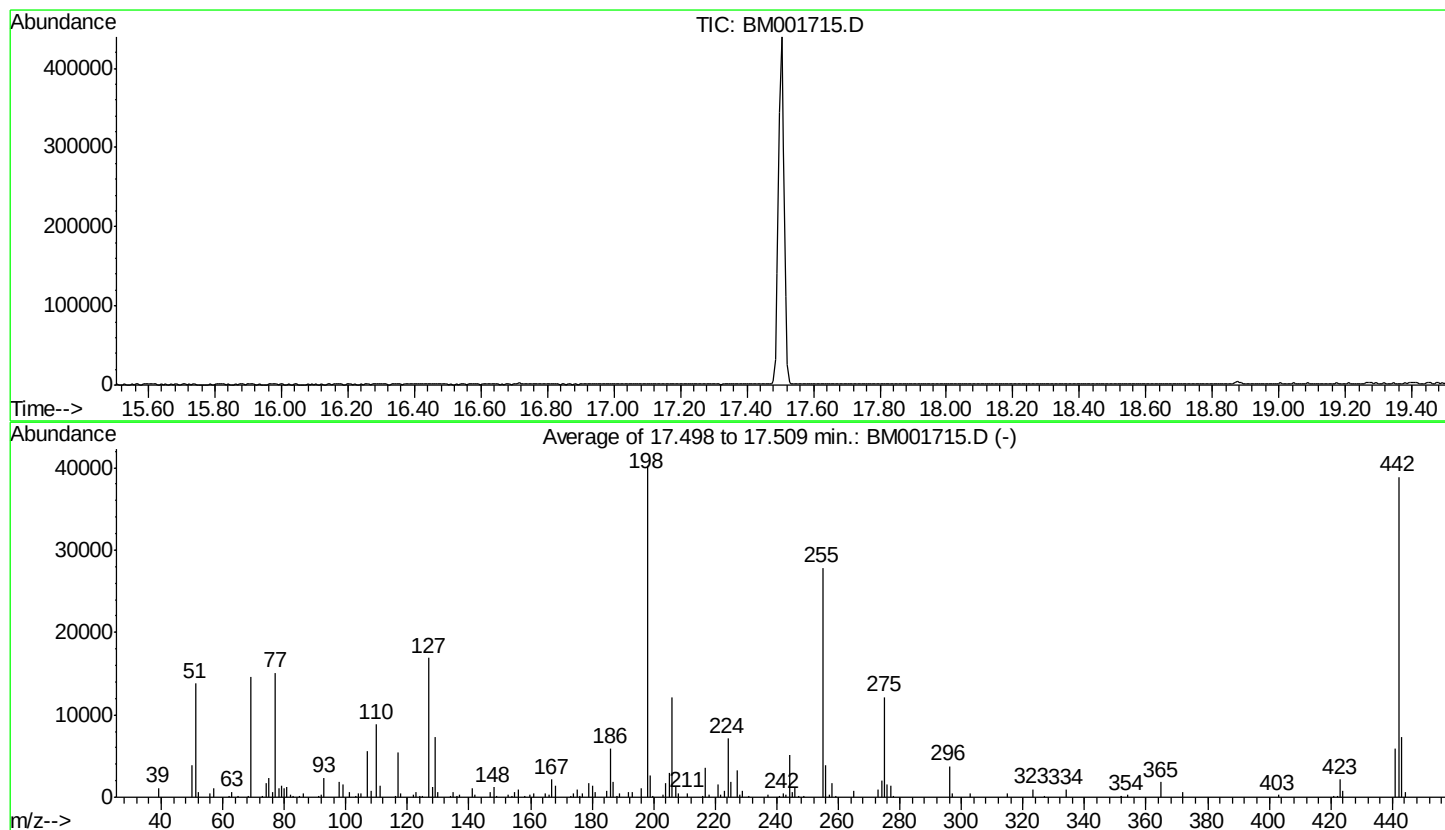

AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2513

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.3	13826	PASS
68	69	0.00	2	1.0	148	PASS
69	198	0.00	100	36.3	14626	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.0	16925	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	40256	PASS
199	198	5	9	6.7	2692	PASS
275	198	10	60	30.2	12164	PASS
365	198	1	100	4.6	1861	PASS
441	442	0.01	24	15.4	5974	PASS
442	198	50	100	96.6	38893	PASS
443	442	15	24	18.7	7279	PASS

m/z	Abundance
39.00	1321.0
44.00	1026.0
50.10	4325.0
51.10	15259.0
52.10	831.0
56.00	536.0
57.00	1044.0
62.00	332.0
63.00	592.0
69.00	15996.0
74.00	1964.0
75.00	2930.0
76.00	685.0
77.10	16291.0
78.10	1217.0
79.00	1805.0
80.00	1032.0
80.90	1302.0
82.00	400.0
86.00	488.0
91.00	324.0
91.90	456.0
93.00	2501.0
98.00	1948.0
99.00	1908.0
101.00	736.0
103.00	359.0
104.00	631.0
105.00	463.0
107.00	6036.0
108.00	836.0
110.00	9745.0
111.00	1600.0
117.00	5767.0
118.00	596.0
122.00	512.0
122.90	806.0
127.00	17256.0
128.00	1448.0
129.00	7513.0
130.10	570.0
134.00	305.0
135.00	528.0
137.10	411.0
141.00	1225.0
141.90	333.0
146.90	632.0
147.90	1151.0
149.10	323.0
155.00	561.0
156.10	785.0
159.90	490.0
160.90	535.0
165.00	487.0
167.00	2112.0
168.00	1724.0
174.00	501.0
175.00	824.0
175.90	300.0
176.90	389.0
178.90	1579.0
179.90	1286.0
180.90	543.0
184.90	764.0
186.00	5871.0
187.00	1513.0
189.00	572.0
191.90	689.0
193.00	606.0
196.00	750.0
197.90	39456.0
199.00	2420.0
202.90	418.0
204.00	1635.0
205.00	3009.0
206.10	11947.0
207.10	1913.0
208.00	368.0
211.00	490.0
215.90	337.0
217.00	3278.0
221.00	1584.0
221.70	407.0
223.00	701.0
224.10	6468.0
225.00	1982.0
227.00	2900.0
228.00	453.0
228.90	797.0
237.00	488.0
242.00	361.0

Instrument :
BNA_M
ClientSampleId :
DFTPP61

243.00	426.0
244.00	4620.0
245.00	662.0
246.00	1157.0
255.00	25488.0
256.00	3489.0
258.00	1340.0
265.10	943.0
273.00	877.0
274.00	1631.0
275.00	10982.0
276.00	1285.0
276.90	1321.0
296.00	3590.0
297.00	413.0
303.00	434.0
314.90	458.0
323.00	666.0
334.00	843.0
365.00	1441.0
372.10	471.0
403.00	447.0
423.00	1463.0
424.00	552.0
441.10	4436.0
442.10	27240.0
443.10	5791.0
444.10	562.0

Instrument :
BNA_M
ClientSampleId :
DFTPP61

m/z	Abundance
39.00	1195.0
44.00	1115.0
50.10	4713.0
51.10	16536.0
52.00	796.0
56.00	561.0
57.00	1288.0
63.00	775.0
65.00	384.0
68.10	445.0
69.00	17608.0
73.00	364.0
74.00	2294.0
75.00	2627.0
76.10	849.0
77.10	18008.0
78.00	1252.0
79.00	1521.0
80.00	1415.0
81.00	1644.0
82.00	414.0
83.00	376.0
84.90	390.0
85.80	436.0
90.90	361.0
91.90	553.0
93.00	2854.0
98.00	2368.0
99.00	1735.0
101.00	694.0
103.90	529.0
105.00	515.0
107.00	6412.0
108.10	1099.0
110.00	10476.0
111.00	1620.0
116.10	328.0
117.00	6304.0
117.90	378.0
121.90	556.0
123.00	615.0
124.00	352.0
125.00	371.0
127.00	20488.0
128.00	1513.0
129.00	9010.0
130.00	832.0
134.90	773.0
136.00	301.0
137.00	416.0
141.00	1340.0
142.00	456.0
147.00	660.0
147.90	1396.0
149.00	346.0
153.00	362.0
154.00	327.0
154.90	640.0
156.00	1135.0
157.90	331.0
159.80	355.0
161.00	603.0
165.00	397.0
166.00	453.0
167.00	2374.0
168.00	1611.0
173.00	456.0
174.00	661.0
175.00	1178.0
175.90	342.0
176.90	562.0
178.90	2066.0
180.00	1664.0
181.00	701.0
184.90	834.0
186.00	6646.0
187.00	2406.0
187.90	479.0
188.90	425.0
191.90	703.0
192.90	792.0
196.00	1231.0
198.00	48768.0
199.00	3348.0
203.00	315.0
204.00	2128.0
205.00	3764.0
206.00	14640.0
207.00	2098.0
208.00	784.0
211.00	668.0

Instrument :
BNA_M
ClientSampleId :
DFTPP61

215.90	346.0
217.00	4637.0
218.00	569.0
221.00	1933.0
221.80	589.0
223.00	1074.0
224.00	8840.0
225.00	2264.0
227.00	3817.0
227.90	578.0
229.00	972.0
230.90	310.0
237.00	446.0
240.80	305.0
241.90	405.0
243.00	370.0
244.10	6244.0
245.00	779.0
246.10	1432.0
246.90	312.0
255.00	32872.0
256.00	4890.0
256.90	508.0
258.00	2132.0
259.00	384.0
265.00	868.0
273.00	915.0
274.00	2683.0
275.00	14827.0
276.00	2085.0
276.90	1589.0
278.00	353.0
296.00	4212.0
297.00	514.0
303.00	452.0
314.90	485.0
323.10	1356.0
327.00	329.0
334.10	1015.0
352.10	348.0
354.00	421.0
365.00	2325.0
372.10	928.0
403.00	378.0
422.10	436.0
423.10	2456.0
424.00	788.0
441.10	7276.0
442.10	47040.0
443.10	8765.0
444.00	852.0

Instrument :
BNA_M
ClientSampleId :
DFTPP61

m/z	Abundance
39.10	822.0
44.00	973.0
50.00	2827.0
51.10	9684.0
52.00	425.0
55.90	341.0
57.00	806.0
63.00	528.0
69.00	10276.0
74.00	1050.0
75.00	1476.0
76.00	519.0
77.10	11174.0
78.00	704.0
78.90	832.0
80.00	917.0
80.90	942.0
86.00	363.0
93.00	1798.0
97.90	1270.0
99.00	968.0
101.10	512.0
103.90	311.0
104.90	378.0
107.00	4252.0
107.90	534.0
110.00	6241.0
111.00	961.0
117.00	4115.0
118.00	370.0
122.90	465.0
127.00	13031.0
127.90	868.0
129.00	5637.0
129.90	527.0
134.90	603.0
141.00	866.0
147.10	404.0
148.00	1179.0
152.80	355.0
154.90	465.0
156.00	668.0
160.00	302.0
161.00	417.0
164.90	410.0
166.00	385.0
166.90	1883.0
168.00	1052.0
174.10	418.0
175.00	659.0
177.00	371.0
179.00	1414.0
180.00	1044.0
181.00	426.0
184.90	669.0
186.00	5011.0
187.00	1560.0
188.90	357.0
191.80	412.0
193.00	606.0
196.00	1183.0
198.00	32544.0
199.00	2310.0
199.80	364.0
204.00	1523.0
205.00	2081.0
206.00	9932.0
207.00	1941.0
208.10	416.0
211.00	408.0
216.90	2772.0
217.90	338.0
221.10	1119.0
223.00	624.0
224.00	5944.0
225.00	1317.0
227.00	3059.0
229.00	562.0
241.90	429.0
243.00	367.0
244.00	4605.0
245.00	608.0
246.00	1044.0
248.90	340.0
255.00	25296.0
256.00	3189.0
257.00	396.0
258.00	1473.0
264.90	764.0
272.90	800.0
274.00	1728.0

Instrument :
BNA_M
ClientSampleId :
DFTPP61

275.00	10684.0
276.00	1188.0
276.90	1176.0
296.00	3526.0
296.90	471.0
303.00	555.0
314.90	455.0
323.00	833.0
334.00	808.0
351.80	300.0
353.90	358.0
365.00	1818.0
372.00	622.0
421.00	335.0
423.00	2396.0
424.00	807.0
441.10	6211.0
442.10	42400.0
443.10	7283.0
444.10	610.0

Instrument :
BNA_M
ClientSampleId :
DFTPP61

Scan 2513 (17.468 min): BM001715.D
DFTPP61

m/z	Abundance
44.00	1041.0
207.00	682.0

Instrument :
BNA_M
ClientSampleId :
DFTPP61