




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061716\
Data File : BM005841.D
Acq On : 16 Jun 2016 23:14
Operator : UM/SJ
Sample : H3535-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9XW6

Quant Time: Jun 17 01:57:35 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061716.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 17 01:56:56 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

sohil
6/17/2016 7:27:39 PM

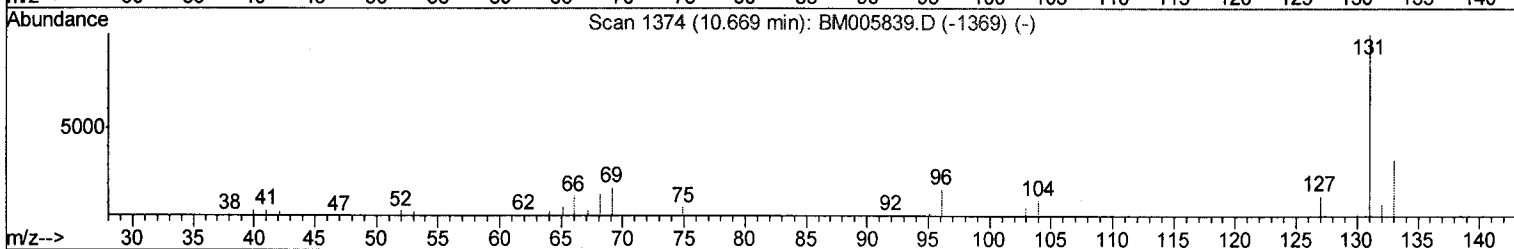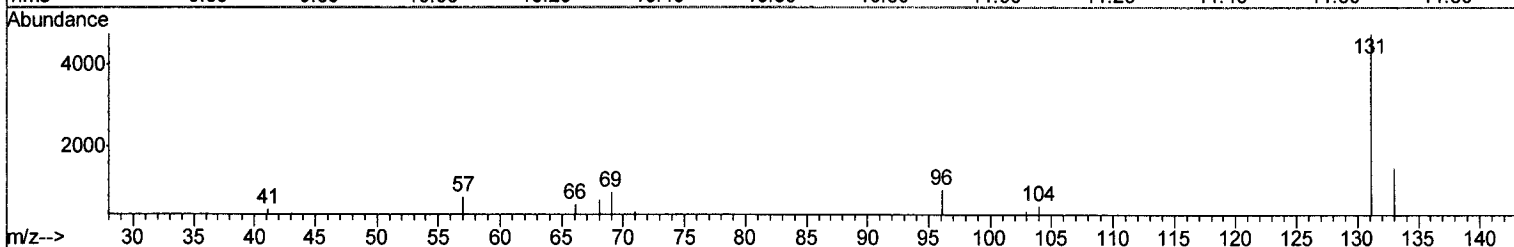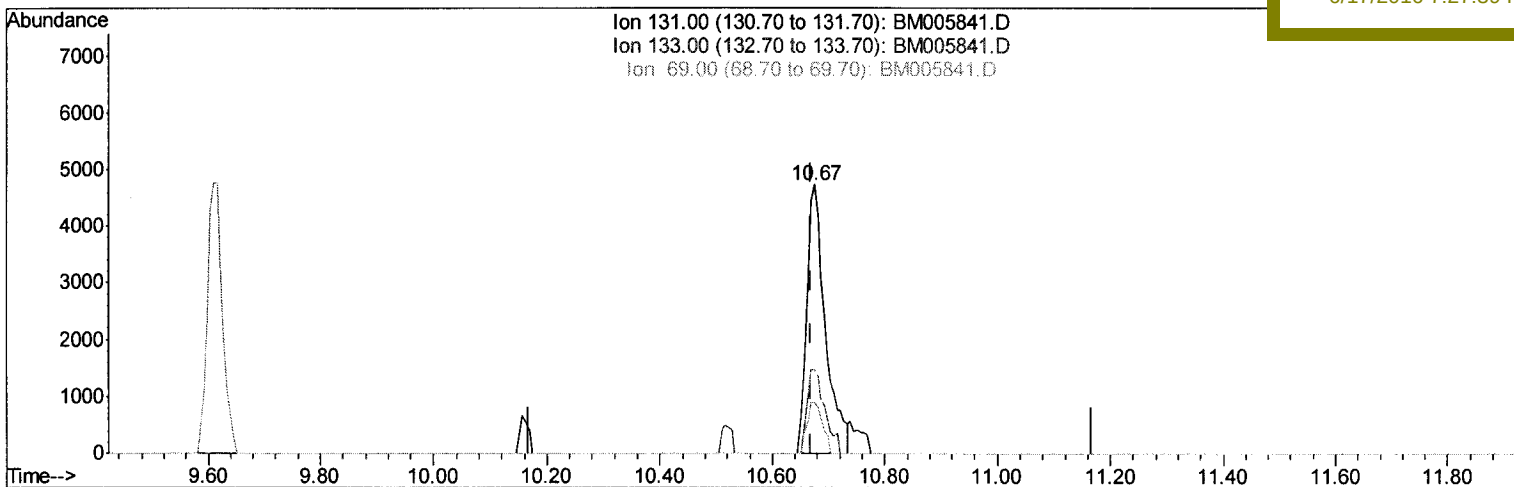

TIC: BM005841.D

(12) 4-Chloroaniline-d4 (S)

10.675min (+0.006) 8.23ng/ul

response 10843

Ion	Exp%	Act%
131.00	100	100
133.00	30.80	31.22
69.00	17.50	18.73
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061716\
 Data File : BM005841.D
 Acq On : 16 Jun 2016 23:14
 Operator : UM/SJ
 Sample : H3535-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9XW6

Manual Integrations
 APPROVED

sohil
 6/17/2016 7:27:39 PM

Quant Time: Jun 17 01:57:35 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061716.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 17 01:56:56 2016
 Response via : Initial Calibration

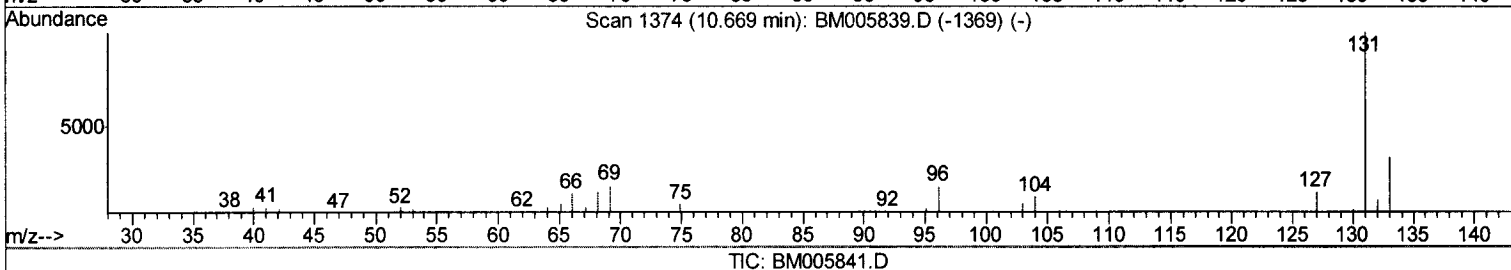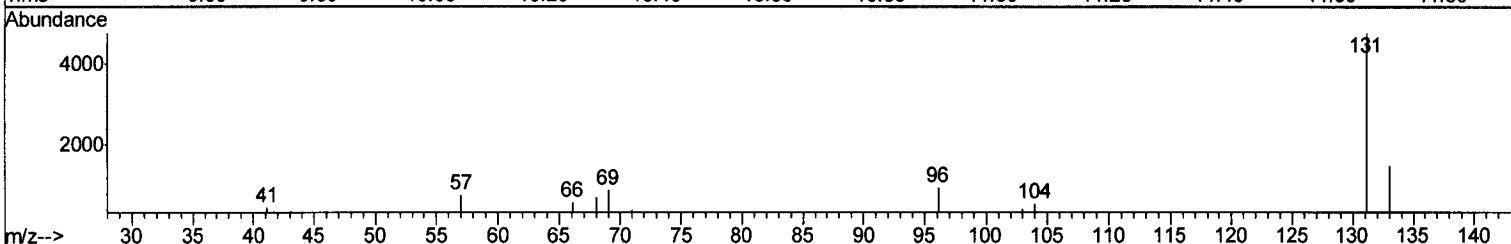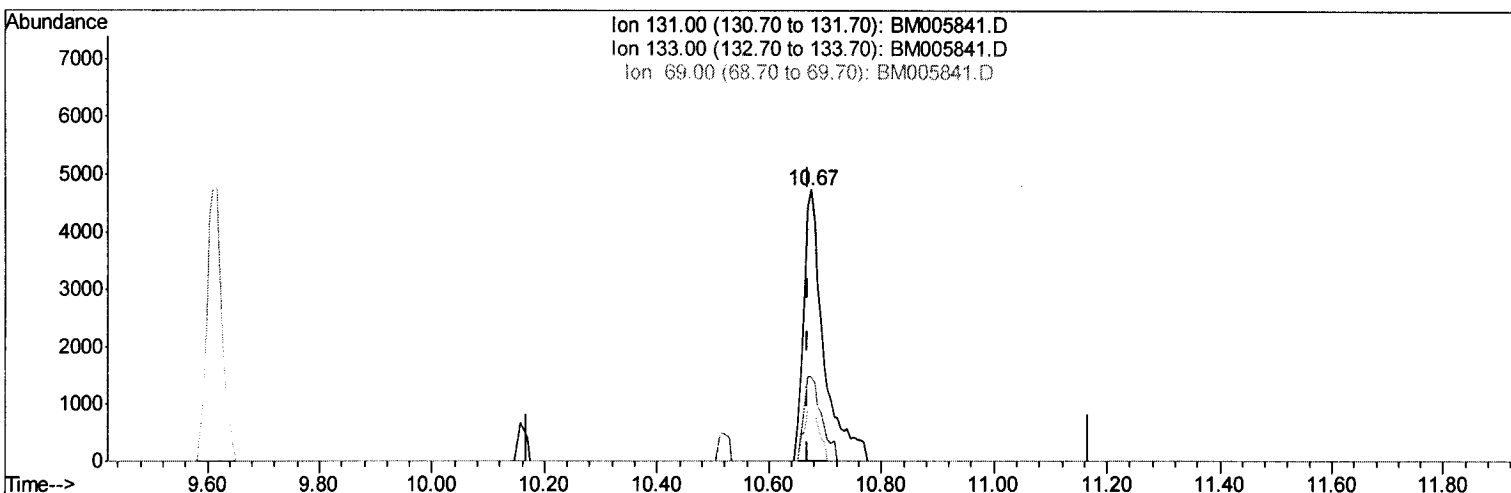

TIC: BM005841.D

(12) 4-Chloroaniline-d4 (S)

10.675min (+0.006) 8.89ng/ul m

response 11706

Ion	Exp%	Act%
131.00	100	100
133.00	30.80	31.22
69.00	17.50	18.73
0.00	0.00	0.00

> U.M
 06/20/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061716\
 Data File : BM005841.D
 Acq On : 16 Jun 2016 23:14
 Operator : UM/SJ
 Sample : H3535-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9XW6

Quant Time: Jun 17 01:57:35 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061716.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 17 01:56:56 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

sohil
 6/17/2016 7:27:39 PM

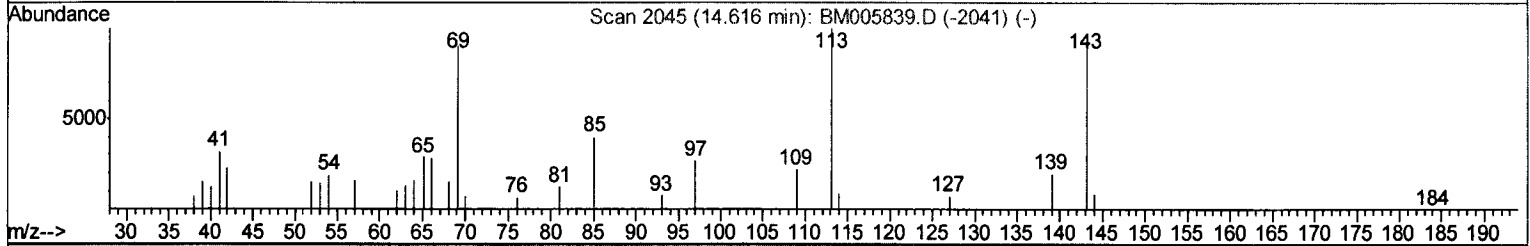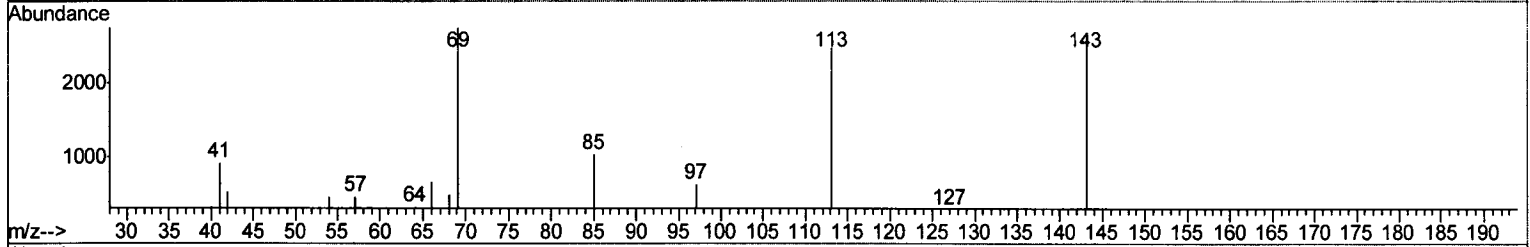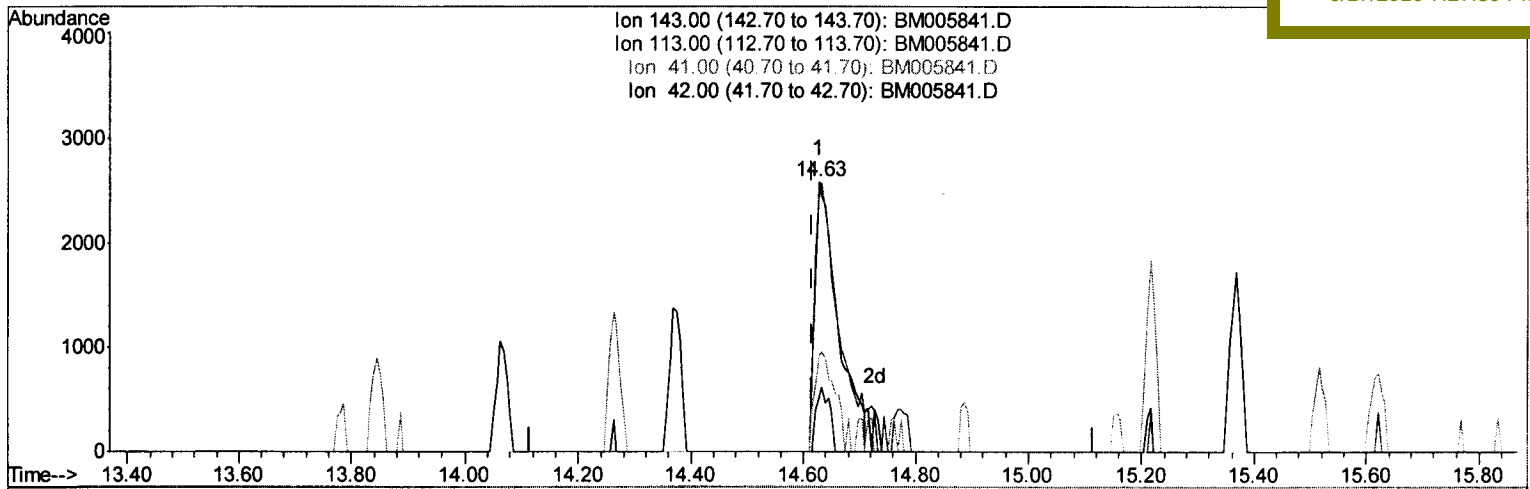

TIC: BM005841.D

(20) 4-Nitrophenol-d4 (S)

14.627min (+0.012) 8.54ng/ul

response 7487

Ion	Exp%	Act%
143.00	100	100
113.00	97.50	96.45
41.00	32.50	35.62
42.00	23.00	20.22

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061716\
 Data File : BM005841.D
 Acq On : 16 Jun 2016 23:14
 Operator : UM/SJ
 Sample : H3535-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9XW6

Manual Integrations
 APPROVED

sohil
 6/17/2016 7:27:39 PM

Quant Time: Jun 17 01:57:35 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061716.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 17 01:56:56 2016
 Response via : Initial Calibration

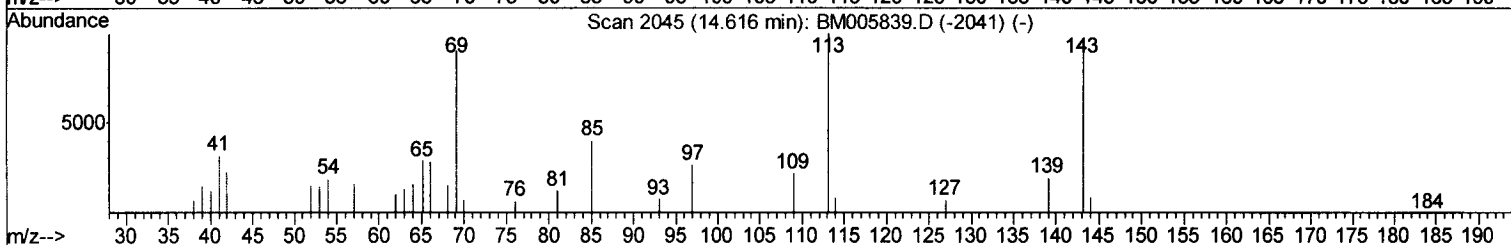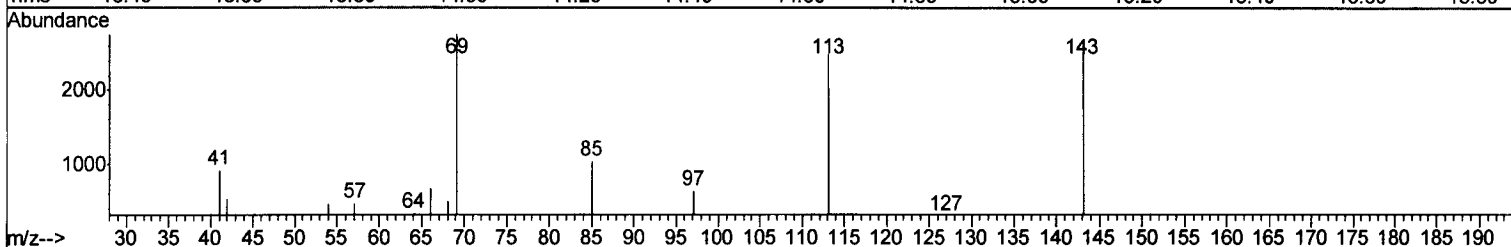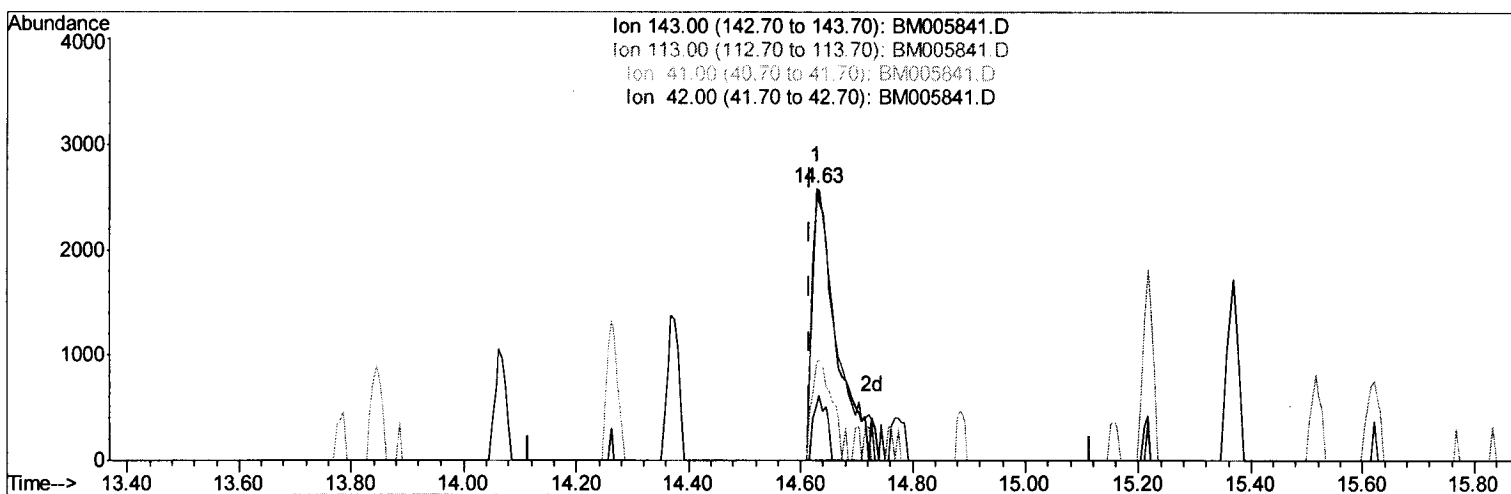

TIC: BM005841.D

(20) 4-Nitrophenol-d4 (S)

14.627min (+0.012) 8.71ng/ul m

response 7634

> U.M
 06/20/16

Ion	Exp%	Act%
143.00	100	100
113.00	97.50	96.45
41.00	32.50	35.62
42.00	23.00	20.22

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061716\
 Data File : BM005841.D
 Acq On : 16 Jun 2016 23:14
 Operator : UM/SJ
 Sample : H3535-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9XW6

Quant Time: Jun 17 02:04:48 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061716.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 17 01:56:56 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

sohil
 6/17/2016 7:27:39 PM

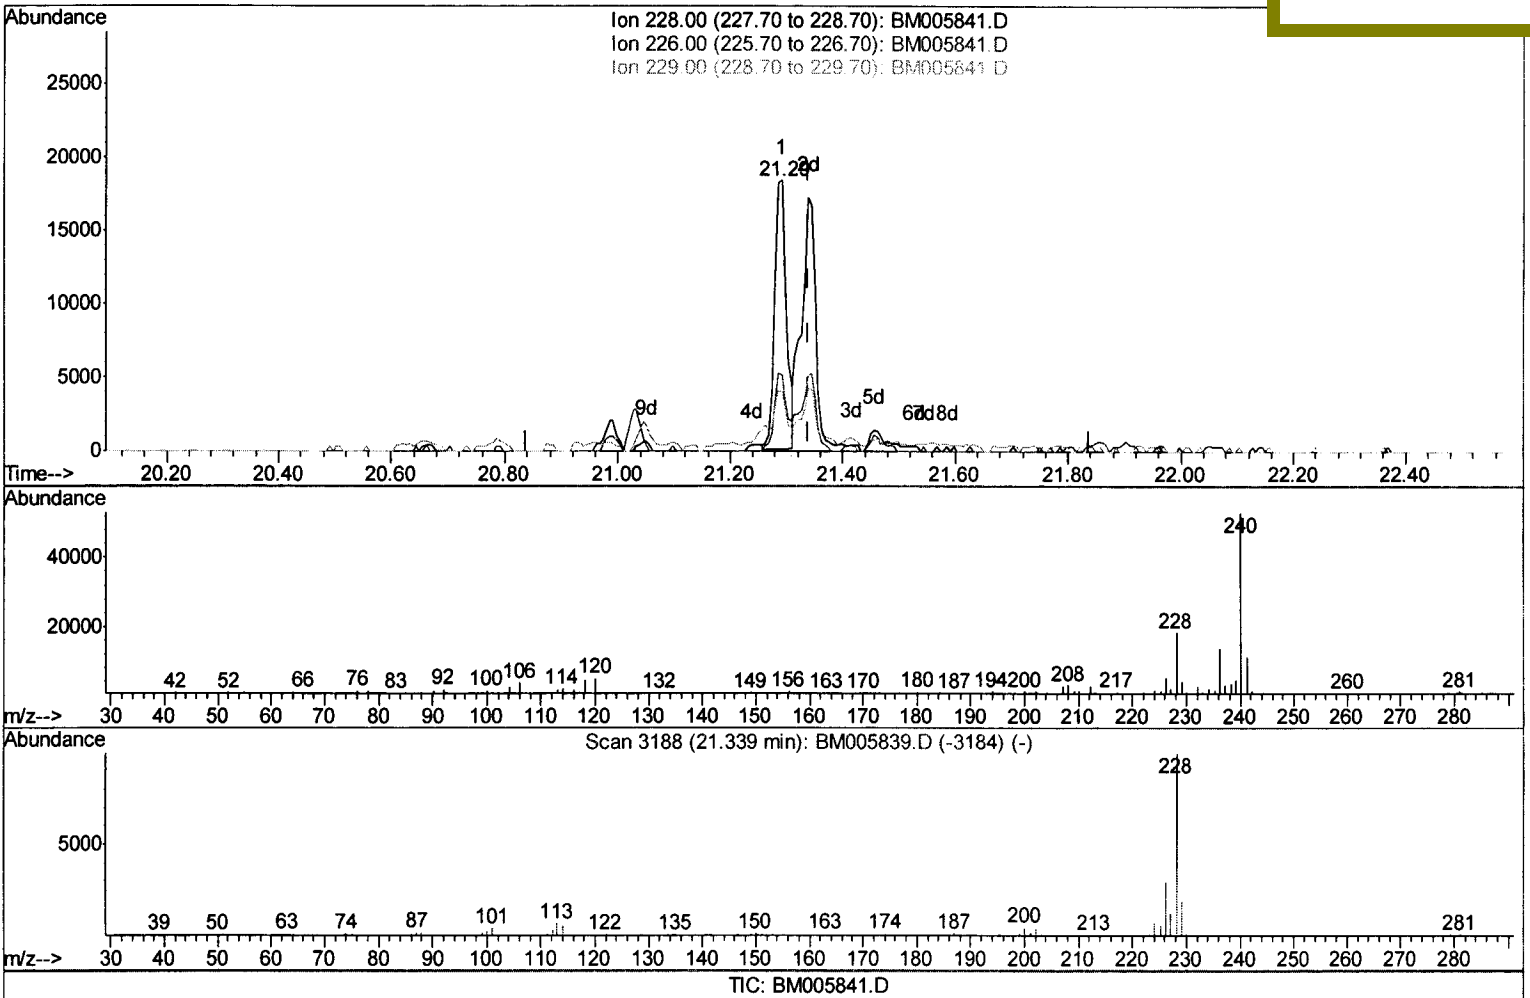

(33) Chrysene

21.291min (-0.047) 1.94ng/ul

response 26566

Ion	Exp%	Act%
228.00	100	100
226.00	29.40	28.10
229.00	19.20	22.04
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061716\
 Data File : BM005841.D
 Acq On : 16 Jun 2016 23:14
 Operator : UM/SJ
 Sample : H3535-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9XW6

Manual Integrations
 APPROVED

sohil
 6/17/2016 7:27:39 PM

Quant Time: Jun 17 02:04:48 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061716.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 17 01:56:56 2016
 Response via : Initial Calibration

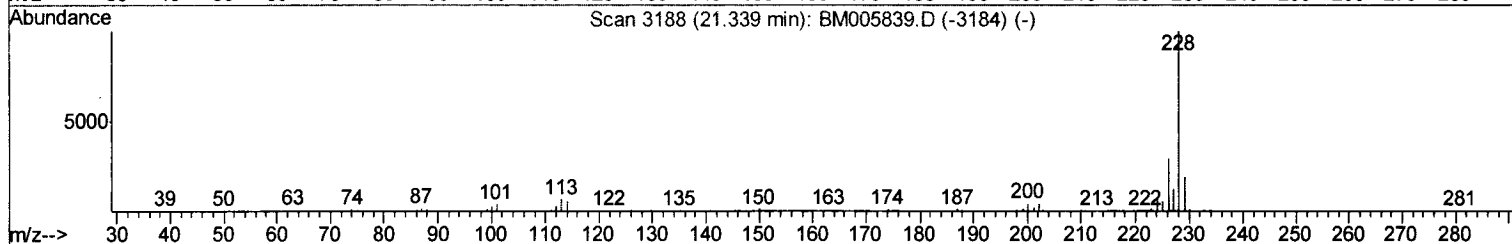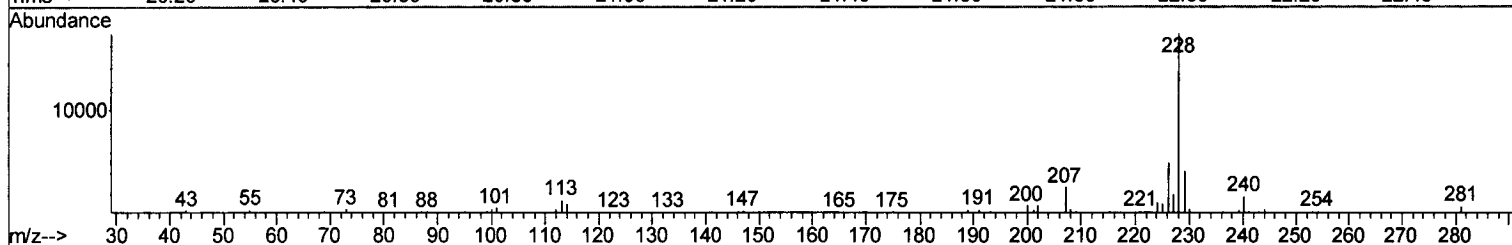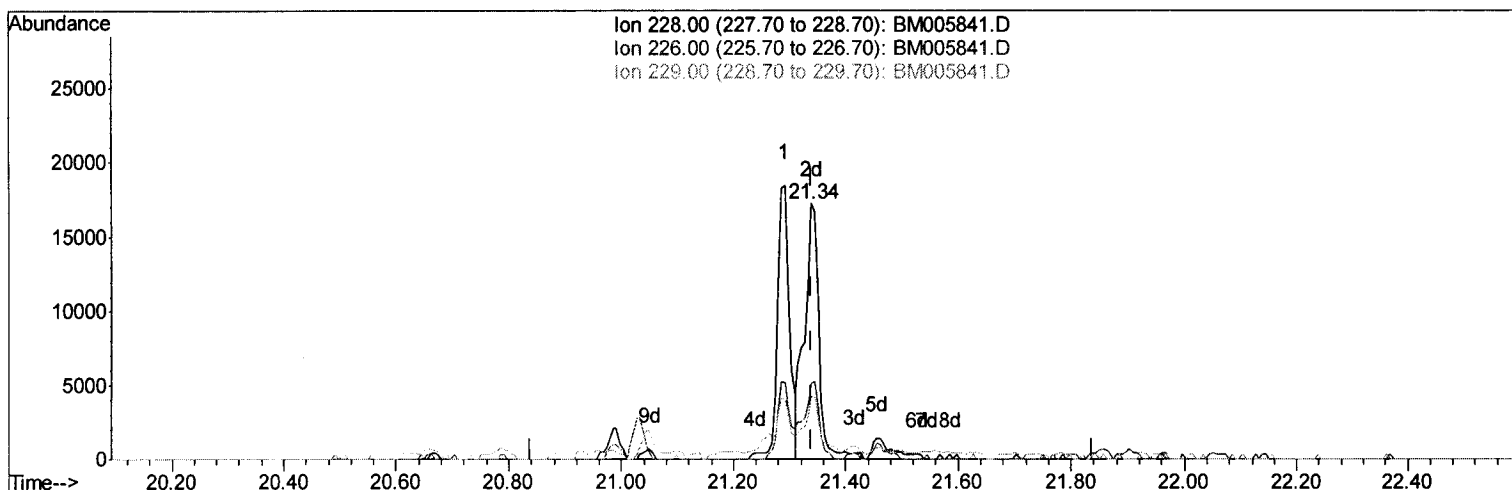

TIC: BM005841.D

(33) Chrysene

21.339min (-0.000) 2.30ng/ul m

response 31507

Ion Exp% Act%

228.00 100 100

226.00 29.40 29.56

229.00 19.20 24.76#

0.00 0.00 0.00

> U.M
 06/20/16

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061716\
 Data File : BM005841.D
 Acq On : 16 Jun 2016 23:14
 Operator : UM/SJ
 Sample : H3535-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9XW6

Quant Time: Jun 17 02:06:25 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061716.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 17 01:56:56 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

sohil
 6/17/2016 7:27:39 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	23457	20.00	ng/ul	0.00
7) Naphthalene-d8	10.52	136	114231	20.00	ng/ul	0.00
15) Acenaphthene-d10	14.37	164	76868	20.00	ng/ul	0.00
23) Phenanthrene-d10	17.12	188	183273	20.00	ng/ul	0.00
29) Chrysene-d12	21.30	240	227348	20.00	ng/ul	0.00
34) Perylene-d12	23.56	264	228569	20.00	ng/ul	0.00

System Monitoring Compounds

2) 1,4-Dioxane-d8	3.17	96	521	2.88	ng/uL	0.00
3) Phenol-d5	6.92	99	29726	15.14	ng/ul	0.00
4) Bis-(2-Chloroethyl) ether-d	7.06	67	17233	16.93	ng/ul	0.00
5) 2-Chlorophenol-d4	7.27	132	28305	16.93	ng/ul	0.00
6) 4-Methylphenol-d8	8.45	113	19638	11.19	ng/ul	0.00
8) Nitrobenzene-d5	8.89	128	13632	16.91	ng/ul	0.00
9) 2-Nitrophenol-d4	9.61	143	17236	17.49	ng/ul	0.00
10) 2,4-Dichlorophenol-d3	10.16	165	32836	16.87	ng/ul	0.00
12) 4-Chloroaniline-d4	10.67	131	11706m	8.89	ng/ul	0.00
16) Dimethylphthalate-d6	13.78	166	122711	16.87	ng/ul	0.00
17) Acenaphthylene-d8	14.07	160	148489	17.72	ng/ul	0.00
20) 4-Nitrophenol-d4	14.63	143	7634m	8.71	ng/ul	0.01
21) Fluorene-d10	15.37	176	108990	17.59	ng/ul	0.00
24) 4,6-Dinitro-2-methylphenol	15.52	200	16163	13.07	ng/ul	0.00
26) Anthracene-d10	17.22	188	170981	17.87	ng/ul	0.00
30) Pyrene-d10	19.52	212	204898	19.01	ng/ul	0.00
37) Benzo(a)pyrene-d12	23.41	264	204443	17.89	ng/ul	0.00

U.M.
 06/20/16

Target Compounds

					Qvalue
11) Naphthalene	10.57	128	6982	1.14 ng/ul	99
13) 2-Methylnaphthalene	12.19	142	7288	1.56 ng/ul	91
14) 1-Methylnaphthalene	12.41	142	6650	1.37 ng/ul#	94
25) Phenanthrene	17.16	178	20776	1.90 ng/ul	96
28) Fluoranthene	19.18	202	37623	2.74 ng/ul	98
31) Pyrene	19.54	202	36308	2.70 ng/ul	98
32) Benzo(a)anthracene	21.29	228	26566	1.87 ng/ul	97
33) Chrysene	21.34	228	31507m	2.30 ng/ul	
35) Benzo(b)fluoranthene	22.88	252	47481	3.34 ng/ul	98
38) Benzo(a)pyrene	23.46	252	24757	1.77 ng/ul#	98

U.M.
 06/20/16

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (QT Reviewed)

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061716\
 Data File : BM005841.D
 Acq On : 16 Jun 2016 23:14
 Operator : UM/SJ
 Sample : H3535-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 D9XW6

Manual Integrations
 APPROVED

sohil
 6/17/2016 7:27:39 PM

Quant Time: Jun 17 02:06:25 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061716.M
 Quant Title : SVOA CALIBRATION
 Qlast Update : Fri Jun 17 01:56:56 2016
 Response via : Initial Calibration

