

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061716\
 Data File : BM005853.D
 Acq On : 17 Jun 2016 06:26
 Operator : UM/SJ
 Sample : H3537-17
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9Y47

Manual Integrations
 APPROVED

sohil
 6/17/2016 7:28:36 PM

Quant Time: Jun 17 07:18:40 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061716.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 17 01:56:56 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	29611	20.00	ng/ul	0.00
7) Naphthalene-d8	10.52	136	138812	20.00	ng/ul	0.00
15) Acenaphthene-d10	14.37	164	89092	20.00	ng/ul	0.00
23) Phenanthrene-d10	17.12	188	205375	20.00	ng/ul	0.00
29) Chrysene-d12	21.31	240	196595	20.00	ng/ul	0.00
34) Perylene-d12	23.57	264	184619	20.00	ng/ul	0.01

System Monitoring Compounds

2) 1,4-Dioxane-d8	3.18	96	631	2.76	ng/uL	0.00
3) Phenol-d5	6.92	99	40358	16.28	ng/ul	0.00
4) Bis-(2-Chloroethyl)ether-d	7.06	67	23335	18.16	ng/ul	0.00
5) 2-Chlorophenol-d4	7.27	132	39201	18.58	ng/ul	0.00
6) 4-Methylphenol-d8	8.45	113	29478	13.30	ng/ul	0.00
8) Nitrobenzene-d5	8.89	128	19209	19.61	ng/ul	0.00
9) 2-Nitrophenol-d4	9.61	143	23310	19.47	ng/ul	0.00
10) 2,4-Dichlorophenol-d3	10.16	165	41109	17.38	ng/ul	0.00
12) 4-Chloroaniline-d4	10.67	131	15429m	9.64	ng/ul	0.00
16) Dimethylphthalate-d6	13.79	166	140900	16.72	ng/ul	0.00
17) Acenaphthylene-d8	14.07	160	172433	17.76	ng/ul	0.00
20) 4-Nitrophenol-d4	14.63	143	9818m	9.67	ng/ul	0.02
21) Fluorene-d10	15.37	176	122516	17.06	ng/ul	0.00
24) 4,6-Dinitro-2-methylphenol	15.52	200	12311	8.88	ng/ul	0.00
26) Anthracene-d10	17.22	188	188506	17.58	ng/ul	0.00
30) Pyrene-d10	19.52	212	207717	22.29	ng/ul	0.00
37) Benzo(a)pyrene-d12	23.43	264	157685	17.08	ng/ul	0.01

Target Compounds

						Qvalue
25) Phenanthrene	17.16	178	84671	6.93	ng/ul	98
27) Anthracene	17.26	178	14659	1.17	ng/ul	99
28) Fluoranthene	19.19	202	369122	24.02	ng/ul	98
31) Pyrene	19.55	202	602818	51.88	ng/ul	99
32) Benzo(a)anthracene	21.30	228	279743	22.78	ng/ul	96
33) Chrysene	21.35	228	340967	28.83	ng/ul	96
35) Benzo(b)fluoranthene	22.89	252	245437	21.36	ng/ul	99
36) Benzo(k)fluoranthene	22.93	252	63050m	5.68	ng/ul	
38) Benzo(a)pyrene	23.47	252	172452	15.28	ng/ul	100
39) Indeno(1,2,3-cd)pyrene	25.85	276	86368	6.26	ng/ul	97
40) Dibenzo(a,h)anthracene	25.84	278	32815	2.89	ng/ul#	88
41) Benzo(g,h,i)perylene	26.55	276	87969	7.49	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061716\
Data File : BM005853.D
Acq On : 17 Jun 2016 06:26
Operator : UM/SJ
Sample : H3537-17
Misc :
ALS Vial : 24 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
D9Y47

Manual Integrations
APPROVED

sohil
6/17/2016 7:28:36 PM

Quant Time: Jun 17 07:18:40 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061716.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 17 01:56:56 2016
Response via : Initial Calibration

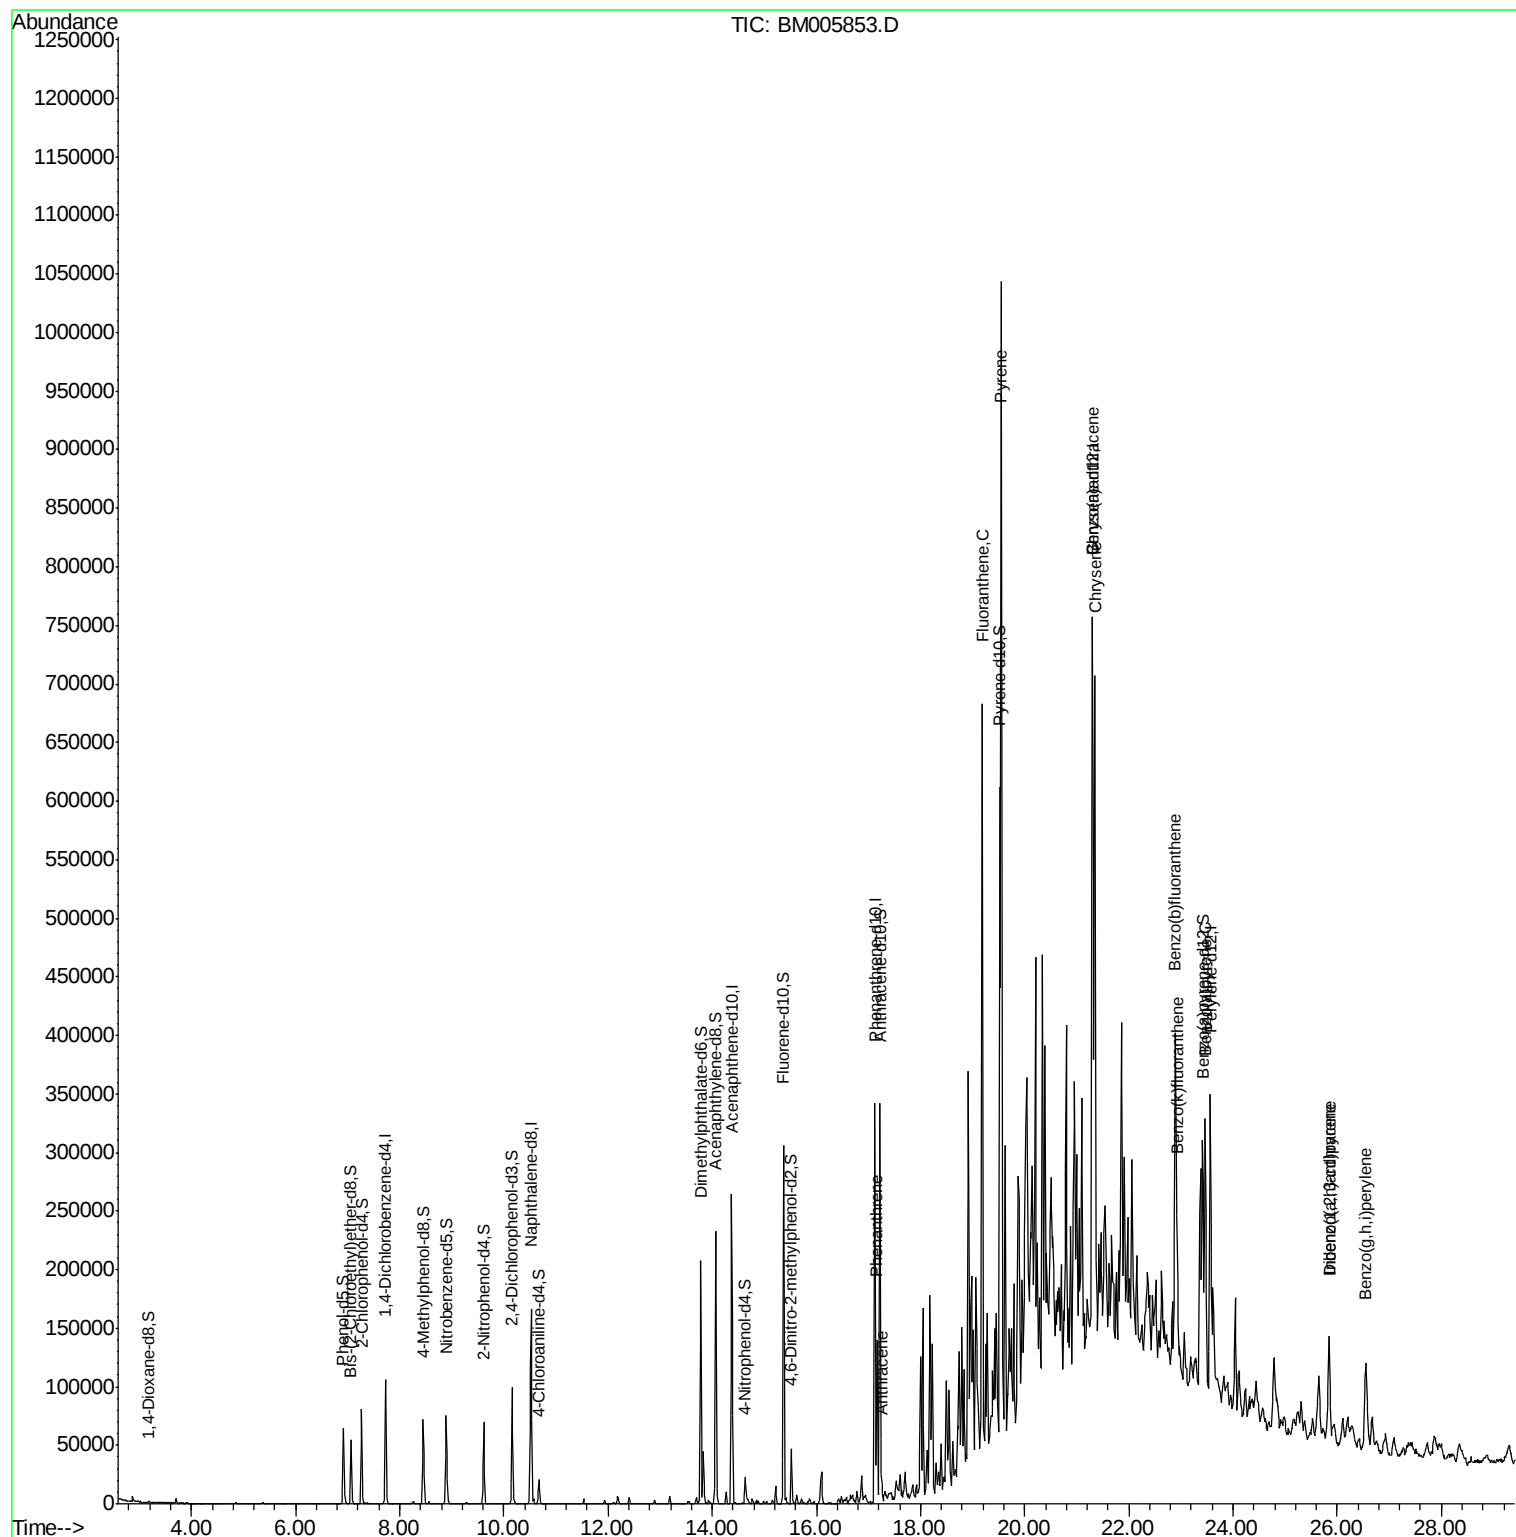







#25
Phenanthrene
Concen: 6.93 ng/ul
RT: 17.16 min Scan# 2478
Delta R.T. -0.00 min
Lab File: BM005853.D
Acq: 17 Jun 2016 06:26

Instrument :
BNA_M
ClientSampleId :
D9Y47

Tgt Ion	Ratio	Lower	Upper
178	100		
179	16.0	12.0	18.0
176	19.7	14.9	22.3




Manual Integrations
APPROVED


sohil
6/17/2016 7:28:36 PM

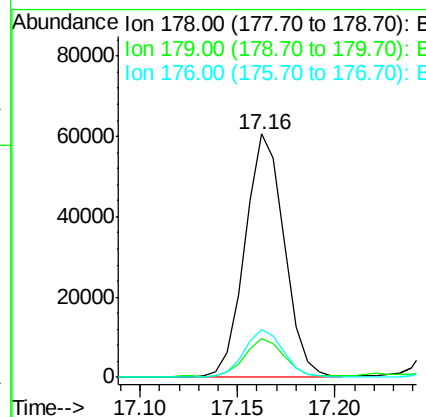

#27
Anthracene
Concen: 1.17 ng/ul
RT: 17.26 min Scan# 2494
Delta R.T. -0.00 min
Lab File: BM005853.D
Acq: 17 Jun 2016 06:26

Tgt Ion	Ratio	Lower	Upper
178	100		
179	14.0	11.9	17.9
176	18.8	14.8	22.2

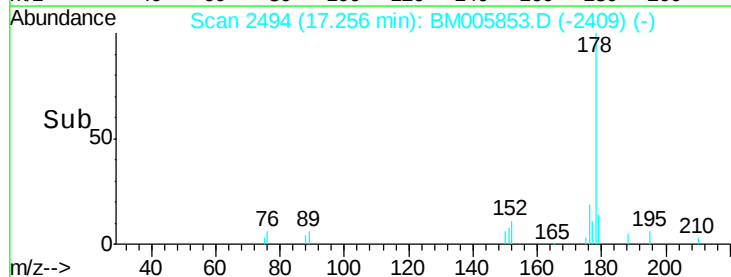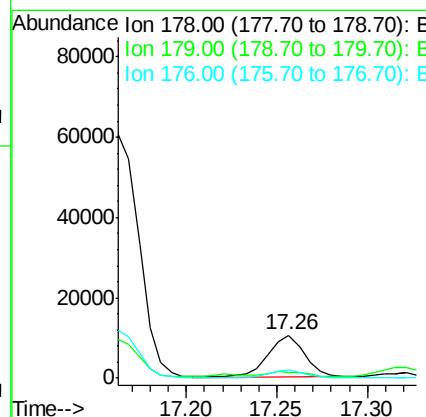



#28

Fluoranthene

Concen: 24.02 ng/ul

RT: 19.19 min Scan# 2822

Delta R.T. 0.01 min

Lab File: BM005853.D

Acq: 17 Jun 2016 06:26

Instrument :

BNA_M





ClientSampleId :

D9Y47

Tgt	Ion	Ratio	Resp	Lower	Upper
202	100		369122		
101	6.7	6.1	9.1		
100	5.0	4.2	6.2		

Manual Integrations
APPROVED

sohil
6/17/2016 7:28:36 PM

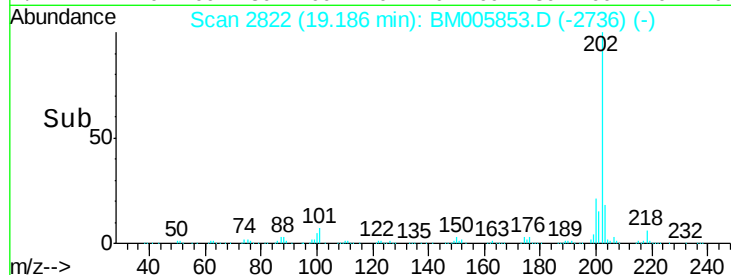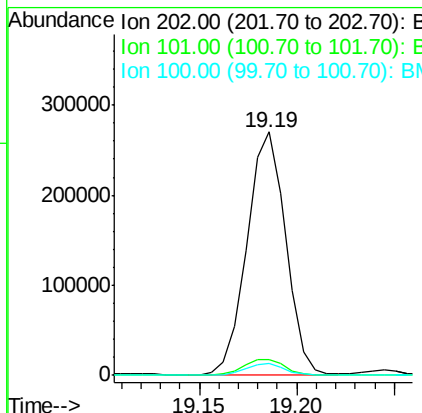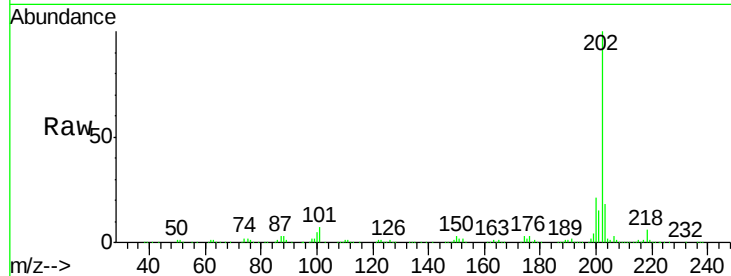

#31

Pyrene

Concen: 51.88 ng/ul




RT: 19.55 min Scan# 2884


Delta R.T. 0.01 min

Lab File: BM005853.D

Acq: 17 Jun 2016 06:26

Tgt	Ion	Ratio	Resp	Lower	Upper
202	100		602818		
101	8.1	6.5	9.7		
100	6.3	5.4	8.2		

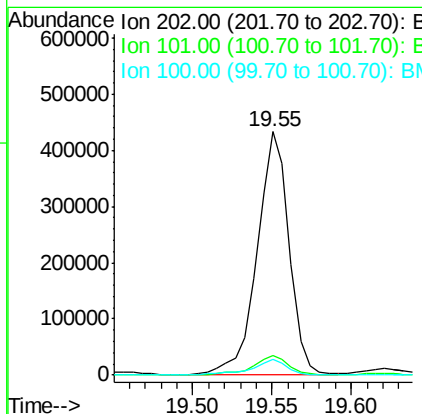







#32
Benzo(a)anthracene
Concen: 22.78 ng/u1
RT: 21.30 min Scan# 3181
Delta R.T. 0.01 min
Lab File: BM005853.D
Acq: 17 Jun 2016 06:26

Instrument :
BNA_M
ClientSampled :
D9Y47

Tgt Ion	Ratio	Lower	Upper
228	100		
229	23.0	15.8	23.6
226	28.5	21.8	32.6




Manual Integrations
APPROVED


sohil
6/17/2016 7:28:36 PM

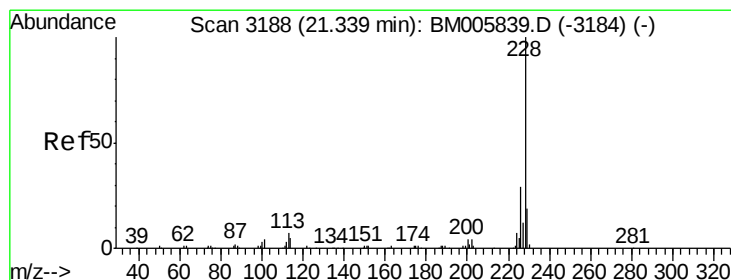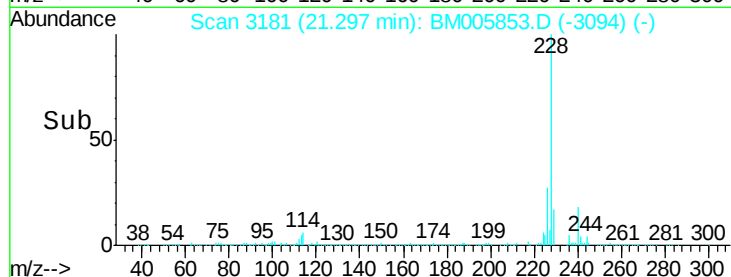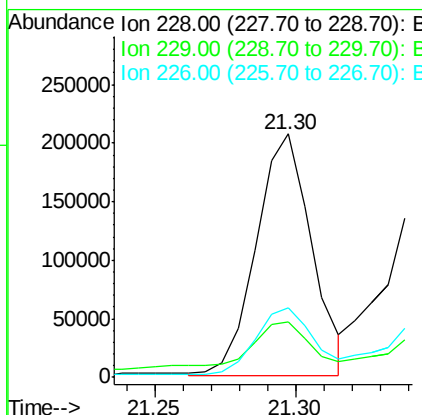

#33
Chrysene
Concen: 28.83 ng/u1
RT: 21.35 min Scan# 3190
Delta R.T. 0.01 min
Lab File: BM005853.D
Acq: 17 Jun 2016 06:26

Tgt Ion	Ratio	Lower	Upper
228	100		
226	31.2	23.5	35.3
229	21.2	15.4	23.0

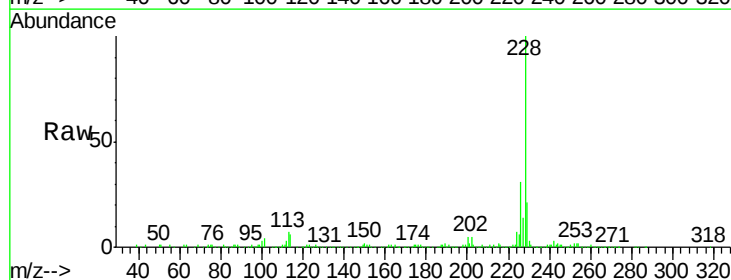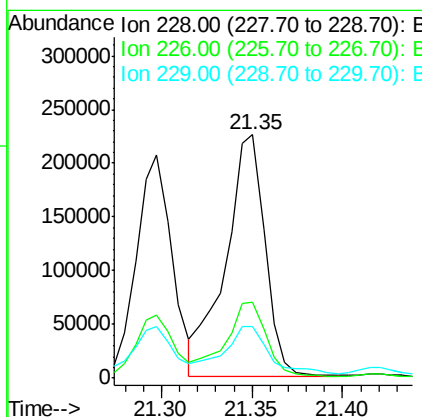



#35

Benzo(b)fluoranthene

Concen: 21.36 ng/ul

RT: 22.89 min Scan# 3452

Delta R.T. 0.01 min

Lab File: BM005853.D

Acq: 17 Jun 2016 06:26

Instrument :

BNA_M


ClientSampled :

D9Y47




Tgt Ion:	252	Resp:	245437
Ion Ratio	Lower	Upper	
252	100		
253	21.9	17.1	25.7
125	6.7	4.9	7.3

Manual Integrations
APPROVED

sohil
6/17/2016 7:28:36 PM

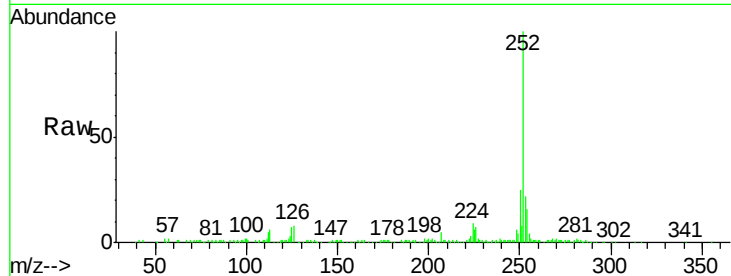

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

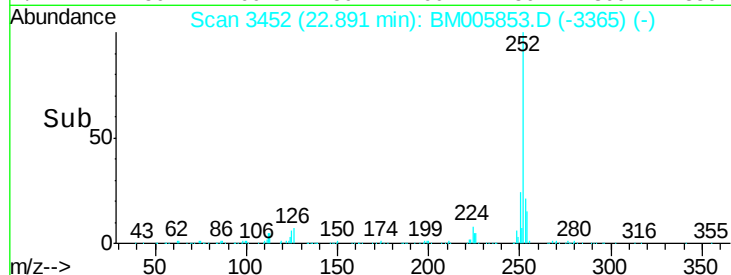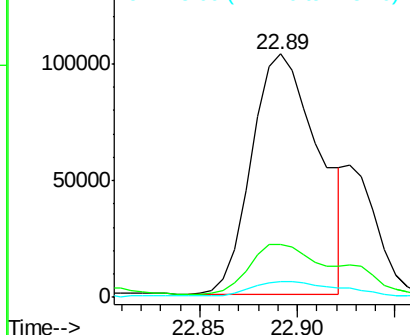

#36

Benzo(k)fluoranthene

Concen: 5.68 ng/ul m

RT: 22.93 min Scan# 3458




Delta R.T. 0.01 min


Lab File: BM005853.D

Acq: 17 Jun 2016 06:26

Tgt Ion:	252	Resp:	63050
Ion Ratio	Lower	Upper	
252	100		
253	24.1	17.5	26.3
125	7.2	4.8	7.2#

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

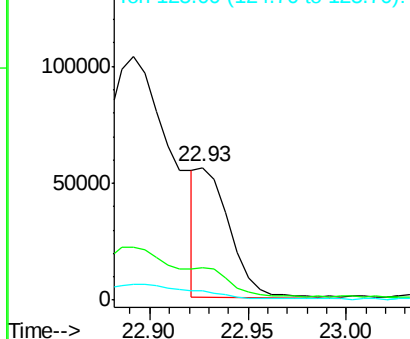







#38
Benzo(a)pyrene
Concen: 15.28 ng/u1
RT: 23.47 min Scan# 3550
Delta R.T. 0.01 min
Lab File: BM005853.D
Acq: 17 Jun 2016 06:26

Instrument :
BNA_M
ClientSampleId :
D9Y47

Tgt Ion	Ratio	Resp	Lower	Upper
252	100	172452		
253	22.5	18.0	27.0	
125	7.1	5.1	7.7	




Manual Integrations
APPROVED


sohil
6/17/2016 7:28:36 PM

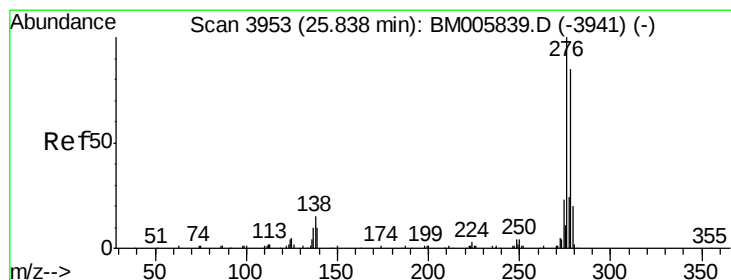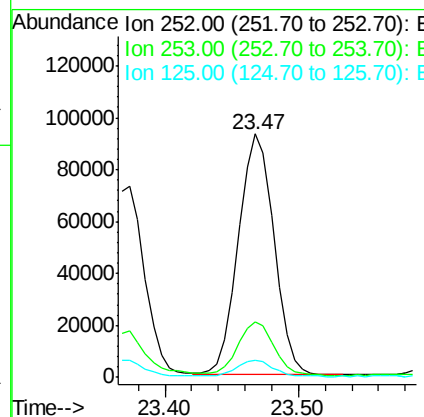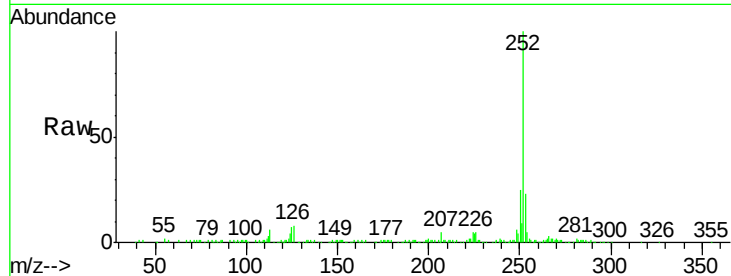

#39
Indeno(1,2,3-cd)pyrene
Concen: 6.26 ng/u1
RT: 25.85 min Scan# 3955
Delta R.T. 0.01 min
Lab File: BM005853.D
Acq: 17 Jun 2016 06:26

Tgt Ion	Ratio	Resp	Lower	Upper
276	100	86368		
138	14.7	11.9	17.9	
277	24.1	21.0	31.6	

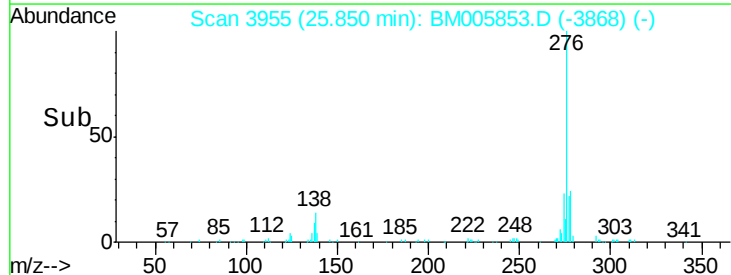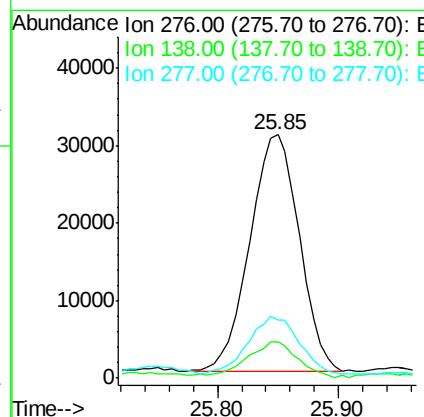



#40

Dibenzo(a,h)anthracene

Concen: 2.89 ng/ul

RT: 25.84 min Scan# 3953

Delta R.T. -0.01 min

Lab File: BM005853.D

Acq: 17 Jun 2016 06:26

Instrument :

BNA_M





ClientSampleId :

D9Y47

Tgt Ion:	278	Resp:	32815
Ion Ratio	Lower	Upper	
278	100		
139	13.1	8.2	12.4#
279	30.3	18.6	27.8#

Manual Integrations
APPROVED

sohil
6/17/2016 7:28:36 PM

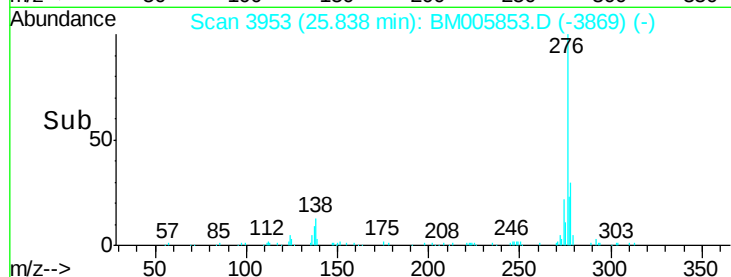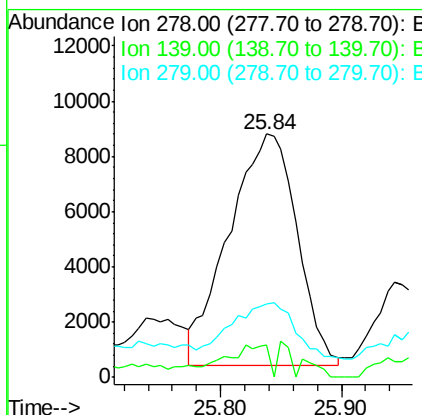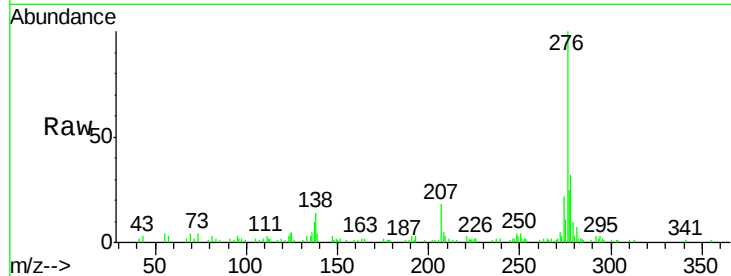

#41

Benzo(g,h,i)perylene

Concen: 7.49 ng/ul

RT: 26.55 min Scan# 4074

Delta R.T. 0.02 min

Lab File: BM005853.D

Acq: 17 Jun 2016 06:26

Tgt Ion:	276	Resp:	87969
Ion Ratio	Lower	Upper	
276	100		
138	13.6	10.6	15.8
277	24.8	19.6	29.4

