


Data Path : Z:\HPCHEM1\BNA_M\Data\BM061716\
 Data File : BM005838.D
 Acq On : 16 Jun 2016 21:26
 Operator : UM/SJ
 Sample : DFTPP60
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP60

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061716.M
 Title : SVOA CALIBRATION
 Last Update : Fri Jun 17 10:48:37 2016

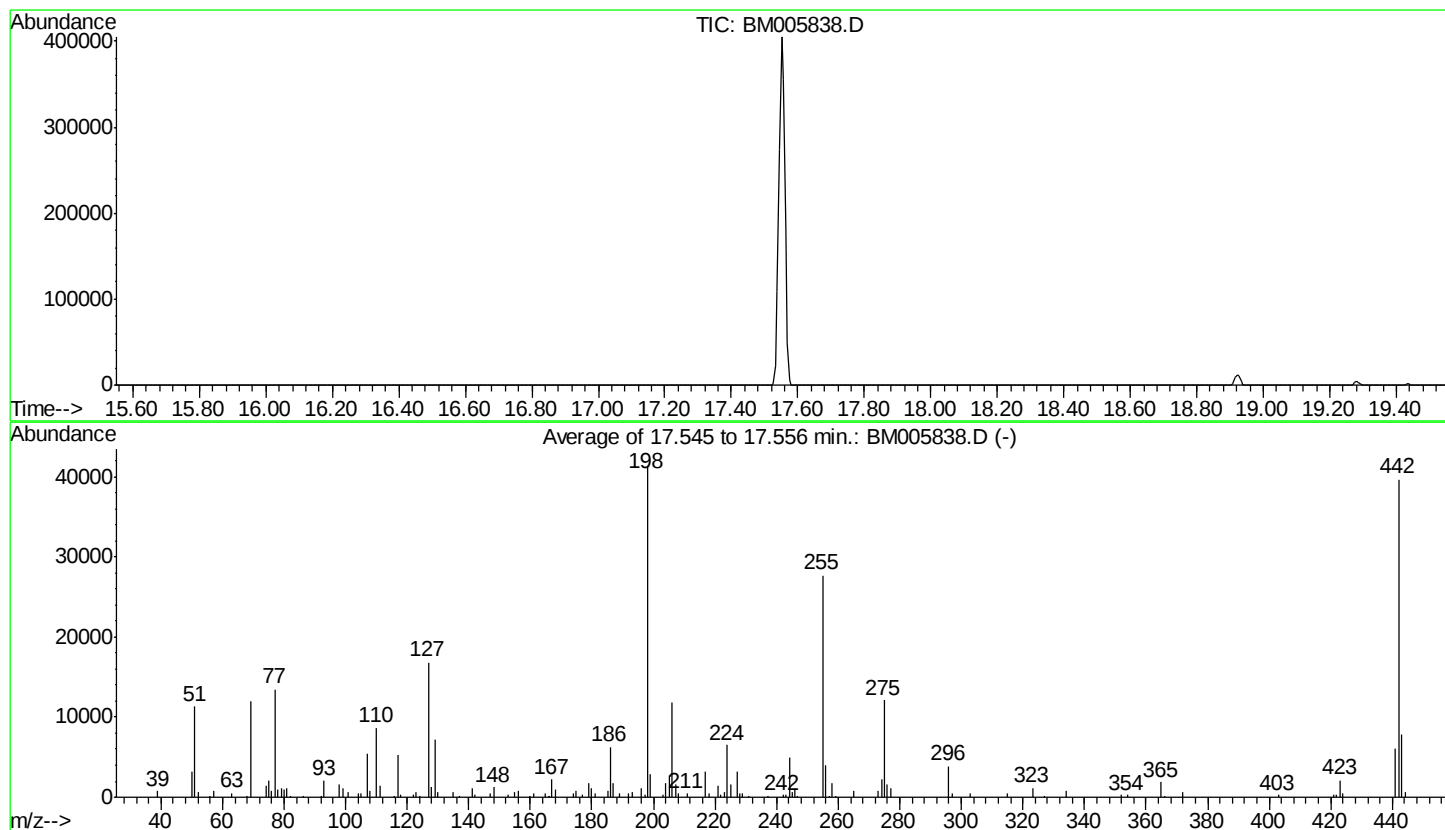

AutoFind: Scans 2543, 2544, 2545; Background Corrected with Scan 2538

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.3	11290	PASS
68	69	0.00	2	0.9	111	PASS
69	198	0.00	100	29.0	12004	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.6	16784	PASS
197	198	0.00	2	0.9	362	PASS
198	198	100	100	100.0	41386	PASS
199	198	5	9	7.1	2920	PASS
275	198	10	60	29.3	12139	PASS
365	198	1	100	4.6	1898	PASS
441	443	0.01	100	77.6	6130	PASS
442	198	50	100	95.8	39648	PASS
443	442	15	24	19.9	7898	PASS

m/z	Abundance
39.00	717.0
50.10	2917.0
51.10	10642.0
52.00	505.0
57.00	745.0
63.00	498.0
69.00	11254.0
74.00	1285.0
75.00	2171.0
76.10	744.0
77.10	12552.0
78.00	804.0
79.00	1003.0
80.00	838.0
81.00	1052.0
93.00	1718.0
98.00	1519.0
99.00	1105.0
100.90	601.0
104.00	416.0
105.00	359.0
107.00	4703.0
108.00	677.0
110.00	7713.0
111.00	1394.0
116.00	355.0
117.00	4685.0
117.90	354.0
121.90	306.0
123.00	515.0
127.00	14809.0
128.00	1135.0
129.00	6395.0
130.00	550.0
134.90	523.0
137.00	327.0
141.00	947.0
142.00	414.0
147.00	497.0
148.00	973.0
152.90	347.0
155.00	552.0
156.10	614.0
159.90	320.0
160.90	394.0
164.90	345.0
167.00	1744.0
168.00	905.0
174.00	434.0
175.00	718.0
179.00	1548.0
180.00	824.0
180.90	452.0
185.00	709.0
186.00	5367.0
187.00	1364.0
188.90	371.0
192.00	431.0
193.00	482.0
196.00	884.0
197.10	342.0
198.00	33640.0
199.00	2645.0
203.00	318.0
204.00	1351.0
205.00	2337.0
206.00	9431.0
207.00	1321.0
208.00	309.0
210.90	441.0
217.00	2613.0
218.00	401.0
221.00	1086.0
221.90	307.0
223.10	513.0
224.00	5165.0
225.00	1366.0
227.00	2619.0
228.00	329.0
229.00	402.0
244.00	3982.0
245.10	466.0
246.00	932.0
255.00	21776.0
256.00	3190.0
258.00	1372.0
265.00	594.0
272.90	584.0
274.00	1747.0
275.00	8678.0
276.00	1283.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60

277.00	903.0
296.00	2875.0
297.00	357.0
303.00	313.0
323.00	838.0
334.00	560.0
365.00	1273.0
372.00	450.0
423.10	1424.0
424.00	399.0
441.00	3903.0
442.10	24640.0
443.10	5019.0
444.00	484.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60

m/z	Abundance
39.10	866.0
50.00	3667.0
51.10	13219.0
52.00	621.0
56.00	432.0
57.00	920.0
63.00	623.0
68.00	335.0
69.00	13983.0
74.10	1710.0
75.00	2435.0
76.00	750.0
77.10	15805.0
78.00	1118.0
79.00	1418.0
80.00	930.0
81.00	1371.0
81.90	351.0
86.00	399.0
92.00	405.0
93.00	2530.0
98.00	1985.0
99.00	1335.0
101.00	667.0
103.90	517.0
105.00	523.0
107.00	6560.0
108.00	926.0
110.00	9966.0
111.00	1747.0
117.00	6300.0
118.00	439.0
121.90	437.0
122.90	658.0
124.00	337.0
127.00	19600.0
128.00	1532.0
129.00	8119.0
130.00	678.0
135.00	729.0
137.00	359.0
141.00	1167.0
142.00	376.0
147.00	606.0
148.00	1470.0
152.90	437.0
155.00	790.0
156.00	1084.0
160.00	394.0
161.00	644.0
165.00	504.0
165.90	398.0
167.00	2758.0
168.00	1080.0
174.00	493.0
175.00	860.0
177.00	517.0
179.00	1986.0
180.00	1379.0
181.00	580.0
185.00	842.0
186.00	7454.0
187.00	2089.0
189.00	522.0
192.00	693.0
193.00	725.0
196.00	1328.0
197.10	434.0
198.00	48904.0
199.00	3326.0
203.00	451.0
204.00	1885.0
205.10	3184.0
206.10	13877.0
207.10	1727.0
208.00	678.0
211.00	551.0
217.00	3714.0
218.00	534.0
221.00	1671.0
222.00	462.0
223.00	720.0
224.10	7550.0
225.00	1930.0
227.00	3792.0
227.90	500.0
229.00	633.0
231.00	320.0
237.00	302.0
242.00	391.0
243.00	370.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60

244.10	5580.0
245.00	816.0
246.00	1423.0
246.90	321.0
255.00	32424.0
256.00	4580.0
257.00	330.0
258.00	2067.0
259.00	301.0
265.00	894.0
273.00	934.0
274.00	2607.0
275.00	14425.0
276.00	1967.0
277.00	1305.0
296.00	4354.0
297.00	597.0
303.00	525.0
315.00	700.0
323.10	1376.0
326.90	300.0
334.00	947.0
352.00	369.0
354.00	406.0
365.00	2131.0
365.90	306.0
372.00	698.0
403.00	420.0
420.90	367.0
421.90	365.0
423.00	2340.0
424.00	530.0
441.00	6978.0
442.10	45112.0
443.10	9059.0
444.10	799.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60

m/z	Abundance
39.00	654.0
50.10	2808.0
51.00	10009.0
52.00	587.0
56.90	764.0
63.00	399.0
69.00	10776.0
74.00	1242.0
75.00	1778.0
76.10	720.0
77.10	12074.0
78.00	896.0
79.00	962.0
80.00	905.0
81.00	1079.0
86.10	316.0
93.00	1952.0
98.00	1459.0
99.00	1099.0
101.00	654.0
103.90	411.0
105.00	401.0
107.00	4944.0
107.90	754.0
110.00	8355.0
111.00	1202.0
115.90	313.0
117.00	4969.0
118.00	364.0
122.00	418.0
123.00	619.0
127.00	15945.0
128.00	1113.0
129.00	7227.0
129.90	565.0
135.00	629.0
140.90	1028.0
146.90	580.0
148.00	1212.0
153.00	301.0
155.00	568.0
156.00	902.0
161.00	532.0
164.90	435.0
166.10	306.0
167.00	2120.0
168.00	979.0
173.90	445.0
175.00	836.0
177.00	358.0
179.00	1595.0
180.00	982.0
181.00	534.0
185.00	814.0
186.00	6103.0
187.00	1797.0
188.90	461.0
191.90	562.0
193.00	682.0
196.00	1181.0
197.10	312.0
198.00	41616.0
199.00	2789.0
203.00	323.0
204.00	1872.0
205.00	2717.0
206.00	12019.0
207.00	1643.0
208.00	536.0
211.00	415.0
217.00	3310.0
217.90	475.0
221.00	1368.0
221.90	384.0
223.00	748.0
224.00	6837.0
225.00	1700.0
227.00	3426.0
228.00	409.0
229.00	610.0
242.00	372.0
243.10	376.0
244.00	5343.0
245.10	640.0
246.00	1121.0
255.00	28800.0
256.00	4421.0
257.00	407.0
258.00	1756.0
259.00	383.0
265.00	817.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60

273.10	918.0
274.00	2432.0
275.00	13314.0
276.00	1738.0
277.00	1284.0
296.00	4529.0
297.00	547.0
303.00	460.0
315.00	529.0
323.10	1318.0
334.00	972.0
352.10	474.0
354.00	443.0
365.00	2291.0
366.00	300.0
372.10	712.0
403.00	400.0
421.00	393.0
422.00	413.0
423.10	2565.0
424.00	555.0
441.00	7509.0
442.10	49192.0
443.10	9618.0
444.10	787.0

Instrument :
BNA_M
ClientSampleId :
DFTPP60

m/z	Abundance
197.90	565.0
255.00	332.0

Instrument :

BNA_M

ClientSampleId :

DFTPP60