

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061721\
 Data File : BM030488.D
 Acq On : 17 Jun 2021 10:46
 Operator : CG/JU
 Sample : PB137067BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK067

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM060621.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030488.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	36	41	50	rVB2	39818	95028	2.09%	0.206%
2	3.746	107	112	136	rBV	388606	1119559	24.62%	2.422%
3	6.816	631	634	638	rBV5	4561	7116	0.16%	0.015%
4	6.910	647	650	654	rBV4	3609	5681	0.12%	0.012%
5	6.998	657	665	674	rBV	798179	1414419	31.11%	3.060%
6	7.157	684	692	709	rBV	650020	1112259	24.46%	2.407%
7	7.363	719	727	735	rBV	873386	1514447	33.31%	3.277%
8	7.828	798	806	817	rBV	634840	1094918	24.08%	2.369%
9	8.110	849	854	856	rVB4	3081	4859	0.11%	0.011%
10	8.528	917	925	934	rBV	1027719	1666719	36.66%	3.606%
11	8.981	993	1002	1010	rBV	770251	1328798	29.23%	2.875%
12	9.392	1069	1072	1075	rBV5	3689	4570	0.10%	0.010%
13	9.698	1117	1124	1136	rBV	639580	1102207	24.24%	2.385%
14	10.234	1207	1215	1227	rBV	976456	1711800	37.65%	3.704%
15	10.610	1270	1279	1287	rVB	844082	1398306	30.75%	3.026%
16	10.745	1293	1302	1315	rBV	903503	1623184	35.70%	3.512%
17	12.198	1544	1549	1556	rVB3	18627	32538	0.72%	0.070%
18	13.857	1824	1831	1846	rVV	1554477	2246673	49.41%	4.861%
19	14.139	1871	1879	1888	rBV	1913799	2833118	62.31%	6.130%
20	14.445	1925	1931	1938	rBV	1126000	1723119	37.90%	3.728%
21	14.651	1959	1966	1991	rBV	542566	1040904	22.89%	2.252%
22	14.810	1991	1993	1995	rVV2	6403	6916	0.15%	0.015%
23	14.863	1999	2002	2007	rVB7	2842	5515	0.12%	0.012%
24	15.439	2092	2100	2114	rVB	2455520	3424945	75.33%	7.411%
25	15.557	2114	2120	2134	rBV	656702	972595	21.39%	2.104%
26	15.674	2137	2140	2145	rVV2	28557	44764	0.98%	0.097%
27	15.910	2177	2180	2182	rBV4	3731	4778	0.11%	0.010%
28	16.221	2228	2233	2237	rVB5	9327	14591	0.32%	0.032%
29	16.863	2338	2342	2344	rBV5	3423	4769	0.10%	0.010%
30	16.974	2355	2361	2366	rBB5	6159	9248	0.20%	0.020%
31	17.186	2391	2397	2407	rVV	1352149	1889695	41.56%	4.089%
32	17.286	2407	2414	2423	rVV	2569709	3600033	79.18%	7.789%
33	18.080	2542	2549	2555	rBV5	30224	63360	1.39%	0.137%
34	18.610	2637	2639	2642	rBV4	4983	6139	0.14%	0.013%
35	19.209	2736	2741	2745	rBV	33522	50216	1.10%	0.109%
36	19.462	2780	2784	2787	rBV	22656	30892	0.68%	0.067%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061721\
Data File : BM030488.D
Acq On : 17 Jun 2021 10:46
Operator : CG/JU
Sample : PB137067BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK067

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM060621.M
Title : SVOA CALIBRATION

37	19.574	2796	2803	2813	rBV	2993209	4164222	91.59%	9.010%
38	21.351	3101	3105	3111	rBV	1595707	2057270	45.25%	4.451%
39	23.486	3461	3468	3479	rVB	2325175	4546777	100.00%	9.838%
40	23.627	3487	3492	3502	rVB2	1150630	2240404	49.27%	4.848%




Sum of corrected areas: 46217351

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061721\
Data File : BM030488.D
Acq On : 17 Jun 2021 10:46
Operator : CG/JU
Sample : PB137067BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK067

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM060621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

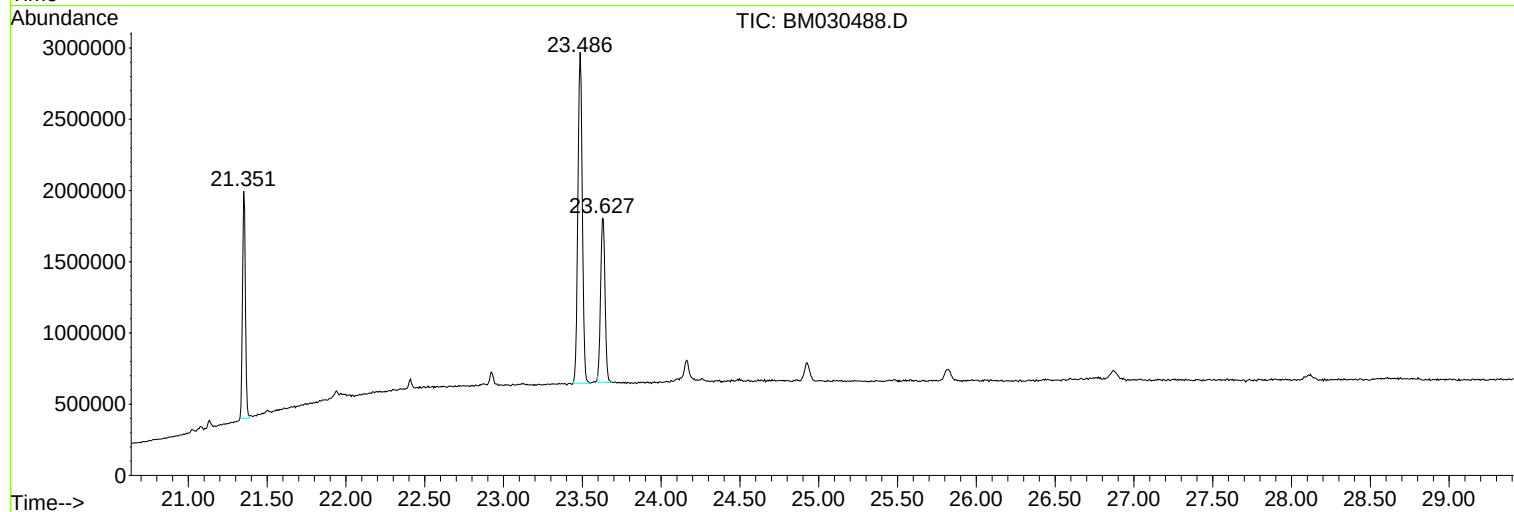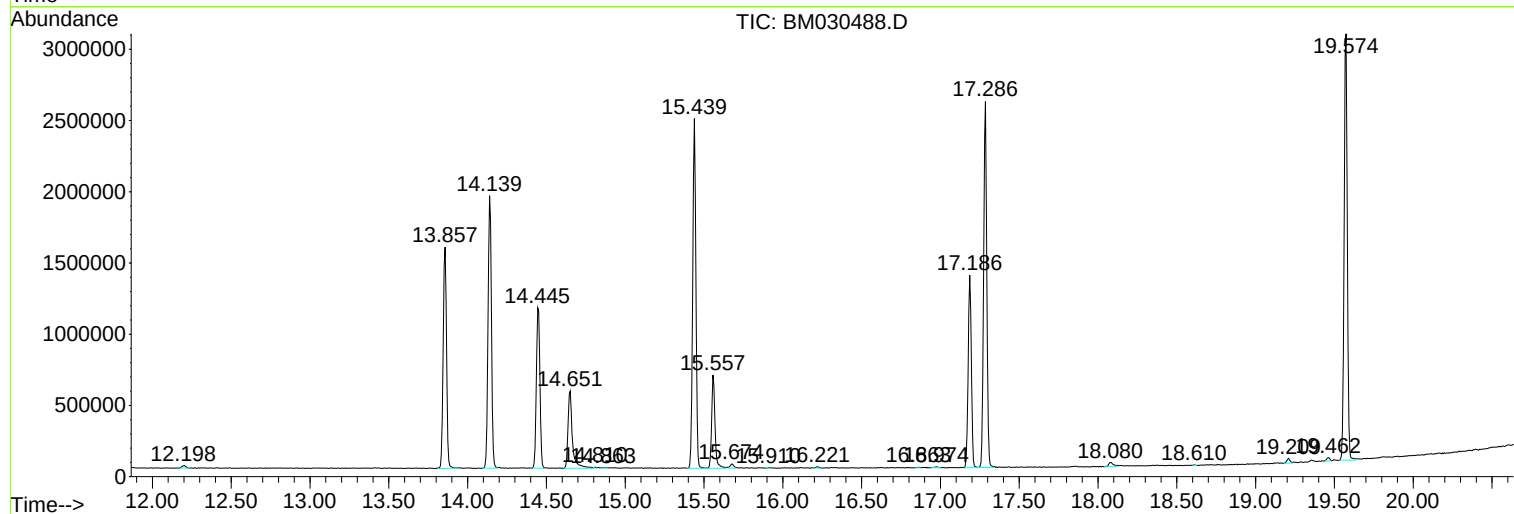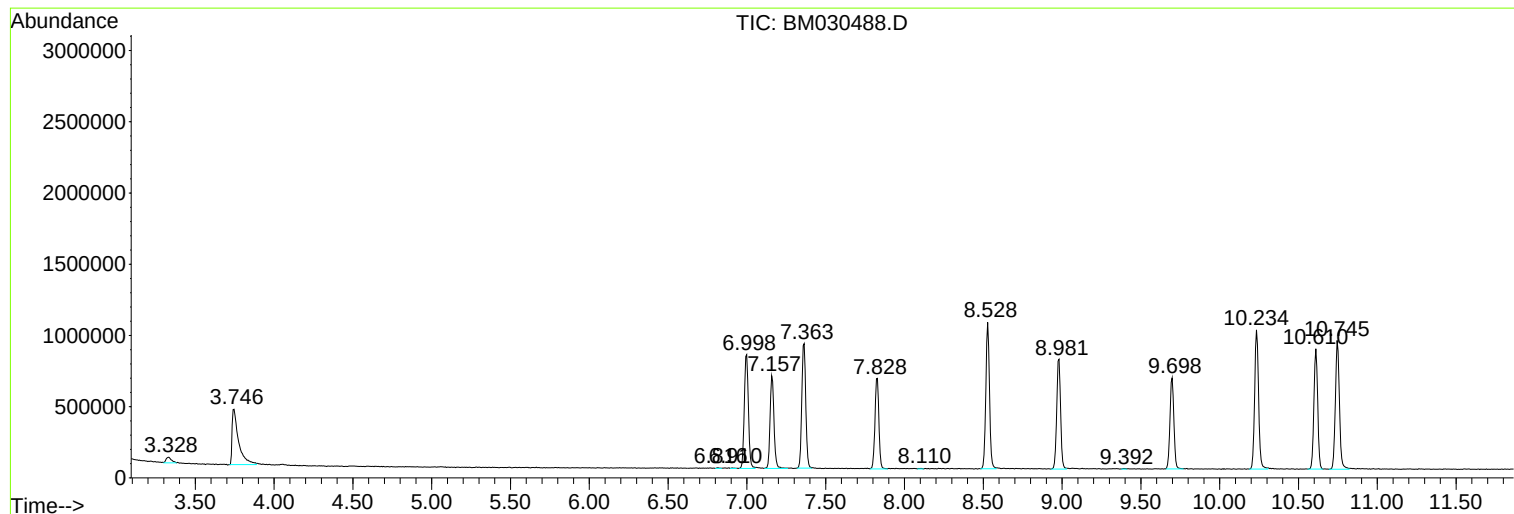

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061721\
Data File : BM030488.D
Acq On : 17 Jun 2021 10:46
Operator : CG/JU
Sample : PB137067BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK067

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM060621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061721\
Data File : BM030488.D
Acq On : 17 Jun 2021 10:46
Operator : CG/JU
Sample : PB137067BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK067

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM060621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
