

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061721\
 Data File : BM030490.D
 Acq On : 17 Jun 2021 12:02
 Operator : CG/JU
 Sample : M2690-10
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GCP2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM060621.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030490.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.051	161	164	170	rBV4	8201	13170	0.52%	0.108%
2	4.269	196	201	209	rVB5	21472	39527	1.55%	0.324%
3	4.675	265	270	275	rBV2	19327	35650	1.40%	0.292%
4	4.857	300	301	304	rBV3	3493	3876	0.15%	0.032%
5	5.234	363	365	367	rVB3	3575	3145	0.12%	0.026%
6	5.798	459	461	463	rBV3	2213	2776	0.11%	0.023%
7	6.216	529	532	533	rBV3	5228	6451	0.25%	0.053%
8	6.475	573	576	578	rBV3	2622	3603	0.14%	0.029%
9	6.975	660	661	665	rVB4	2650	2867	0.11%	0.023%
10	7.010	665	667	675	rVB9	3791	5933	0.23%	0.049%
11	7.428	735	738	741	rBV5	2561	3715	0.15%	0.030%
12	7.663	776	778	780	rBV3	2463	2569	0.10%	0.021%
13	7.822	797	805	814	rBV	728204	1240980	48.77%	10.157%
14	7.934	823	824	830	rVB4	2732	2804	0.11%	0.023%
15	8.422	904	907	909	rBV4	3559	3456	0.14%	0.028%
16	8.975	999	1001	1006	rBV5	1942	2997	0.12%	0.025%
17	9.216	1041	1042	1045	rVB3	2969	2795	0.11%	0.023%
18	9.239	1045	1046	1048	rBV2	2932	2844	0.11%	0.023%
19	9.592	1104	1106	1111	rVB5	2261	2572	0.10%	0.021%
20	9.886	1152	1156	1159	rBV4	1948	2640	0.10%	0.022%
21	10.122	1192	1196	1198	rVB5	1927	2708	0.11%	0.022%
22	10.451	1248	1252	1254	rBV5	2529	2817	0.11%	0.023%
23	10.610	1272	1279	1294	rBV	928888	1577618	62.00%	12.913%
24	11.045	1351	1353	1356	rBV4	2593	3185	0.13%	0.026%
25	11.139	1368	1369	1374	rVB5	2140	2863	0.11%	0.023%
26	11.651	1454	1456	1458	rBV3	2830	2942	0.12%	0.024%
27	11.874	1490	1494	1496	rBV4	3126	3309	0.13%	0.027%
28	12.304	1564	1567	1570	rBV5	2432	2596	0.10%	0.021%
29	13.874	1830	1834	1836	rBV3	4194	4896	0.19%	0.040%
30	14.186	1884	1887	1892	rVB6	2233	2764	0.11%	0.023%
31	14.445	1923	1931	1944	rVV	1278420	1945853	76.48%	15.927%
32	14.904	2007	2009	2013	rBV4	2544	2622	0.10%	0.021%
33	15.468	2103	2105	2109	rVB5	2987	3128	0.12%	0.026%
34	15.857	2169	2171	2174	rBV4	2768	3112	0.12%	0.025%
35	16.327	2248	2251	2252	rBV2	2826	2725	0.11%	0.022%
36	16.374	2256	2259	2261	rBV4	2366	2547	0.10%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061721\
 Data File : BM030490.D
 Acq On : 17 Jun 2021 12:02
 Operator : CG/JU
 Sample : M2690-10
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GCP2-BLANK

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM060621.M
 Title : SVOA CALIBRATION

37	16.474	2274	2276	2279	rBV3	2654	4016	0.16%	0.033%
38	16.792	2327	2330	2331	rBV2	3620	2920	0.11%	0.024%
39	16.904	2347	2349	2352	rVB4	2590	3305	0.13%	0.027%
40	16.939	2352	2355	2357	rBV4	2981	3645	0.14%	0.030%
41	16.980	2357	2362	2365	rVV4	6327	9010	0.35%	0.074%
42	17.186	2390	2397	2410	rBV	1473524	2140680	84.13%	17.521%
43	17.292	2410	2415	2418	rVV7	7275	10549	0.41%	0.086%
44	17.356	2421	2426	2427	rBV4	1780	2820	0.11%	0.023%
45	17.833	2504	2507	2508	rBV3	3020	3417	0.13%	0.028%
46	17.903	2517	2519	2522	rBV4	2023	3176	0.12%	0.026%
47	18.080	2543	2549	2555	rBV10	16309	34930	1.37%	0.286%
48	19.139	2725	2729	2730	rBV4	5437	5713	0.22%	0.047%
49	21.133	3065	3068	3075	rBV	123791	179839	7.07%	1.472%
50	21.356	3101	3106	3112	rBV	1783737	2319206	91.15%	18.982%
51	23.633	3486	3493	3503	rVB2	1303760	2544391	100.00%	20.825%




Sum of corrected areas: 12217672

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061721\
Data File : BM030490.D
Acq On : 17 Jun 2021 12:02
Operator : CG/JU
Sample : M2690-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GCP2-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM060621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

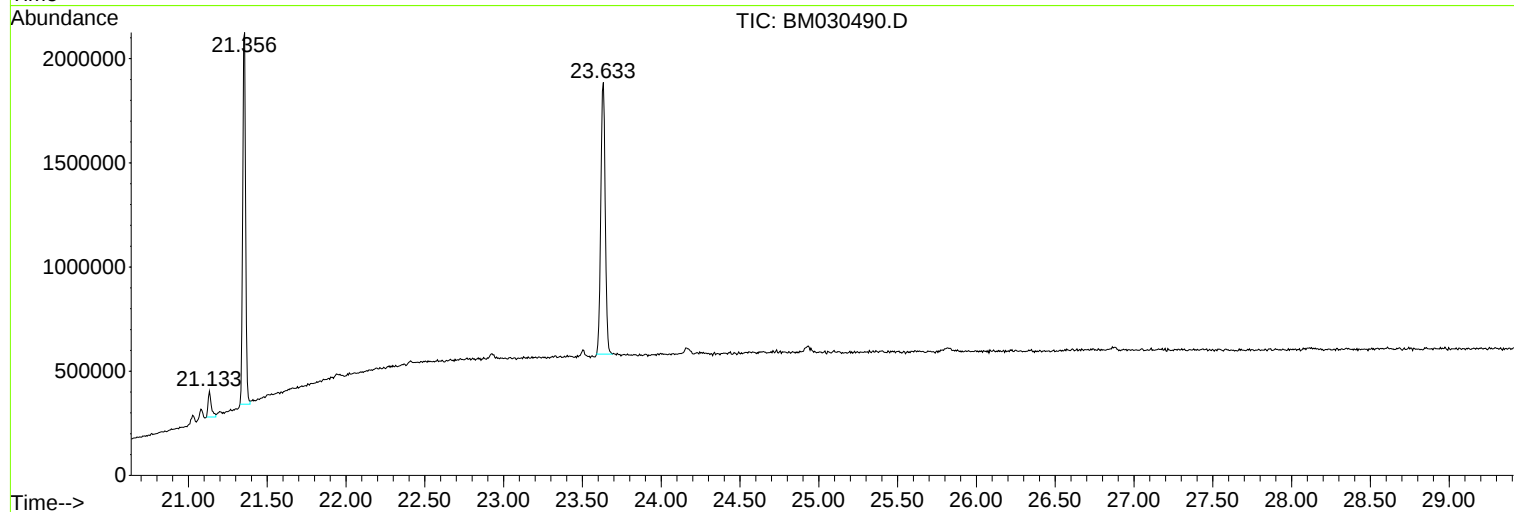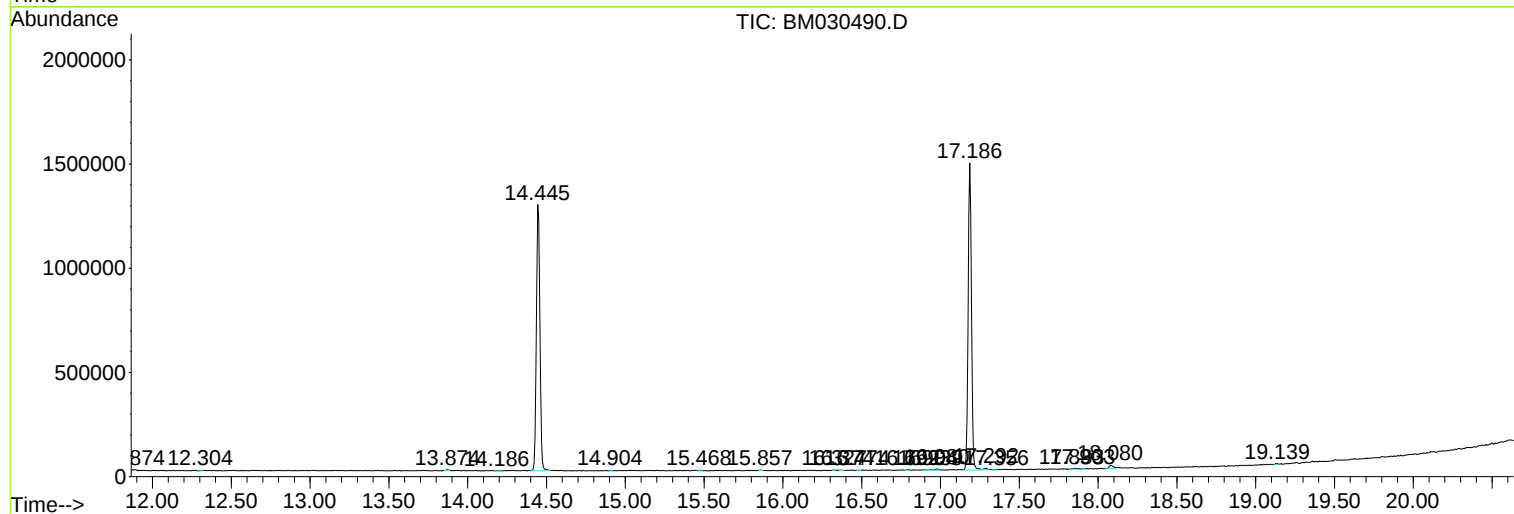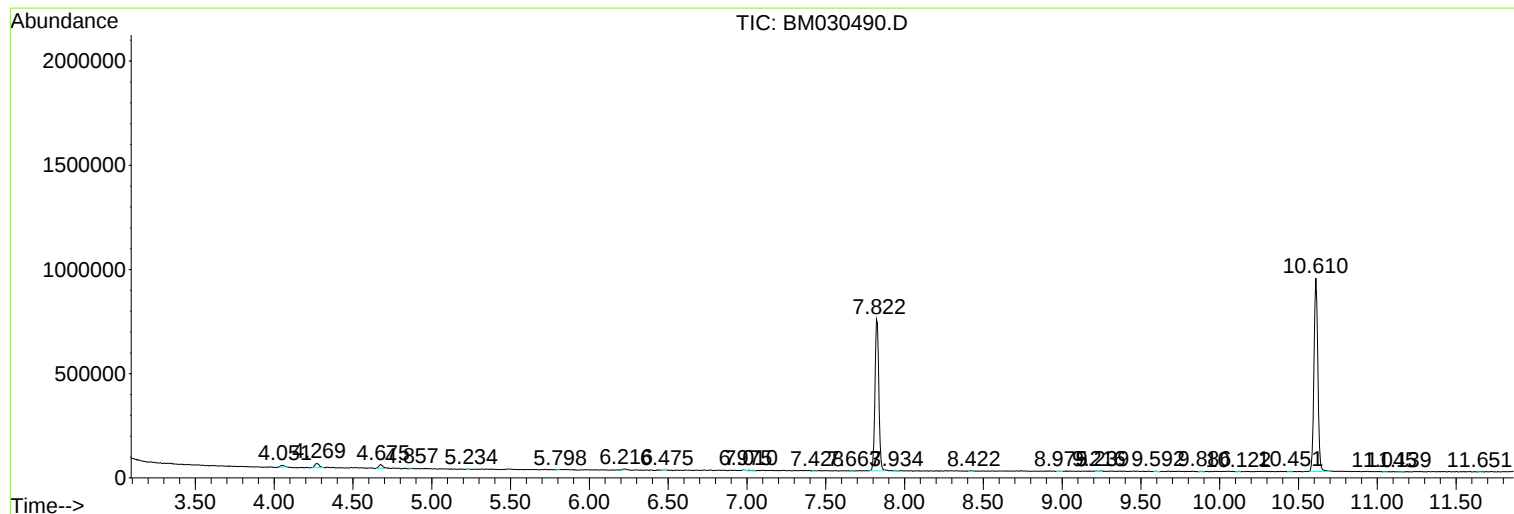

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061721\
Data File : BM030490.D
Acq On : 17 Jun 2021 12:02
Operator : CG/JU
Sample : M2690-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GCP2-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM060621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061721\
Data File : BM030490.D
Acq On : 17 Jun 2021 12:02
Operator : CG/JU
Sample : M2690-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GCP2-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM060621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
