


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061815\
Data File : BM001724.D
Acq On : 17 Jun 2015 18:52
Operator : TP/IZ
Sample : DFTPP62
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP62

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM031115.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Mar 28 05:37:34 2015

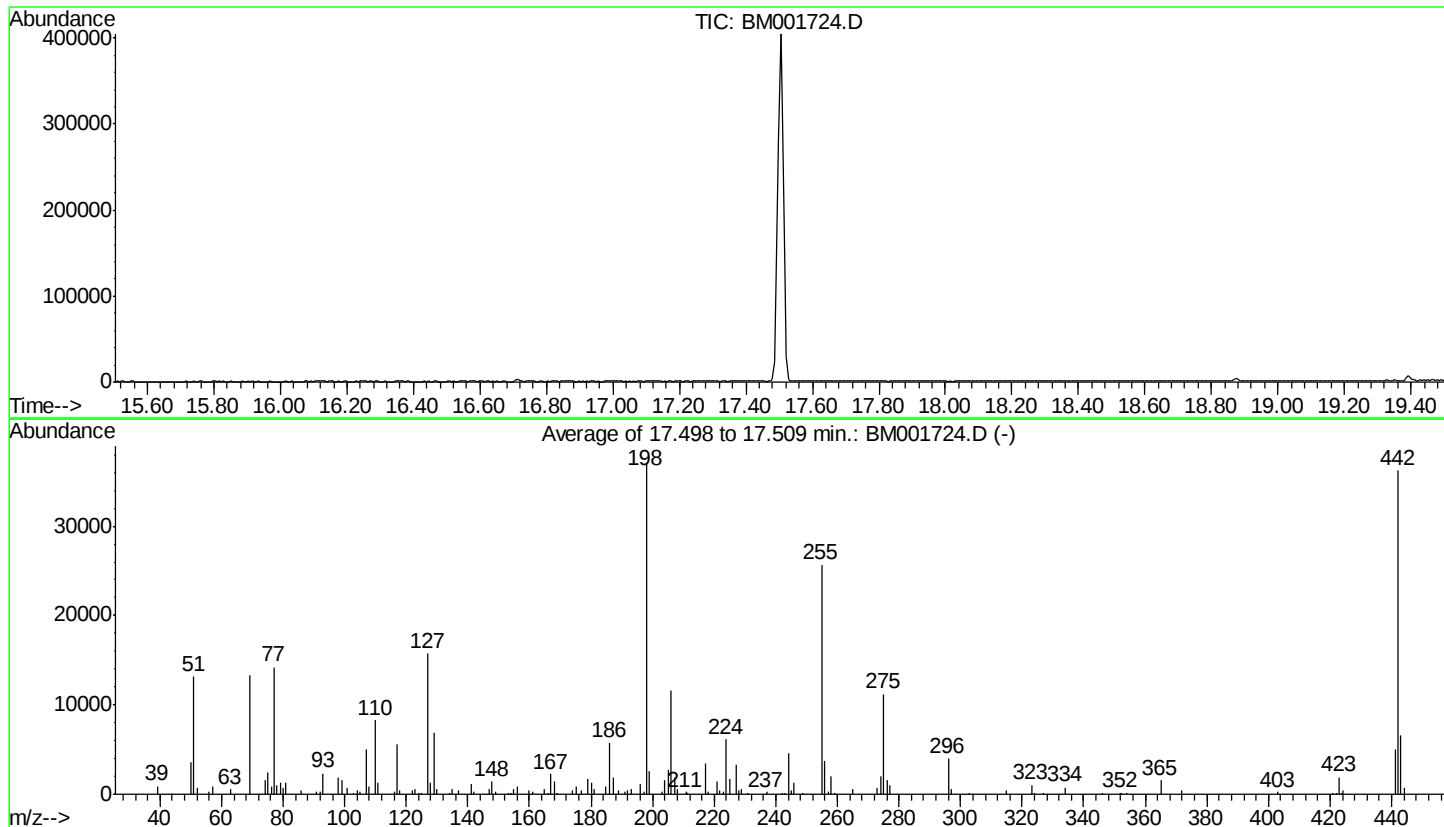

AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2512

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.5	13155	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.0	13374	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.3	15691	PASS
197	198	0.00	2	0.6	226	PASS
198	198	100	100	100.0	37104	PASS
199	198	5	9	6.9	2572	PASS
275	198	10	60	30.3	11238	PASS
365	198	1	100	4.2	1553	PASS
441	442	0.01	24	13.8	5007	PASS
442	198	50	100	97.5	36181	PASS
443	442	15	24	18.3	6626	PASS

m/z	Abundance
39.10	891.0
44.00	942.0
50.10	3686.0
51.10	12879.0
52.10	592.0
56.00	427.0
57.00	761.0
62.90	508.0
69.00	12456.0
74.00	1540.0
75.00	2278.0
76.00	799.0
77.00	13638.0
78.00	1015.0
79.00	1132.0
80.00	765.0
81.00	1208.0
86.00	390.0
91.00	342.0
92.00	389.0
93.00	2248.0
98.00	1667.0
99.00	1842.0
101.00	662.0
104.00	417.0
107.00	5022.0
108.00	830.0
110.00	7720.0
111.00	1326.0
116.00	303.0
117.00	5029.0
118.00	368.0
122.00	414.0
122.90	422.0
127.00	14191.0
128.00	1075.0
129.00	6129.0
129.90	537.0
134.90	519.0
136.90	322.0
140.90	845.0
141.90	393.0
147.00	523.0
147.90	1051.0
149.00	331.0
153.80	306.0
154.90	673.0
156.10	854.0
159.90	400.0
161.00	381.0
165.00	365.0
167.00	2019.0
168.00	1423.0
174.00	383.0
175.00	926.0
177.00	324.0
179.00	1526.0
180.00	1143.0
181.00	314.0
184.90	624.0
186.10	5207.0
187.00	1869.0
188.90	451.0
192.00	444.0
193.00	599.0
196.00	1003.0
198.00	32256.0
198.90	2326.0
204.00	1421.0
204.90	2418.0
206.00	9730.0
207.00	1742.0
208.10	524.0
210.90	304.0
217.00	2961.0
221.00	1141.0
221.80	426.0
222.90	451.0
224.00	4796.0
225.00	1418.0
227.00	2895.0
228.10	412.0
229.00	443.0
244.00	3506.0
245.10	309.0
246.00	918.0
255.00	20480.0
256.00	3063.0
257.10	334.0
257.90	1693.0
265.00	397.0

Instrument :
BNA_M
ClientSampleId :
DFTPP62

273.00	754.0
274.00	1458.0
275.00	8936.0
276.00	1553.0
276.90	763.0
296.00	2889.0
296.90	364.0
303.00	309.0
314.90	324.0
323.00	820.0
327.00	343.0
334.10	564.0
364.90	943.0
372.10	449.0
423.00	1136.0
423.90	569.0
441.10	3207.0
442.10	23576.0
443.00	4624.0
444.00	512.0

Instrument :
BNA_M
ClientSampleId :
DFTPP62

m/z	Abundance
39.00	1051.0
44.00	534.0
50.10	4197.0
51.10	15881.0
52.00	956.0
56.00	451.0
56.90	859.0
63.00	521.0
69.00	15825.0
74.00	1812.0
75.00	3240.0
76.10	971.0
77.10	17424.0
78.10	1155.0
79.00	1611.0
80.00	801.0
81.00	1482.0
85.90	495.0
91.00	321.0
92.00	351.0
93.00	3019.0
98.00	2248.0
99.00	1563.0
101.00	677.0
103.00	301.0
104.00	562.0
104.90	500.0
107.00	5612.0
108.00	1086.0
110.00	10213.0
110.90	1608.0
115.90	560.0
117.00	6838.0
117.90	507.0
121.90	371.0
123.00	846.0
124.00	378.0
127.00	19136.0
128.00	1451.0
129.00	8466.0
130.00	598.0
133.90	341.0
135.00	885.0
136.90	522.0
140.90	1425.0
142.00	370.0
147.00	682.0
148.00	1864.0
149.00	399.0
153.00	329.0
155.00	768.0
156.00	884.0
159.90	429.0
160.90	475.0
164.90	760.0
166.00	558.0
167.00	2686.0
167.90	1430.0
169.00	339.0
173.90	578.0
175.00	986.0
176.90	449.0
178.90	2104.0
180.00	1656.0
181.00	583.0
184.90	1089.0
186.00	6765.0
187.10	2299.0
188.90	540.0
191.00	308.0
191.90	526.0
193.00	584.0
196.00	1313.0
197.10	351.0
197.90	43880.0
198.90	3174.0
202.90	378.0
204.00	1808.0
205.00	3351.0
206.10	14136.0
207.10	2088.0
208.10	649.0
211.20	544.0
217.00	3933.0
217.90	526.0
221.00	1682.0
221.90	537.0
222.90	597.0
224.00	7316.0
225.10	2081.0
227.00	4106.0

Instrument :
BNA_M
ClientSampleId :
DFTPP62

228.00	529.0
229.00	841.0
231.00	368.0
236.90	430.0
242.10	381.0
244.10	5843.0
245.00	640.0
246.00	1650.0
248.90	302.0
255.00	30424.0
256.00	4275.0
257.00	379.0
258.00	2489.0
259.00	361.0
265.00	832.0
273.00	721.0
274.00	2641.0
275.00	13520.0
276.00	1917.0
276.90	1274.0
296.00	4861.0
296.90	702.0
302.90	330.0
315.00	551.0
323.00	1264.0
334.00	932.0
346.00	363.0
351.90	437.0
354.10	439.0
365.00	2004.0
371.90	578.0
403.00	311.0
423.10	2425.0
424.10	731.0
441.10	5929.0
442.10	42096.0
443.10	7749.0
443.90	736.0

Instrument :
BNA_M
ClientSampleId :
DFTPP62

m/z	Abundance
39.00	797.0
44.00	709.0
50.00	2985.0
51.10	10707.0
52.00	536.0
57.00	815.0
63.00	615.0
69.00	11843.0
74.00	1421.0
75.00	1874.0
76.00	614.0
77.10	11485.0
78.10	873.0
79.00	1043.0
79.90	812.0
80.90	1012.0
85.90	363.0
91.00	325.0
93.00	1767.0
97.90	1644.0
99.00	1395.0
100.80	645.0
104.00	347.0
105.00	418.0
107.00	4567.0
107.90	745.0
110.00	6888.0
111.00	1145.0
117.00	4876.0
117.90	322.0
121.90	357.0
123.00	473.0
124.90	307.0
127.00	13747.0
128.00	1193.0
129.00	5998.0
129.90	605.0
135.00	393.0
137.00	315.0
140.90	1101.0
147.00	438.0
147.90	1298.0
155.00	360.0
156.10	690.0
159.90	319.0
164.90	466.0
167.00	2097.0
168.00	1344.0
174.00	387.0
175.00	745.0
176.80	409.0
178.90	1597.0
180.00	993.0
180.90	629.0
184.90	723.0
186.00	5402.0
187.00	1541.0
189.00	366.0
191.00	467.0
191.90	479.0
193.00	448.0
195.90	952.0
197.10	329.0
198.00	35176.0
198.90	2218.0
202.90	350.0
204.00	1426.0
205.00	2266.0
206.00	10955.0
207.00	1795.0
207.90	601.0
210.90	437.0
217.00	3495.0
217.90	425.0
221.10	1470.0
221.90	370.0
223.10	546.0
224.00	6194.0
225.00	1688.0
227.00	3083.0
228.00	529.0
228.90	589.0
237.00	339.0
242.90	302.0
244.10	4310.0
245.00	505.0
246.00	1281.0
255.00	26232.0
256.00	3819.0
258.00	1825.0
265.10	643.0

Instrument :
BNA_M
ClientSampleId :
DFTPP62

272.90	579.0
273.90	1938.0
275.00	11258.0
276.00	1208.0
277.00	1018.0
296.00	4240.0
296.90	642.0
315.00	411.0
323.00	1093.0
324.00	337.0
334.00	719.0
352.10	487.0
365.00	1712.0
372.00	483.0
403.00	388.0
421.00	393.0
422.00	391.0
423.00	2113.0
424.00	745.0
441.10	5885.0
442.10	42872.0
443.00	7505.0
444.10	775.0

Instrument :
BNA_M
ClientSampleId :
DFTPP62

m/z	Abundance
44.00	673.0

Instrument :
BNA_M
ClientSampleId :
DFTPP62