


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061815\
 Data File : BM001731.D
 Acq On : 18 Jun 2015 09:09
 Operator : TP/IZ
 Sample : DFTPP63
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP63

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM031115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Mar 28 05:37:34 2015

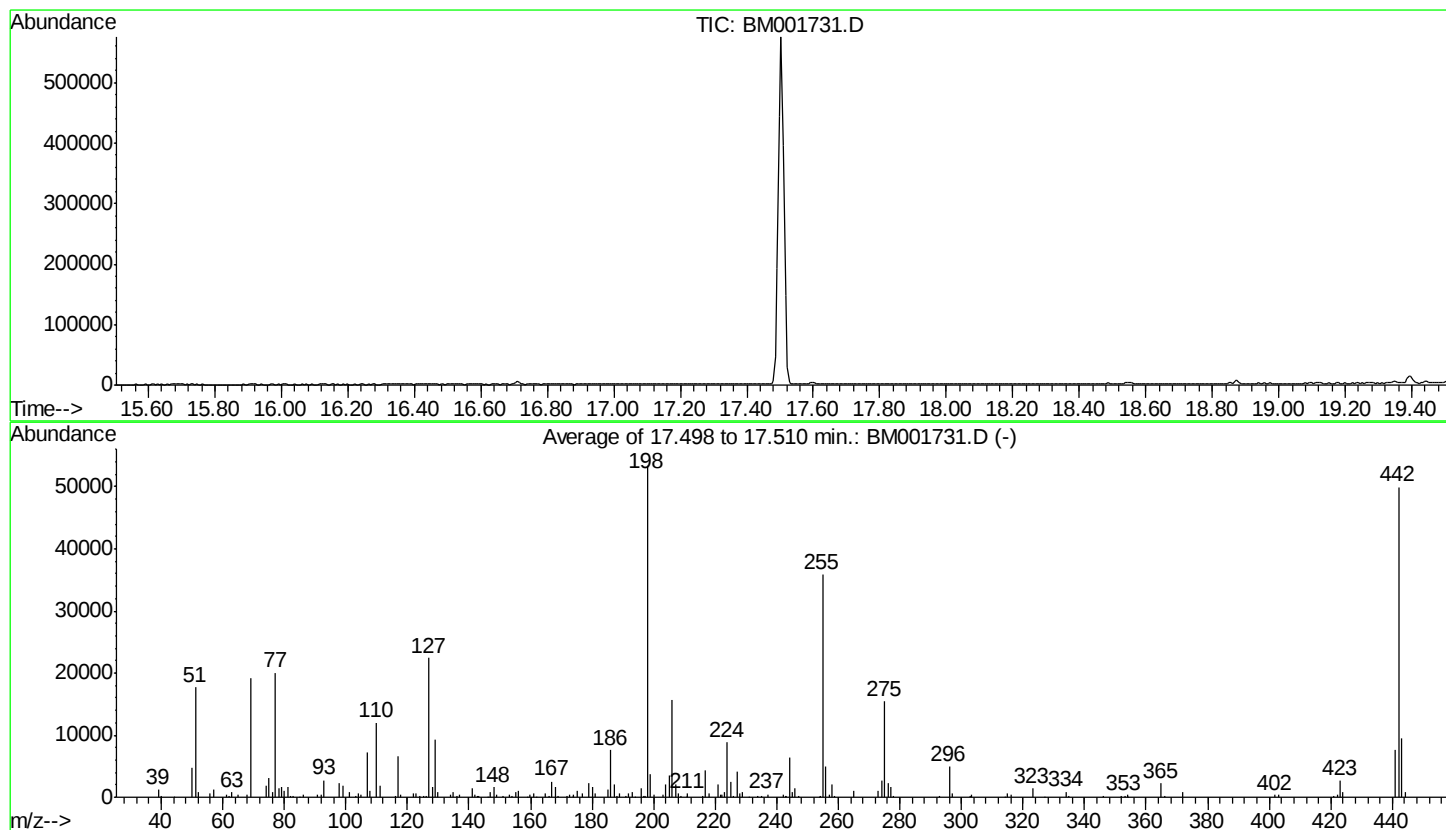

AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2512


Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.1	17698	PASS
68	69	0.00	2	1.8	350	PASS
69	198	0.00	100	36.1	19269	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.9	22389	PASS
197	198	0.00	2	0.3	138	PASS
198	198	100	100	100.0	53405	PASS
199	198	5	9	6.9	3696	PASS
275	198	10	60	28.9	15410	PASS
365	198	1	100	4.1	2182	PASS
441	442	0.01	24	15.5	7731	PASS
442	198	50	100	93.6	49992	PASS
443	442	15	24	19.0	9485	PASS

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061815\
 Data File : BM001731.D
 Acq On : 18 Jun 2015 09:09
 Operator : TP/IZ
 Sample : DFTPP63
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP63

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM031115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Mar 28 05:37:34 2015

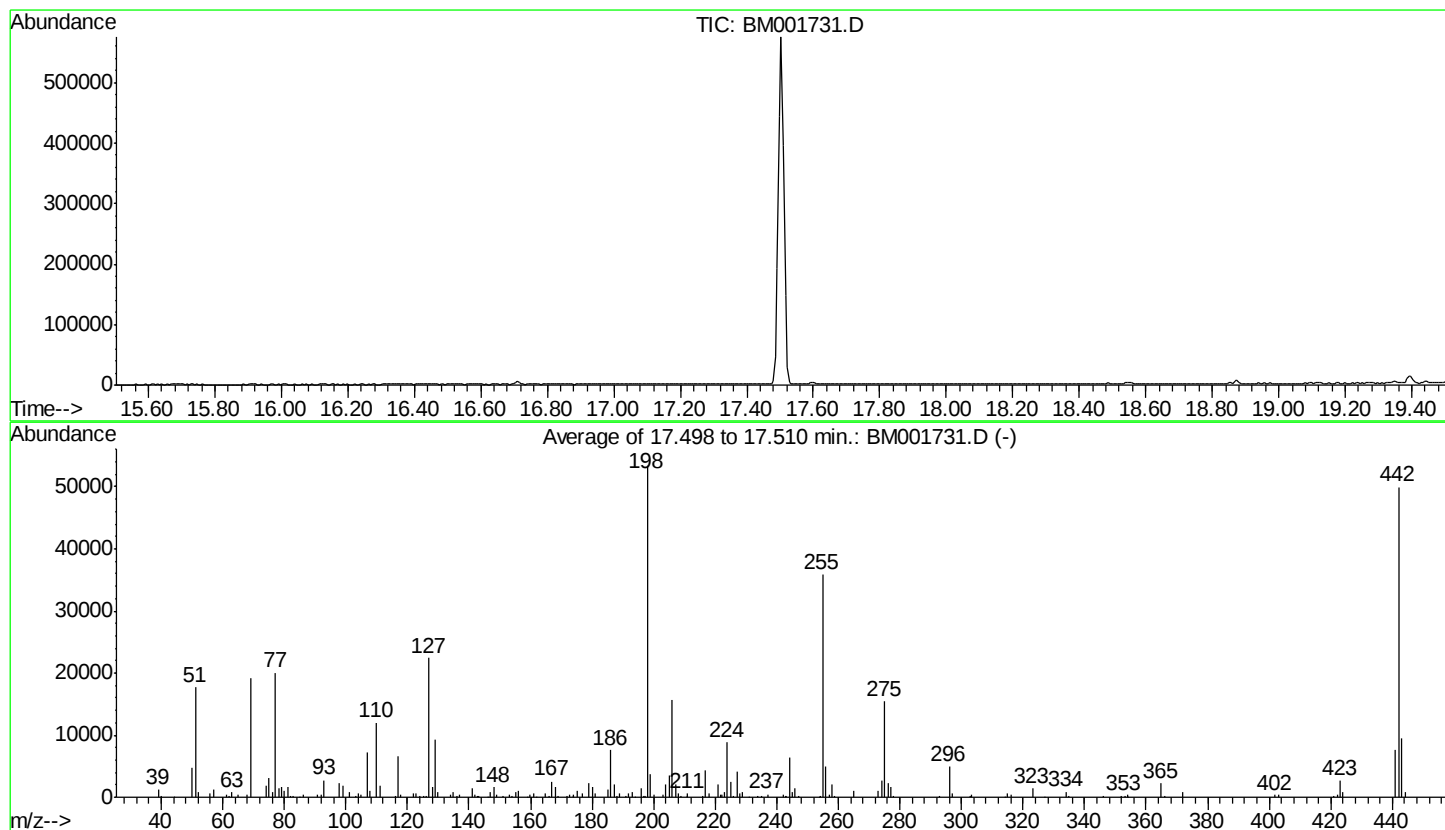

AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2512

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.1	17698	PASS
68	69	0.00	2	1.8	350	PASS
69	198	0.00	100	36.1	19269	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.9	22389	PASS
197	198	0.00	2	0.3	138	PASS
198	198	100	100	100.0	53405	PASS
199	198	5	9	6.9	3696	PASS
275	198	10	60	28.9	15410	PASS
365	198	1	100	4.1	2182	PASS
441	442	0.01	24	15.5	7731	PASS
442	198	50	100	93.6	49992	PASS
443	442	15	24	19.0	9485	PASS

m/z	Abundance
39.00	1219.0
44.00	812.0
50.10	5411.0
51.10	19808.0
52.00	1020.0
56.00	745.0
57.00	1382.0
61.00	377.0
62.10	326.0
63.00	814.0
65.00	389.0
68.10	516.0
69.00	20672.0
73.10	392.0
74.00	2088.0
75.00	3245.0
76.10	1078.0
77.10	21416.0
78.00	1541.0
79.00	1530.0
80.00	1182.0
81.00	1680.0
81.90	499.0
82.90	393.0
86.10	493.0
90.90	440.0
92.00	594.0
93.00	3001.0
98.00	2513.0
99.00	1973.0
101.00	938.0
104.00	933.0
105.10	434.0
107.00	7705.0
107.90	1201.0
110.00	12342.0
111.00	1989.0
116.10	372.0
117.00	6518.0
118.00	555.0
122.00	511.0
122.90	643.0
123.90	353.0
125.10	310.0
127.00	23256.0
128.00	1698.0
129.00	8738.0
129.90	843.0
134.00	397.0
134.90	753.0
136.90	505.0
141.00	1347.0
142.00	373.0
145.90	317.0
146.90	843.0
148.00	1595.0
149.00	613.0
152.90	362.0
155.00	747.0
156.10	825.0
160.00	472.0
160.90	609.0
164.90	557.0
167.00	2507.0
168.00	1735.0
169.00	442.0
172.00	366.0
172.90	361.0
173.90	553.0
175.10	1263.0
177.00	582.0
179.00	1997.0
180.00	1642.0
180.90	671.0
185.00	1149.0
186.00	6673.0
187.00	2013.0
188.90	595.0
190.90	384.0
192.00	502.0
193.00	737.0
196.00	1630.0
196.70	353.0
198.00	52552.0
199.00	3570.0
200.00	321.0
202.90	491.0
204.00	2511.0
205.00	3577.0
206.10	15556.0
207.00	1973.0

Instrument :
BNA_M
ClientSampleId :
DFTPP63

208.10	667.0
210.80	488.0
211.10	467.0
217.00	4152.0
218.00	498.0
221.00	1903.0
221.70	652.0
222.00	649.0
223.00	783.0
224.00	8392.0
225.10	2311.0
227.00	3816.0
228.00	503.0
228.90	855.0
231.00	314.0
237.10	441.0
242.00	390.0
243.10	458.0
244.00	5198.0
245.10	896.0
245.90	1224.0
255.00	32176.0
256.00	4903.0
257.00	529.0
258.00	1874.0
258.90	324.0
264.90	875.0
273.00	999.0
274.10	2452.0
275.00	14274.0
276.10	1986.0
277.00	1559.0
296.00	4201.0
297.00	641.0
302.90	517.0
315.10	320.0
316.10	314.0
323.10	1065.0
334.10	765.0
334.90	331.0
353.90	313.0
365.00	1640.0
372.00	567.0
402.00	317.0
423.10	1693.0
424.10	931.0
441.10	5329.0
442.10	35800.0
443.10	7578.0
444.00	638.0

Instrument :
BNA_M
ClientSampleId :
DFTPP63

m/z	Abundance
39.00	1554.0
39.90	345.0
44.10	954.0
50.10	5533.0
51.10	20824.0
52.00	1167.0
56.00	731.0
57.00	1589.0
61.00	359.0
61.90	313.0
63.00	896.0
65.00	383.0
68.00	536.0
69.00	23784.0
73.00	410.0
74.00	2185.0
75.00	3889.0
76.10	993.0
77.00	24768.0
78.10	1781.0
79.00	2234.0
80.00	1256.0
81.00	1717.0
82.00	386.0
83.00	457.0
84.90	314.0
86.00	617.0
91.00	655.0
91.90	542.0
93.00	3380.0
98.00	2791.0
99.00	2449.0
100.90	1048.0
103.00	464.0
104.00	852.0
105.00	563.0
107.00	8560.0
108.00	1301.0
110.00	14642.0
111.00	2036.0
116.10	495.0
117.00	7748.0
117.90	569.0
122.00	721.0
122.90	1038.0
124.00	427.0
125.00	337.0
126.20	331.0
127.00	27408.0
128.00	2098.0
129.00	11812.0
129.90	1183.0
133.90	489.0
135.00	970.0
136.00	392.0
136.90	534.0
141.00	1726.0
142.10	487.0
142.90	375.0
147.00	1131.0
148.00	1898.0
149.00	434.0
151.10	347.0
152.90	401.0
154.10	385.0
155.00	799.0
156.00	1260.0
158.80	317.0
159.90	491.0
160.90	707.0
162.00	326.0
164.90	737.0
165.90	493.0
167.00	2849.0
168.00	1894.0
169.00	348.0
171.90	339.0
172.80	315.0
174.10	847.0
175.10	1246.0
176.90	778.0
179.00	2752.0
180.00	1962.0
180.90	686.0
185.00	1560.0
186.00	9479.0
187.10	2568.0
187.90	352.0
188.90	722.0
191.00	406.0
191.90	695.0

Instrument :
BNA_M
ClientSampleId :
DFTPP63

193.00	963.0
193.90	311.0
196.00	1933.0
197.10	416.0
198.00	64088.0
199.00	4456.0
199.90	371.0
203.00	526.0
204.00	2238.0
205.00	3926.0
206.00	18472.0
207.10	2900.0
208.00	793.0
209.00	443.0
211.00	578.0
216.00	497.0
217.00	5330.0
218.00	701.0
221.10	2634.0
221.80	840.0
223.00	947.0
224.00	10371.0
225.00	3101.0
226.00	375.0
227.00	5038.0
227.90	781.0
229.00	911.0
233.80	394.0
235.00	440.0
237.00	597.0
242.00	546.0
243.10	430.0
244.00	8367.0
245.00	1071.0
246.00	1841.0
246.90	334.0
253.90	305.0
255.00	44232.0
256.00	5681.0
257.10	504.0
258.00	2589.0
258.90	429.0
264.90	1031.0
273.00	1381.0
274.00	3160.0
275.00	18576.0
276.00	2990.0
277.00	1996.0
278.00	352.0
293.00	367.0
296.00	6338.0
297.00	896.0
303.10	672.0
314.00	302.0
315.00	759.0
316.00	539.0
323.00	1860.0
327.00	326.0
334.00	1131.0
335.00	398.0
352.00	400.0
353.00	376.0
354.10	643.0
365.00	2843.0
372.00	757.0
401.90	469.0
403.00	622.0
421.00	515.0
422.00	601.0
423.00	3131.0
424.10	965.0
441.10	10015.0
442.10	58840.0
443.10	11334.0
444.10	1228.0

Instrument :
BNA_M
ClientSampleId :
DFTPP63

m/z	Abundance
39.00	857.0
44.00	1229.0
50.00	3300.0
51.10	12462.0
52.00	612.0
56.00	416.0
56.90	838.0
61.00	461.0
63.10	725.0
65.00	327.0
69.00	13353.0
74.00	1458.0
75.00	2307.0
76.10	649.0
77.10	14024.0
78.00	942.0
79.00	1212.0
80.00	829.0
81.00	1475.0
86.00	395.0
90.80	336.0
92.10	350.0
93.00	1950.0
98.00	1782.0
98.90	1315.0
101.00	733.0
103.80	381.0
105.00	396.0
107.00	5359.0
108.00	826.0
110.00	9099.0
111.00	1703.0
117.00	5342.0
117.90	354.0
121.90	373.0
123.00	479.0
127.00	16504.0
128.00	1116.0
129.00	7046.0
129.90	725.0
134.00	405.0
134.90	498.0
137.00	332.0
141.00	994.0
142.00	408.0
143.10	401.0
147.00	711.0
148.00	1329.0
148.90	320.0
153.00	333.0
154.00	321.0
155.00	761.0
156.00	974.0
160.00	432.0
161.00	605.0
164.90	478.0
166.00	385.0
167.00	2227.0
168.00	1136.0
172.90	311.0
173.90	437.0
175.00	899.0
177.00	403.0
179.00	1864.0
180.00	1177.0
181.00	511.0
185.00	888.0
186.00	6612.0
187.00	1867.0
189.00	411.0
191.90	700.0
193.00	774.0
196.00	1011.0
198.00	43576.0
198.90	3062.0
200.00	329.0
203.10	475.0
203.90	1386.0
205.10	3025.0
206.10	12806.0
207.00	2440.0
208.00	644.0
211.00	692.0
215.80	300.0
216.90	3830.0
217.90	566.0
221.00	1553.0
221.90	401.0
223.00	890.0
224.00	7708.0
225.10	2117.0

Instrument :
BNA_M
ClientSampleId :
DFTPP63

227.00	3373.0
227.90	427.0
229.00	588.0
235.00	375.0
236.90	440.0
242.10	387.0
242.80	343.0
244.00	5399.0
245.00	751.0
246.00	1217.0
254.10	391.0
255.00	31184.0
256.00	4268.0
256.90	437.0
257.90	1879.0
264.90	940.0
273.00	1042.0
274.00	2705.0
275.00	13382.0
276.00	1567.0
277.00	1324.0
296.00	4119.0
297.00	481.0
303.10	501.0
314.90	582.0
316.10	301.0
323.10	1356.0
334.00	845.0
346.00	331.0
352.10	308.0
353.00	364.0
354.00	395.0
365.00	2064.0
365.90	419.0
372.10	1129.0
402.00	312.0
403.00	373.0
421.00	411.0
422.00	454.0
423.00	3083.0
424.00	848.0
441.10	7851.0
442.10	55336.0
443.10	9543.0
444.00	718.0

Instrument :

BNA_M

ClientSampleId :

DFTPP63

Scan 2512 (17.463 min): BM001731.D
DFTPP63

m/z	Abundance
44.00	961.0
73.00	347.0
206.90	416.0

Instrument :
BNA_M
ClientSampleId :
DFTPP63