


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061816\
 Data File : BM005855.D
 Acq On : 17 Jun 2016 09:11
 Operator : UM/SJ
 Sample : DFTPP61
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP61

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061716.M
 Title : SVOA CALIBRATION
 Last Update : Sat Jun 18 23:47:00 2016

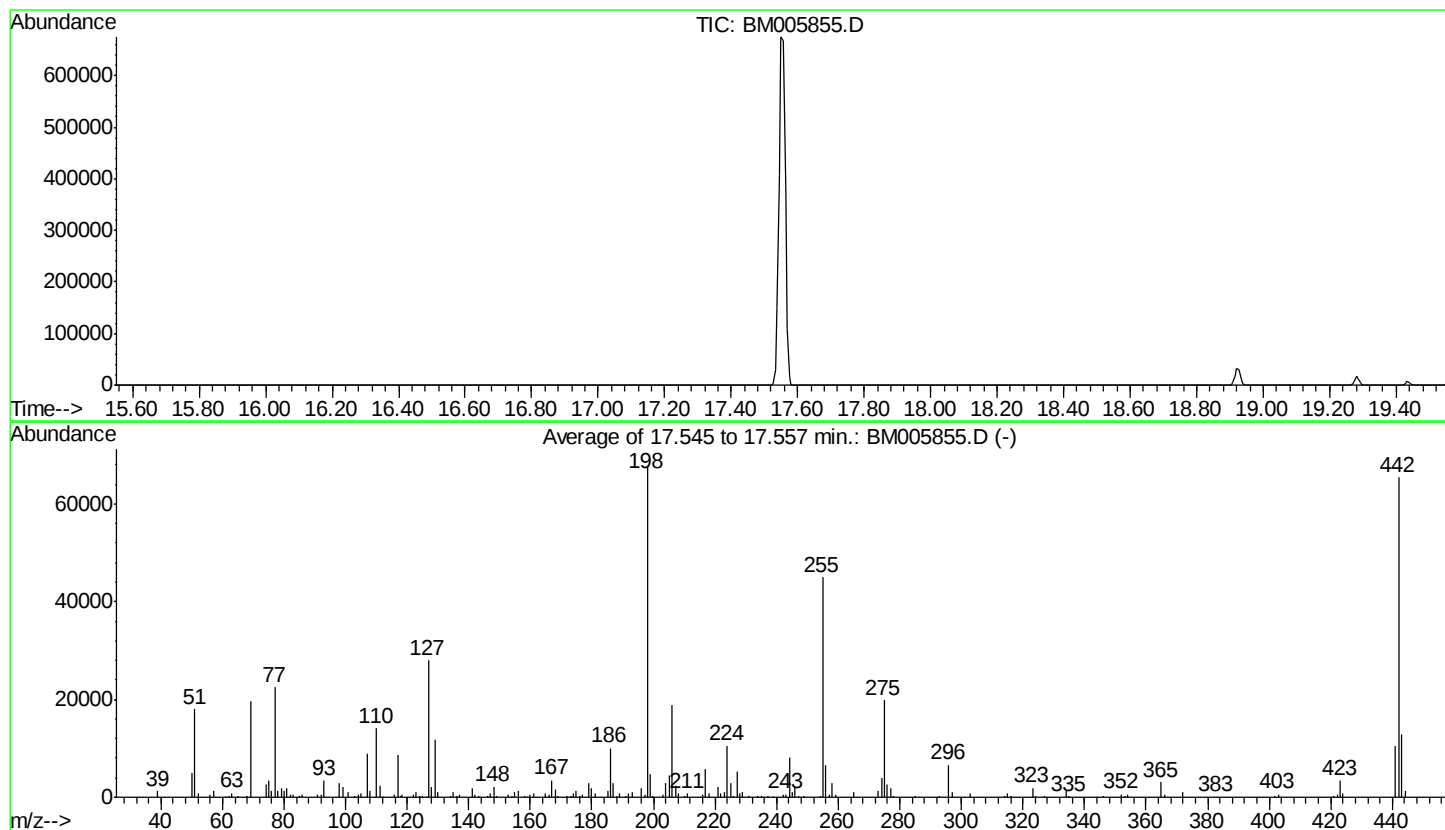

AutoFind: Scans 2543, 2544, 2545; Background Corrected with Scan 2538

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.5	17964	PASS
68	69	0.00	2	1.4	281	PASS
69	198	0.00	100	29.0	19698	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.1	27909	PASS
197	198	0.00	2	0.7	480	PASS
198	198	100	100	100.0	67845	PASS
199	198	5	9	6.9	4710	PASS
275	198	10	60	29.3	19887	PASS
365	198	1	100	4.6	3128	PASS
441	443	0.01	100	81.4	10542	PASS
442	198	50	100	96.4	65394	PASS
443	442	15	24	19.8	12948	PASS

m/z	Abundance
39.00	1085.0
50.00	4224.0
51.10	15046.0
52.10	767.0
56.00	424.0
57.00	933.0
63.00	754.0
67.90	335.0
69.00	16335.0
74.00	2121.0
75.00	2868.0
76.00	1039.0
77.10	18616.0
78.00	1104.0
79.00	1607.0
80.00	1088.0
81.00	1465.0
82.00	366.0
83.00	355.0
86.00	490.0
91.00	340.0
92.00	444.0
93.00	2783.0
98.00	2259.0
99.00	1698.0
100.90	786.0
104.00	533.0
104.90	577.0
107.00	6956.0
108.00	1050.0
110.00	11231.0
111.00	1917.0
116.00	454.0
117.00	7068.0
117.90	527.0
121.90	555.0
123.00	813.0
124.90	305.0
127.00	21592.0
128.00	1665.0
129.00	9199.0
129.90	930.0
135.00	848.0
137.00	389.0
141.00	1450.0
142.00	435.0
146.90	592.0
148.00	1713.0
153.00	497.0
155.00	802.0
156.00	1108.0
160.00	427.0
161.00	582.0
165.00	572.0
166.00	405.0
167.00	2433.0
168.00	1307.0
173.00	300.0
174.00	533.0
175.00	1102.0
176.90	470.0
179.00	2091.0
180.00	1310.0
181.00	659.0
185.00	1017.0
186.00	7497.0
187.00	2374.0
188.90	459.0
192.00	636.0
193.00	776.0
196.00	1449.0
198.00	49368.0
199.00	3385.0
203.00	434.0
204.00	2201.0
205.00	3194.0
206.10	13219.0
207.10	1761.0
208.00	596.0
211.10	554.0
216.00	382.0
217.00	4181.0
218.00	586.0
221.00	1642.0
221.80	543.0
223.00	710.0
224.00	7689.0
225.00	2120.0
227.00	3416.0
227.90	552.0
228.90	669.0

Instrument :
BNA_M
ClientSampleId :
DFTPP61

242.00	327.0
243.10	433.0
244.10	5425.0
245.00	743.0
246.00	1323.0
247.00	307.0
255.00	30368.0
256.00	4846.0
257.00	329.0
258.00	2023.0
259.00	361.0
265.00	784.0
273.00	912.0
274.00	2392.0
275.00	13325.0
276.00	2024.0
277.00	1264.0
296.00	4411.0
297.00	636.0
303.00	436.0
315.00	527.0
323.00	1159.0
334.00	891.0
352.10	346.0
354.10	392.0
365.00	1686.0
366.00	341.0
372.00	590.0
403.00	408.0
422.00	303.0
423.10	1815.0
424.00	419.0
441.10	5873.0
442.10	35736.0
443.10	7112.0
444.00	836.0

Instrument :
BNA_M
ClientSampleId :
DFTPP61

m/z	Abundance
39.00	1594.0
50.10	6148.0
51.10	21184.0
52.00	1046.0
56.00	608.0
57.00	1525.0
60.90	321.0
61.90	400.0
63.00	981.0
65.00	380.0
68.10	422.0
69.00	22496.0
74.00	3025.0
75.00	3991.0
76.00	1529.0
77.10	26264.0
78.00	1774.0
79.00	2183.0
80.00	1513.0
81.00	2146.0
82.00	554.0
82.90	471.0
85.00	361.0
86.00	620.0
90.90	499.0
92.00	552.0
93.00	3660.0
98.00	3280.0
99.00	2272.0
101.00	1251.0
103.00	453.0
104.00	742.0
105.00	732.0
107.00	10512.0
108.00	1589.0
110.00	16384.0
111.00	2630.0
112.00	322.0
116.00	615.0
117.00	10115.0
118.10	622.0
121.90	648.0
123.00	1185.0
123.90	577.0
125.00	444.0
126.20	393.0
127.00	32912.0
128.00	2501.0
129.00	13801.0
130.00	1225.0
134.00	470.0
135.00	1162.0
136.00	463.0
137.00	584.0
141.00	2016.0
142.00	530.0
143.00	438.0
145.90	411.0
147.00	1061.0
148.00	2369.0
148.90	492.0
153.00	588.0
154.00	555.0
155.00	1217.0
156.00	1629.0
158.00	431.0
160.00	709.0
161.00	963.0
164.90	841.0
166.00	611.0
167.00	4273.0
168.00	1933.0
169.00	420.0
172.00	450.0
173.00	478.0
174.00	771.0
175.00	1681.0
176.00	397.0
177.00	805.0
179.00	3322.0
180.00	2284.0
181.00	971.0
185.00	1612.0
186.00	11775.0
187.00	3289.0
188.00	463.0
189.00	812.0
191.00	438.0
191.90	1012.0
193.00	1150.0
196.00	2123.0

Instrument :
BNA_M
ClientSampleId :
DFTPP61

197.10	740.0
198.00	78200.0
199.00	5626.0
200.00	365.0
203.00	534.0
204.00	3200.0
205.10	5459.0
206.10	21912.0
207.10	2936.0
207.90	768.0
210.00	402.0
211.00	810.0
216.00	508.0
217.00	6505.0
218.00	761.0
221.00	2504.0
221.90	953.0
223.00	1203.0
224.00	12637.0
225.10	3169.0
226.10	366.0
227.00	6073.0
228.00	838.0
229.00	1356.0
231.00	492.0
234.00	358.0
235.00	405.0
237.00	426.0
238.90	310.0
242.00	643.0
243.00	571.0
244.10	9333.0
245.10	1395.0
246.00	2412.0
247.00	403.0
248.90	356.0
254.20	579.0
255.00	52224.0
256.00	7667.0
257.00	554.0
258.00	3245.0
259.00	577.0
265.00	1316.0
273.00	1466.0
274.00	4515.0
275.00	22336.0
276.00	3098.0
277.00	2319.0
277.90	413.0
285.00	406.0
292.90	439.0
296.00	7784.0
297.00	1099.0
303.10	810.0
314.00	339.0
315.00	847.0
316.00	351.0
323.10	2327.0
324.00	372.0
326.90	420.0
334.10	1324.0
335.00	419.0
345.90	501.0
352.00	580.0
353.10	433.0
354.10	741.0
365.00	3548.0
366.00	490.0
372.00	1228.0
402.00	428.0
403.00	647.0
421.00	491.0
422.10	558.0
423.10	3658.0
424.10	859.0
441.10	11529.0
442.10	71744.0
443.10	14470.0
444.10	1383.0

Instrument :
BNA_M
ClientSampleId :
DFTPP61

m/z	Abundance
39.10	1248.0
50.10	4727.0
51.10	17664.0
52.00	808.0
55.90	576.0
57.00	1300.0
62.00	344.0
63.00	818.0
65.00	344.0
68.10	421.0
69.00	20264.0
74.00	2362.0
75.00	3266.0
76.10	1234.0
77.10	22640.0
78.00	1442.0
79.00	1871.0
80.00	1338.0
81.00	1782.0
82.00	417.0
83.00	393.0
85.00	383.0
86.00	662.0
90.90	570.0
92.00	558.0
93.00	3592.0
98.00	3038.0
99.00	1964.0
101.00	1122.0
102.90	372.0
104.00	687.0
105.00	711.0
107.00	9277.0
108.00	1371.0
110.00	14456.0
111.00	2360.0
115.90	510.0
117.00	8948.0
118.00	658.0
121.90	653.0
122.90	1007.0
123.90	531.0
125.00	352.0
127.00	29224.0
128.00	2236.0
129.00	12416.0
130.00	1118.0
134.00	416.0
135.00	1225.0
136.00	465.0
137.00	527.0
141.00	1860.0
142.00	452.0
143.00	362.0
146.00	326.0
147.00	978.0
148.00	2226.0
149.00	439.0
152.90	641.0
154.00	415.0
155.00	1076.0
156.00	1606.0
158.00	394.0
158.90	323.0
159.90	585.0
161.00	924.0
165.00	839.0
166.00	593.0
167.00	3652.0
168.00	1707.0
169.00	383.0
172.00	369.0
173.00	422.0
174.00	798.0
175.00	1522.0
176.10	330.0
177.00	714.0
179.00	3180.0
180.00	2147.0
180.90	861.0
185.00	1573.0
186.00	10978.0
187.00	3266.0
188.10	353.0
188.90	786.0
191.00	354.0
192.00	950.0
193.00	1253.0
196.00	2245.0
197.10	701.0
198.00	75968.0

Instrument :
BNA_M
ClientSampleId :
DFTPP61

199.00	5119.0
199.90	398.0
202.90	643.0
204.00	3216.0
205.10	5035.0
206.10	21832.0
207.00	2715.0
208.00	803.0
210.10	322.0
211.00	913.0
215.00	328.0
216.00	507.0
217.00	6373.0
218.00	803.0
221.10	2533.0
221.90	848.0
223.00	1248.0
224.00	11516.0
225.00	3127.0
226.00	306.0
227.00	6119.0
228.00	697.0
229.00	1142.0
231.00	410.0
233.90	375.0
235.00	446.0
237.00	421.0
242.10	611.0
243.10	599.0
244.10	9360.0
245.00	1226.0
246.00	2233.0
247.00	423.0
249.00	354.0
254.20	611.0
255.00	52544.0
256.00	7338.0
257.00	690.0
258.00	3651.0
259.00	572.0
265.00	1387.0
273.00	1506.0
274.00	4609.0
275.00	24000.0
276.00	3055.0
277.00	2291.0
277.90	398.0
285.00	362.0
293.00	438.0
296.00	7819.0
297.00	1110.0
303.00	880.0
314.00	358.0
315.00	904.0
316.00	526.0
323.00	2383.0
324.00	424.0
326.90	513.0
334.10	1452.0
335.00	343.0
346.00	523.0
352.10	717.0
353.00	470.0
354.00	799.0
365.00	4151.0
366.00	523.0
372.00	1290.0
383.00	319.0
402.00	526.0
403.00	780.0
404.00	325.0
421.00	648.0
422.00	671.0
423.00	4555.0
424.00	832.0
441.10	14226.0
442.10	88704.0
443.10	17264.0
444.10	1559.0

Instrument :
BNA_M
ClientSampleId :
DFTPP61

Scan 2540 (17.527 min): BM005855.D
DFTPP61

m/z	Abundance
51.00	345.0
69.00	327.0
77.00	313.0
127.00	352.0
197.90	646.0
254.90	309.0

Instrument :
BNA_M
ClientSampleId :
DFTPP61