


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM061915\
 Data File : BM001738.D
 Acq On : 18 Jun 2015 15:46
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\SIM-BM061915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 19 05:05:14 2015

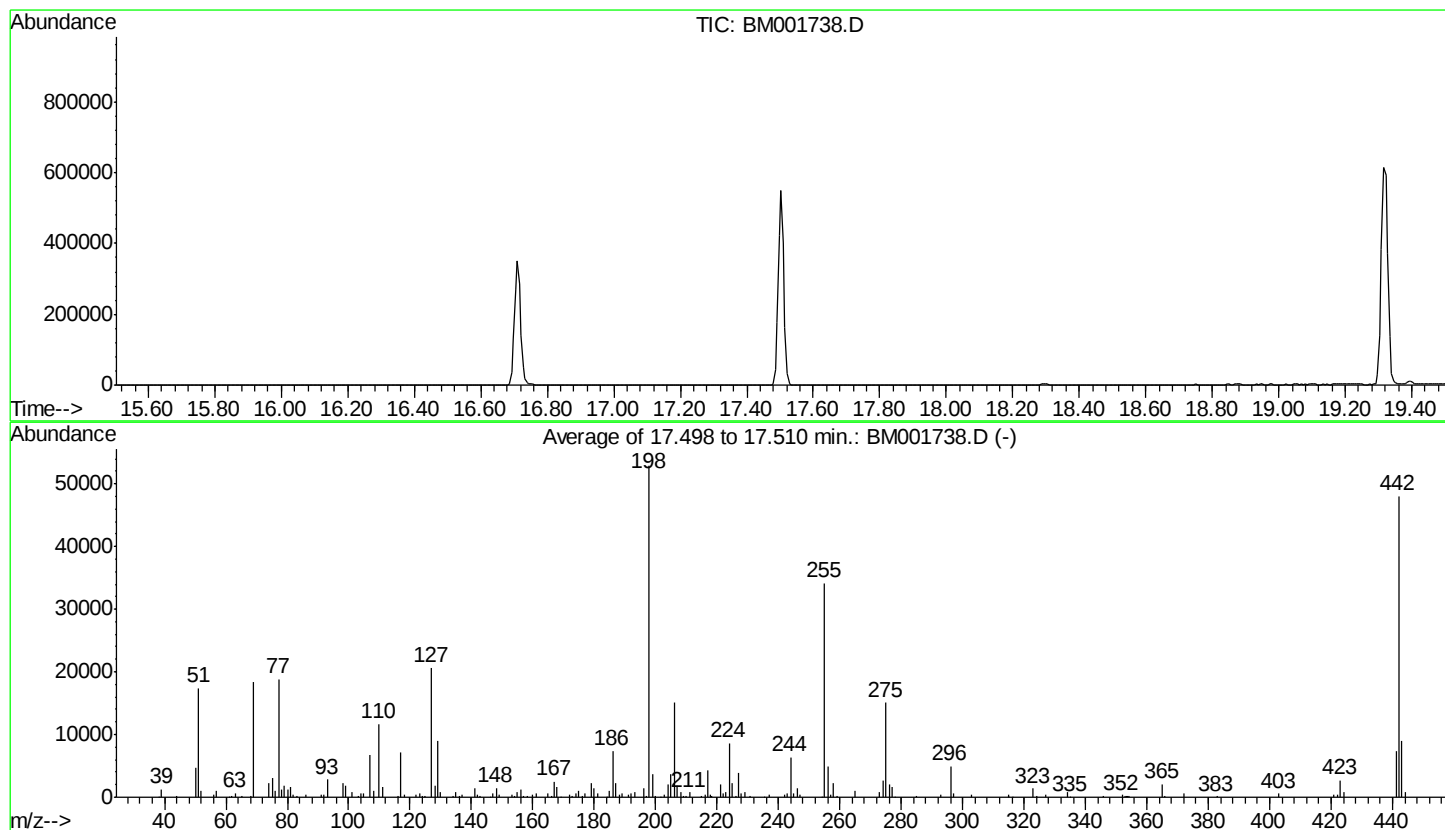

AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2512

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.0	17433	PASS
68	69	0.00	2	1.7	303	PASS
69	198	0.00	100	34.7	18333	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	39.0	20640	PASS
197	198	0.00	2	0.4	208	PASS
198	198	100	100	100.0	52896	PASS
199	198	5	9	6.8	3601	PASS
275	198	10	60	28.4	15032	PASS
365	198	1	100	3.9	2083	PASS
441	442	0.01	24	15.3	7354	PASS
442	198	50	100	90.8	48026	PASS
443	442	15	24	18.6	8933	PASS