
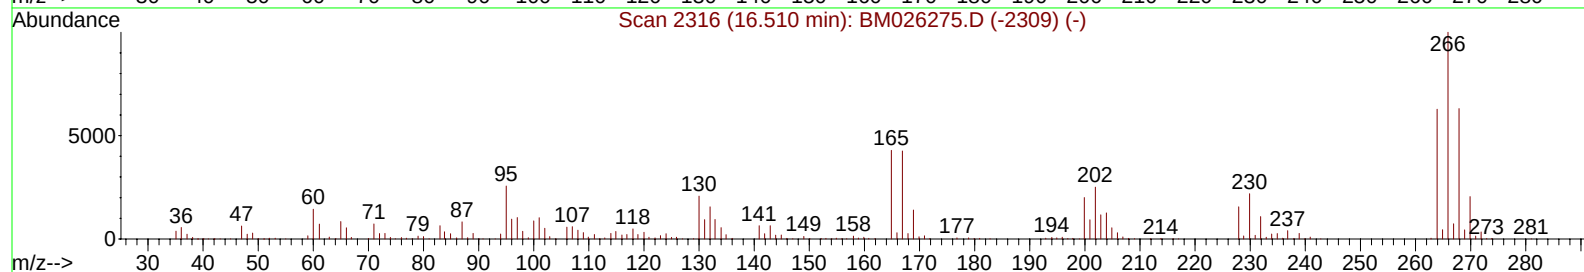
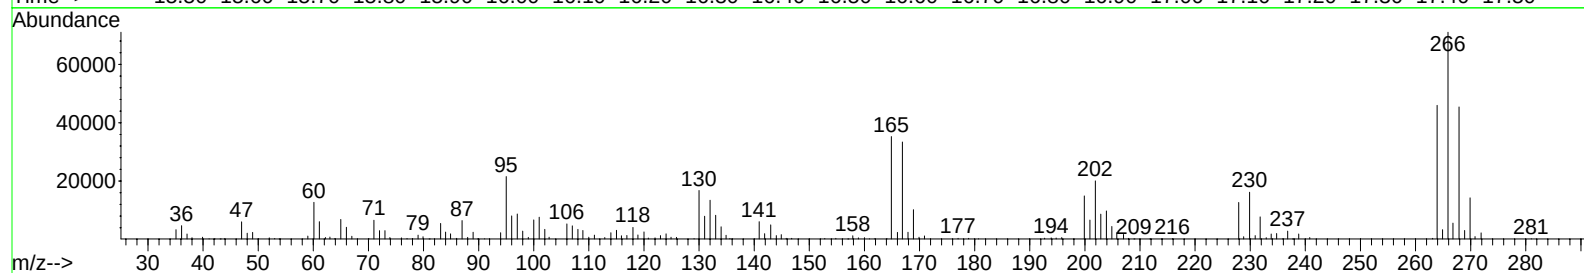


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061920\
 Data File : BM026461.D
 Acq On : 19 Jun 2020 08:29
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 19 18:31:55 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM060520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 19 10:20:20 2020
 Response via : Initial Calibration

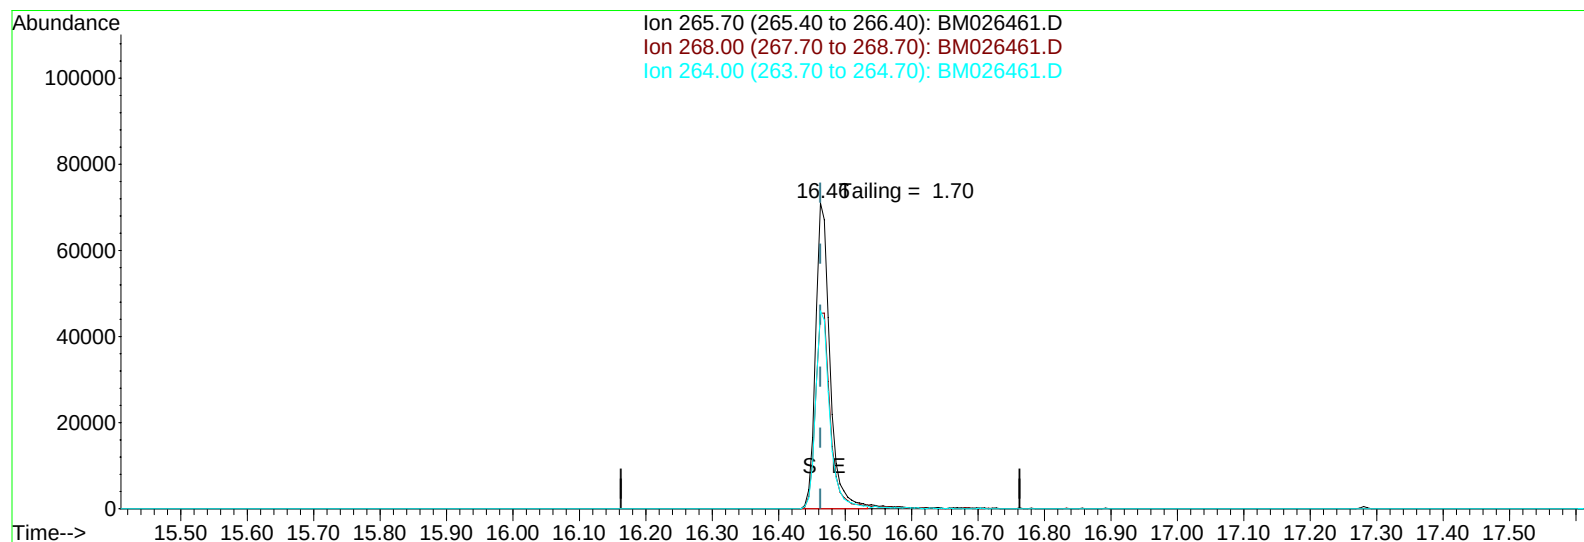

TIC: BM026461.D

(70) Pentachlorophenol (C)




16.463min (+0.000) 31344.02ng

response 109061

Ion	Exp%	Act%
265.70	100	100
268.00	62.80	63.96
264.00	63.20	64.70
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061920\
Data File : BM026461.D
Acq On : 19 Jun 2020 08:29
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 19 18:31:55 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 19 10:20:20 2020
Response via : Initial Calibration

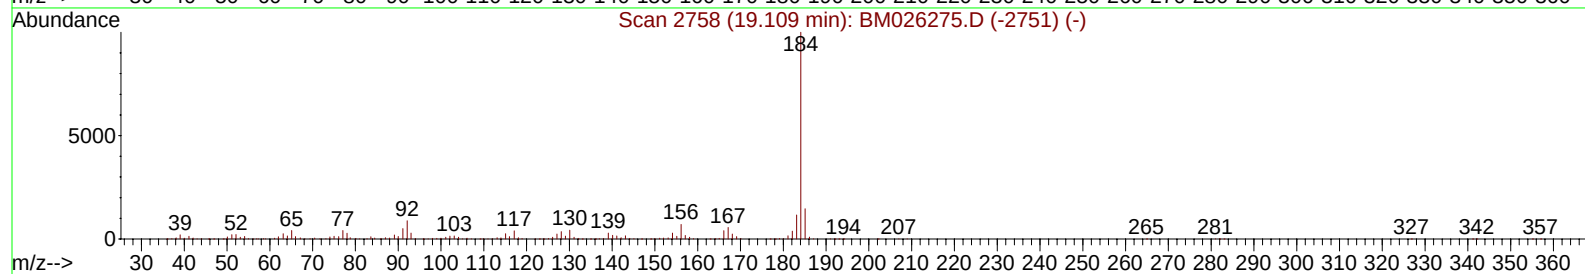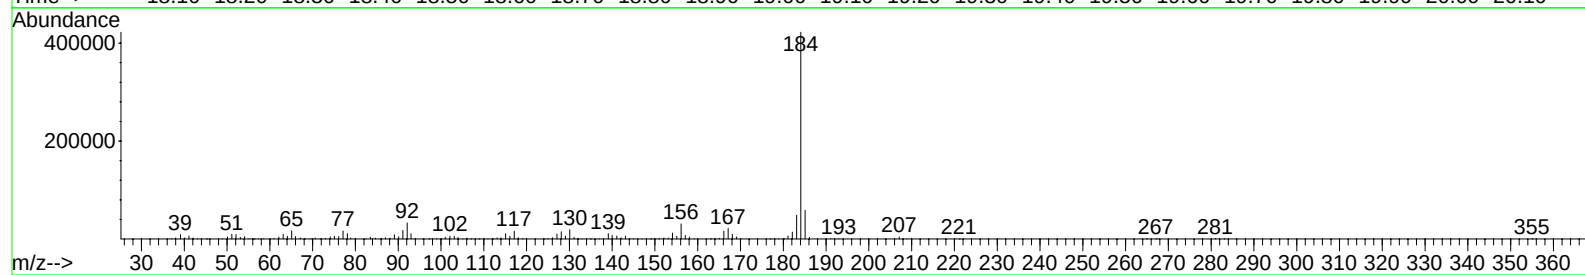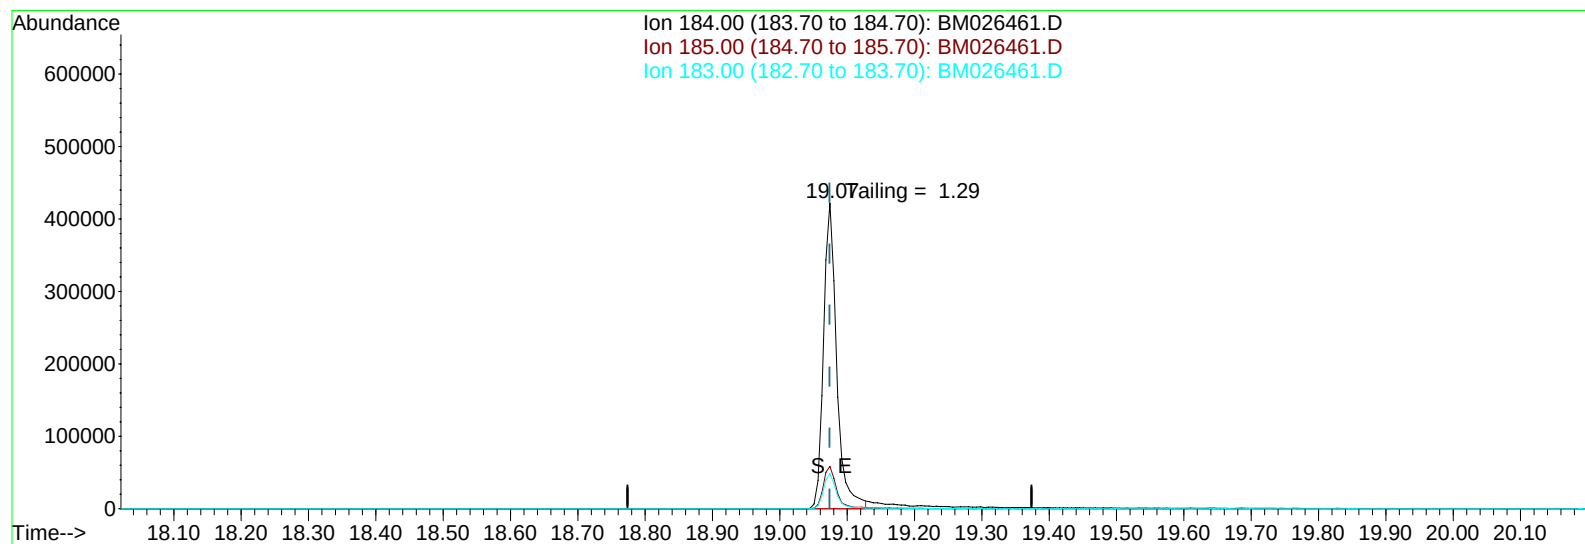

TIC: BM026461.D

(77) Benzidine

19.074min (+0.000) 28204.05ng

response 599902

Ion	Exp%	Act%
184.00	100	100
185.00	14.00	13.85
183.00	11.80	11.52
0.00	0.00	0.00