

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061920\
 Data File : BM026463.D
 Acq On : 19 Jun 2020 09:41
 Operator : JU/CG
 Sample : PB129455BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB129455BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM060520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.022	356	363	381	rBV	2272183	3292179	32.37%	7.578%
2	6.593	623	630	647	rBV	2366912	3642207	35.81%	8.384%
3	7.387	758	765	774	rBV	480786	728370	7.16%	1.677%
4	7.698	811	818	830	rBV	1905037	2978991	29.29%	6.857%
5	8.534	952	960	975	rBV	1602410	2628663	25.85%	6.051%
6	10.145	1227	1234	1247	rBV	607407	1014112	9.97%	2.334%
7	12.651	1653	1660	1678	rBV	3761987	5572618	54.79%	12.828%
8	14.045	1890	1897	1906	rBV	927671	1375405	13.52%	3.166%
9	15.551	2146	2153	2170	rBV	3312304	4709110	46.30%	10.840%
10	16.798	2359	2365	2381	rBV	1202458	1715246	16.87%	3.948%
11	19.462	2811	2818	2829	rBV	8619429	10170384	100.00%	23.412%
12	21.009	3076	3081	3092	rBV	1699171	2153118	21.17%	4.956%
13	22.515	3334	3337	3342	rVB	112543	151202	1.49%	0.348%
14	23.033	3421	3425	3430	rBV	153913	226023	2.22%	0.520%
15	23.103	3430	3437	3462	rVB	1282394	2619916	25.76%	6.031%
16	23.621	3521	3525	3530	rVB	143991	223536	2.20%	0.515%
17	24.286	3634	3638	3645	rVB	125042	240524	2.36%	0.554%


Sum of corrected areas: 43441604

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM061920\
Data File : BM026463.D
Acq On : 19 Jun 2020 09:41
Operator : JU/CG
Sample : PB129455BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB129455BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

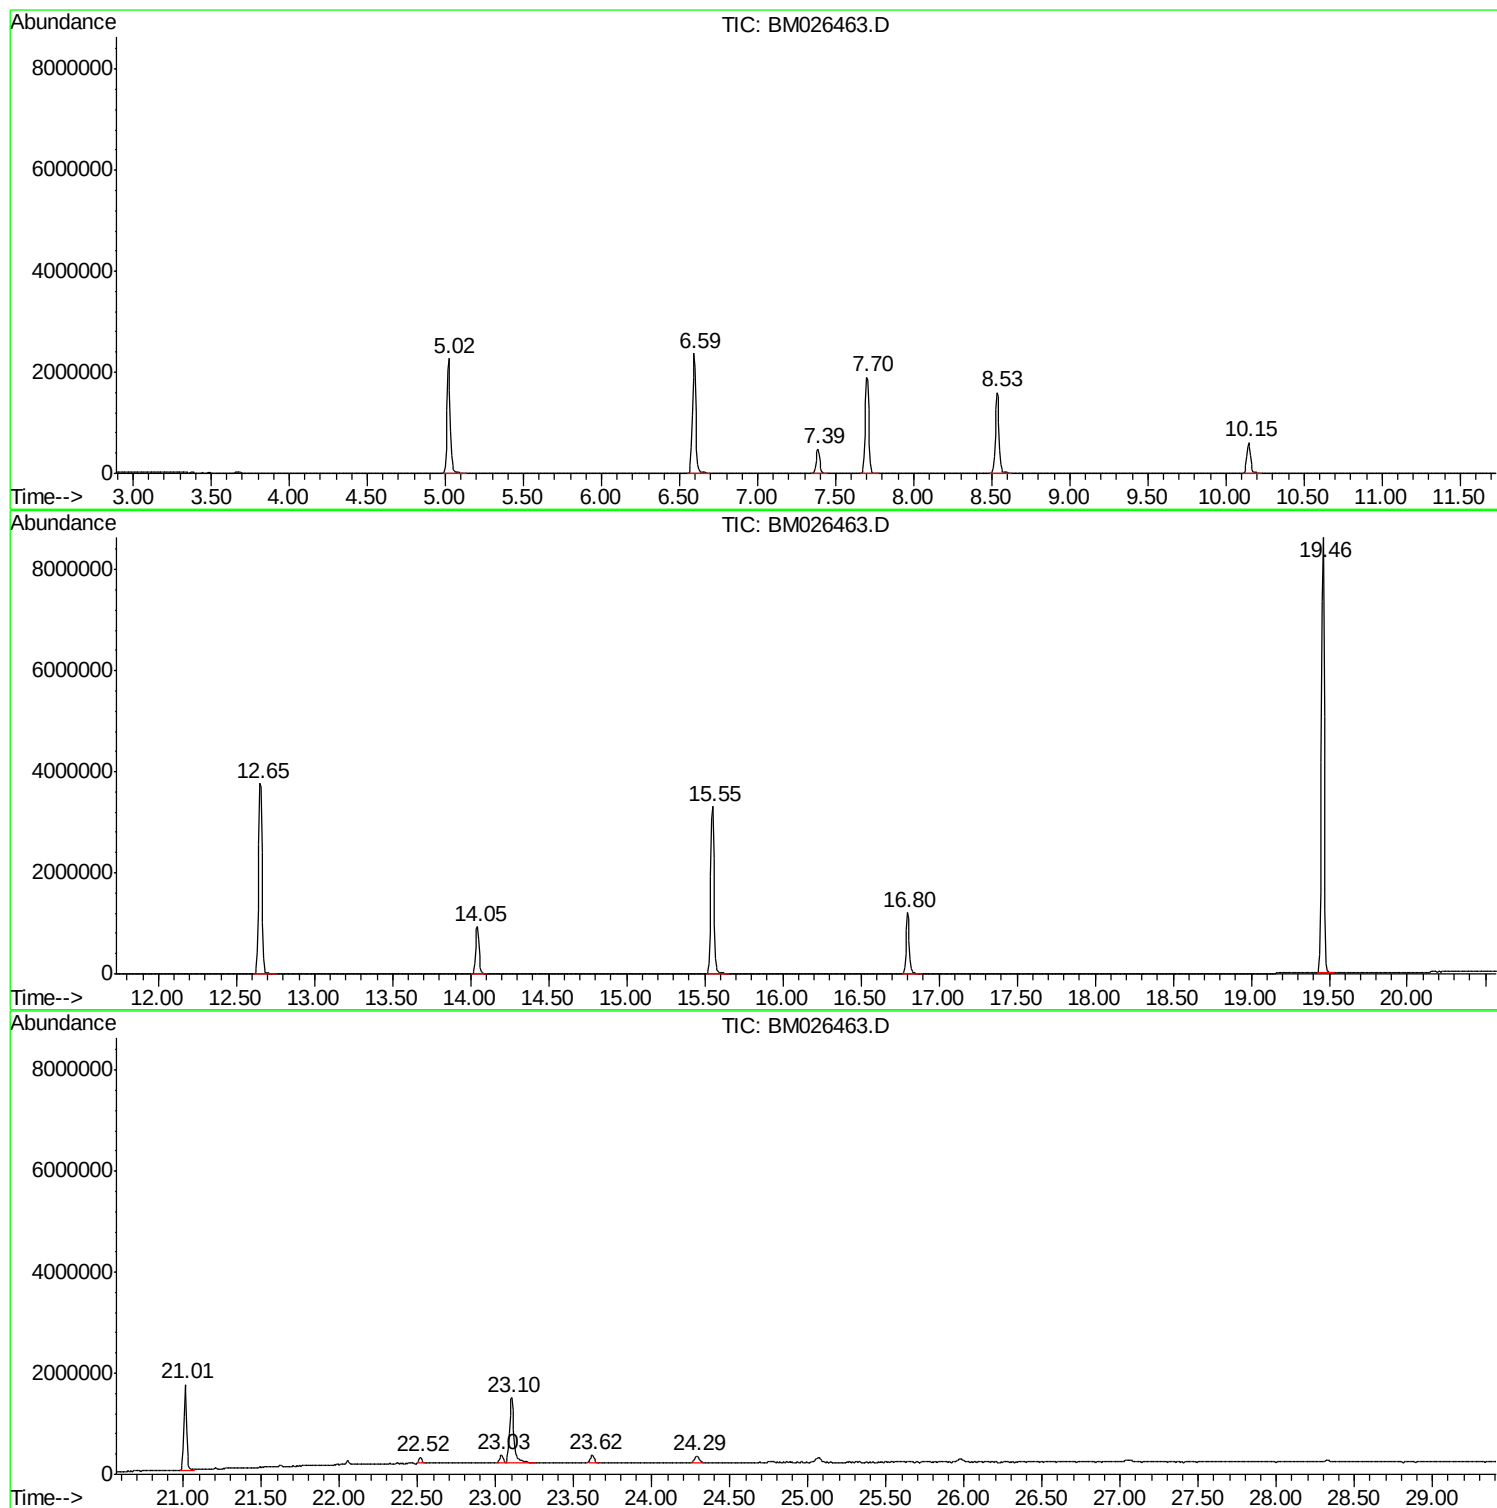

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM061920\
Data File : BM026463.D
Acq On : 19 Jun 2020 09:41
Operator : JU/CG
Sample : PB129455BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB129455BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM061920\
Data File : BM026463.D
Acq On : 19 Jun 2020 09:41
Operator : JU/CG
Sample : PB129455BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB129455BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM060520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc