


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM061920\
 Data File : BM026461.D
 Acq On : 19 Jun 2020 08:29
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM060520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 19 10:20:20 2020

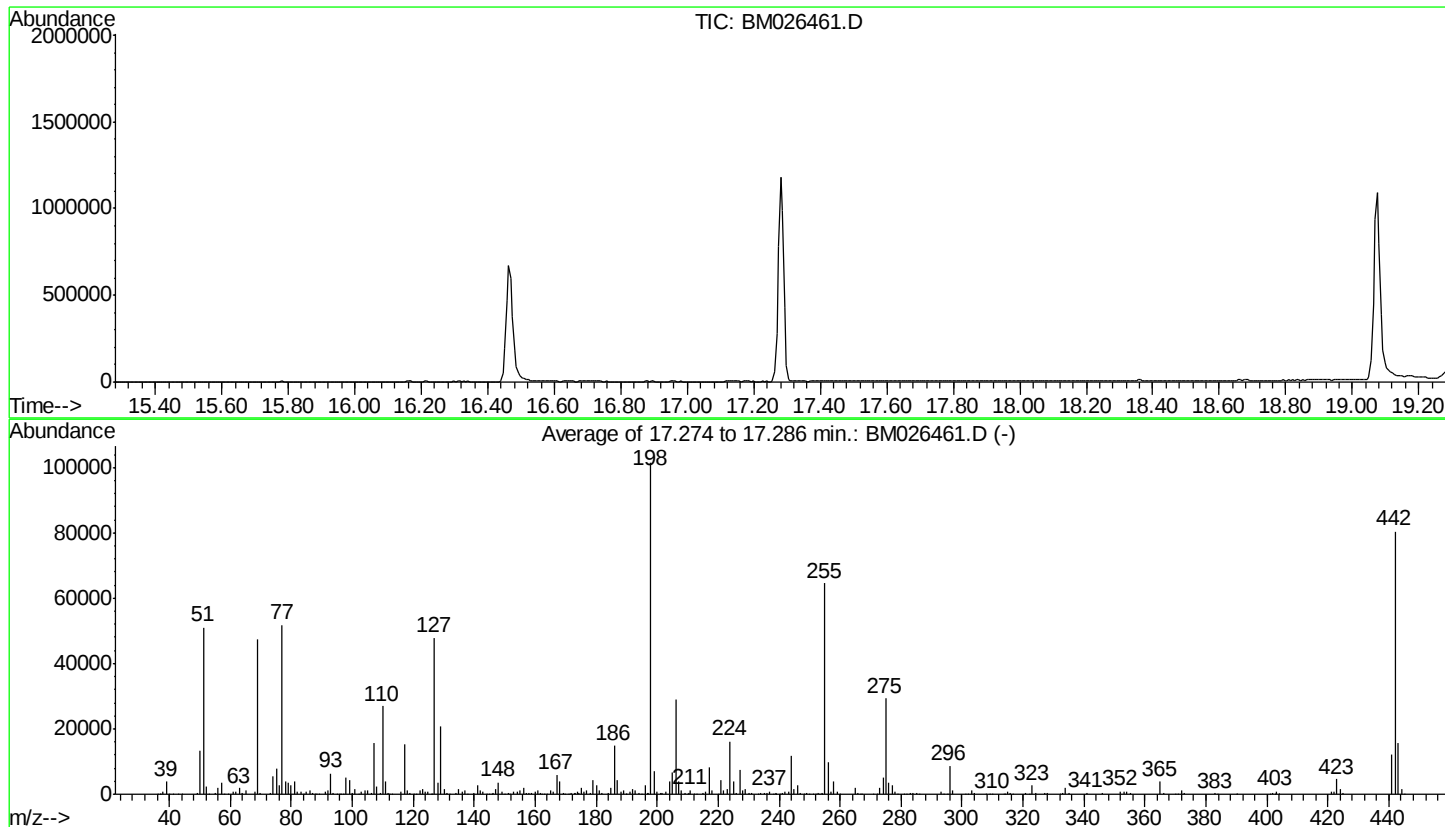

AutoFind: Scans 2446, 2447, 2448; Background Corrected with Scan 2440

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.3	51042	PASS
68	69	0.00	2	1.7	801	PASS
69	198	0.00	100	46.7	47336	PASS
70	69	0.00	2	0.6	273	PASS
127	198	10	80	47.1	47808	PASS
197	198	0.00	2	0.5	457	PASS
198	198	100	100	100.0	101464	PASS
199	198	5	9	6.8	6911	PASS
275	198	10	60	28.9	29296	PASS
365	198	1	100	3.7	3794	PASS
441	198	0.01	100	11.9	12026	PASS
442	198	50	100	79.3	80434	PASS
443	442	15	24	19.4	15614	PASS