


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM061920\
 Data File : BM026472.D
 Acq On : 19 Jun 2020 18:27
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM060520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 19 10:20:20 2020

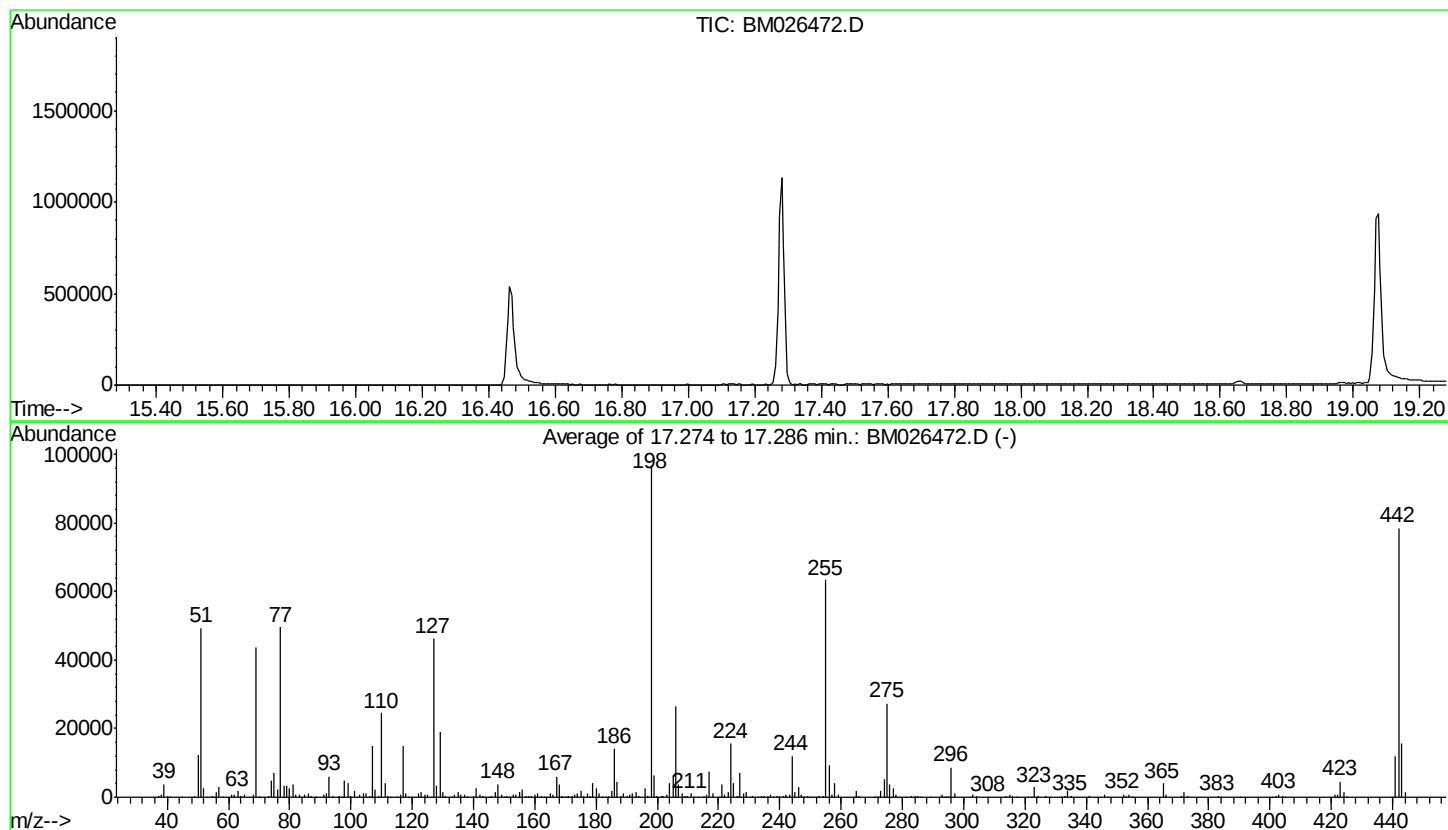

AutoFind: Scans 2446, 2447, 2448; Background Corrected with Scan 2439

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.0	49330	PASS
68	69	0.00	2	1.8	768	PASS
69	198	0.00	100	45.2	43661	PASS
70	69	0.00	2	0.2	101	PASS
127	198	10	80	47.9	46274	PASS
197	198	0.00	2	0.4	368	PASS
198	198	100	100	100.0	96685	PASS
199	198	5	9	6.8	6542	PASS
275	198	10	60	28.2	27264	PASS
365	198	1	100	4.2	4037	PASS
441	198	0.01	100	12.2	11804	PASS
442	198	50	100	81.2	78533	PASS
443	442	15	24	20.1	15761	PASS