

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
 Data File : BM035538.D
 Acq On : 20 Jun 2022 17:16
 Operator : CG/JU
 Sample : N3226-18
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4N8

Quant Time: Jun 21 01:29:01 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.829	152	5194	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.616	136	17061	0.400	ng/ul	-0.03
9) Acenaphthene-d10	14.459	164	9878	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.208	188	20920	0.400	ng/ul	-0.02
17) Chrysene-d12	21.409	240	13467	0.400	ng/ul	0.00
23) Perylene-d12	23.742	264	13915	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.268	96	18091	2.475	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.250	152	3727	0.147	ng/ul	0.00
18) Fluoranthene-d10	19.243	212	8086	0.179	ng/ul	-0.01
Target Compounds						
26) Benzo(a)pyrene	23.575	252	2284	0.036	ng/ul#	Qvalue 12


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
Data File : BM035538.D
Acq On : 20 Jun 2022 17:16
Operator : CG/JU
Sample : N3226-18
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4N8


Quant Time: Jun 21 01:29:01 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

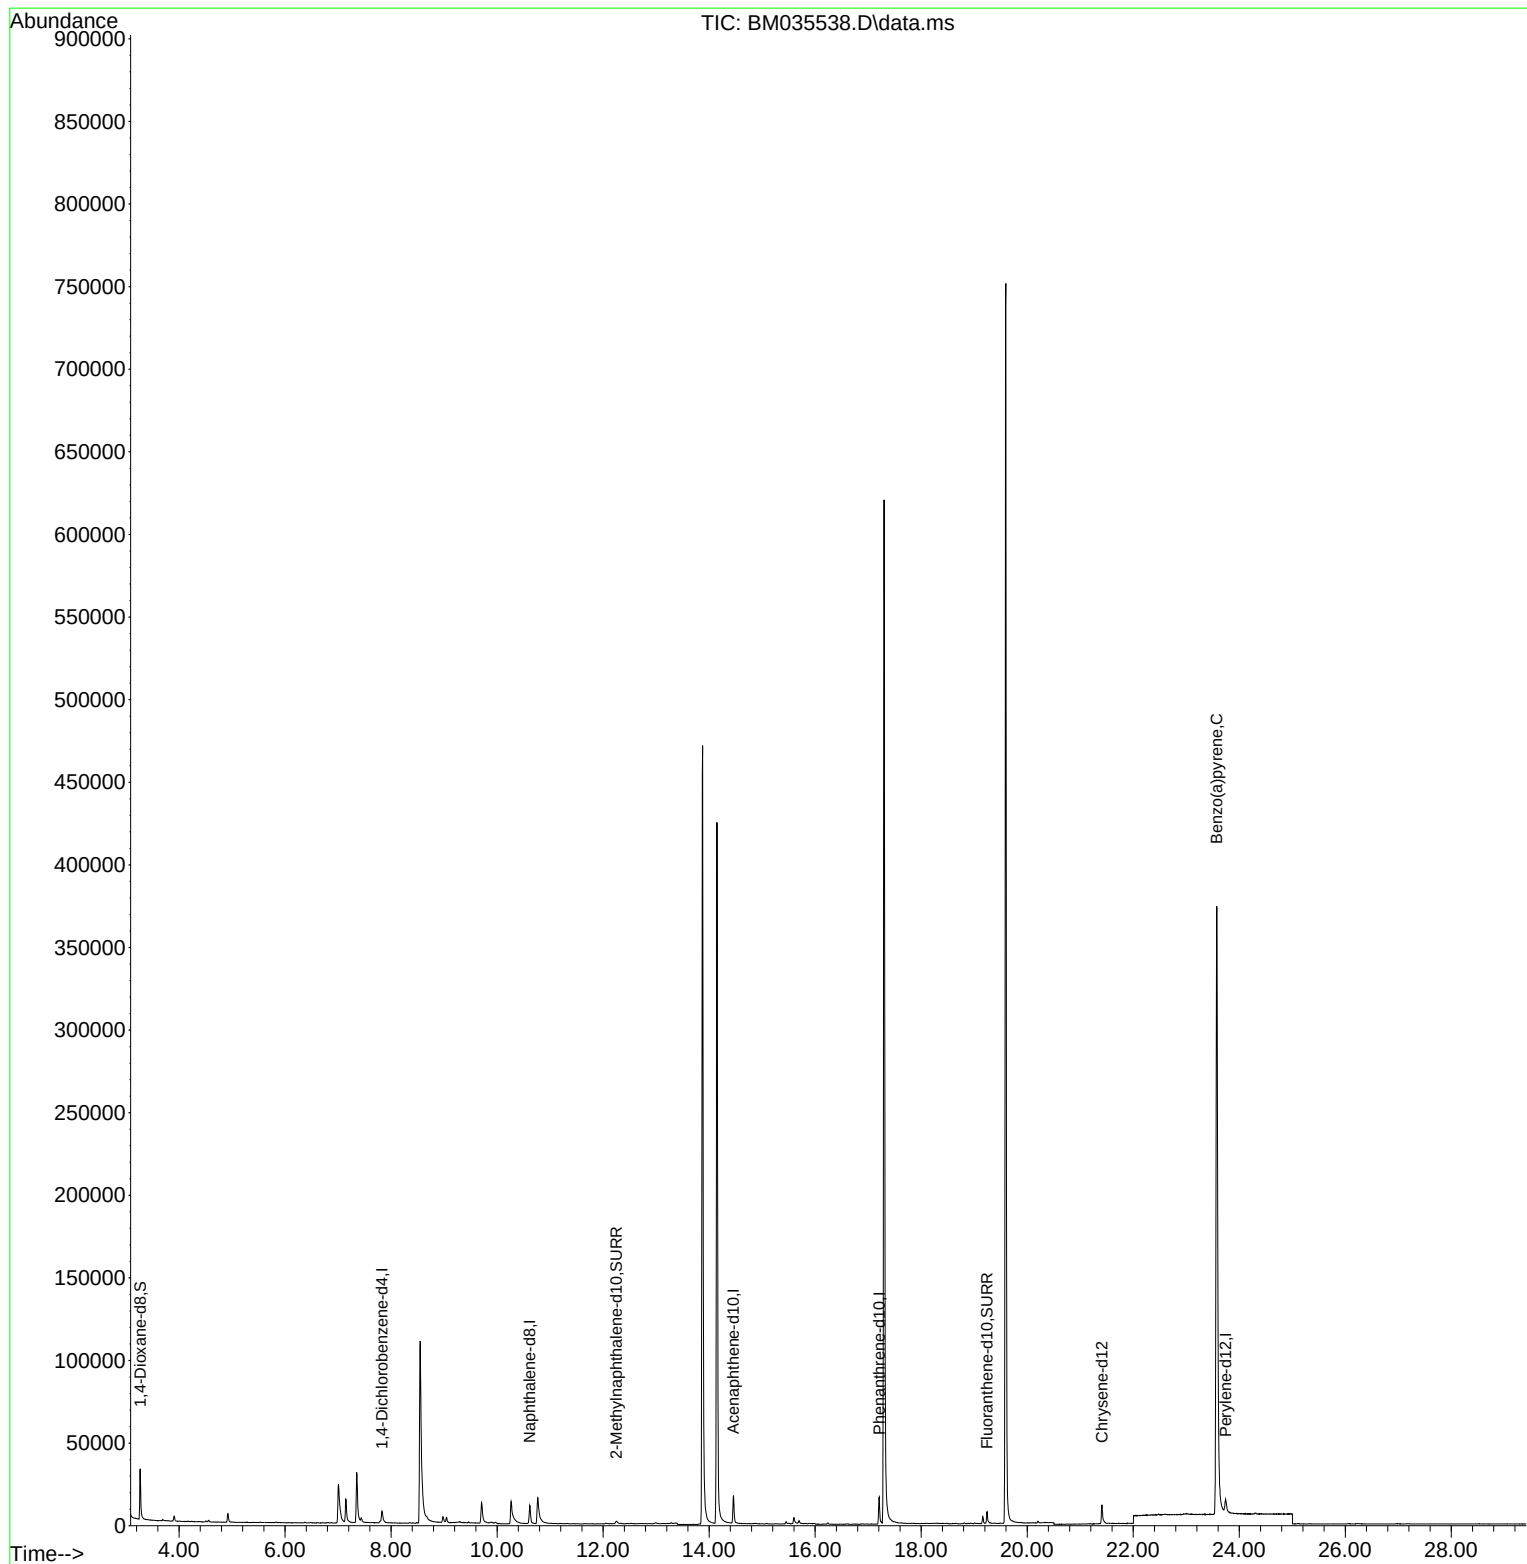

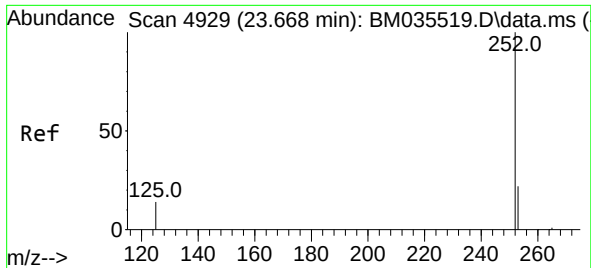

#26
Benzo(a)pyrene
Concen: 0.036 ng/ul
RT: 23.575 min Scan# 41
Delta R.T. -0.093 min
Lab File: BM035538.D
Acq: 20 Jun 2022 17:16

Instrument :
BNA_M
ClientSampleId :
EW4N8

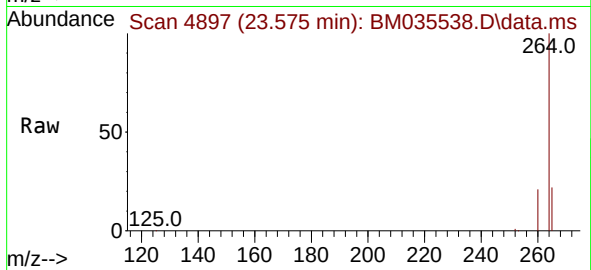

Tgt Ion:252 Resp: 2284
Ion Ratio Lower Upper
252 100
253 80.9 27.8 41.6#
125 81.1 23.3 34.9#

