

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
 Data File : BM035540.D
 Acq On : 20 Jun 2022 18:29
 Operator : CG/JU
 Sample : N3226-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4L6

Quant Time: Jun 21 01:29:08 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.829	152	5302	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.611	136	18415	0.400	ng/ul	-0.03
9) Acenaphthene-d10	14.459	164	11047	0.400	ng/ul	-0.01
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-17.23
17) Chrysene-d12	21.409	240	13802	0.400	ng/ul	0.00
23) Perylene-d12	23.745	264	14434	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	38166	5.116	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.244	152	9785	0.358	ng/ul	0.00
18) Fluoranthene-d10	19.243	212	19148	0.413	ng/ul	-0.01
Target Compounds						
					Qvalue	
7) 2-Methylnaphthalene	12.321	142	808	0.023	ng/ul	96
19) Fluoranthene	19.271	202	3913	0.055	ng/ul#	69
20) Pyrene	19.624	202	3476	0.047	ng/ul#	67
21) Benzo(a)anthracene	21.400	228	1562	0.030	ng/ul#	79
22) Chrysene	21.450	228	1943	0.031	ng/ul#	86
24) Benzo(b)fluoranthene	23.034	252	2290	0.036	ng/ul#	1
26) Benzo(a)pyrene	23.572	252	5861	0.089	ng/ul#	52
29) Benzo(g,h,i)perylene	26.970	276	1442	0.021	ng/ul#	31


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
Data File : BM035540.D
Acq On : 20 Jun 2022 18:29
Operator : CG/JU
Sample : N3226-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4L6

Quant Time: Jun 21 01:29:08 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration




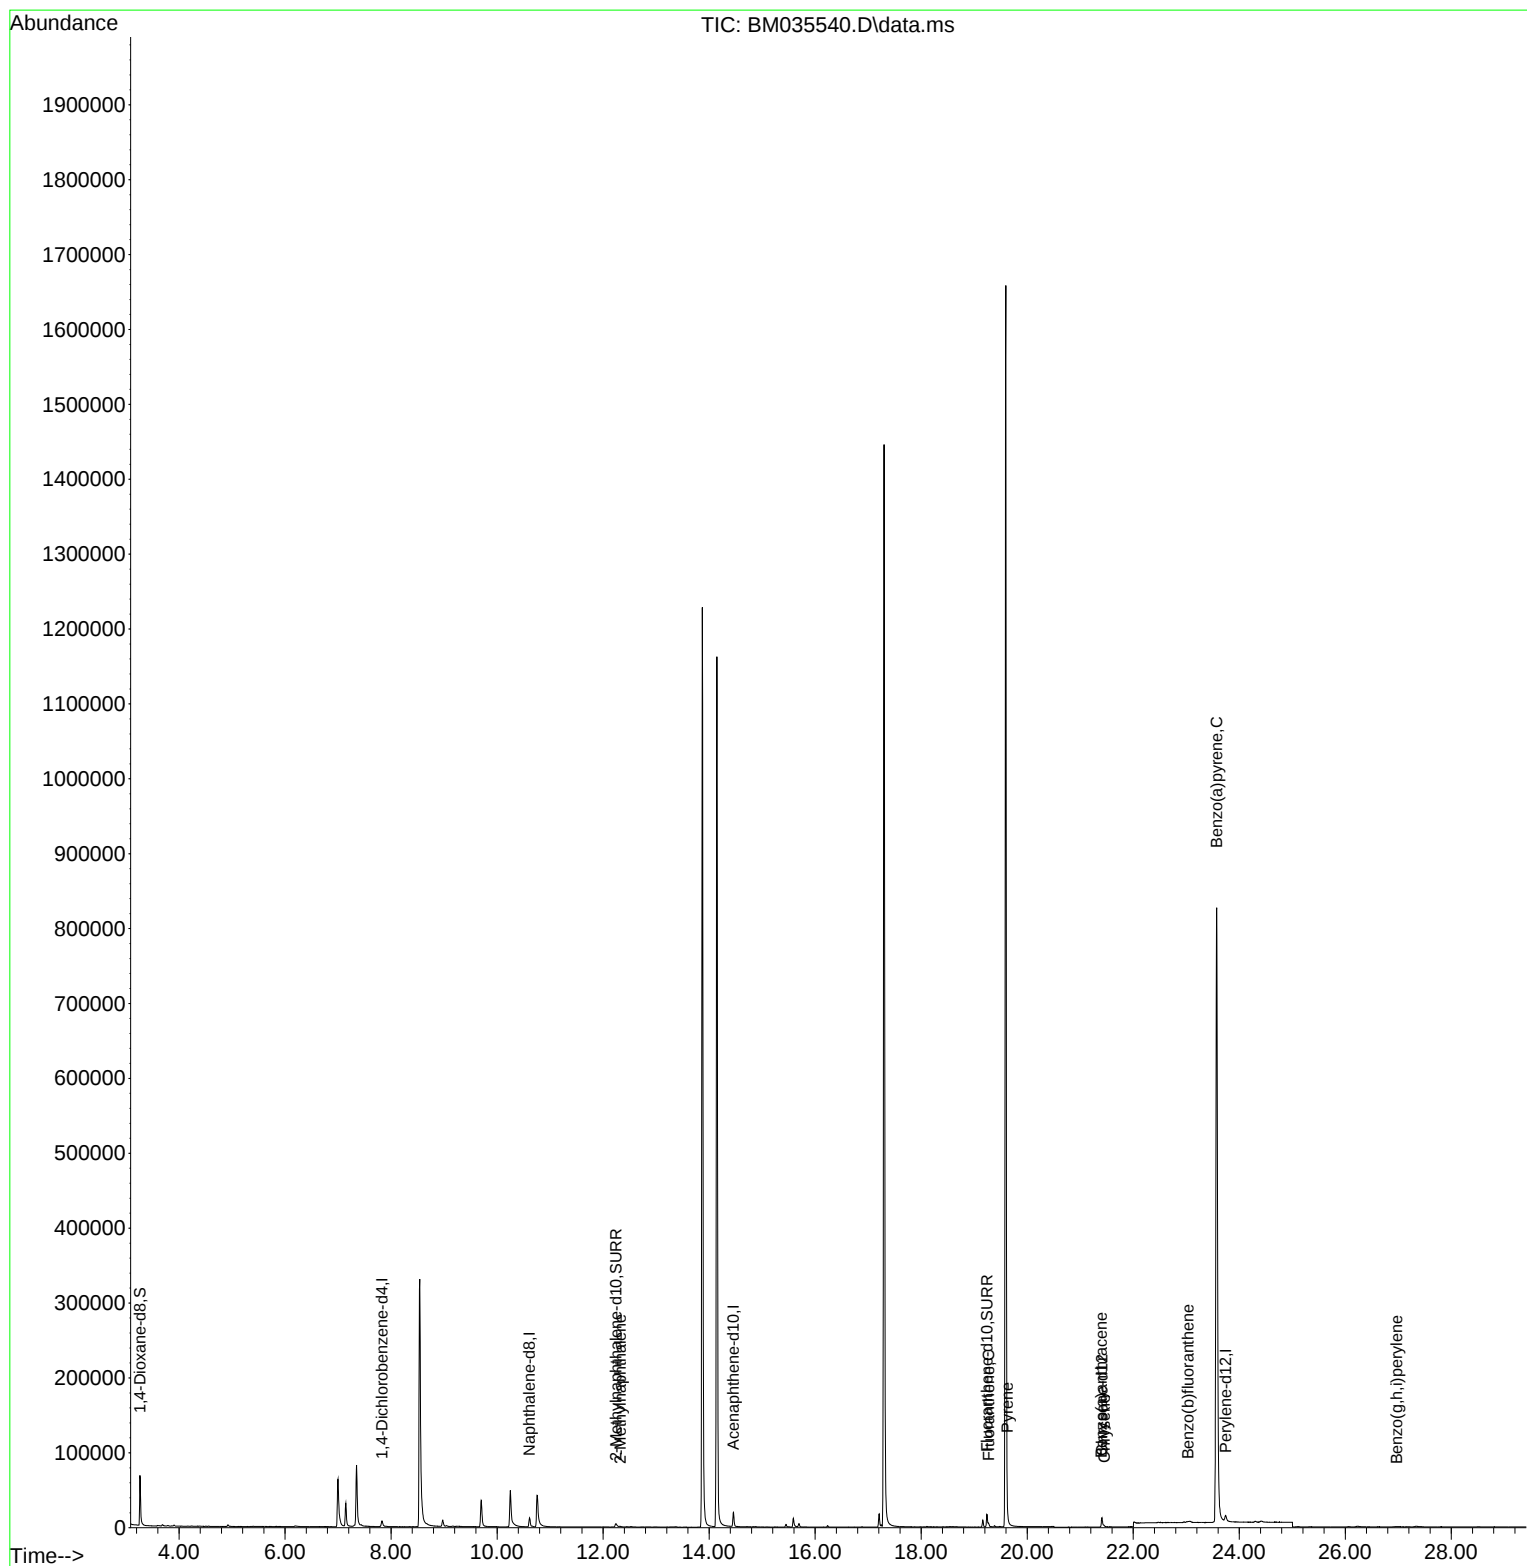


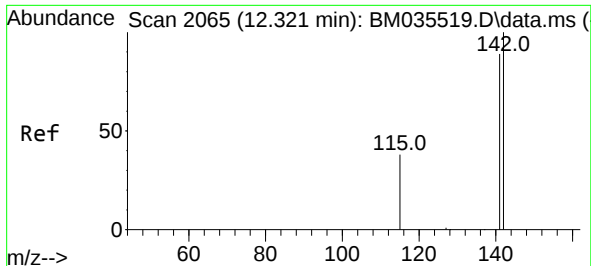

#7
2-Methylnaphthalene
Concen: 0.023 ng/ul
RT: 12.321 min Scan# 2065
Delta R.T. -0.000 min
Lab File: BM035540.D
Acq: 20 Jun 2022 18:29




Instrument :
BNA_M
ClientSampleId :
EW4L6


Tgt Ion:142 Resp: 808
Ion Ratio Lower Upper
142 100
141 96.2 73.8 110.8

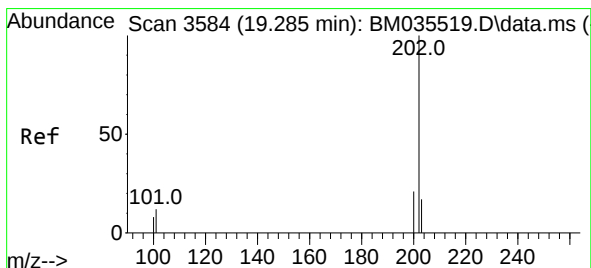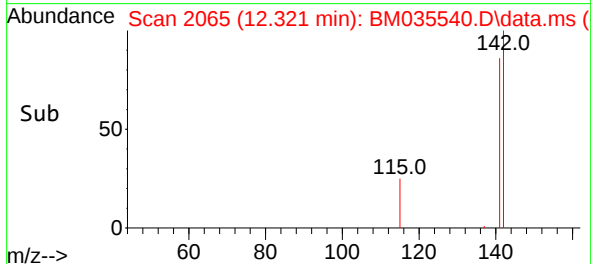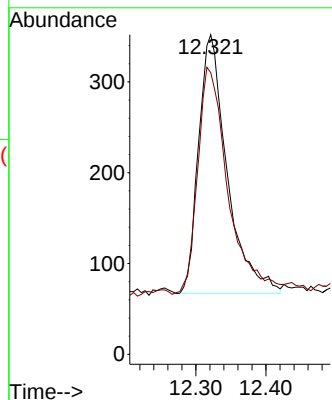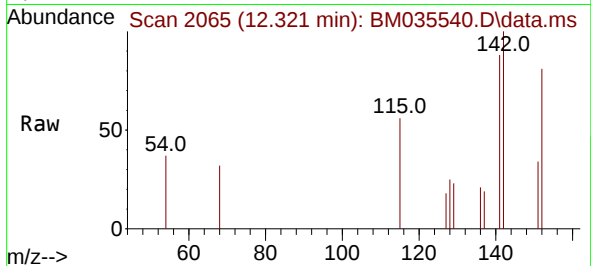

#19
Fluoranthene
Concen: 0.055 ng/ul
RT: 19.271 min Scan# 3581
Delta R.T. -0.015 min
Lab File: BM035540.D
Acq: 20 Jun 2022 18:29

Tgt Ion:202 Resp: 3913
Ion Ratio Lower Upper
202 100
101 25.7 10.0 15.0#
100 19.7 7.5 11.3#


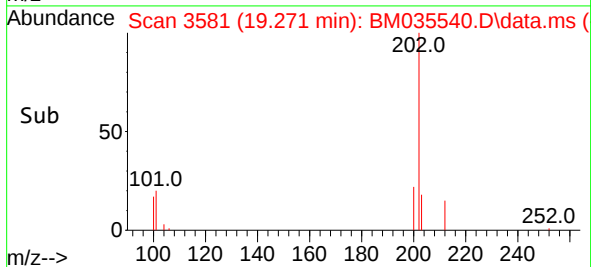
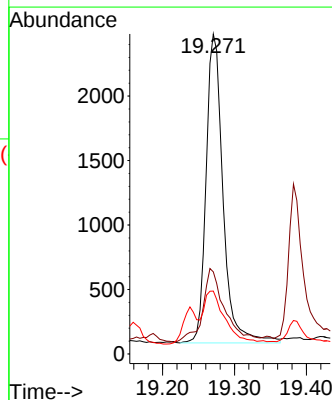
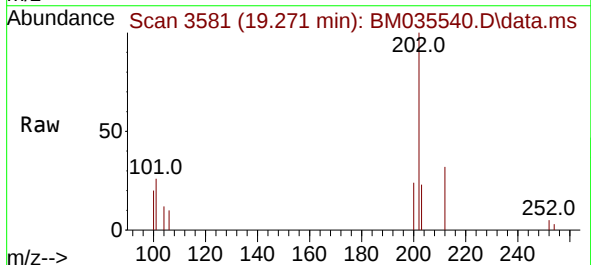


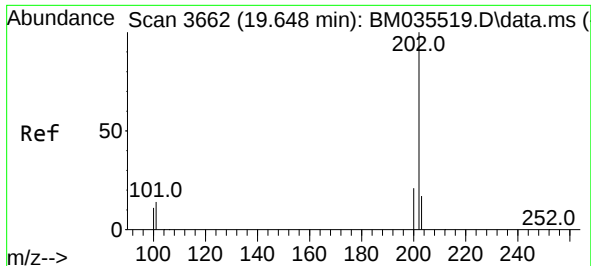

#20
Pyrene
Concen: 0.047 ng/ul
RT: 19.624 min Scan# 3657
Delta R.T. -0.024 min
Lab File: BM035540.D
Acq: 20 Jun 2022 18:29




Instrument :
BNA_M
ClientSampleId :
EW4L6


Tgt Ion:202 Resp: 3476
Ion Ratio Lower Upper
202 100
101 21.0 11.6 17.4#
100 32.6 9.3 13.9#

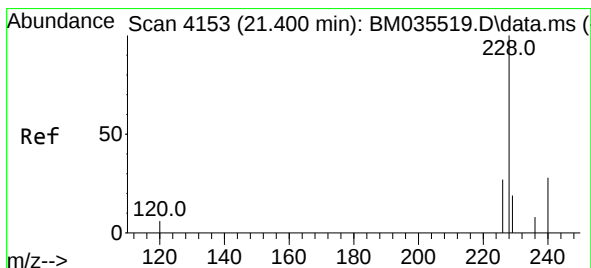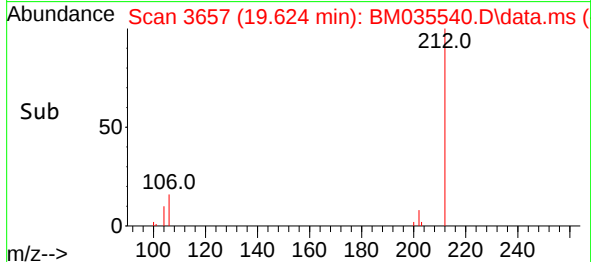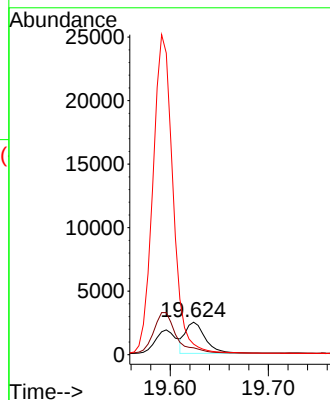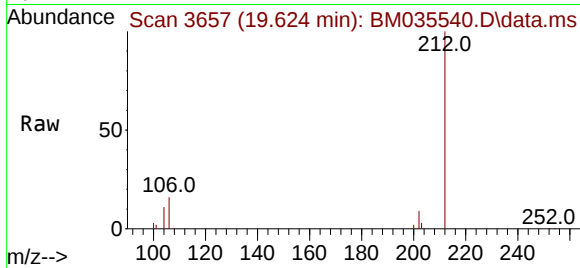

#21
Benzo(a)anthracene
Concen: 0.030 ng/ul
RT: 21.400 min Scan# 4153
Delta R.T. 0.001 min
Lab File: BM035540.D
Acq: 20 Jun 2022 18:29

Tgt Ion:228 Resp: 1562
Ion Ratio Lower Upper
228 100
229 33.0 16.2 24.2#
226 36.2 22.3 33.5#

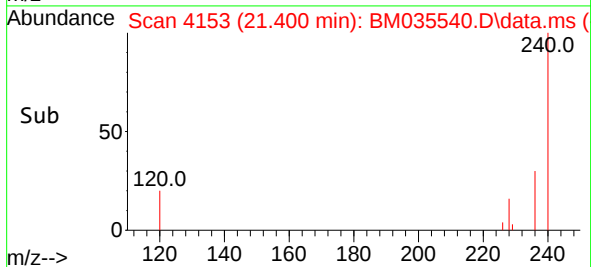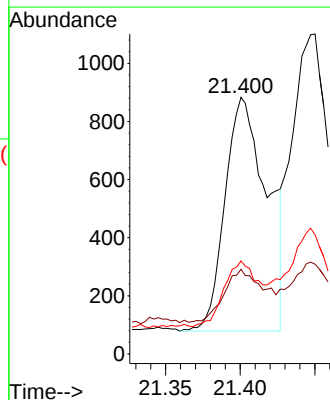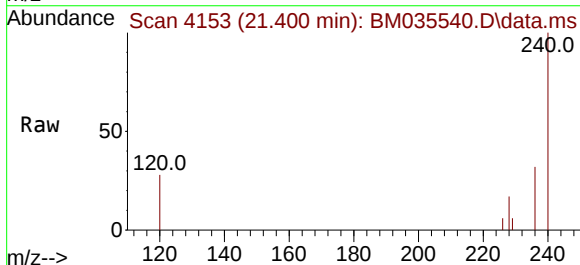

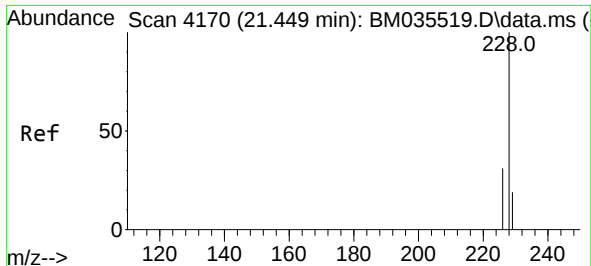

#22

Chrysene

Concen: 0.031 ng/ul

RT: 21.450 min Scan# 4170

Delta R.T. 0.001 min

Lab File: BM035540.D

Acq: 20 Jun 2022 18:29

Instrument :

BNA_M

ClientSampleId :

EW4L6





Tgt Ion:228 Resp: 1943

Ion Ratio Lower Upper

228 100

226 37.2 24.5 36.7#

229 28.1 15.8 23.8#

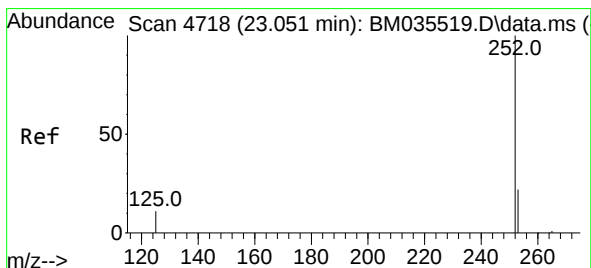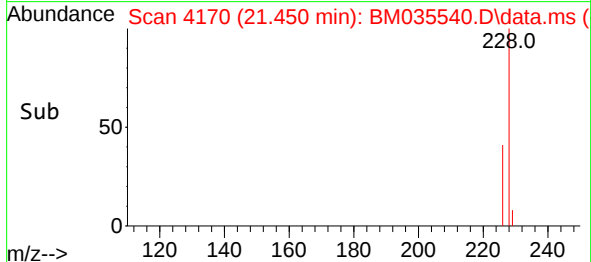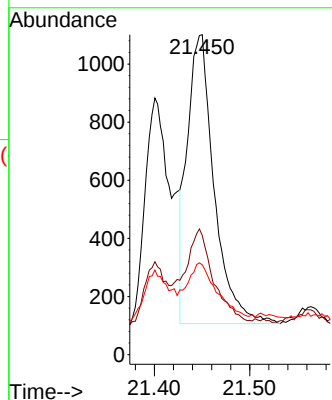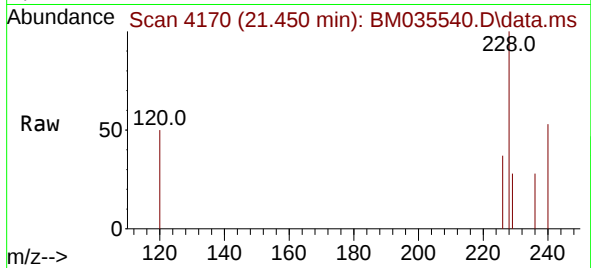

#24

Benzo(b)fluoranthene

Concen: 0.036 ng/ul

RT: 23.034 min Scan# 4712

Delta R.T. -0.017 min

Lab File: BM035540.D

Acq: 20 Jun 2022 18:29




Tgt Ion:252 Resp: 2290


Ion Ratio Lower Upper

252 100

253 75.0 0.0 60.6#

125 88.2 0.0 44.8#


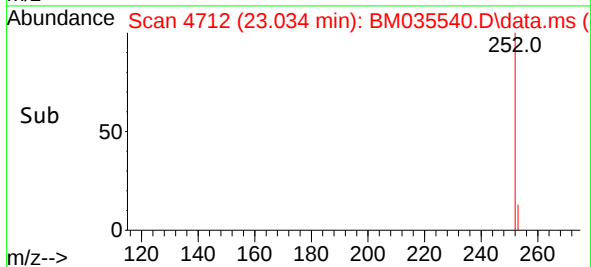
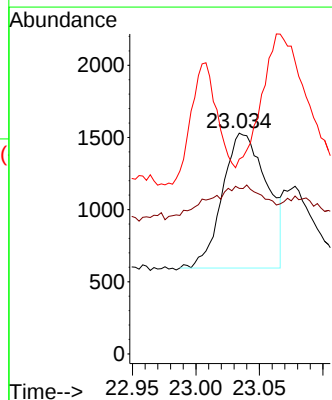
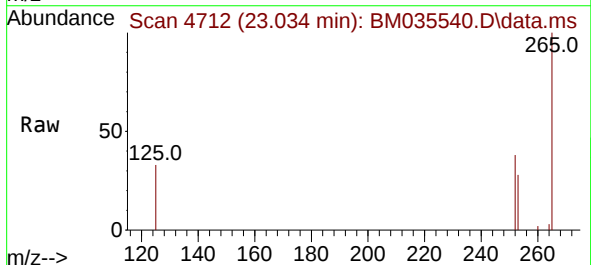


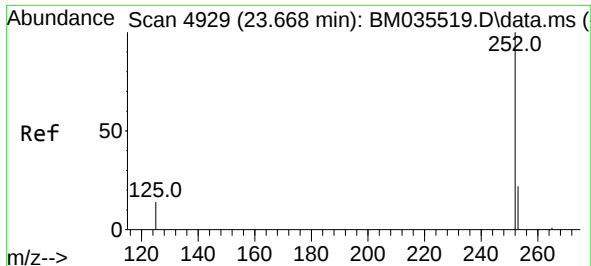

#26
Benzo(a)pyrene
Concen: 0.089 ng/ul
RT: 23.572 min Scan# 4896
Delta R.T. -0.096 min
Lab File: BM035540.D
Acq: 20 Jun 2022 18:29

Instrument :
BNA_M
ClientSampleId :
EW4L6

Tgt Ion:252 Resp: 5861
Ion Ratio Lower Upper
252 100
253 57.4 27.8 41.6#
125 60.0 23.3 34.9#

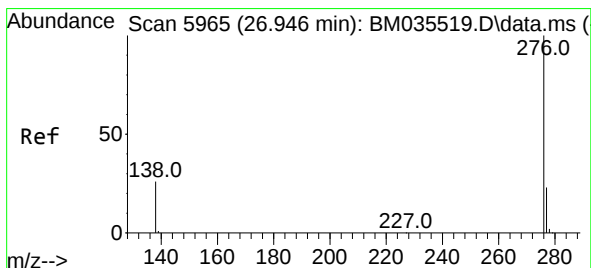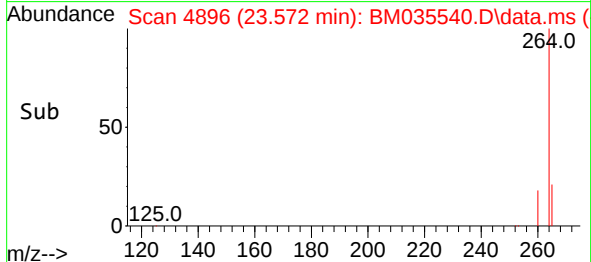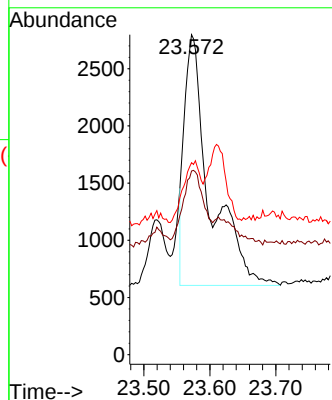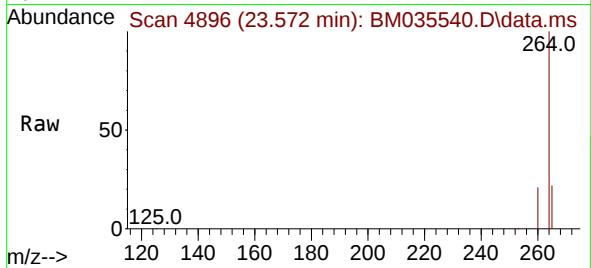

#29
Benzo(g,h,i)perylene
Concen: 0.021 ng/ul
RT: 26.970 min Scan# 5972
Delta R.T. 0.024 min
Lab File: BM035540.D
Acq: 20 Jun 2022 18:29

Tgt Ion:276 Resp: 1442
Ion Ratio Lower Upper
276 100
138 72.2 23.1 34.7#
277 53.2 20.3 30.5#

