

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
 Data File : BM035545.D
 Acq On : 20 Jun 2022 22:07
 Operator : CG/JU
 Sample : N3226-17
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4N7

Quant Time: Jun 21 01:29:26 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.833	152	4709	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.628	136	14610	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.460	164	8109	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.208	188	16221	0.400	ng/ul	-0.02
17) Chrysene-d12	21.421	240	11582	0.400	ng/ul	0.00
23) Perylene-d12	23.748	264	12304	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.268	96	10528	1.589	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.272	152	2085	0.096	ng/ul	0.03
18) Fluoranthene-d10	19.243	212	5067	0.130	ng/ul	0.00
Target Compounds						
26) Benzo(a)pyrene	23.575	252	1598	0.029	ng/ul#	Qvalue 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
Data File : BM035545.D
Acq On : 20 Jun 2022 22:07
Operator : CG/JU
Sample : N3226-17
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4N7


Quant Time: Jun 21 01:29:26 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

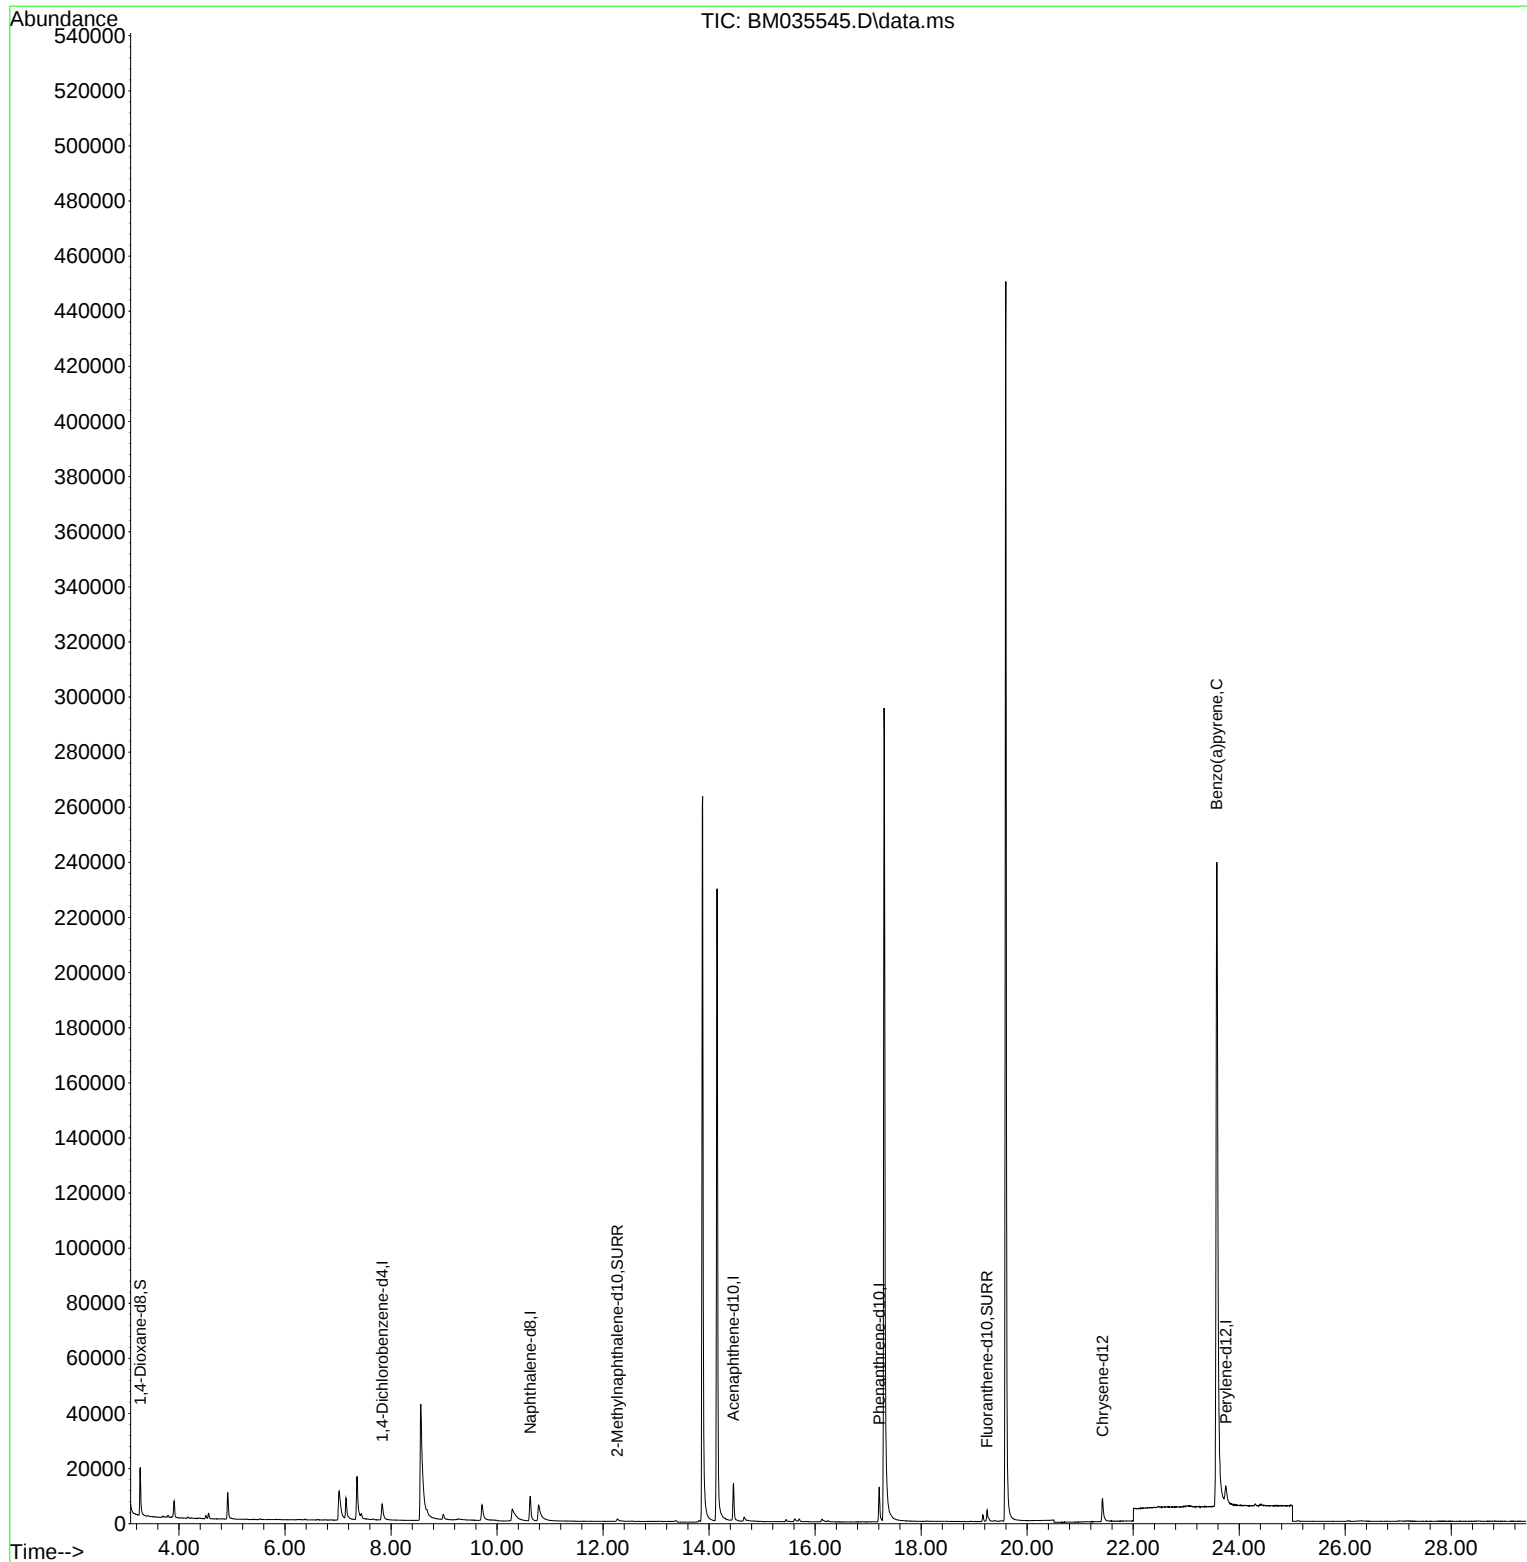

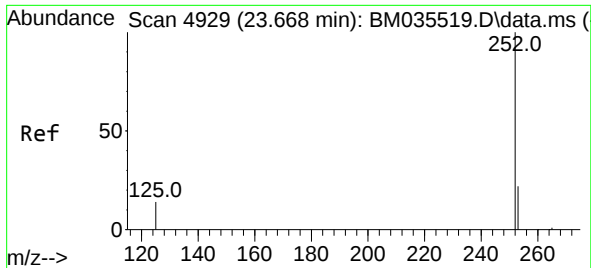

#26
Benzo(a)pyrene
Concen: 0.029 ng/ul
RT: 23.575 min Scan# 41
Delta R.T. -0.092 min
Lab File: BM035545.D
Acq: 20 Jun 2022 22:07

Instrument :
BNA_M
ClientSampleId :
EW4N7

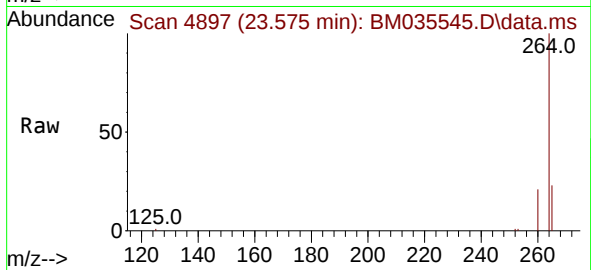

Tgt Ion:252 Resp: 1598
Ion Ratio Lower Upper
252 100
253 87.1 27.8 41.6#
125 91.1 23.3 34.9#

