

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
 Data File : BM035564.D
 Acq On : 21 Jun 2022 10:07
 Operator : CG/JU
 Sample : N3285-09
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4Q3

Quant Time: Jun 22 01:32:08 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.820	152	5455	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.611	136	18737	0.400	ng/ul	#-0.03
9) Acenaphthene-d10	14.456	164	11499	0.400	ng/ul	-0.01
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-17.23
17) Chrysene-d12	21.405	240	16539	0.400	ng/ul	0.00
23) Perylene-d12	23.735	264	20721	0.400	ng/ul	#-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	34399	4.482	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.233	152	10946	0.393	ng/ul	-0.01
18) Fluoranthene-d10	19.234	212	22830	0.411	ng/ul	-0.02
Target Compounds						
					Qvalue	
20) Pyrene	19.592	202	3331	0.038	ng/ul#	1
26) Benzo(a)pyrene	23.571	252	6719	0.071	ng/ul#	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
Data File : BM035564.D
Acq On : 21 Jun 2022 10:07
Operator : CG/JU
Sample : N3285-09
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4Q3

Quant Time: Jun 22 01:32:08 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration




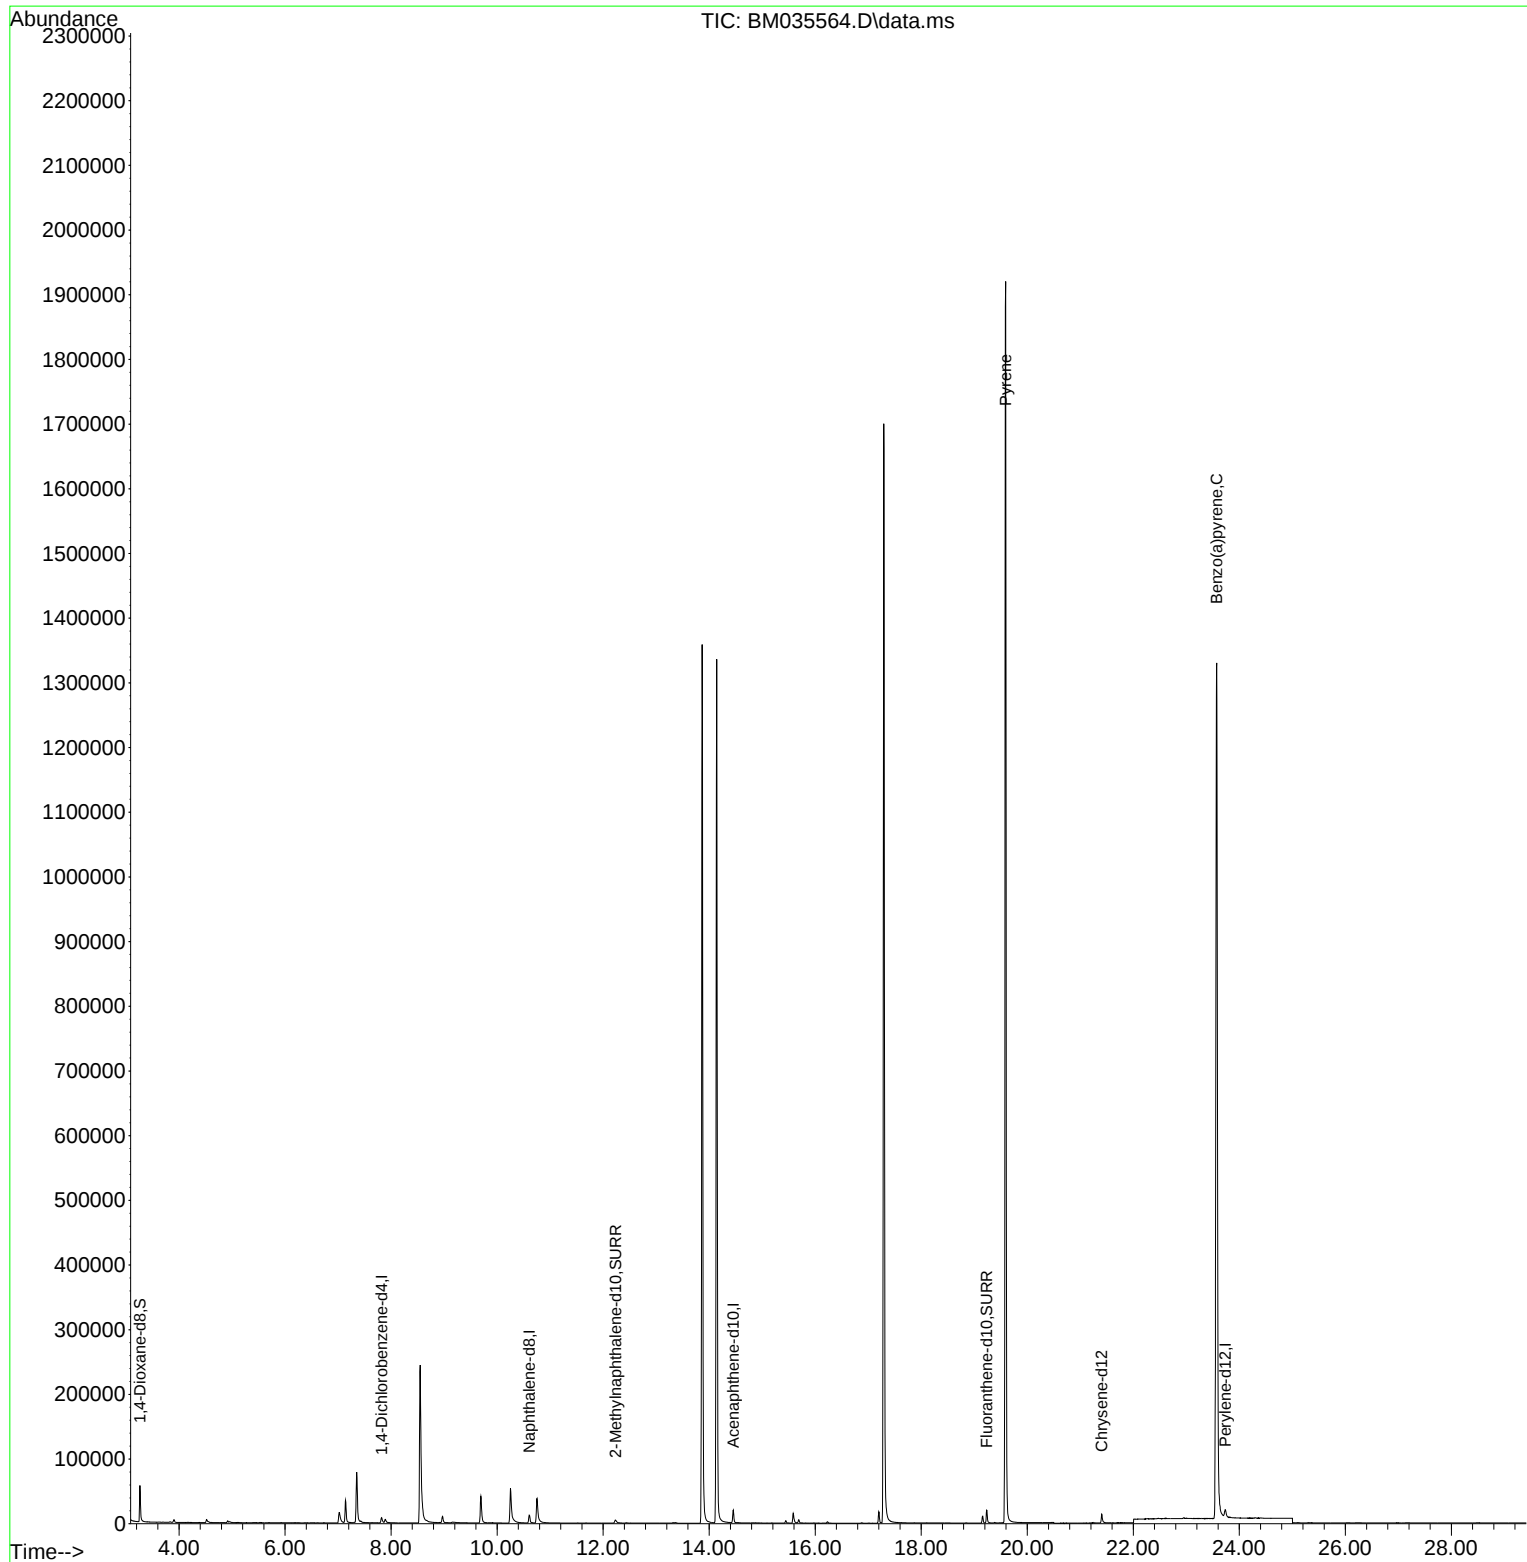


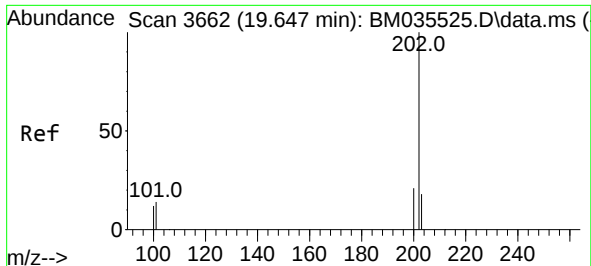

#20
Pyrene
Concen: 0.038 ng/ul
RT: 19.592 min Scan# 3
Delta R.T. -0.056 min
Lab File: BM035564.D
Acq: 21 Jun 2022 10:07

Instrument :
BNA_M
ClientSampleId :
EW4Q3

Tgt Ion:202 Resp: 3331
Ion Ratio Lower Upper
202 100
101 155.3 11.6 17.4#
100 1048.0 9.3 13.9#

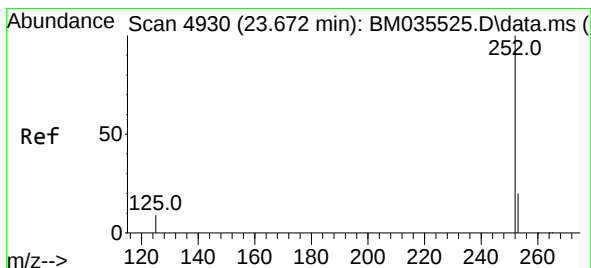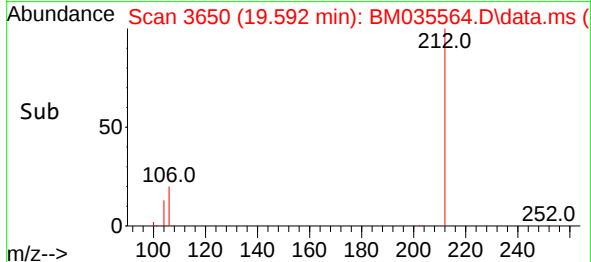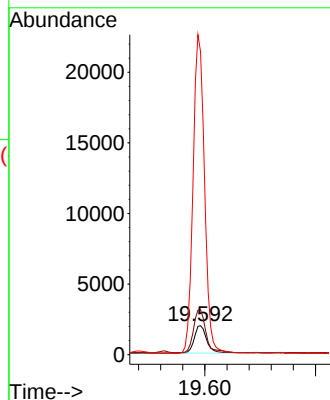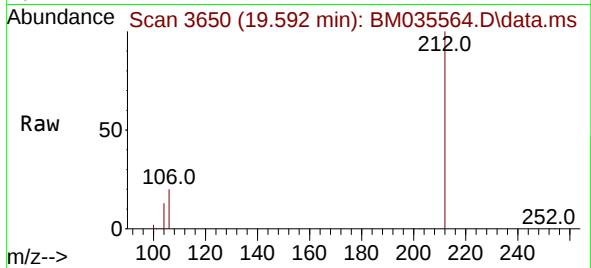

#26
Benzo(a)pyrene
Concen: 0.071 ng/ul
RT: 23.571 min Scan# 4896
Delta R.T. -0.097 min
Lab File: BM035564.D
Acq: 21 Jun 2022 10:07

Tgt Ion:252 Resp: 6719
Ion Ratio Lower Upper
252 100
253 52.2 27.8 41.6#
125 49.3 23.3 34.9#

