

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
 Data File : BM035568.D
 Acq On : 21 Jun 2022 12:31
 Operator : CG/JU
 Sample : N3285-11
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4Q4

Quant Time: Jun 22 01:32:24 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.820	152	5382	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.611	136	19009	0.400	ng/ul	#-0.03
9) Acenaphthene-d10	14.455	164	10769	0.400	ng/ul	-0.01
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-17.23
17) Chrysene-d12	21.402	240	17157	0.400	ng/ul	0.00
23) Perylene-d12	23.735	264	20964	0.400	ng/ul	#-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	31569	4.169	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.233	152	8288	0.293	ng/ul	-0.01
18) Fluoranthene-d10	19.234	212	19514	0.339	ng/ul	-0.02
Target Compounds						
					Qvalue	
20) Pyrene	19.592	202	2899	0.032	ng/ul#	1
26) Benzo(a)pyrene	23.571	252	5969	0.063	ng/ul#	60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
Data File : BM035568.D
Acq On : 21 Jun 2022 12:31
Operator : CG/JU
Sample : N3285-11
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4Q4

Quant Time: Jun 22 01:32:24 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration




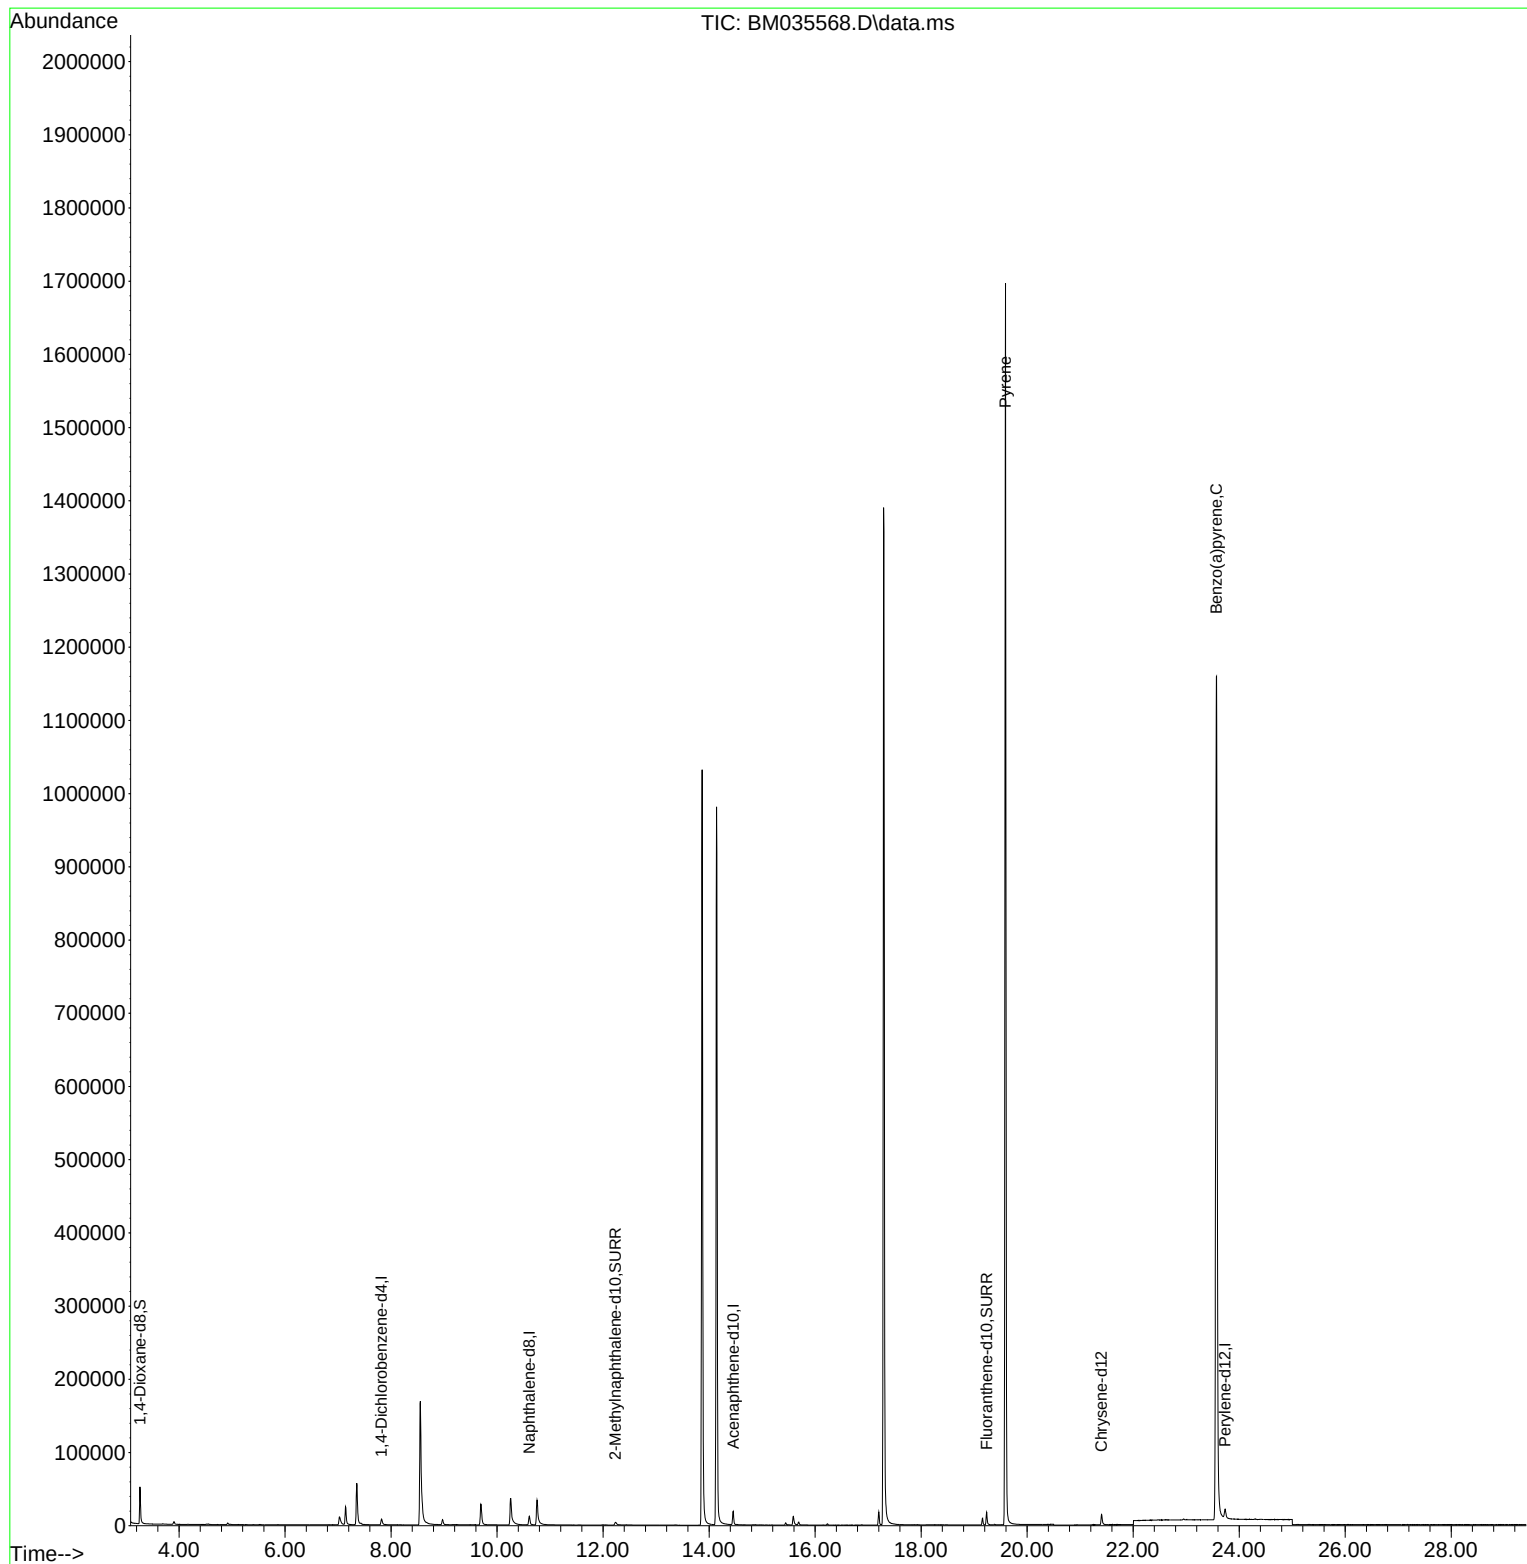


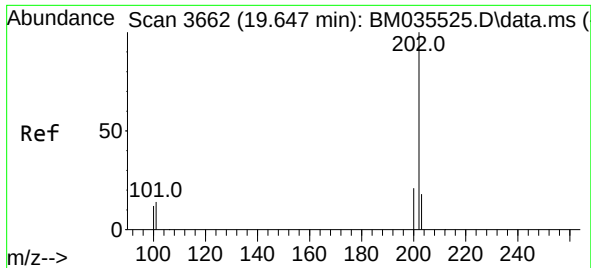

#20
Pyrene
Concen: 0.032 ng/u1
RT: 19.592 min Scan# 3
Delta R.T. -0.056 min
Lab File: BM035568.D
Acq: 21 Jun 2022 12:31

Instrument :
BNA_M
ClientSampleId :
EW4Q4

Tgt Ion:202 Resp: 2899
Ion Ratio Lower Upper
202 100
101 147.6 11.6 17.4#
100 976.5 9.3 13.9#

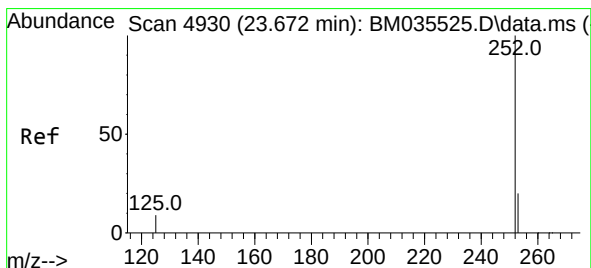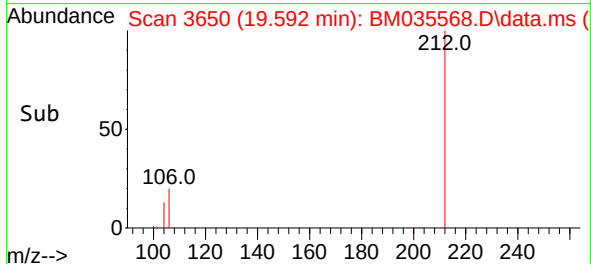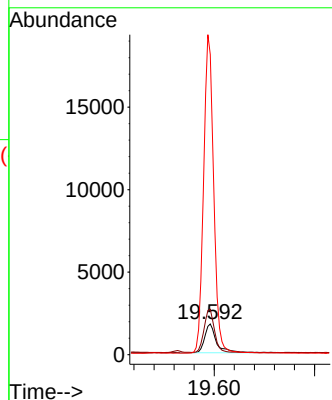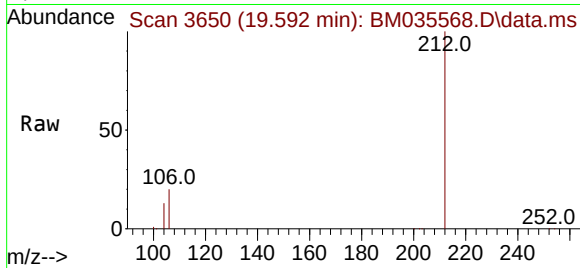

#26
Benzo(a)pyrene
Concen: 0.063 ng/u1
RT: 23.571 min Scan# 4896
Delta R.T. -0.097 min
Lab File: BM035568.D
Acq: 21 Jun 2022 12:31

Tgt Ion:252 Resp: 5969
Ion Ratio Lower Upper
252 100
253 55.4 27.8 41.6#
125 53.1 23.3 34.9#

