

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
 Data File : BM035569.D
 Acq On : 21 Jun 2022 13:07
 Operator : CG/JU
 Sample : N3285-12
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4Q5

Quant Time: Jun 22 01:32:27 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.825	152	5253	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.611	136	19480	0.400	ng/ul	#-0.03
9) Acenaphthene-d10	14.456	164	10444	0.400	ng/ul	-0.01
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-17.23
17) Chrysene-d12	21.406	240	16401	0.400	ng/ul	0.00
23) Perylene-d12	23.735	264	19877	0.400	ng/ul	#-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	30473	4.123	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.233	152	9714	0.336	ng/ul	-0.01
18) Fluoranthene-d10	19.234	212	20633	0.374	ng/ul	-0.02
Target Compounds						
					Qvalue	
20) Pyrene	19.592	202	3057	0.035	ng/ul#	1
26) Benzo(a)pyrene	23.571	252	6186	0.069	ng/ul#	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
Data File : BM035569.D
Acq On : 21 Jun 2022 13:07
Operator : CG/JU
Sample : N3285-12
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4Q5

Quant Time: Jun 22 01:32:27 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration




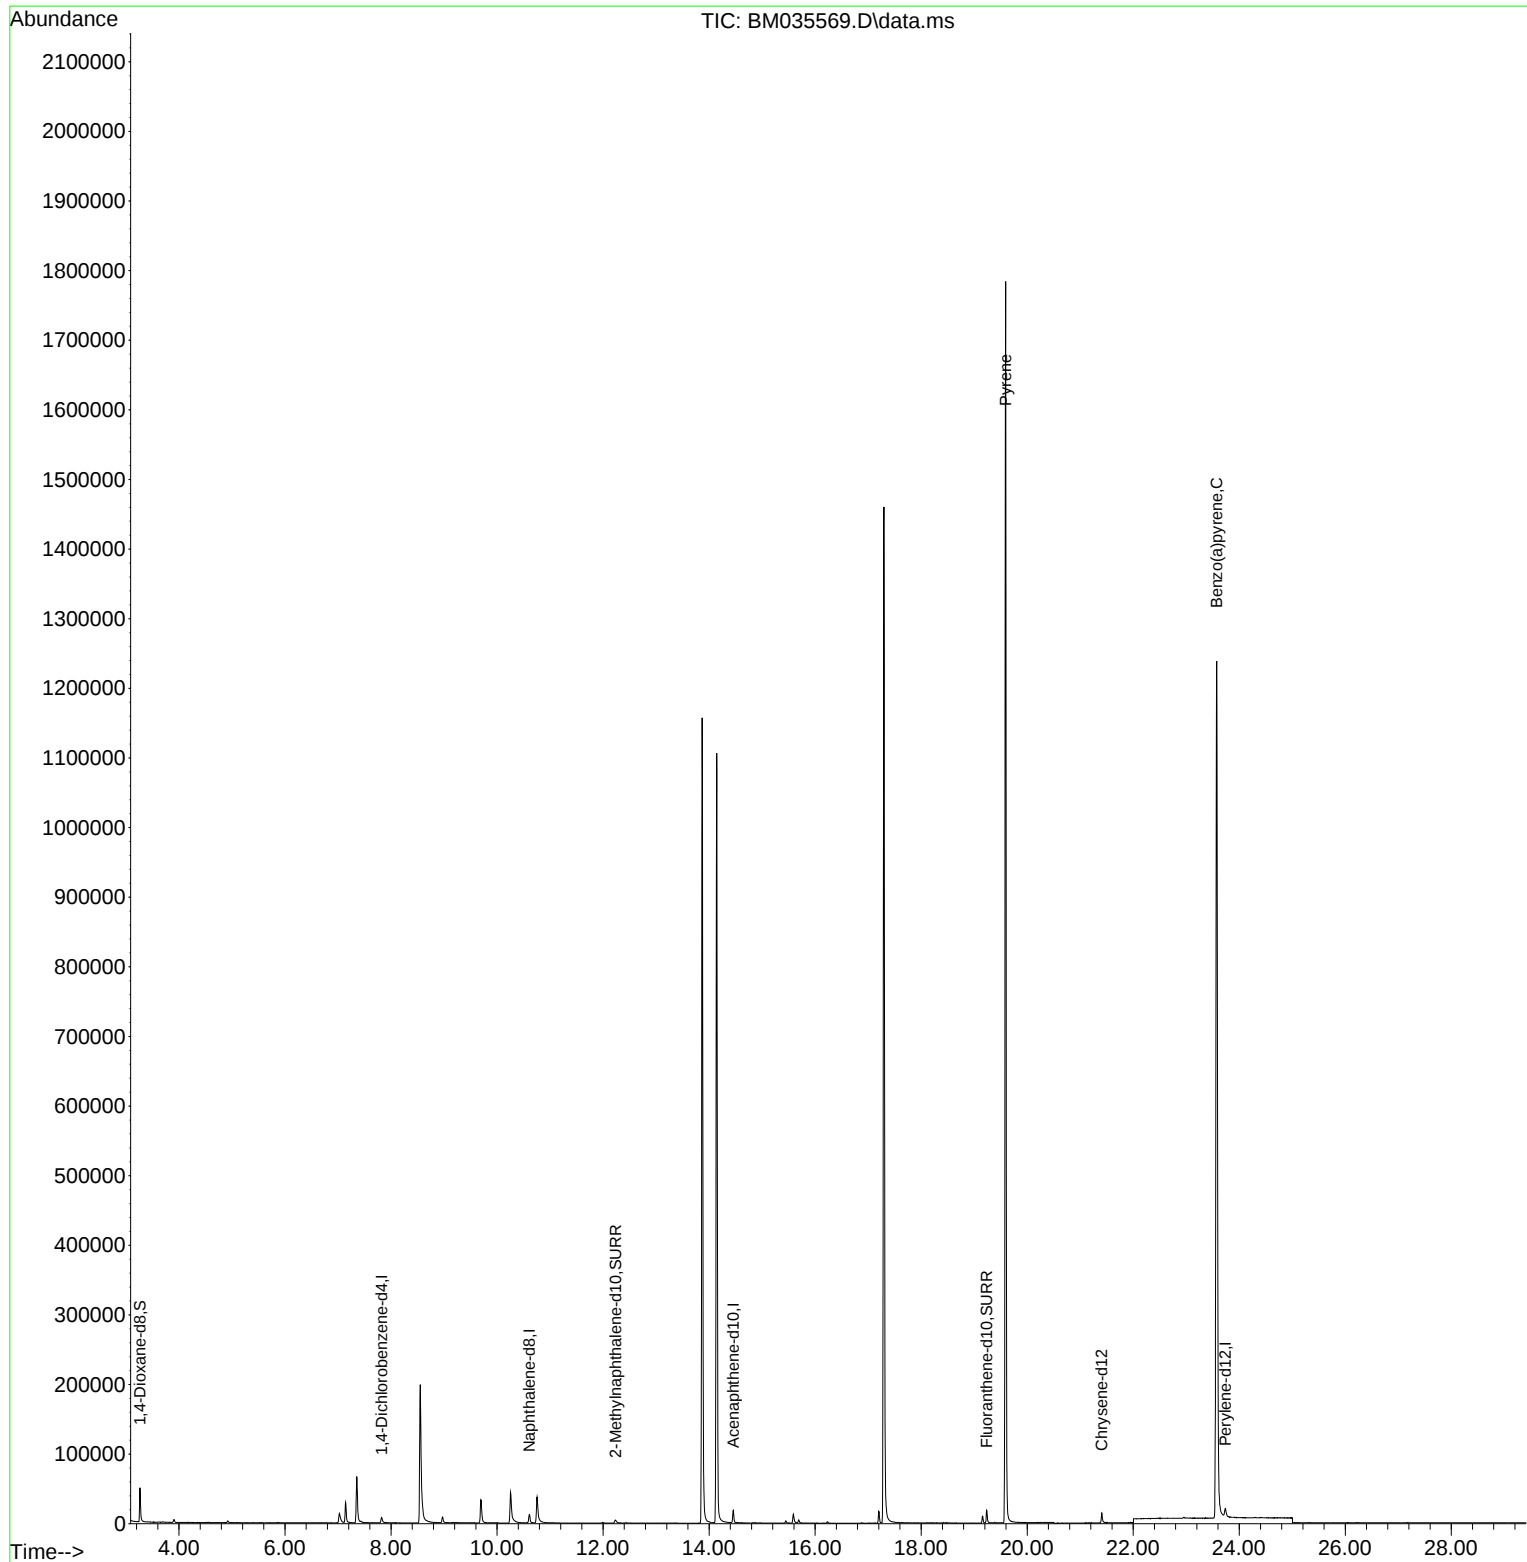


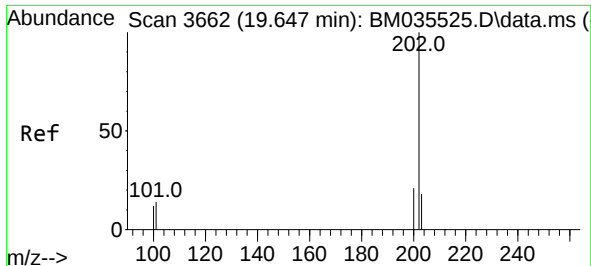

#20
Pyrene
Concen: 0.035 ng/ul
RT: 19.592 min Scan# 3057
Delta R.T. -0.056 min
Lab File: BM035569.D
Acq: 21 Jun 2022 13:07

Instrument :
BNA_M
ClientSampleId :
EW4Q5

Tgt Ion:202 Resp: 3057
Ion Ratio Lower Upper
202 100
101 151.6 11.6 17.4#
100 1039.0 9.3 13.9#

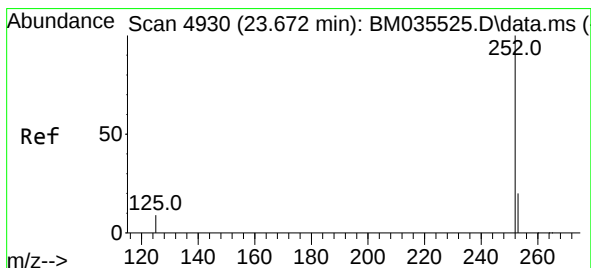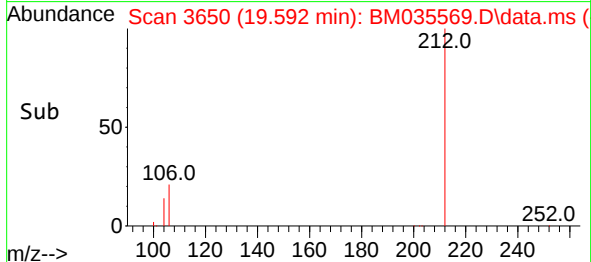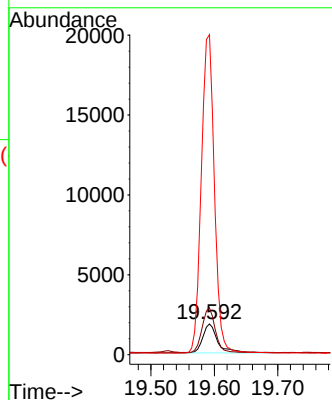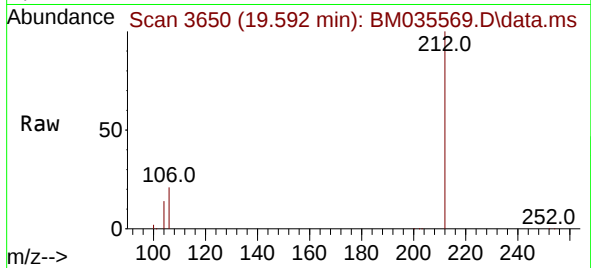

#26
Benzo(a)pyrene
Concen: 0.069 ng/ul
RT: 23.571 min Scan# 4896
Delta R.T. -0.096 min
Lab File: BM035569.D
Acq: 21 Jun 2022 13:07

Tgt Ion:252 Resp: 6186
Ion Ratio Lower Upper
252 100
253 52.3 27.8 41.6#
125 51.1 23.3 34.9#

