

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
 Data File : BM035579.D
 Acq On : 21 Jun 2022 19:48
 Operator : CG/JU
 Sample : PB145592BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK592

Quant Time: Jun 22 01:33:12 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.825	152	5725	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.611	136	19741	0.400	ng/ul	-0.03
9) Acenaphthene-d10	14.455	164	11843	0.400	ng/ul	-0.01
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-17.23
17) Chrysene-d12	21.415	240	16392	0.400	ng/ul	0.00
23) Perylene-d12	23.733	264	18162	0.400	ng/ul	#-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	38163	4.738	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.250	152	8181	0.279	ng/ul	0.00
18) Fluoranthene-d10	19.238	212	17589	0.319	ng/ul	-0.01
Target Compounds						
					Qvalue	
20) Pyrene	19.591	202	2779	0.032	ng/ul#	1
26) Benzo(a)pyrene	23.566	252	3989	0.048	ng/ul#	49


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
Data File : BM035579.D
Acq On : 21 Jun 2022 19:48
Operator : CG/JU
Sample : PB145592BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK592

Quant Time: Jun 22 01:33:12 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration




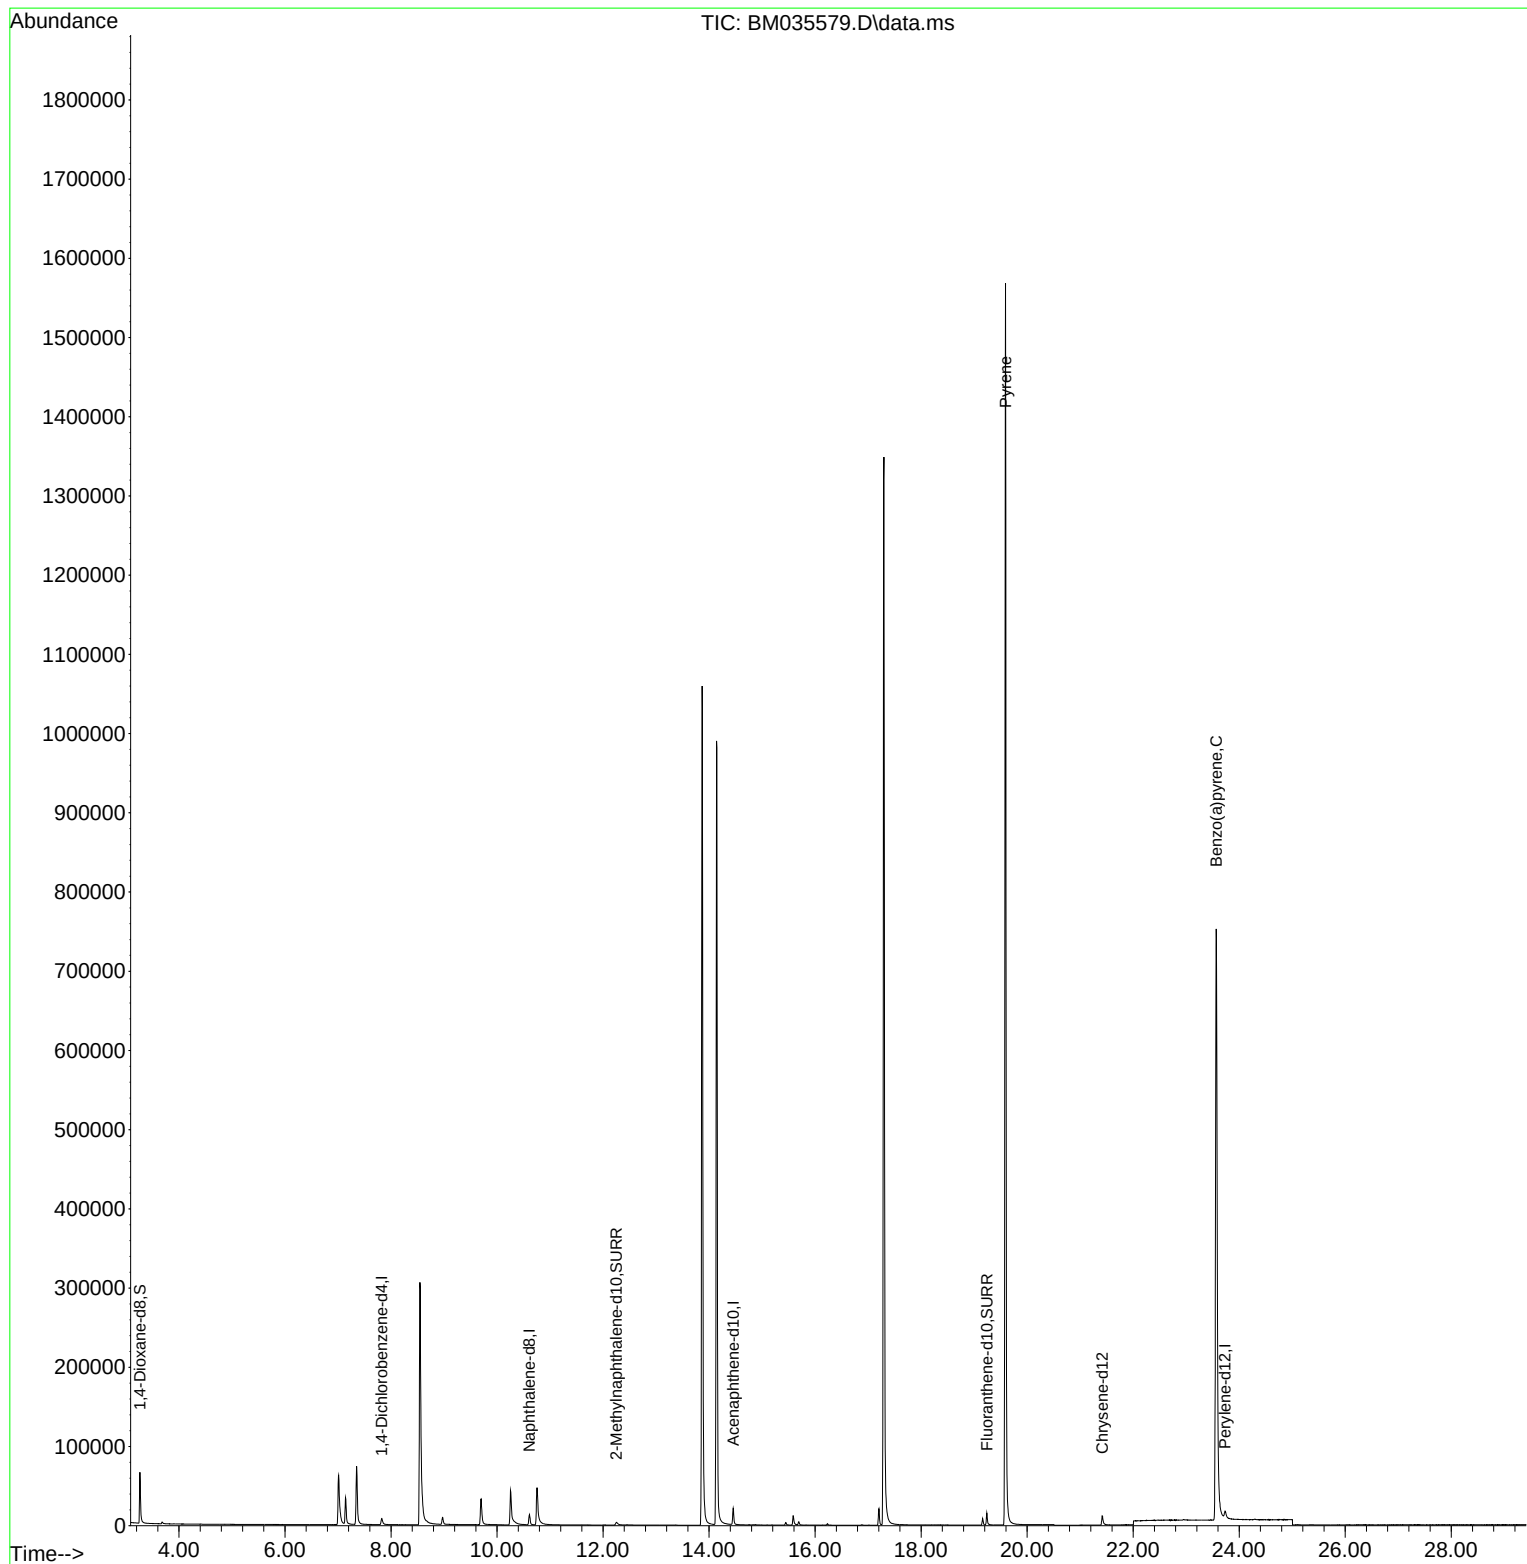


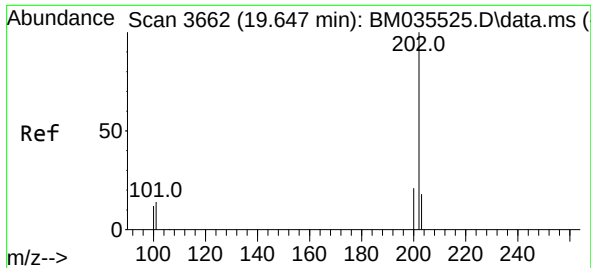

#20
Pyrene
Concen: 0.032 ng/ul
RT: 19.591 min Scan# 3650
Delta R.T. -0.057 min
Lab File: BM035579.D
Acq: 21 Jun 2022 19:48

Instrument :
BNA_M
ClientSampleId :
SBLK592

Tgt Ion:202 Resp: 2779
Ion Ratio Lower Upper
202 100
101 168.2 11.6 17.4#
100 1216.7 9.3 13.9#

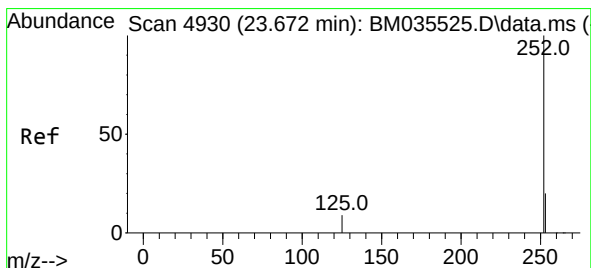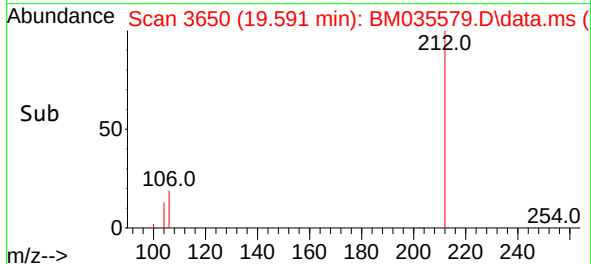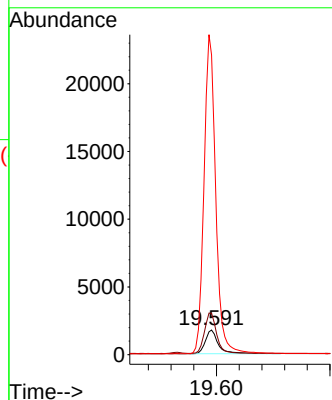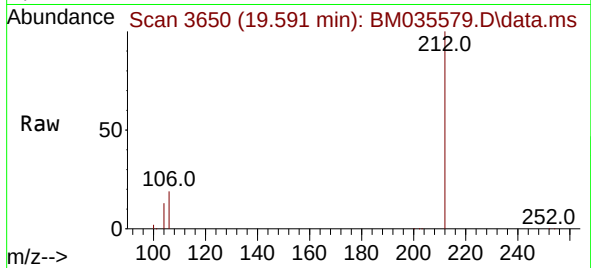

#26
Benzo(a)pyrene
Concen: 0.048 ng/ul
RT: 23.566 min Scan# 4894
Delta R.T. -0.101 min
Lab File: BM035579.D
Acq: 21 Jun 2022 19:48

Tgt Ion:252 Resp: 3989
Ion Ratio Lower Upper
252 100
253 61.9 27.8 41.6#
125 59.1 23.3 34.9#

