

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
 Data File : BM035547.D
 Acq On : 20 Jun 2022 23:20
 Operator : CG/JU
 Sample : N3226-02
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4L3




Manual IntegrationsAPPROVED

Quant Time: Jun 21 01:29:33 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2022
 Supervised By :Yogesh Patel 06/25/2022

06/21/2022
 Supervised By :Yogesh
 Patel

Ion 188.00 (187.70 to 188.70): BM035547.D\data.ms
 Ion 94.00 (93.70 to 94.70): BM035547.D\data.ms
 Ion 80.00 (79.70 to 80.70): BM035547.D\data.ms

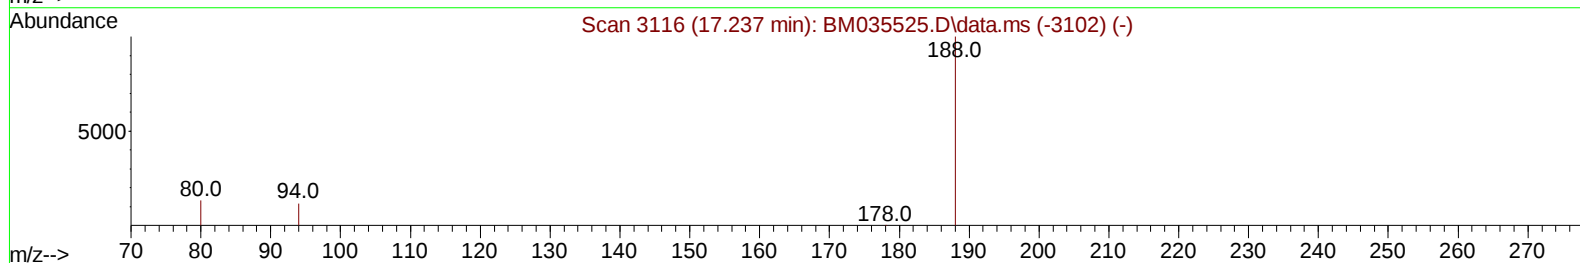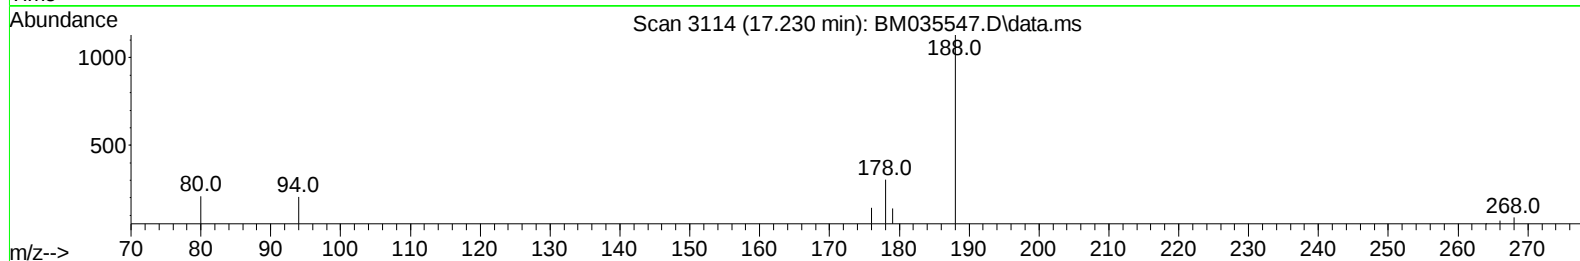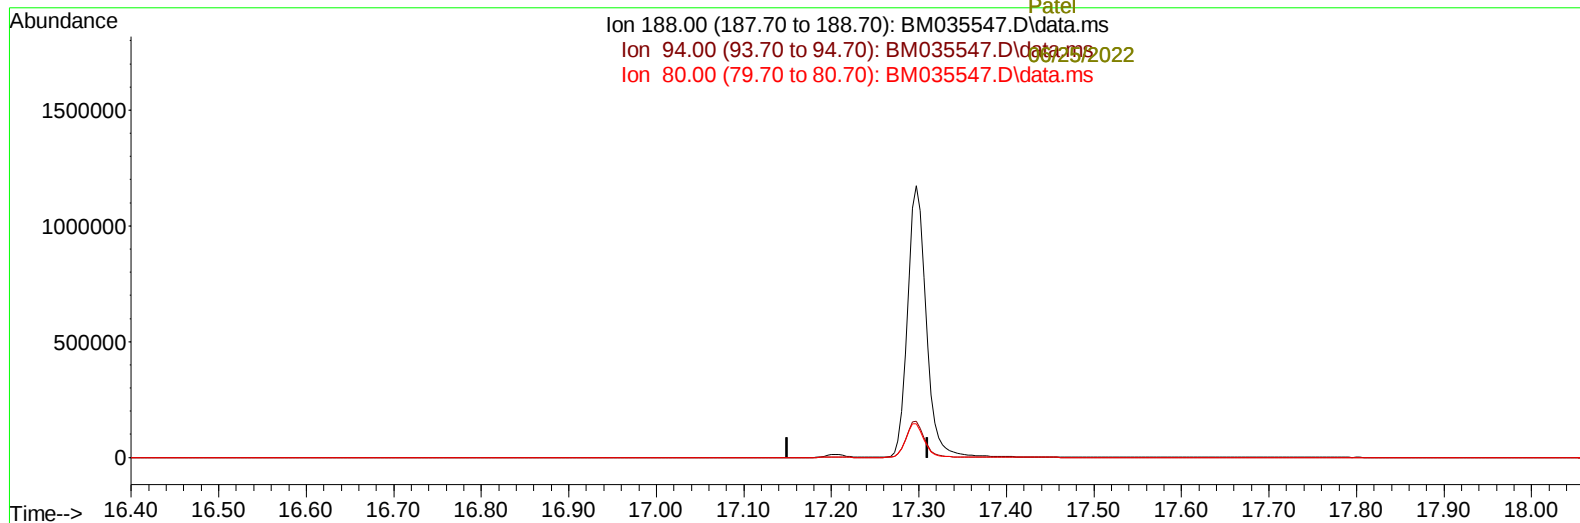

TIC: BM035547.D\data.ms

(13) Phenanthrene-d10 (I)

17.230min (-17.230) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	12.00	0.00#
80.00	13.50	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
 Data File : BM035547.D
 Acq On : 20 Jun 2022 23:20
 Operator : CG/JU
 Sample : N3226-02
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4L3




Manual IntegrationsAPPROVED

Quant Time: Jun 21 01:29:33 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2022
 Supervised By :Yogesh Patel 06/25/2022

06/21/2022
 Supervised By :Yogesh
 Patel

Ion 188.00 (187.70 to 188.70): BM035547.D\data.ms
 Ion 94.00 (93.70 to 94.70): BM035547.D\data.ms
 Ion 80.00 (79.70 to 80.70): BM035547.D\data.ms

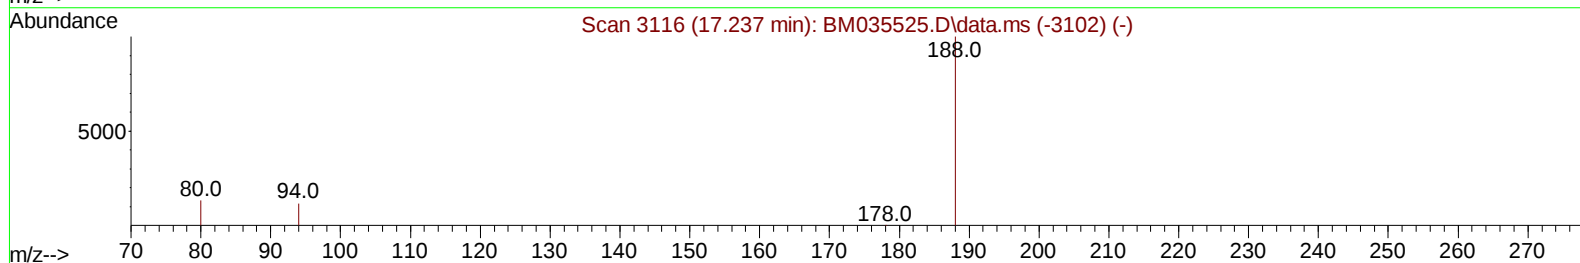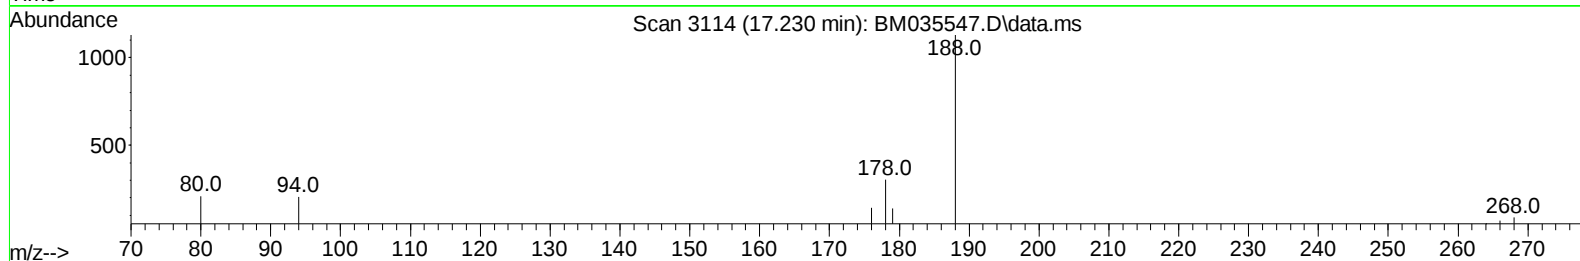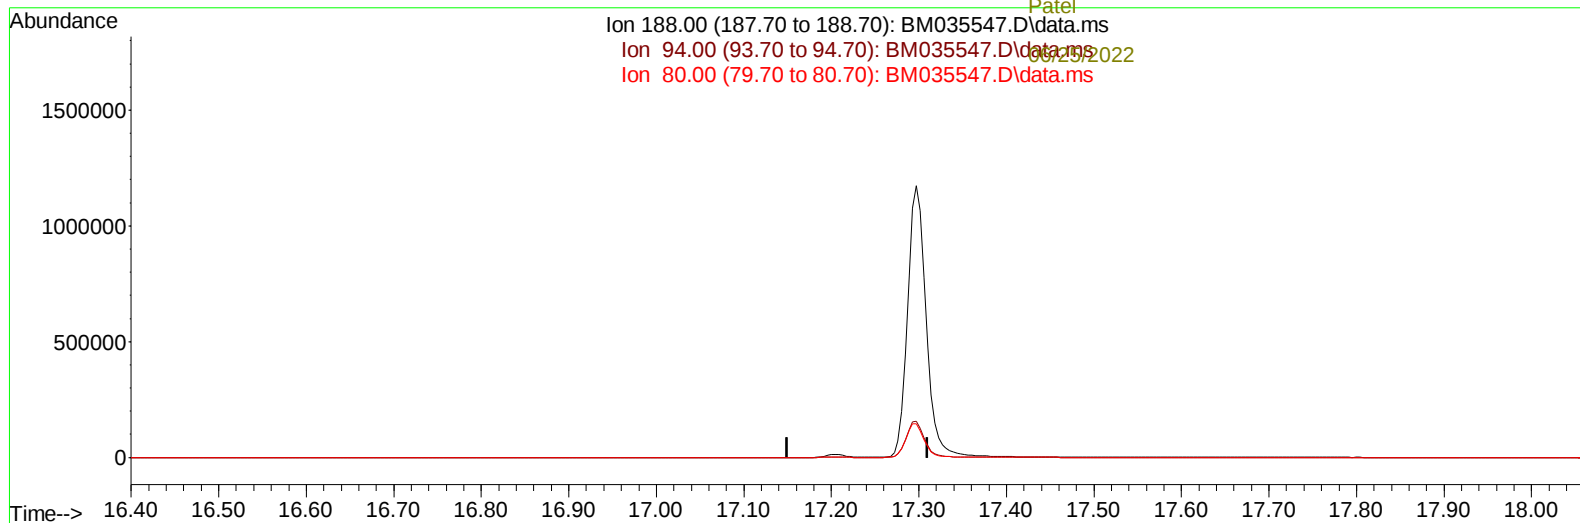

TIC: BM035547.D\data.ms

(13) Phenanthrene-d10 (I)

17.230min (-17.230) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	12.00	0.00#
80.00	13.50	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
 Data File : BM035547.D
 Acq On : 20 Jun 2022 23:20
 Operator : CG/JU
 Sample : N3226-02
 Misc :
 ALS Vial : 25 Sample Multiplier: 1




Instrument :
 BNA_M
 ClientSampleId :
 EW4L3

Manual IntegrationsAPPROVED

Quant Time: Jun 21 01:29:33 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2022
 Supervised By :Yogesh Patel 06/25/2022

06/21/2022
 Supervised By :Yogesh
 Patel

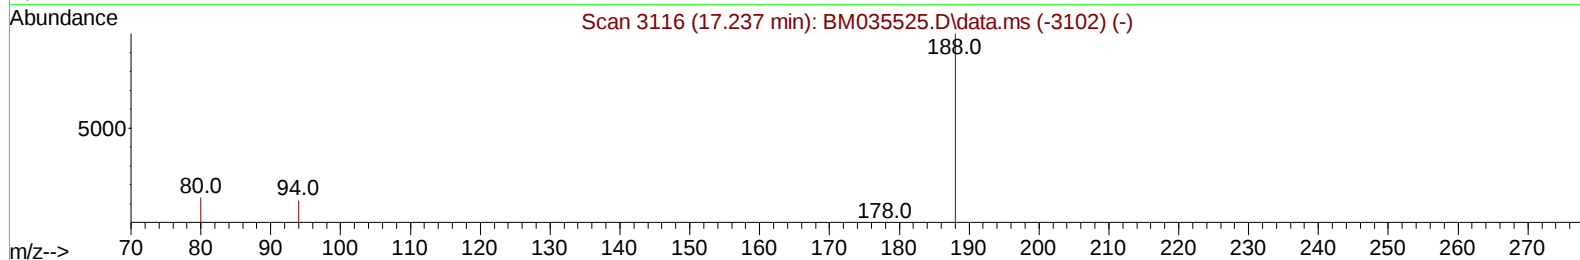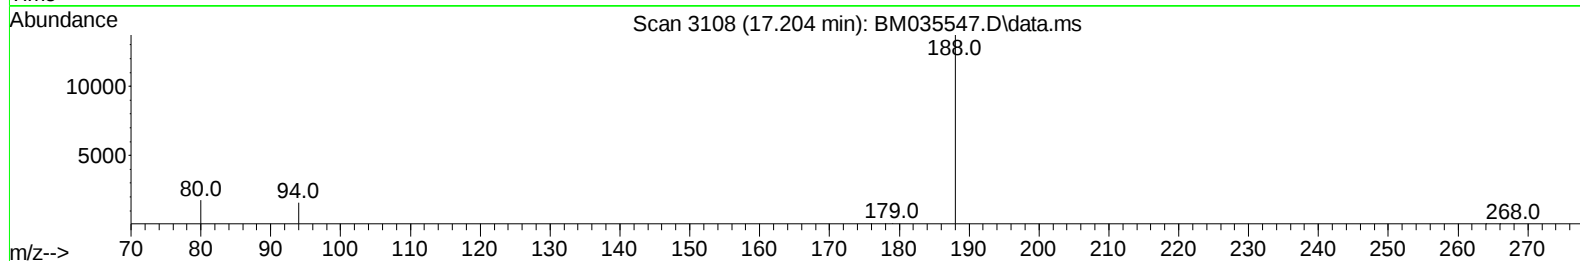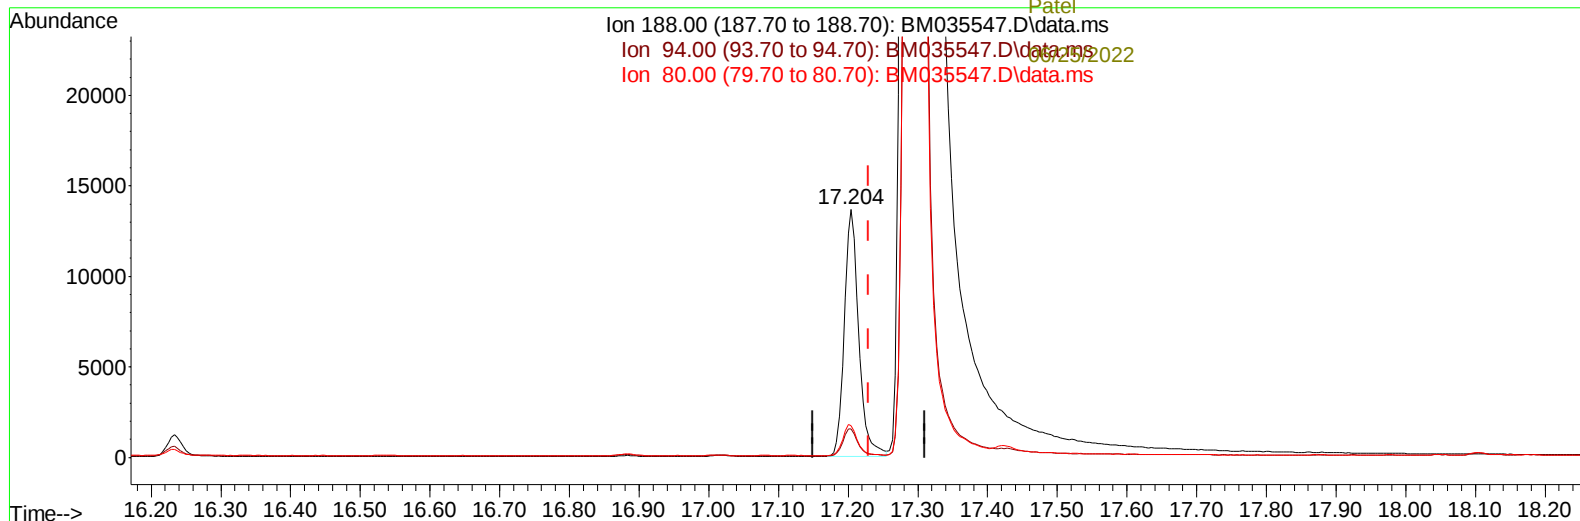

TIC: BM035547.D\data.ms

(13) Phenanthrene-d10 (I)

17.204min (-0.025) 0.40 ng/ul m

response 19748

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.00	11.59
80.00	13.50	12.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
 Data File : BM035547.D
 Acq On : 20 Jun 2022 23:20
 Operator : CG/JU
 Sample : N3226-02
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4L3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/21/2022
 Supervised By :Yogesh Patel 06/25/2022

Quant Time: Jun 21 01:29:33 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----06/25/2022						
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.825	152	5622	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.611	136	18026	0.400	ng/ul	-0.03
9) Acenaphthene-d10	14.456	164	9982	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.204	188	19748m	0.400	ng/ul	-0.03
17) Chrysene-d12	21.411	240	14308	0.400	ng/ul	0.00
23) Perylene-d12	23.741	264	16339	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	45947	5.808	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.239	152	9789	0.365	ng/ul	0.00
18) Fluoranthene-d10	19.239	212	19468	0.405	ng/ul	-0.01
Target Compounds						
					Qvalue	
19) Fluoranthene	19.271	202	2050	0.028	ng/ul#	66
24) Benzo(b)fluoranthene	23.039	252	1525	0.021	ng/ul#	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
Data File : BM035547.D
Acq On : 20 Jun 2022 23:20
Operator : CG/JU
Sample : N3226-02
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4L3

Manual IntegrationsAPPROVED

Quant Time: Jun 21 01:29:33 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/21/2022
Supervised By :Yogesh Patel 06/25/2022

06/21/2022
Supervised By :Yogesh
Patel

06/25/2022

