




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
 Data File : BM035562.D
 Acq On : 21 Jun 2022 08:55
 Operator : CG/JU
 Sample : PB145549BL
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 SBLK549

Manual IntegrationsAPPROVED

Quant Time: Jun 22 01:32:00 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :Yogesh Patel 06/25/2022

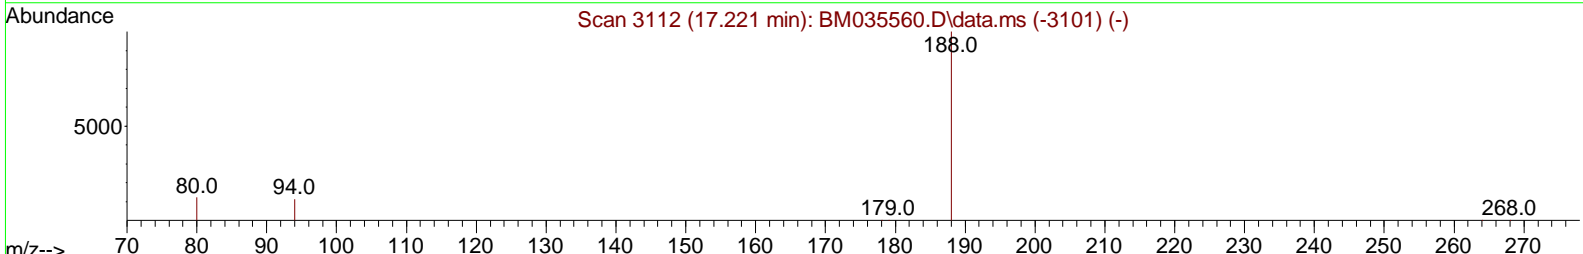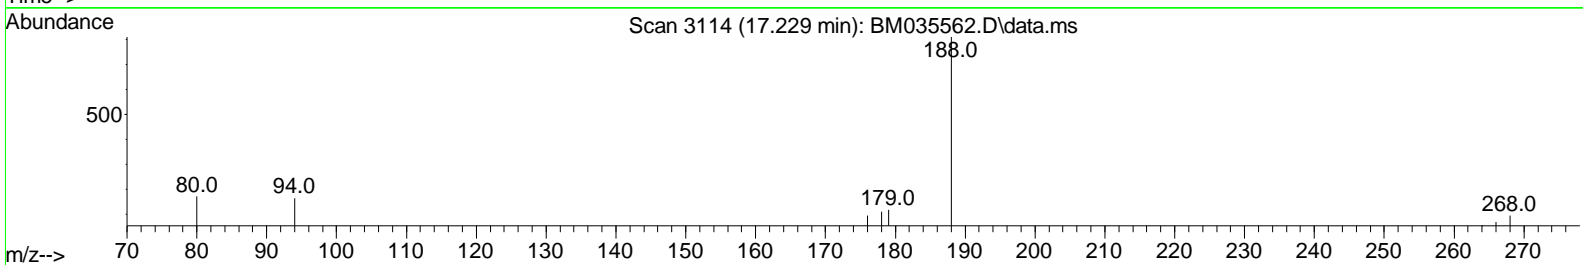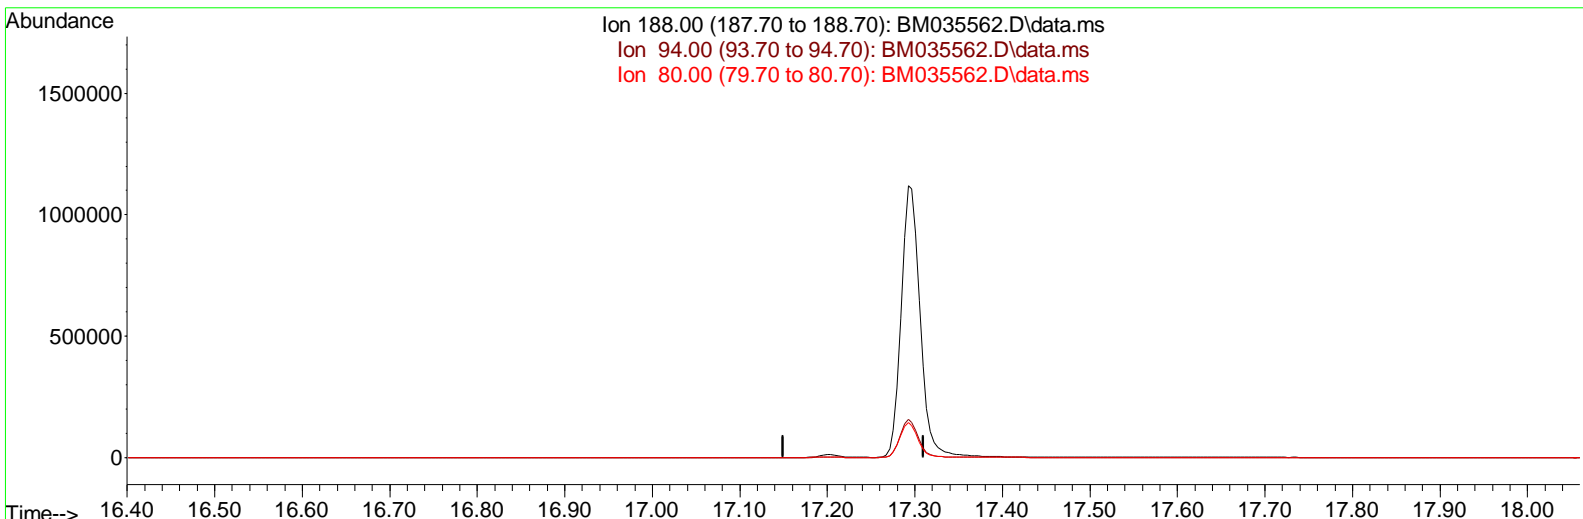

TIC: BM035562.D\data.ms

(13) Phenanthrene-d10 (I)

17.230min (-17.230) 0.00 ng/ul

response	0	
Ion	Exp%	Act%
188.00	100.00	0.00
94.00	12.00	0.00#
80.00	13.50	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
 Data File : BM035562.D
 Acq On : 21 Jun 2022 08:55
 Operator : CG/JU
 Sample : PB145549BL
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 SBLK549

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :Yogesh Patel 06/25/2022

Quant Time: Jun 22 01:32:00 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

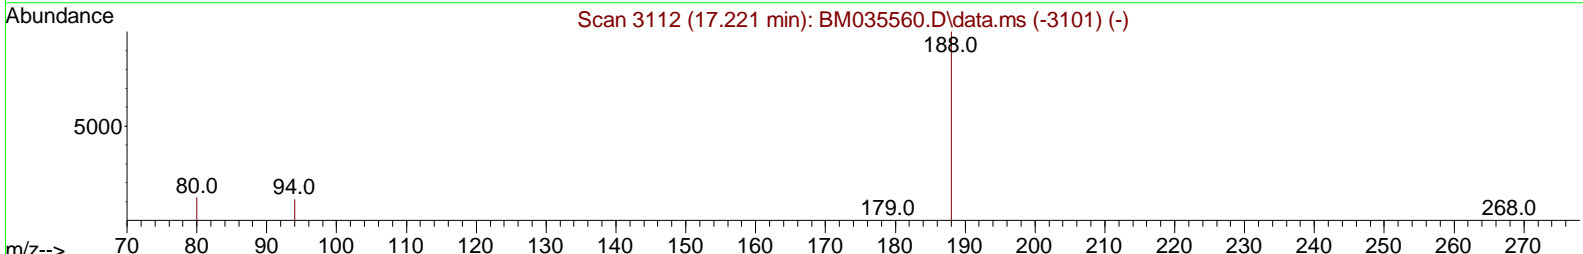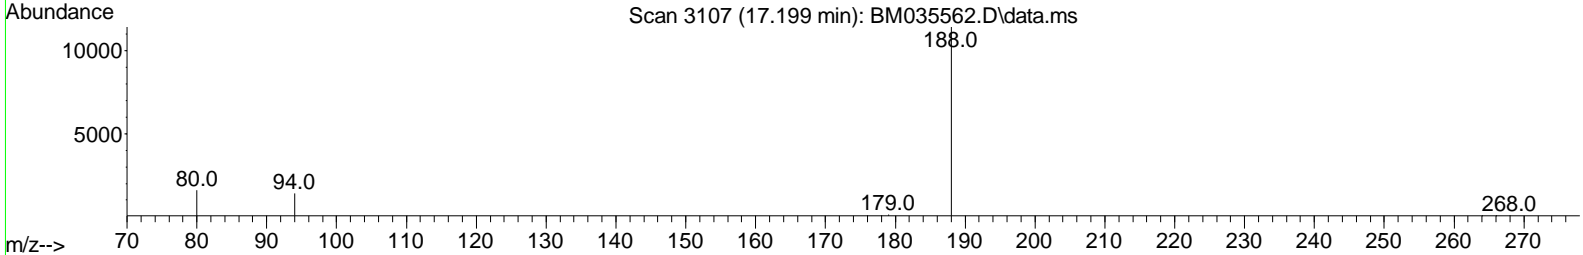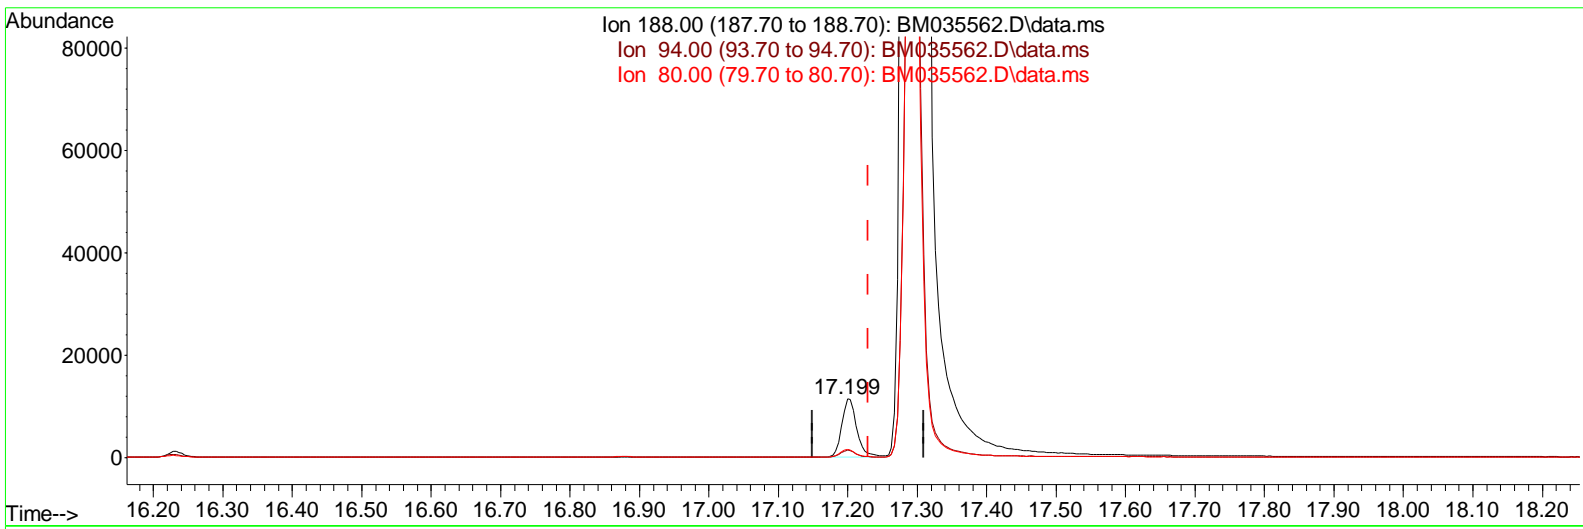

TIC: BM035562.D\data.ms

(13) Phenanthrene-d10 (I)

17.199min (-0.030) 0.40 ng/ul m

response	17061	
Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.00	12.23
80.00	13.50	13.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BMO62022\
 Data File : BMO35562.D
 Acq On : 21 Jun 2022 08:55
 Operator : CG/JU
 Sample : PB145549BL
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 SBLK549

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :Yogesh Patel 06/25/2022

Quant Time: Jun 22 01:32:00 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BMO61822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Compound	R. T.	QI on	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.821	152	4606	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.611	136	15644	0.400	ng/ul	-0.03
9) Acenaphthene-d10	14.455	164	9019	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.199	188	17061m	0.400	ng/ul	-0.03
17) Chrysene-d12	21.412	240	12975	0.400	ng/ul	0.00
23) Perylene-d12	23.736	264	17388	0.400	ng/ul	#-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	48086	7.420	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.239	152	9700	0.417	ng/ul	0.00
18) Fluoranthene-d10	19.238	212	18273	0.419	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BMO62022\
 Data File : BMO35562.D
 Acq On : 21 Jun 2022 08:55
 Operator : CG/JU
 Sample : PB145549BL
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 SBLK549

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :Yogesh Patel 06/25/2022

Quant Time: Jun 22 01:32:00 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BMO61822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

