




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
Data File : BM035570.D
Acq On : 21 Jun 2022 13:43
Operator : CG/JU
Sample : N3285-16
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4Q8

Manual IntegrationsAPPROVED

Quant Time: Jun 22 01:32:30 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/22/2022
Supervised By :Yogesh Patel 06/25/2022

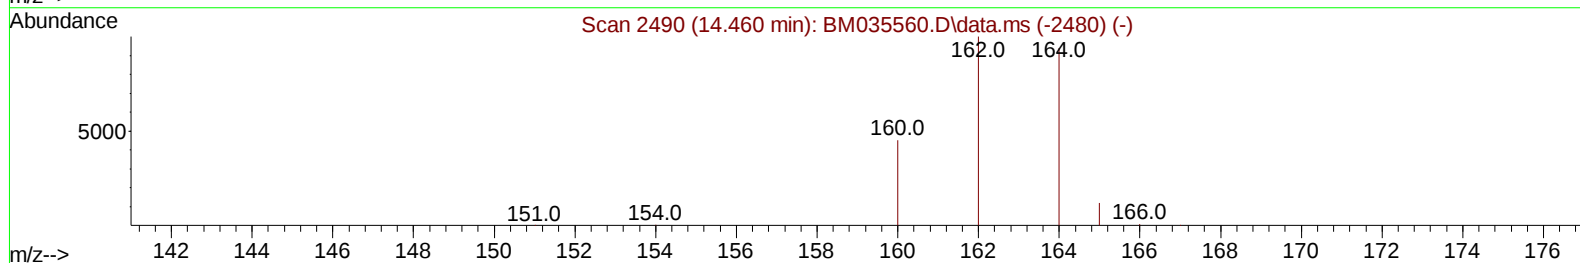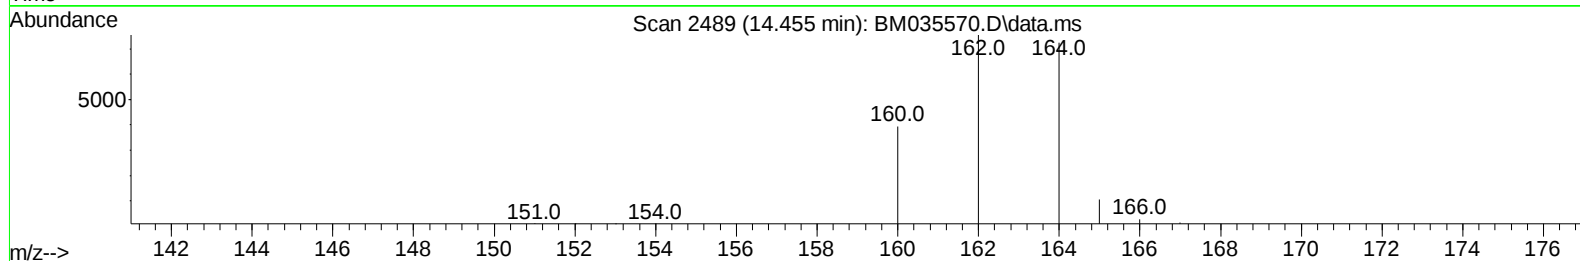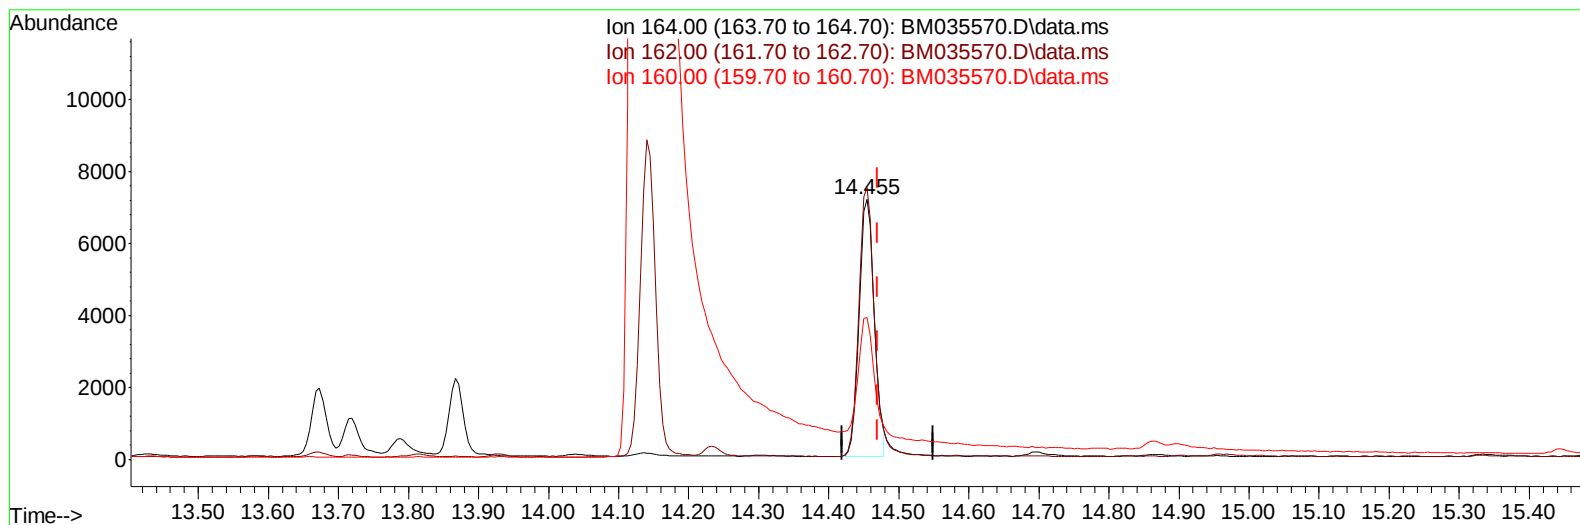

TIC: BM035570.D\data.ms

(9) Acenaphthene-d10 (I)

14.455min (-0.015) 0.40 ng/u1

response 10832

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	106.40	104.23
160.00	49.90	54.36
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
Data File : BM035570.D
Acq On : 21 Jun 2022 13:43
Operator : CG/JU
Sample : N3285-16
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4Q8

Manual IntegrationsAPPROVED

Quant Time: Jun 22 01:32:30 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/22/2022
Supervised By :Yogesh Patel 06/25/2022

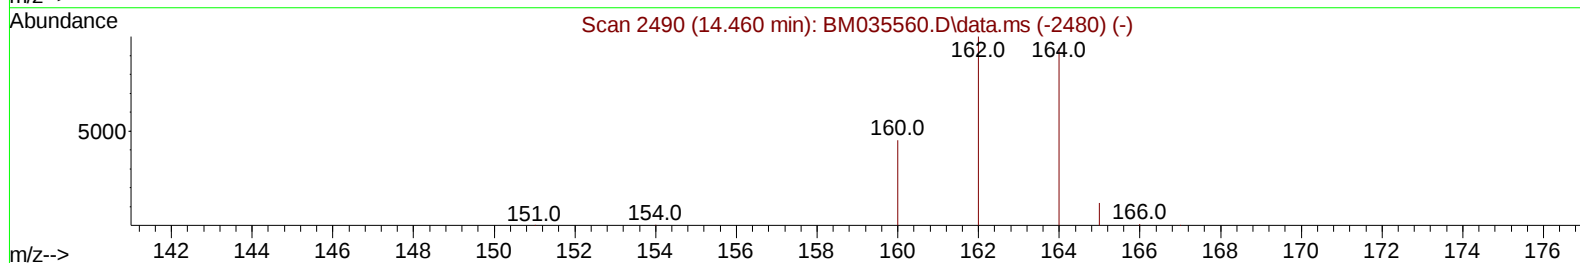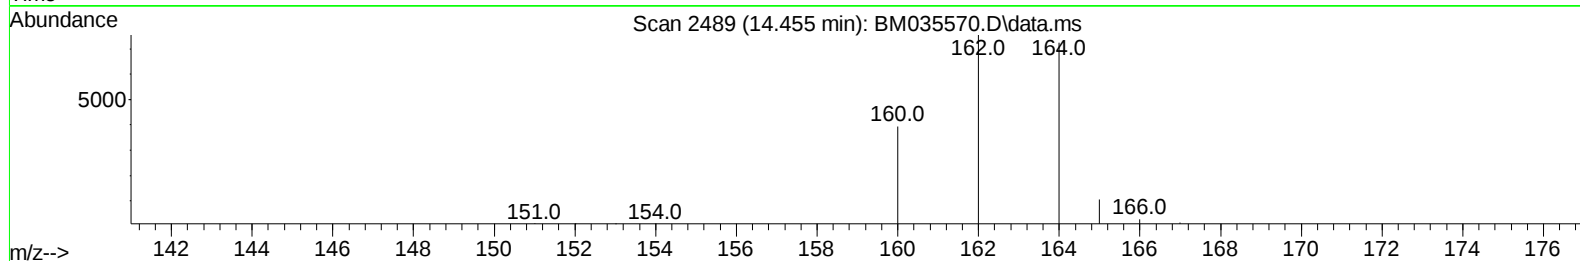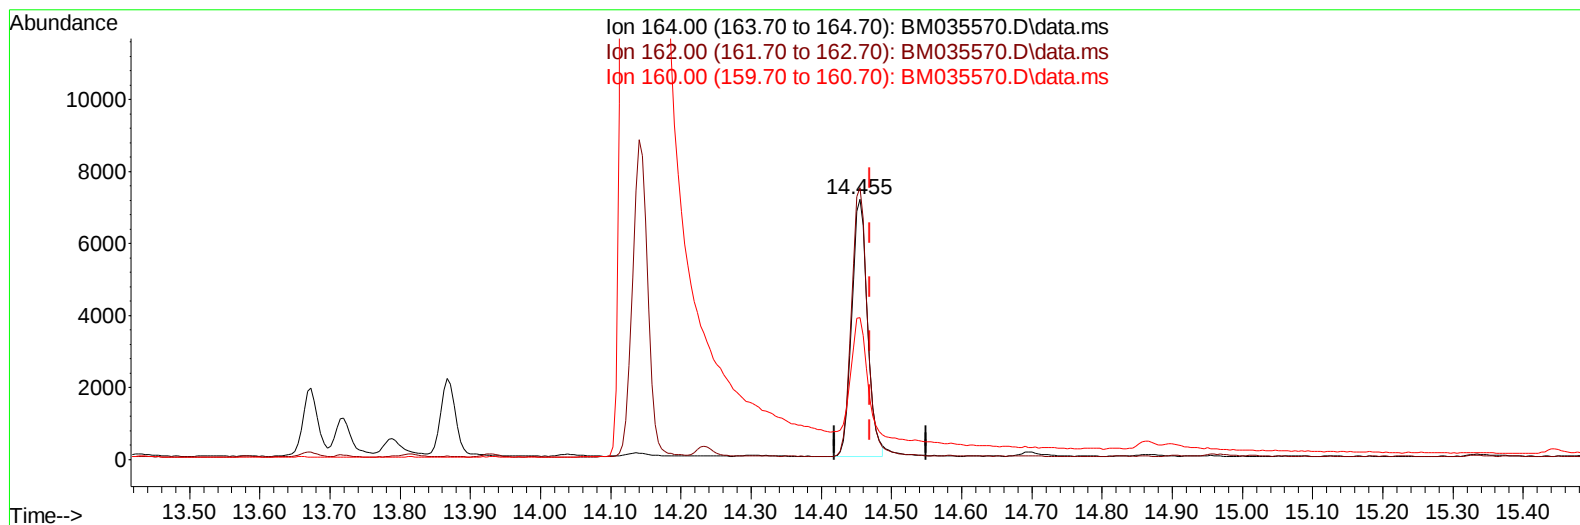

TIC: BM035570.D\data.ms

(9) Acenaphthene-d10 (I)

14.455min (-0.015) 0.40 ng/u1 m

response 11040

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	106.40	104.23
160.00	49.90	54.36
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
 Data File : BM035570.D
 Acq On : 21 Jun 2022 13:43
 Operator : CG/JU
 Sample : N3285-16
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4Q8

Manual IntegrationsAPPROVED

Quant Time: Jun 22 01:32:30 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :Yogesh Patel 06/25/2022

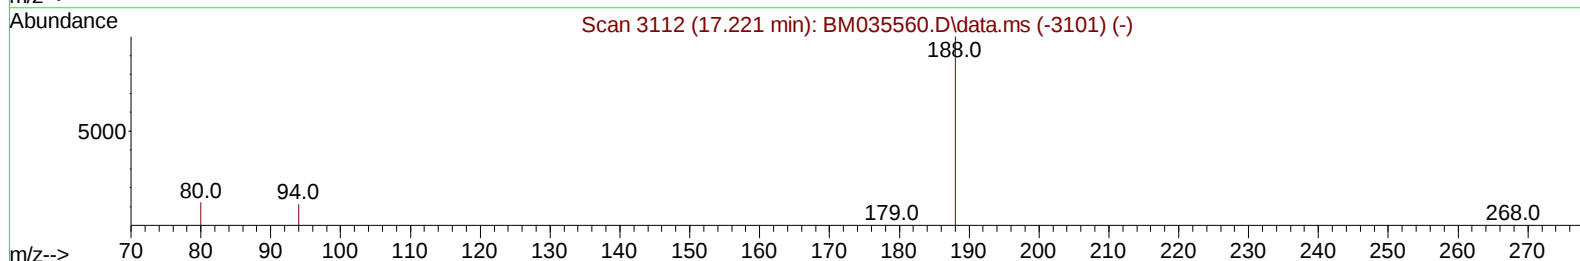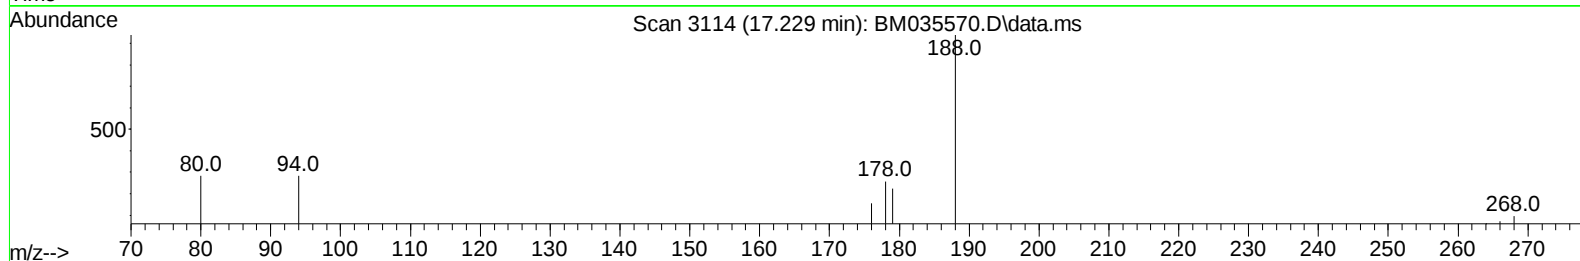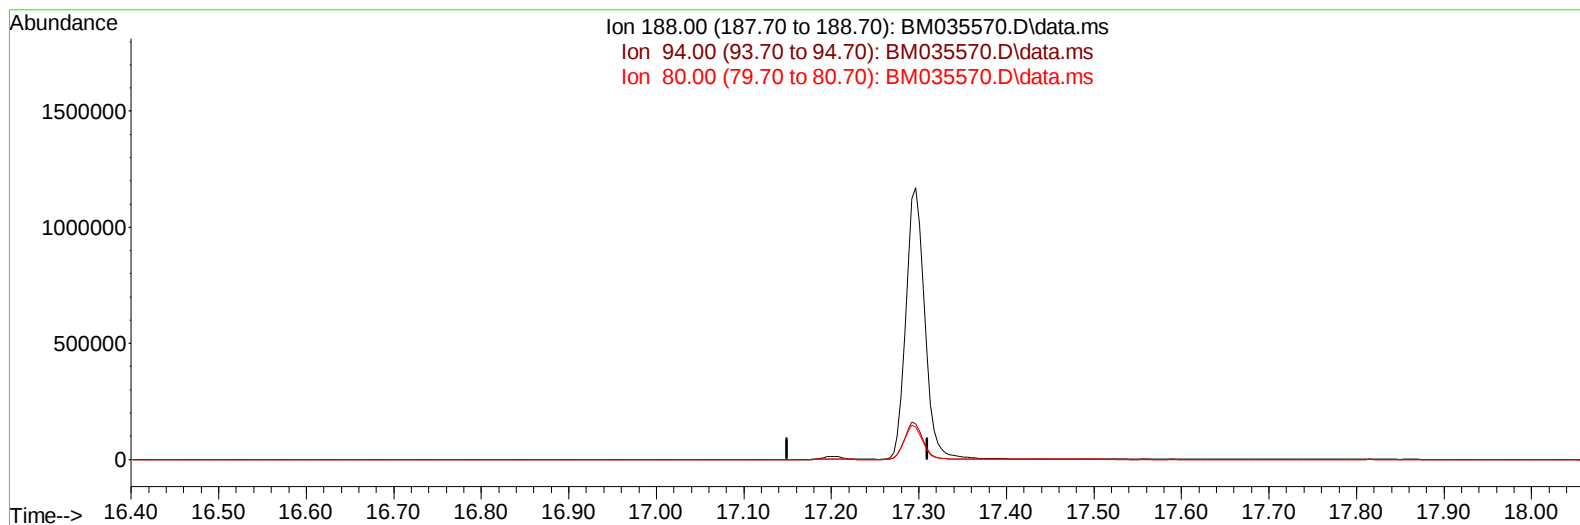

TIC: BM035570.D\data.ms

(13) Phenanthrene-d10 (I)

17.230min (-17.230) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	12.00	0.00#
80.00	13.50	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
 Data File : BM035570.D
 Acq On : 21 Jun 2022 13:43
 Operator : CG/JU
 Sample : N3285-16
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4Q8

Manual IntegrationsAPPROVED

Quant Time: Jun 22 01:32:30 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :Yogesh Patel 06/25/2022

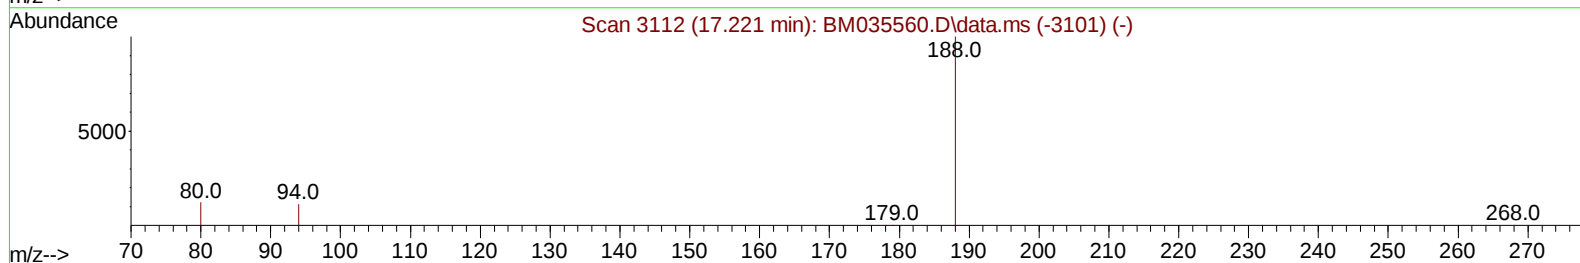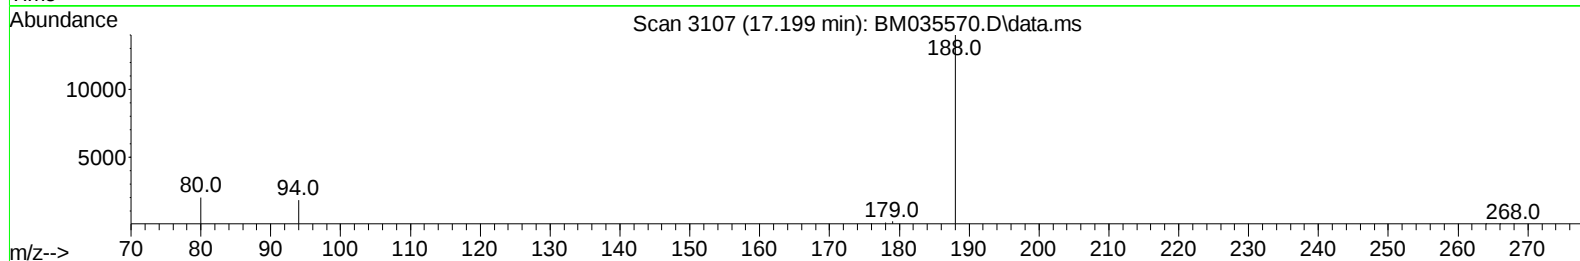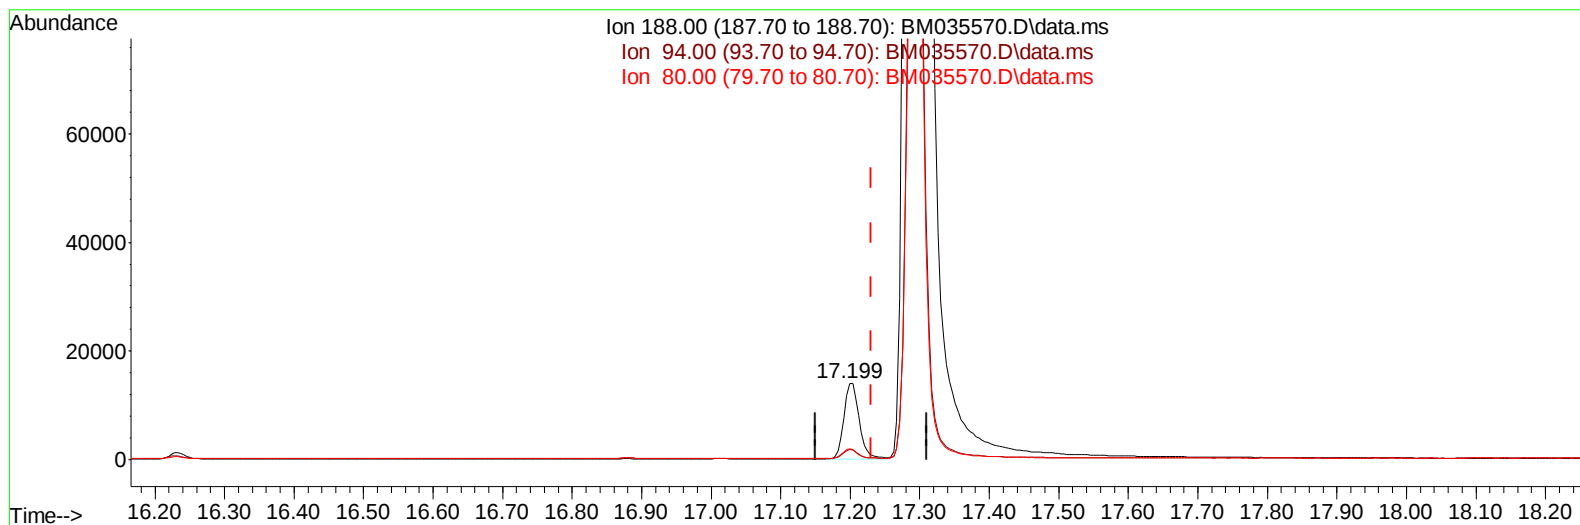

TIC: BM035570.D\data.ms

(13) Phenanthrene-d10 (I)

17.199min (-0.030) 0.40 ng/ul m

response 21400

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.00	13.11
80.00	13.50	14.29
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
 Data File : BM035570.D
 Acq On : 21 Jun 2022 13:43
 Operator : CG/JU
 Sample : N3285-16
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4Q8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :Yogesh Patel 06/25/2022

Quant Time: Jun 22 01:32:30 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.820	152		5274	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.605	136		23927	0.400	ng/ul	-0.04
9) Acenaphthene-d10	14.455	164		11040m	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.199	188		21400m	0.400	ng/ul	-0.03
17) Chrysene-d12	21.401	240		16119	0.400	ng/ul	-0.01
23) Perylene-d12	23.736	264		18745	0.400	ng/ul	#-0.03
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.264	96		30234	4.074	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.211	152		10453	0.294	ng/ul	-0.03
18) Fluoranthene-d10	19.238	212		20827	0.385	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
Data File : BM035570.D
Acq On : 21 Jun 2022 13:43
Operator : CG/JU
Sample : N3285-16
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4Q8

Manual IntegrationsAPPROVED

Quant Time: Jun 22 01:32:30 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/22/2022
Supervised By :Yogesh Patel 06/25/2022

