




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
Data File : BM035583.D
Acq On : 21 Jun 2022 22:13
Operator : CG/JU
Sample : N3285-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4P5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/22/2022
Supervised By :Yogesh Patel 06/25/2022

Quant Time: Jun 22 01:33:28 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

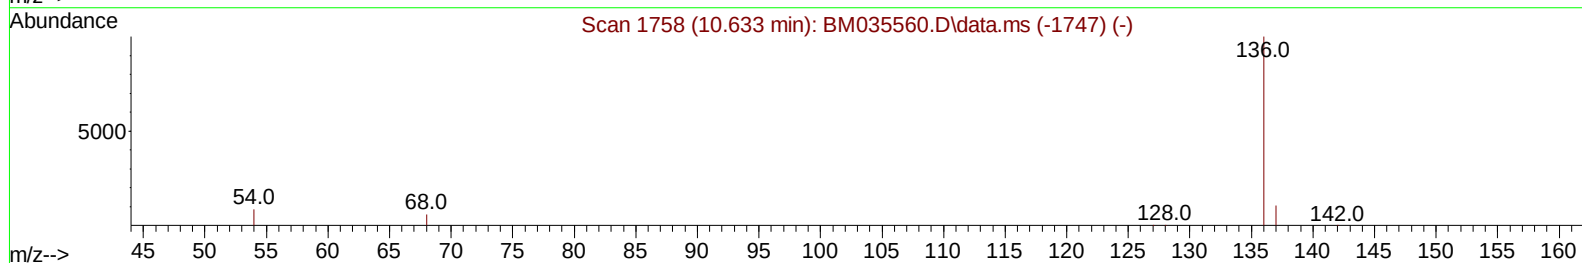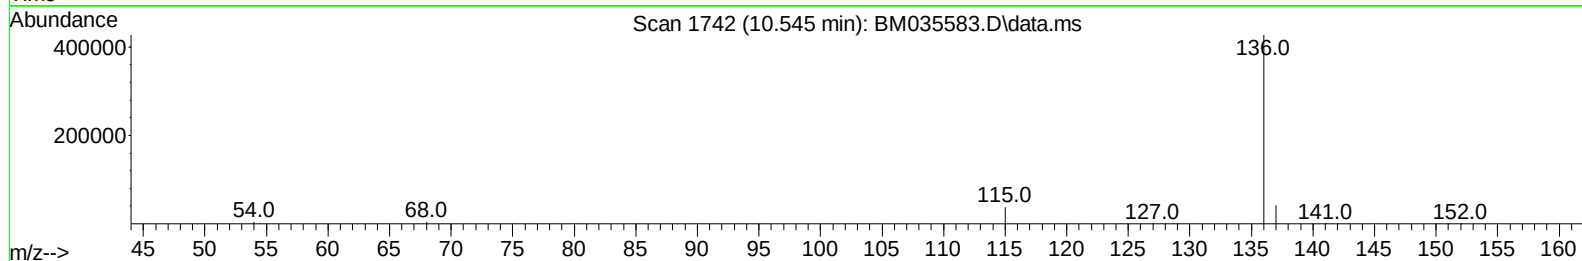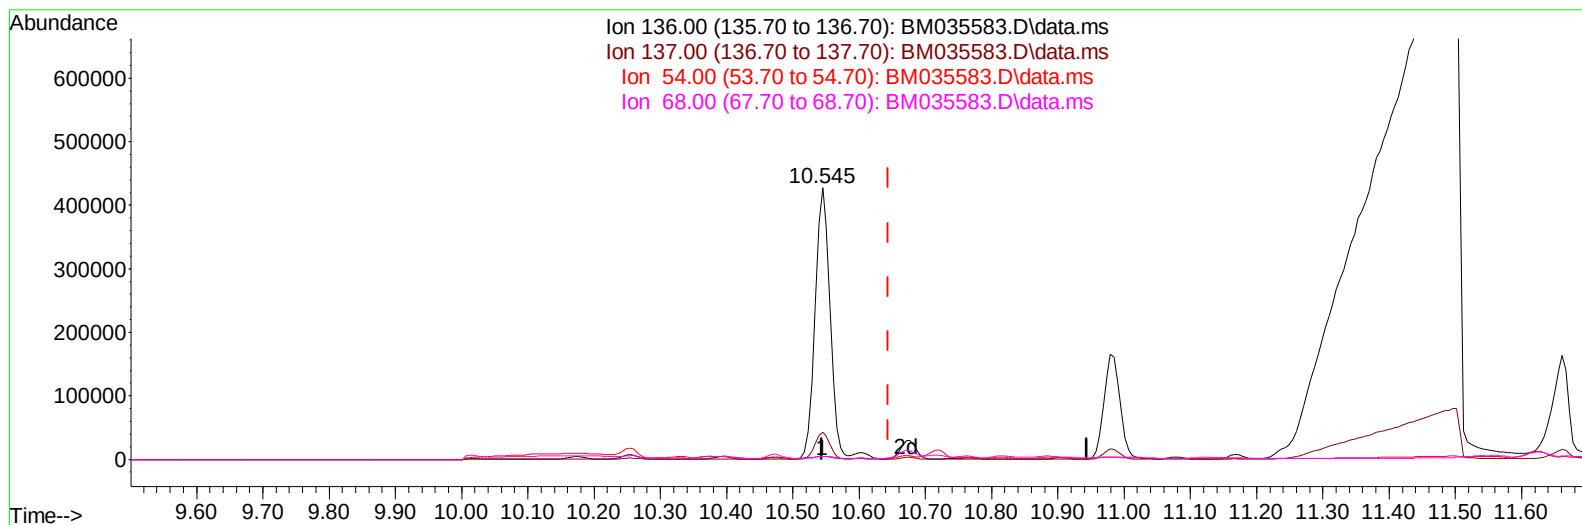

TIC: BM035583.D\data.ms

(4) Naphthalene-d8 (I)

10.545min (-0.099) 0.40 ng/u1

response 667096

Ion	Exp%	Act%
136.00	100.00	100.00
137.00	11.70	9.99
54.00	12.80	1.20#
68.00	8.70	1.17#




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
 Data File : BM035583.D
 Acq On : 21 Jun 2022 22:13
 Operator : CG/JU
 Sample : N3285-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4P5

Manual IntegrationsAPPROVED

Quant Time: Jun 22 01:33:28 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :Yogesh Patel 06/25/2022

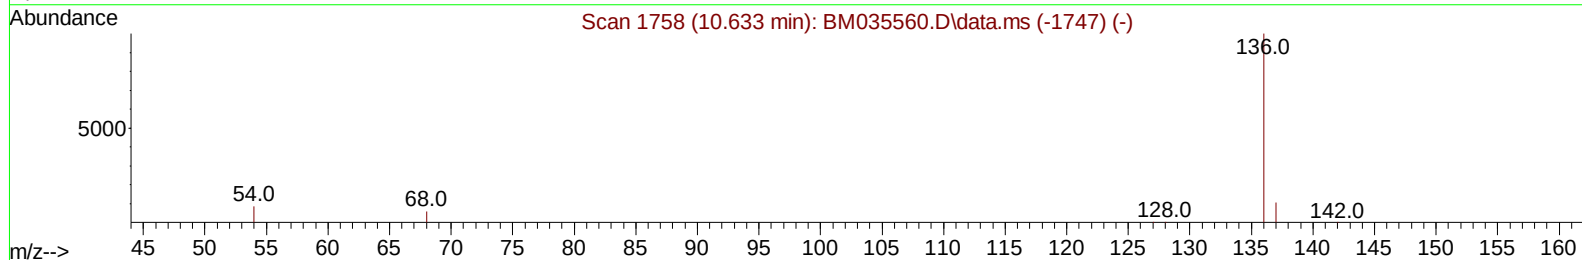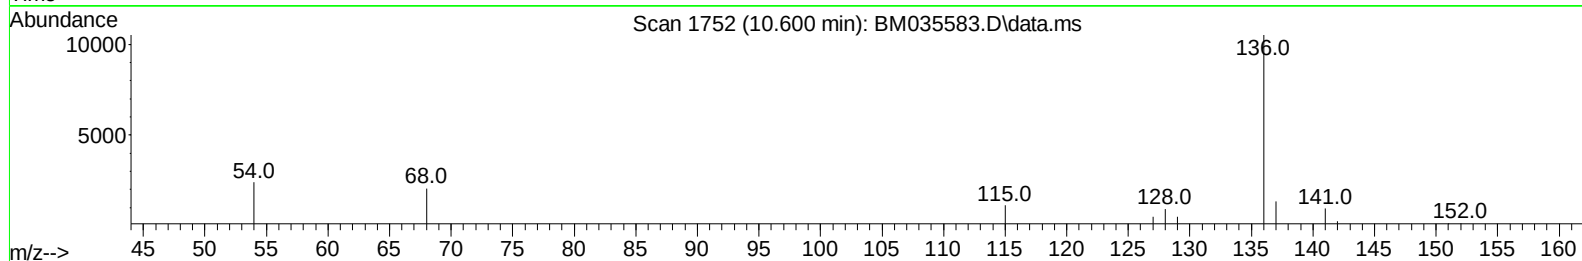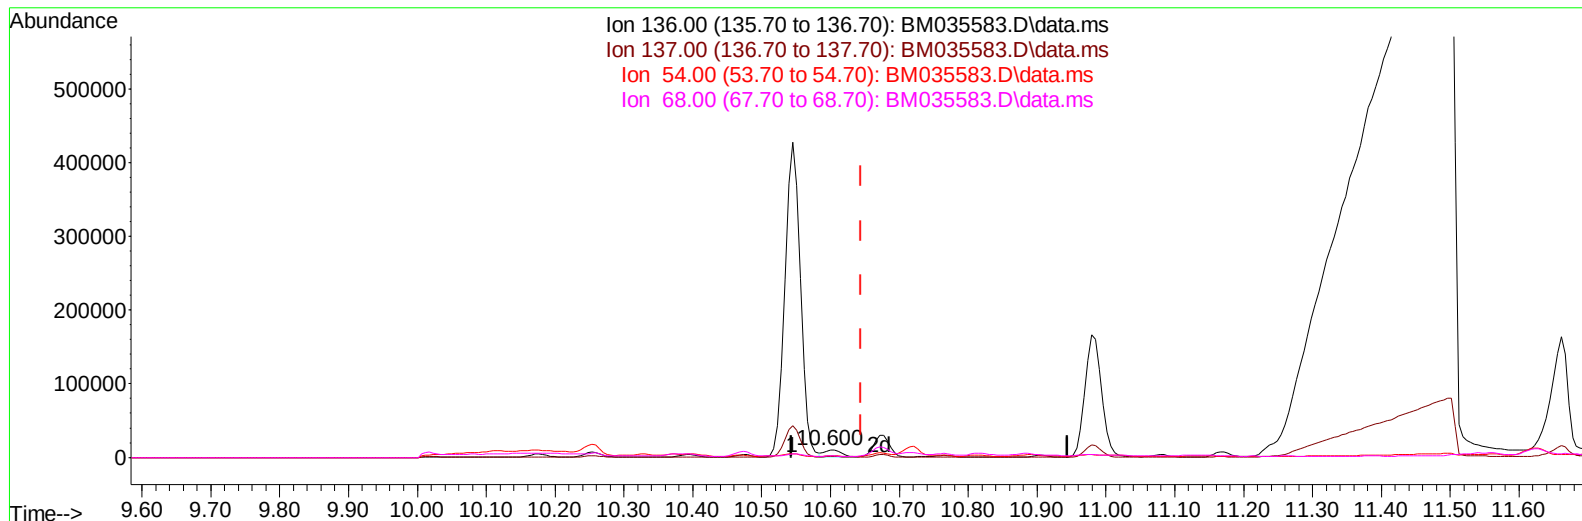

TIC: BM035583.D\data.ms

(4) Naphthalene-d8 (I)

10.600min (-0.044) 0.40 ng/ul m

response 18075

Ion	Exp%	Act%
136.00	100.00	100.00
137.00	11.70	12.72
54.00	12.80	22.70#
68.00	8.70	19.47#




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
 Data File : BM035583.D
 Acq On : 21 Jun 2022 22:13
 Operator : CG/JU
 Sample : N3285-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4P5

Manual IntegrationsAPPROVED

Quant Time: Jun 22 01:33:28 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :Yogesh Patel 06/25/2022

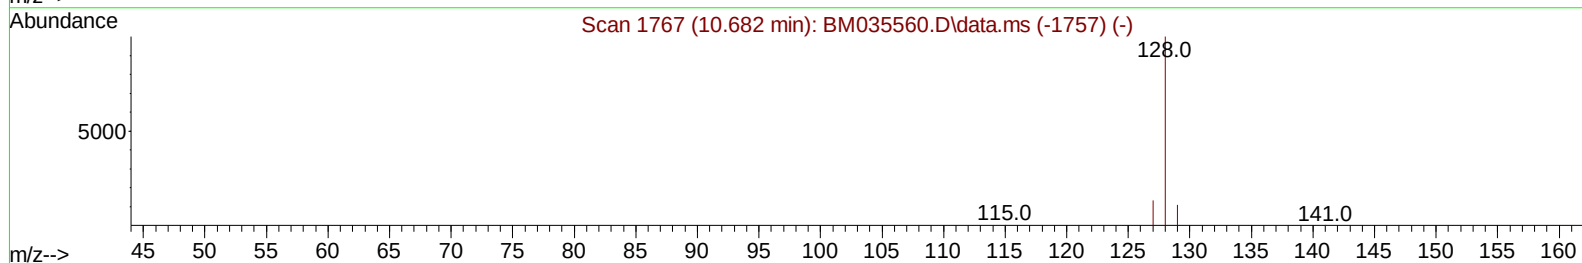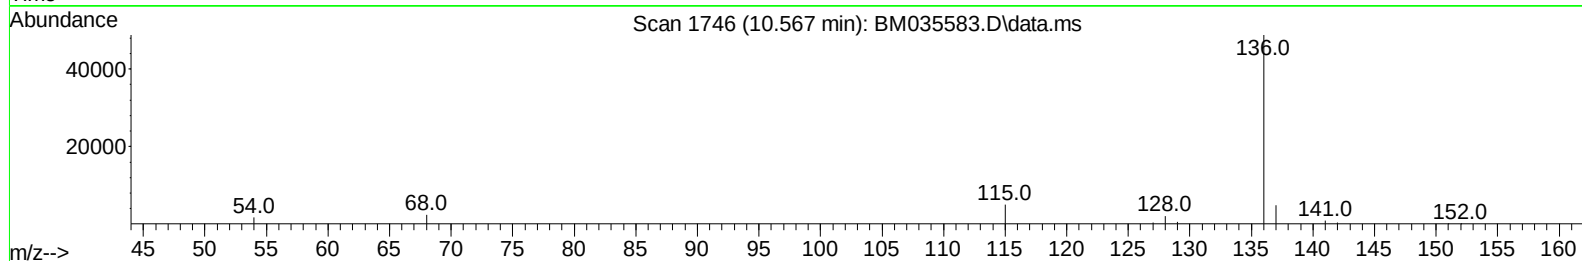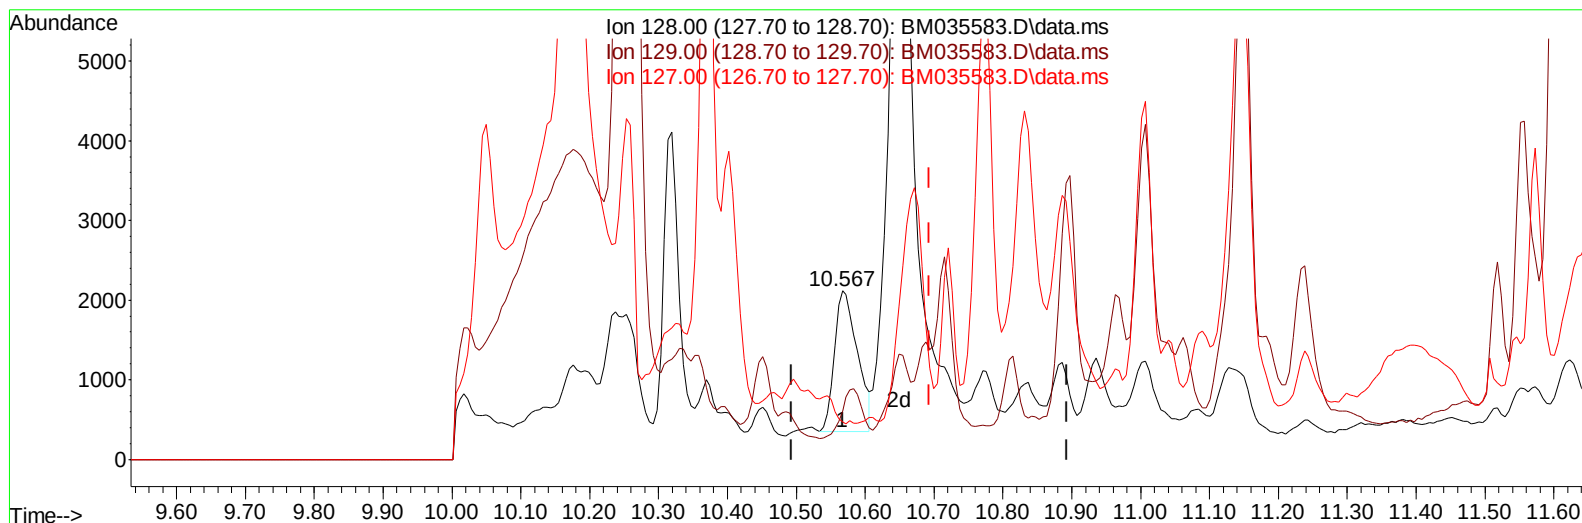

TIC: BM035583.D\data.ms

(5) Naphthalene

10.567min (-0.127) 0.07 ng/u1

response 4152

Ion	Exp%	Act%
128.00	100.00	100.00
129.00	12.60	28.50#
127.00	14.30	22.18#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
 Data File : BM035583.D
 Acq On : 21 Jun 2022 22:13
 Operator : CG/JU
 Sample : N3285-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4P5

Manual IntegrationsAPPROVED

Quant Time: Jun 22 01:33:28 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :Yogesh Patel 06/25/2022

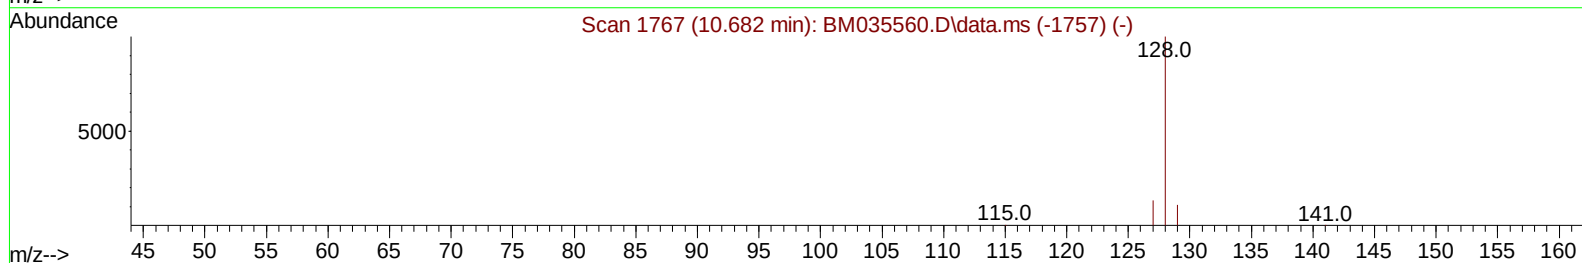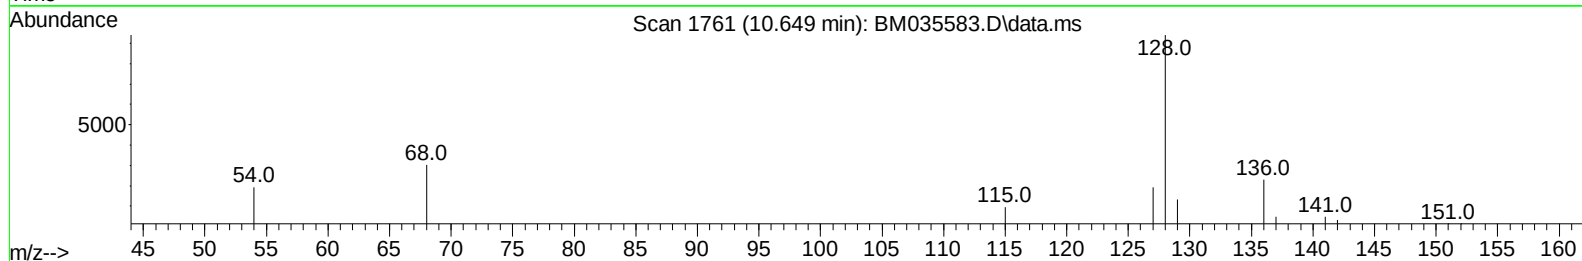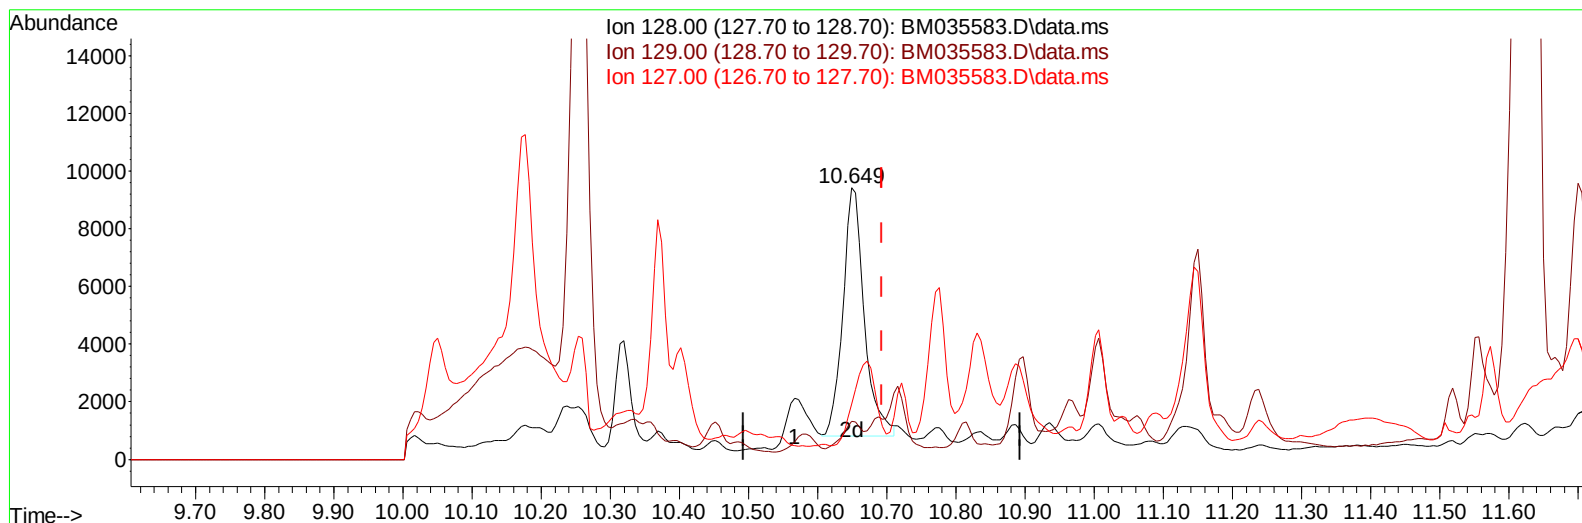

TIC: BM035583.D\data.ms

(5) Naphthalene

10.649min (-0.044) 0.30 ng/ul m

response 18632

Ion	Exp%	Act%
128.00	100.00	100.00
129.00	12.60	14.01
127.00	14.30	20.46#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
 Data File : BM035583.D
 Acq On : 21 Jun 2022 22:13
 Operator : CG/JU
 Sample : N3285-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4P5

Manual IntegrationsAPPROVED

Quant Time: Jun 22 01:33:28 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :Yogesh Patel 06/25/2022

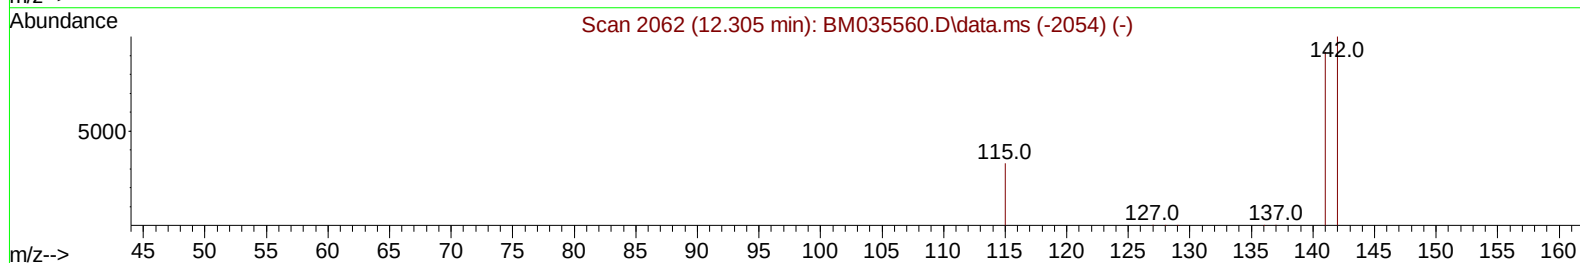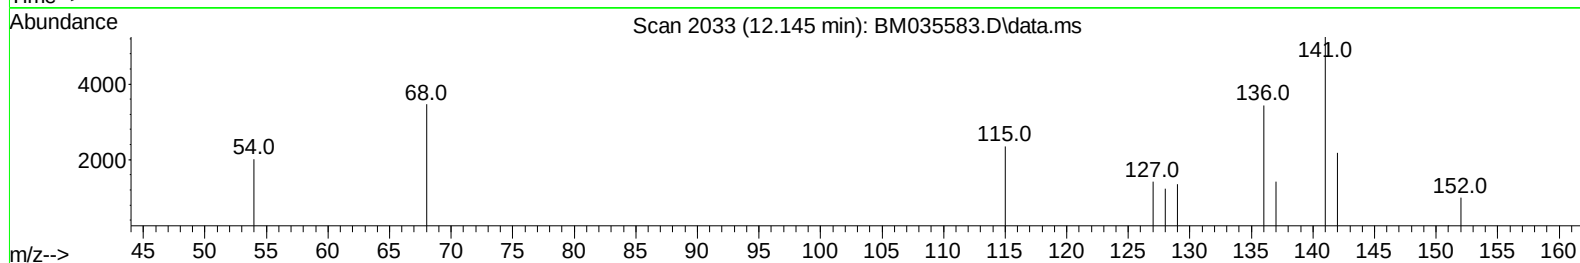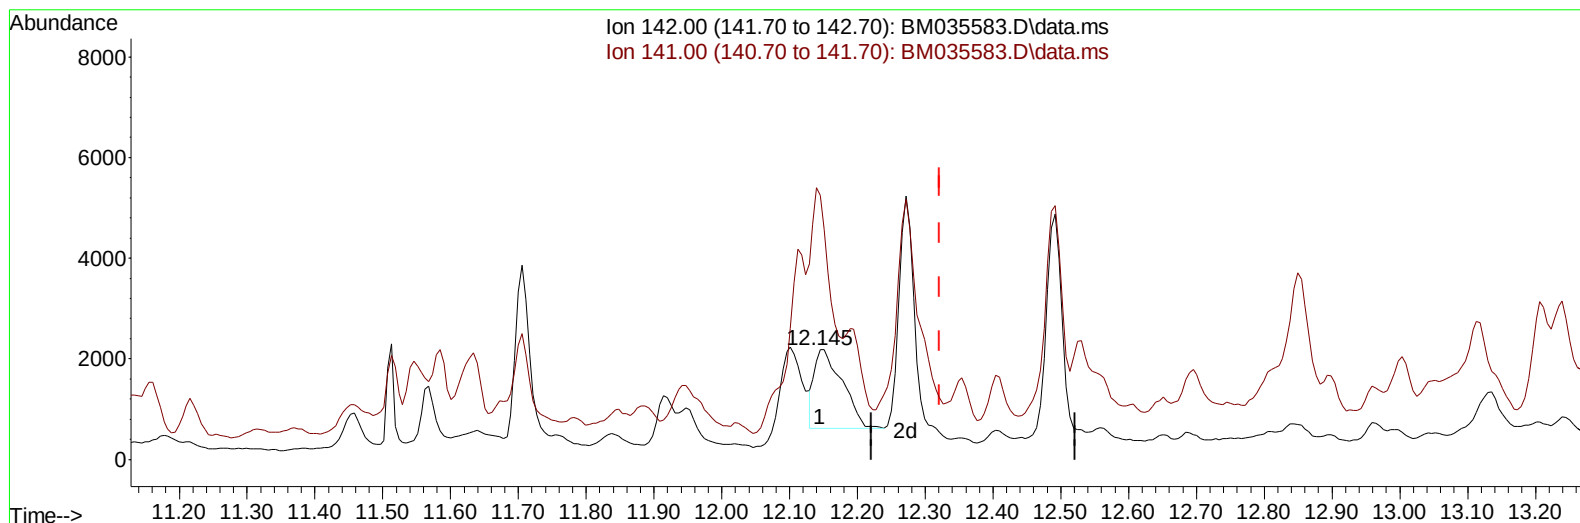

TIC: BM035583.D\data.ms

(7) 2-Methylnaphthalene

12.145min (-0.176) 0.13 ng/u1

response 4525

Ion	Exp%	Act%
142.00	100.00	100.00
141.00	92.30	259.16#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
Data File : BM035583.D
Acq On : 21 Jun 2022 22:13
Operator : CG/JU
Sample : N3285-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4P5

Manual IntegrationsAPPROVED

Quant Time: Jun 22 01:33:28 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/22/2022
Supervised By :Yogesh Patel 06/25/2022

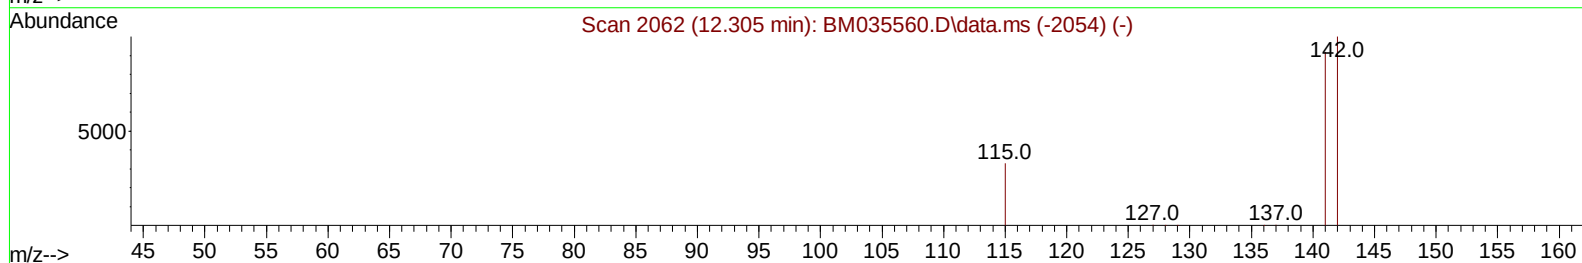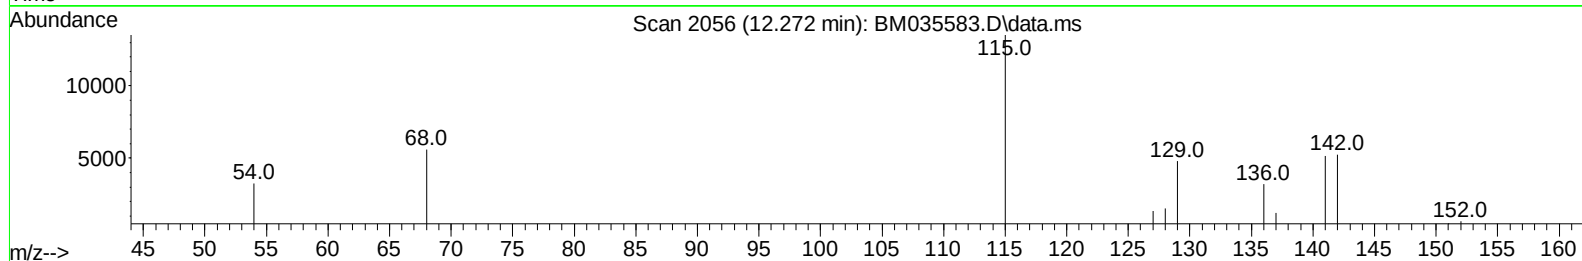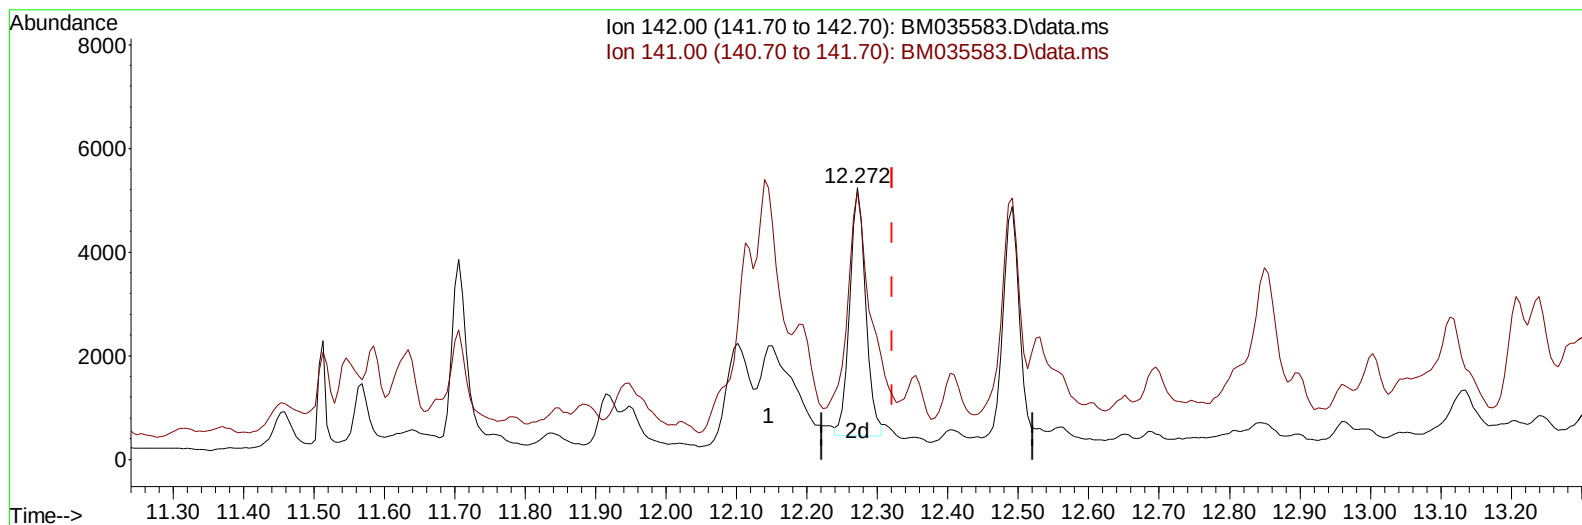

TIC: BM035583.D\data.ms

(7) 2-Methylnaphthalene

12.272min (-0.050) 0.22 ng/ul m

response 7577

Ion	Exp%	Act%
142.00	100.00	100.00
141.00	92.30	154.77#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
 Data File : BM035583.D
 Acq On : 21 Jun 2022 22:13
 Operator : CG/JU
 Sample : N3285-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4P5

Manual IntegrationsAPPROVED

Quant Time: Jun 22 01:33:28 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :Yogesh Patel 06/25/2022

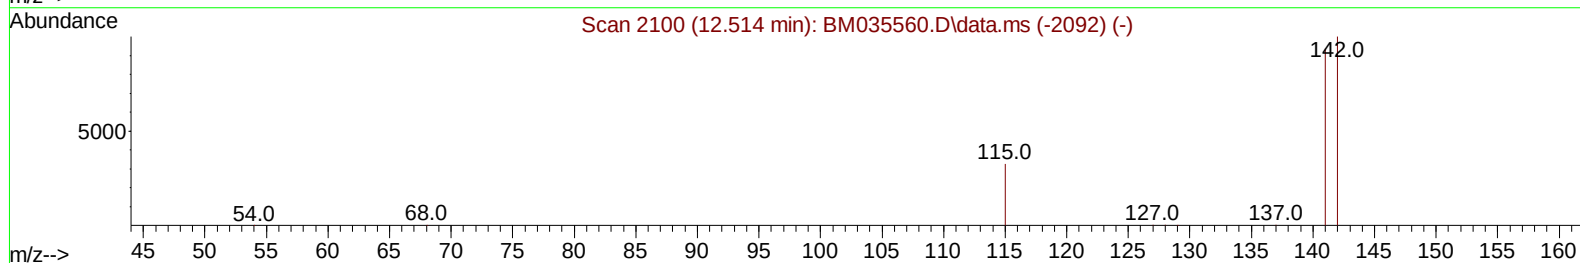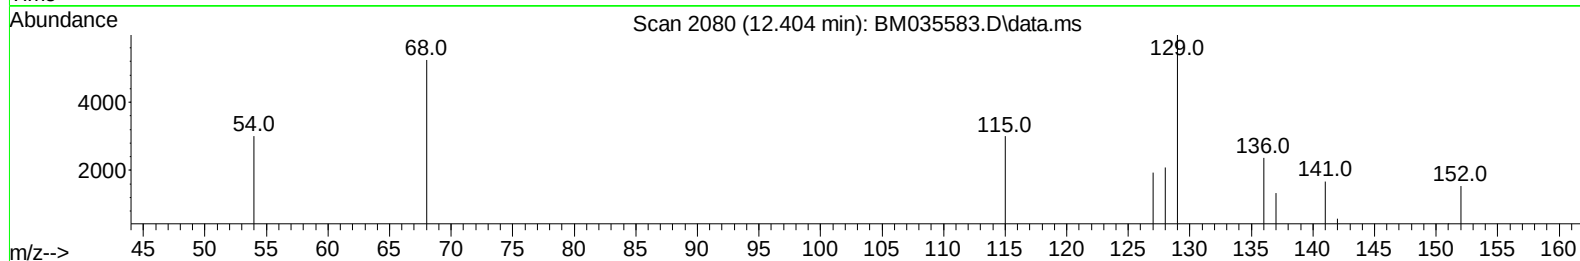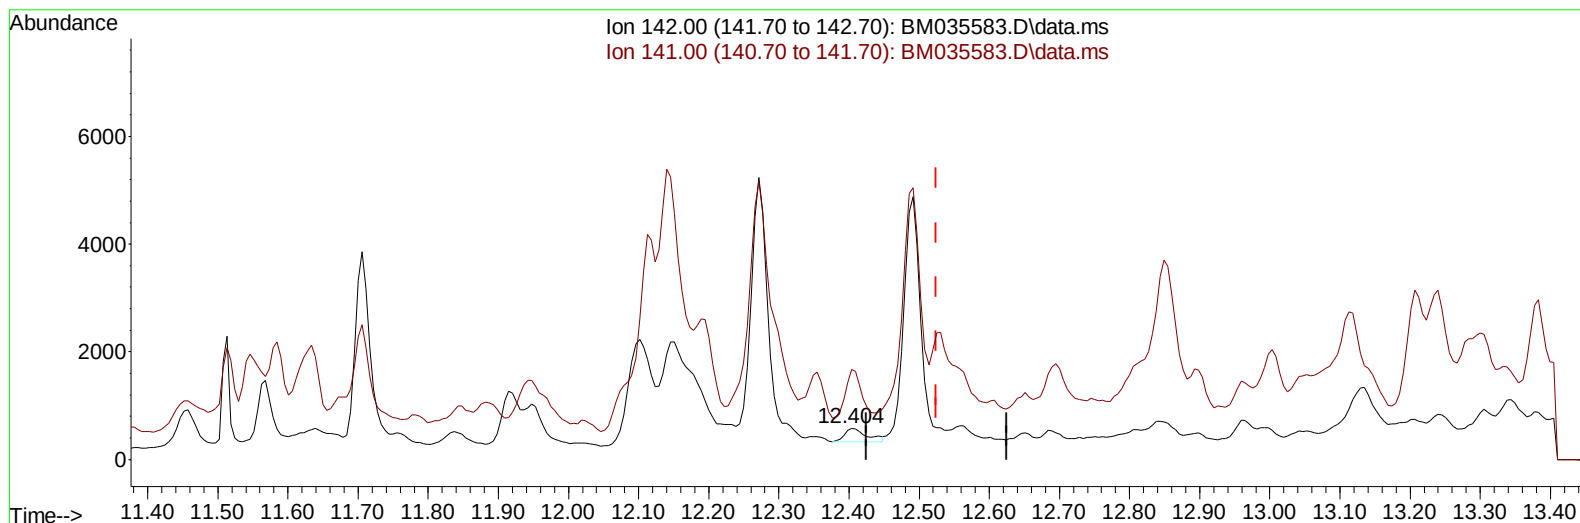

TIC: BM035583.D\data.ms

(8) 1-Methylnaphthalene

12.404min (-0.121) 0.02 ng/uL

response 571

Ion	Exp%	Act%
142.00	100.00	100.00
141.00	93.20	250.26#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
 Data File : BM035583.D
 Acq On : 21 Jun 2022 22:13
 Operator : CG/JU
 Sample : N3285-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4P5

Manual IntegrationsAPPROVED

Quant Time: Jun 22 01:33:28 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :Yogesh Patel 06/25/2022

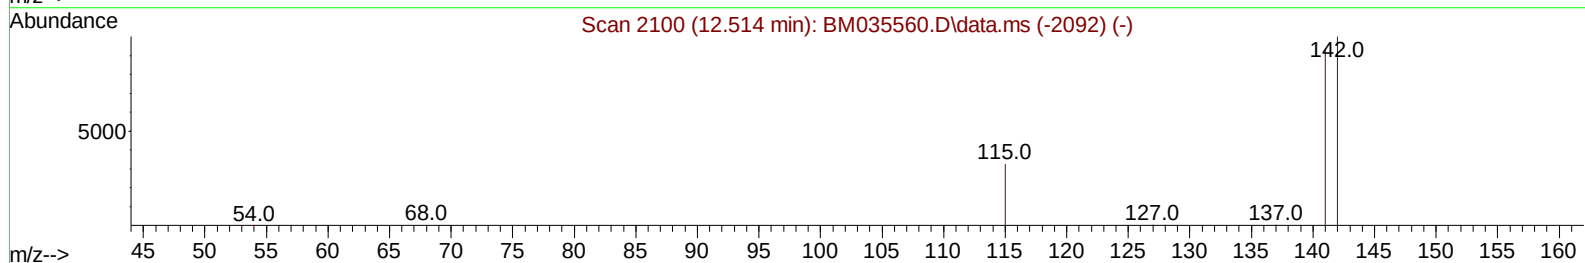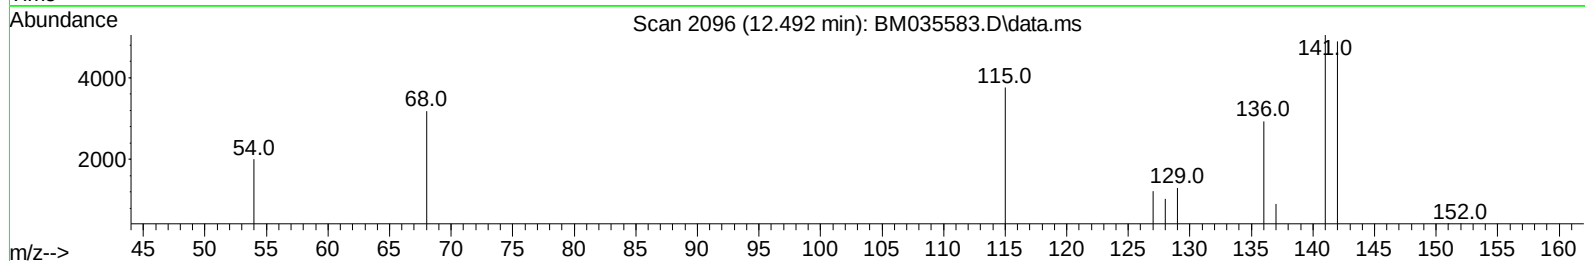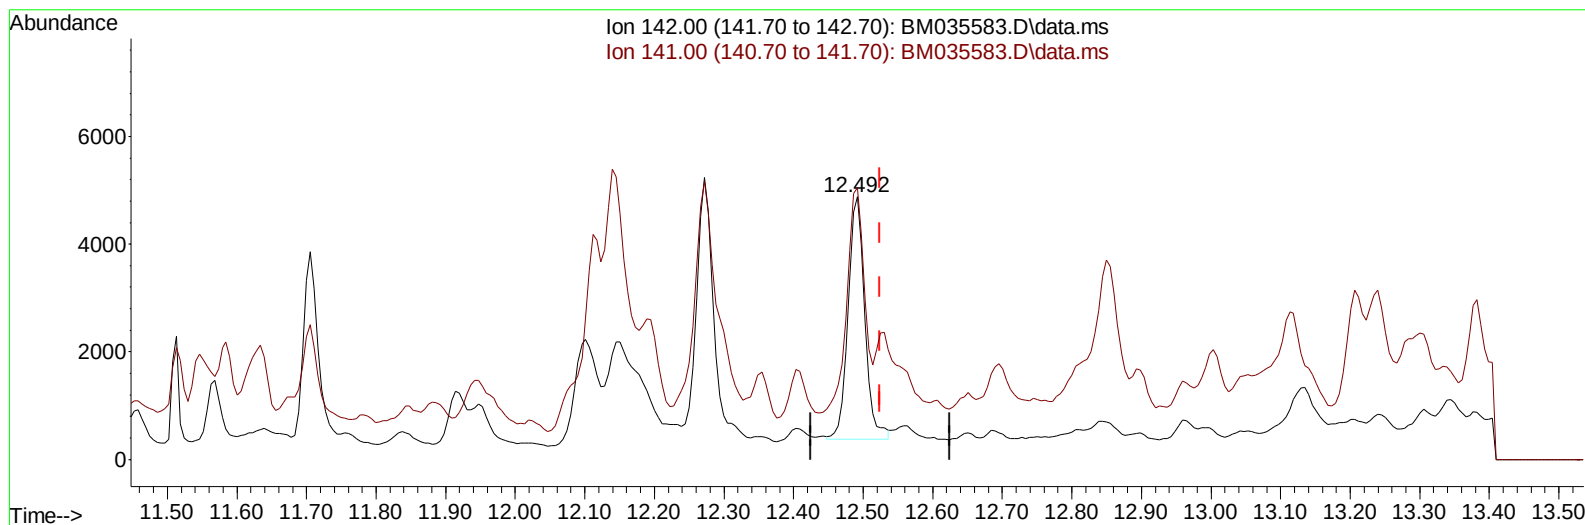

TIC: BM035583.D\data.ms

(8) 1-Methylnaphthalene

12.492min (-0.033) 0.23 ng/ul m

response 7491

Ion	Exp%	Act%
142.00	100.00	100.00
141.00	93.20	19.08#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
 Data File : BM035583.D
 Acq On : 21 Jun 2022 22:13
 Operator : CG/JU
 Sample : N3285-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4P5

Manual IntegrationsAPPROVED

Quant Time: Jun 22 01:33:28 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :Yogesh Patel 06/25/2022

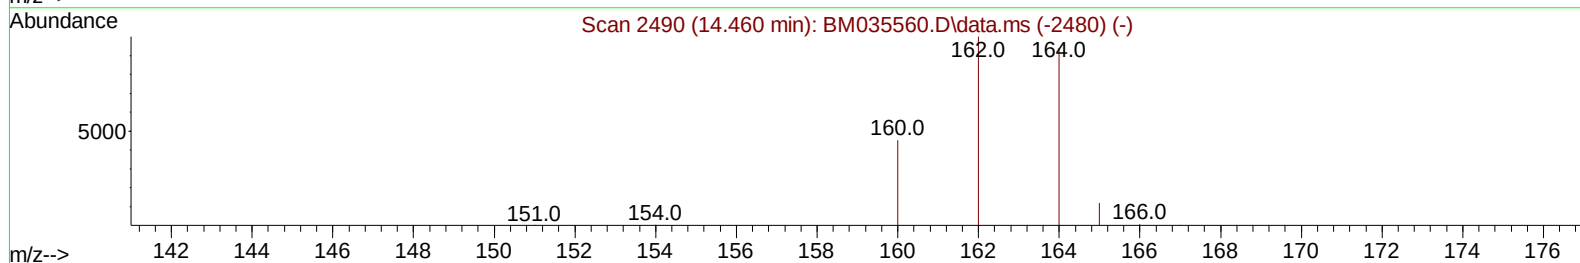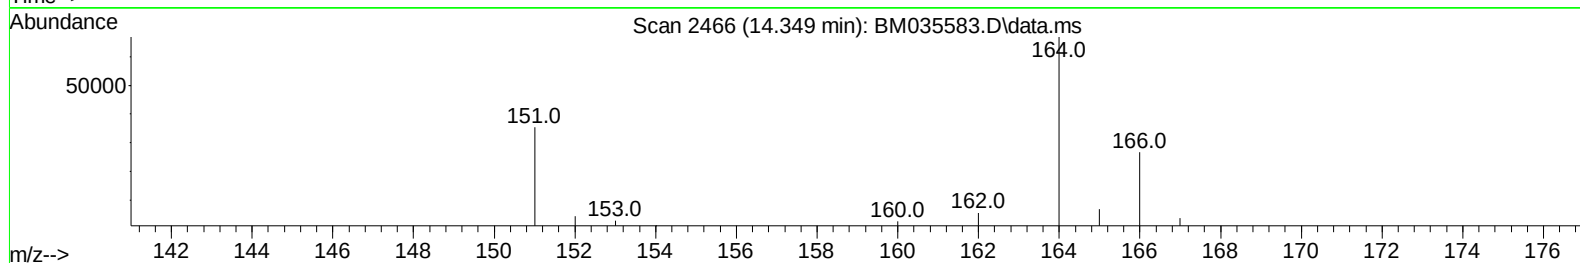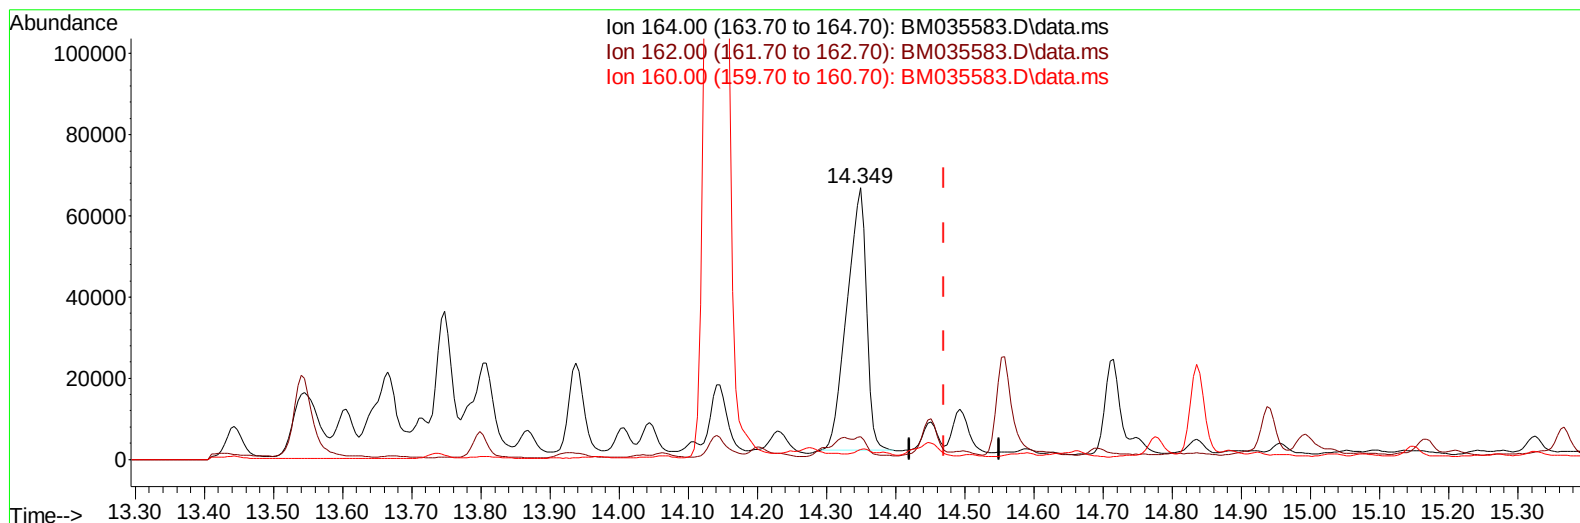

TIC: BM035583.D\data.ms

(9) Acenaphthene-d10 (I)

14.349min (-0.120) 0.40 ng/u1

response 126564

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	106.40	8.33#
160.00	49.90	3.77#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
Data File : BM035583.D
Acq On : 21 Jun 2022 22:13
Operator : CG/JU
Sample : N3285-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4P5

Manual IntegrationsAPPROVED

Quant Time: Jun 22 01:33:28 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/22/2022
Supervised By :Yogesh Patel 06/25/2022

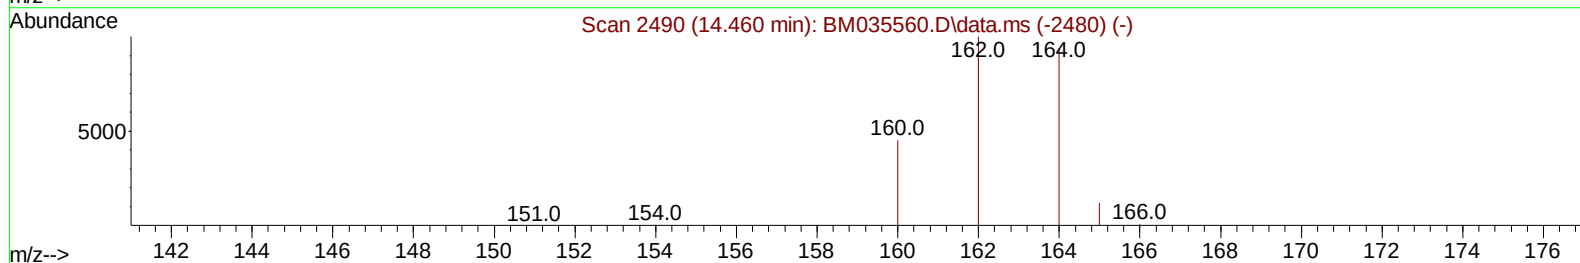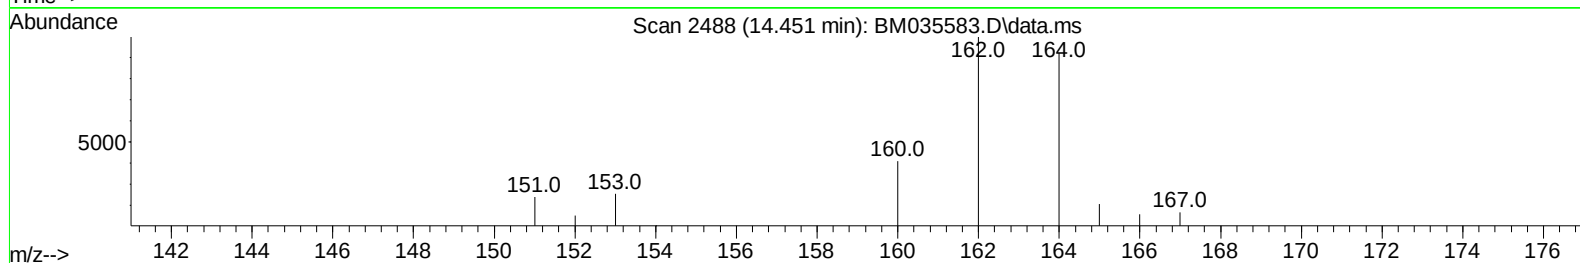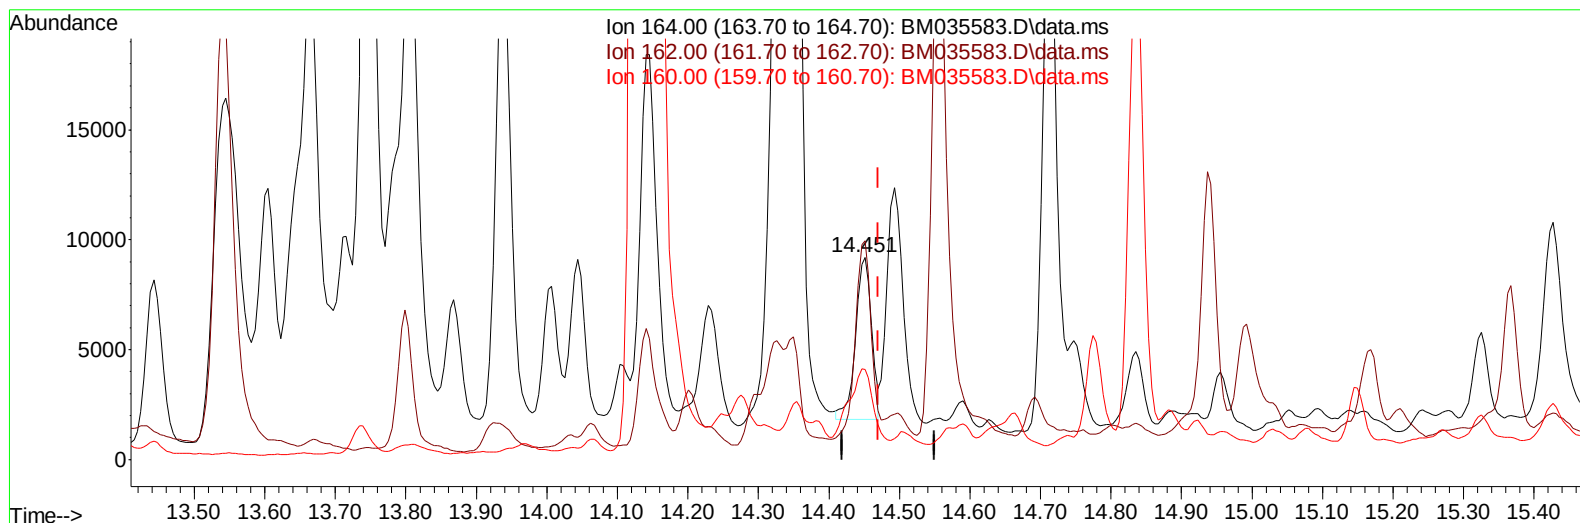

TIC: BM035583.D\data.ms

(9) Acenaphthene-d10 (I)

14.451min (-0.019) 0.40 ng/ul m

response 11539

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	106.40	108.21
160.00	49.90	44.55
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
 Data File : BM035583.D
 Acq On : 21 Jun 2022 22:13
 Operator : CG/JU
 Sample : N3285-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4P5

Manual IntegrationsAPPROVED

Quant Time: Jun 22 01:33:28 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :Yogesh Patel 06/25/2022

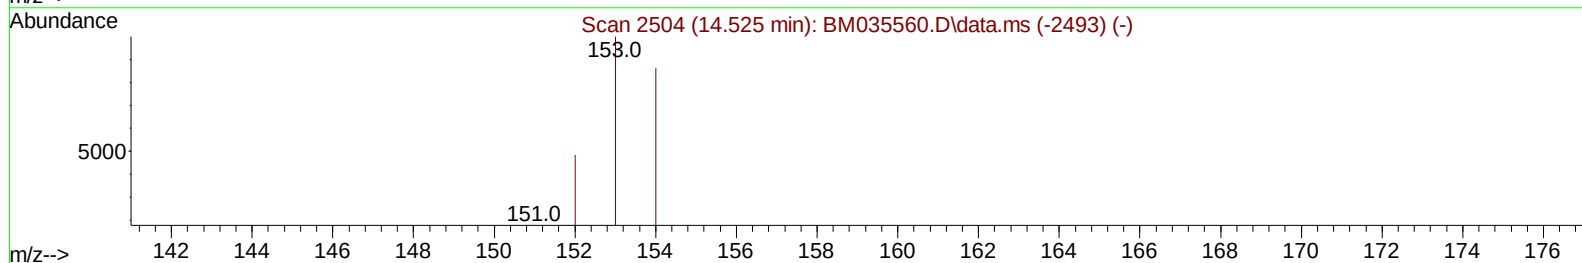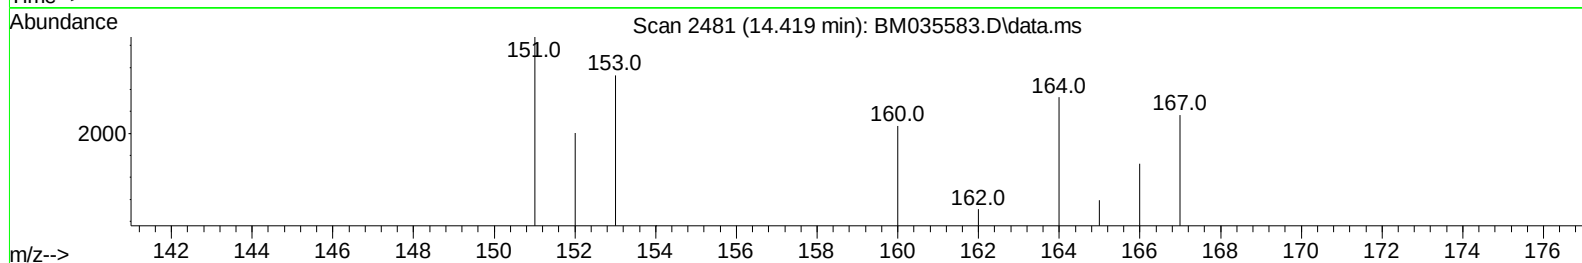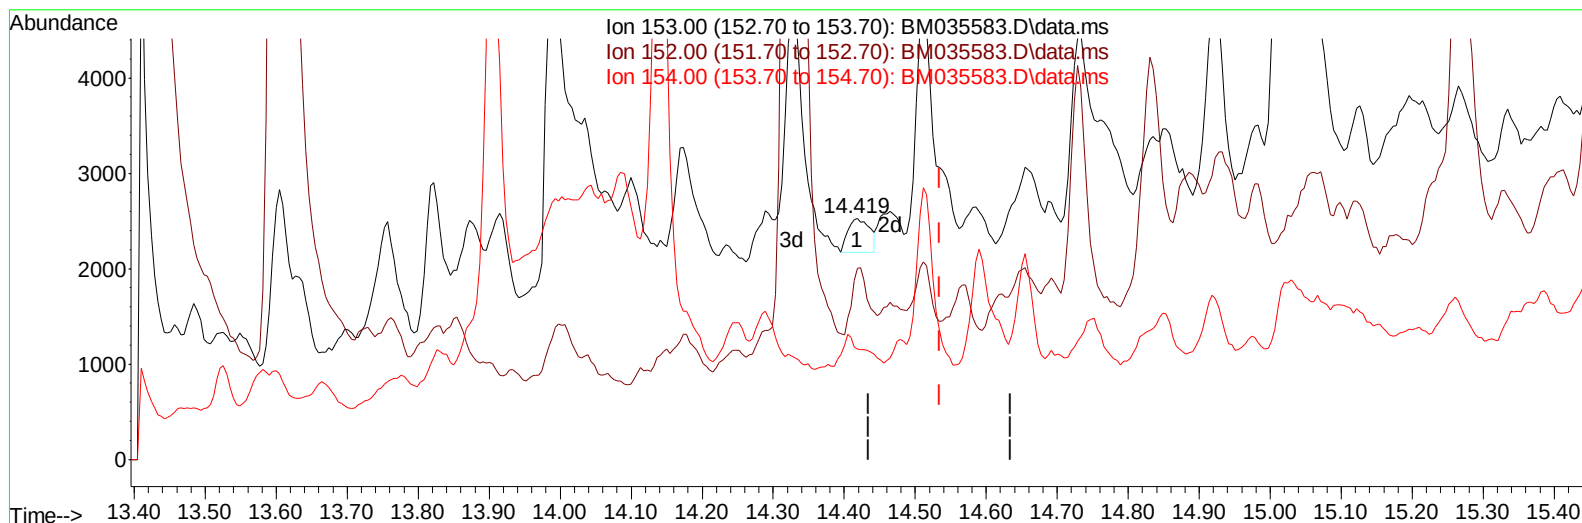

TIC: BM035583.D\data.ms

(11) Acenaphthene (C)

14.419min (-0.116) 0.02 ng/u1

response 753

Ion	Exp%	Act%
153.00	100.00	100.00
152.00	50.00	79.19#
154.00	86.40	45.89#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
 Data File : BM035583.D
 Acq On : 21 Jun 2022 22:13
 Operator : CG/JU
 Sample : N3285-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4P5

Manual IntegrationsAPPROVED

Quant Time: Jun 22 01:33:28 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :Yogesh Patel 06/25/2022

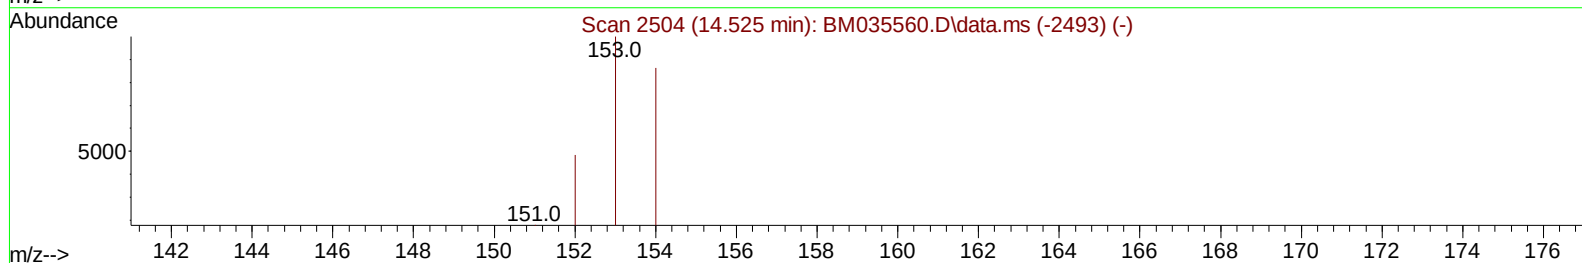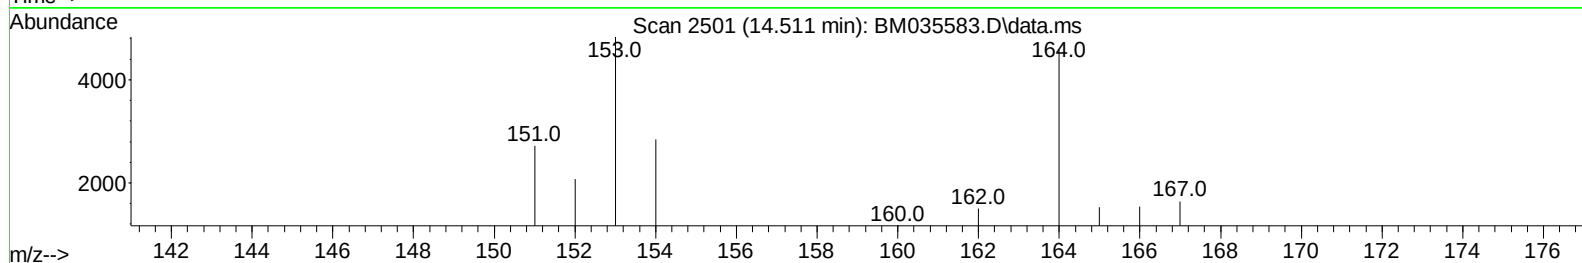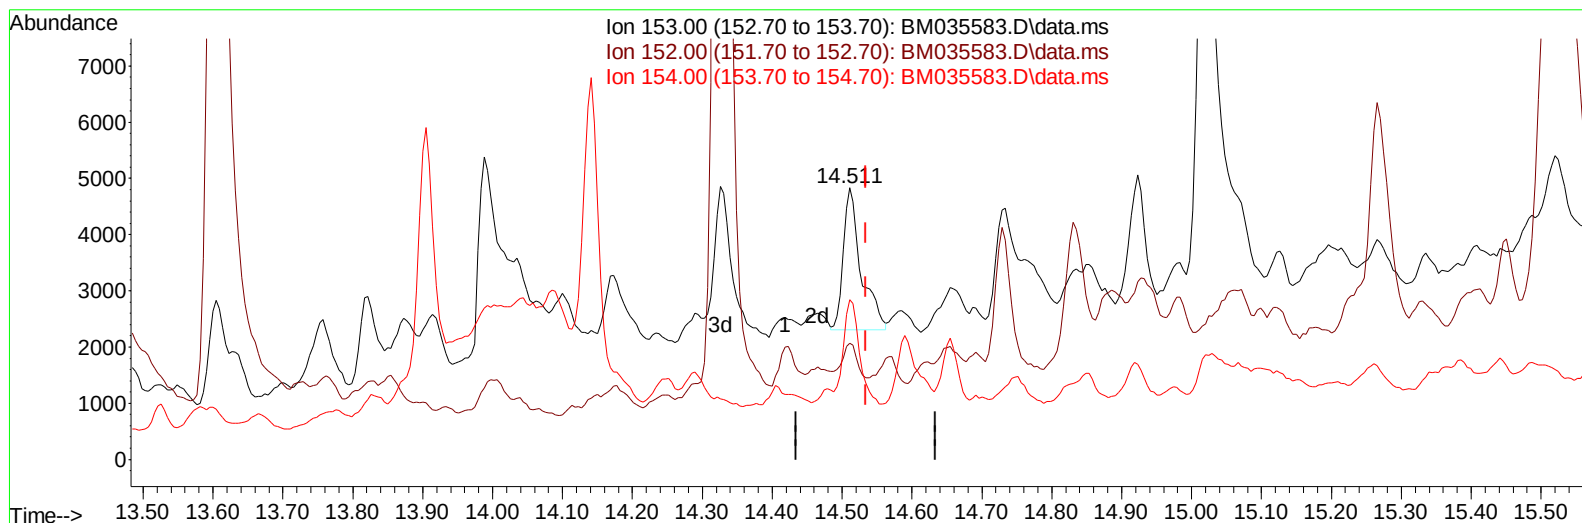

TIC: BM035583.D\data.ms

(11) Acenaphthene (C)

14.511min (-0.023) 0.09 ng/ul m

response 4460

Ion	Exp%	Act%
153.00	100.00	100.00
152.00	50.00	42.84
154.00	86.40	58.94#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
 Data File : BM035583.D
 Acq On : 21 Jun 2022 22:13
 Operator : CG/JU
 Sample : N3285-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4P5

Manual IntegrationsAPPROVED

Quant Time: Jun 22 01:33:28 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :Yogesh Patel 06/25/2022

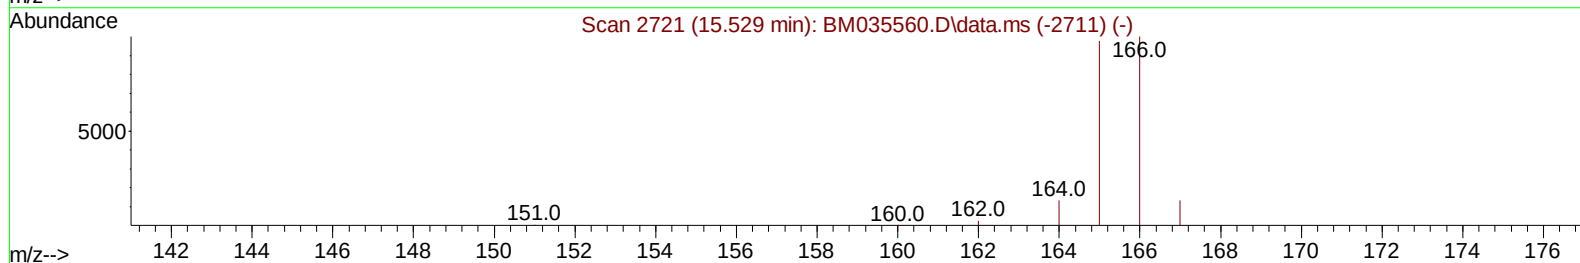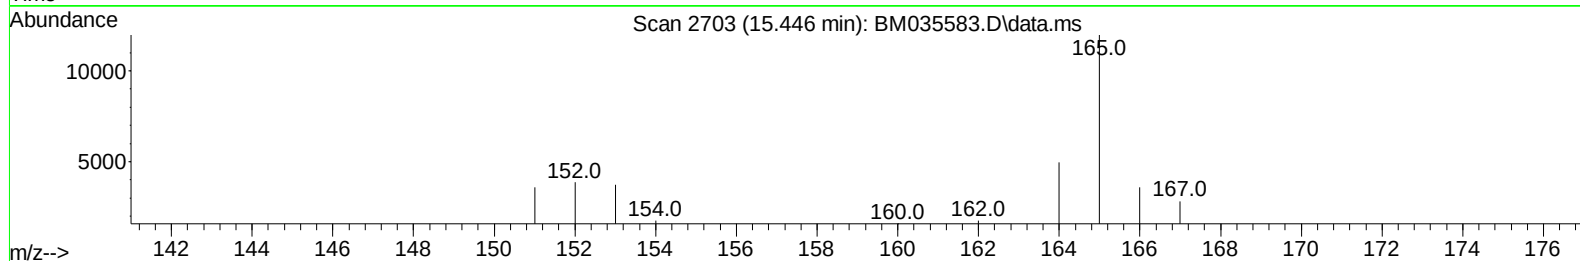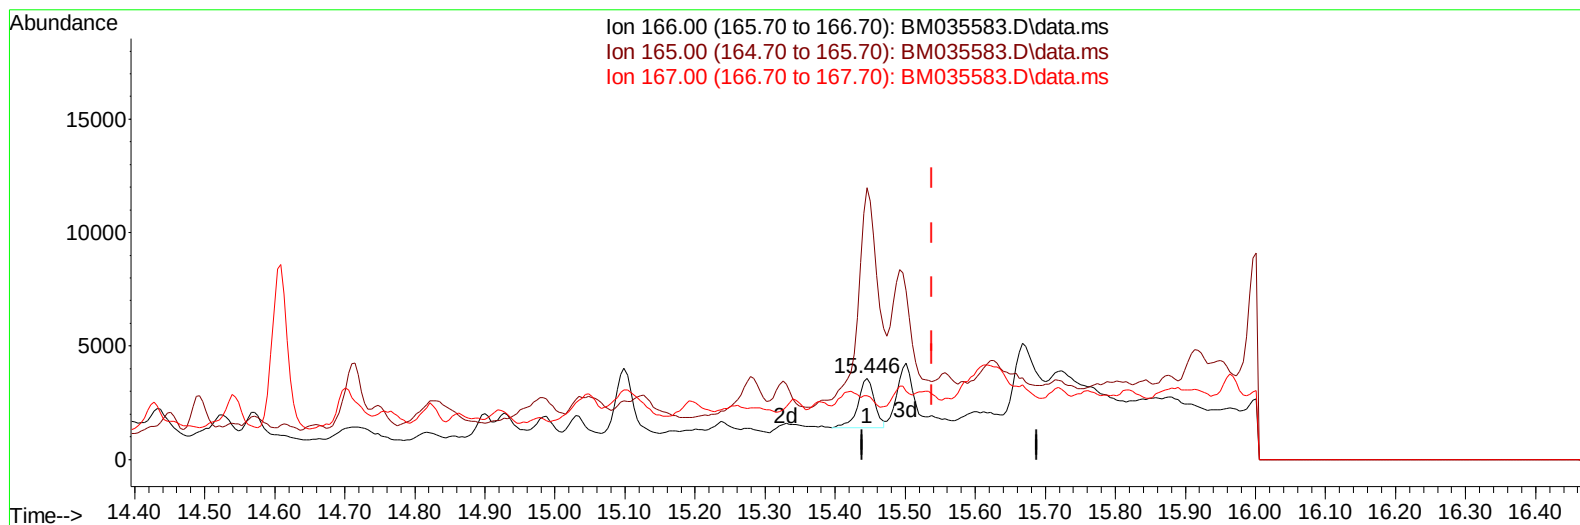

TIC: BM035583.D\data.ms

(12) Fluorene

15.446min (-0.093) 0.07 ng/u1

response 3663

Ion	Exp%	Act%
166.00	100.00	100.00
165.00	98.40	334.58#
167.00	14.50	78.81#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
 Data File : BM035583.D
 Acq On : 21 Jun 2022 22:13
 Operator : CG/JU
 Sample : N3285-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4P5

Manual IntegrationsAPPROVED

Quant Time: Jun 22 01:33:28 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :Yogesh Patel 06/25/2022

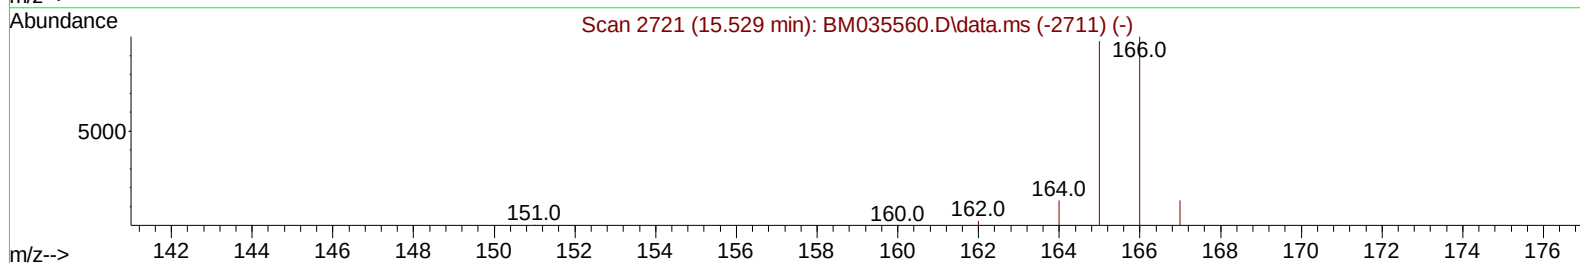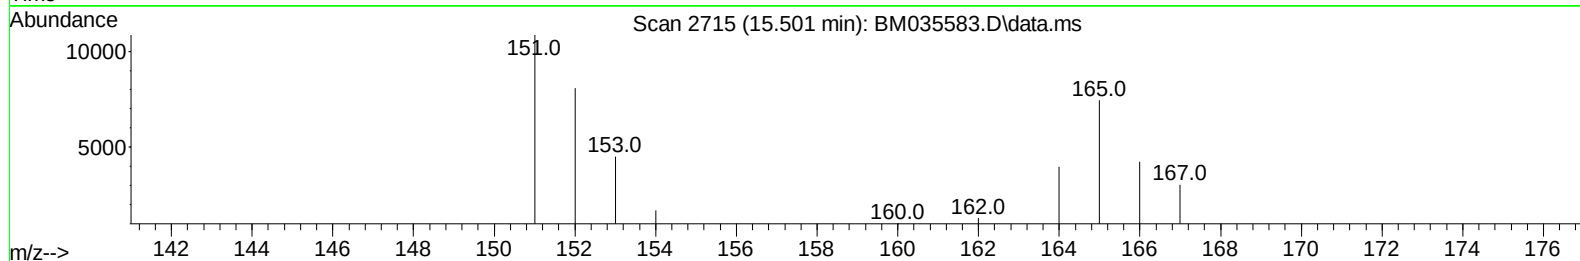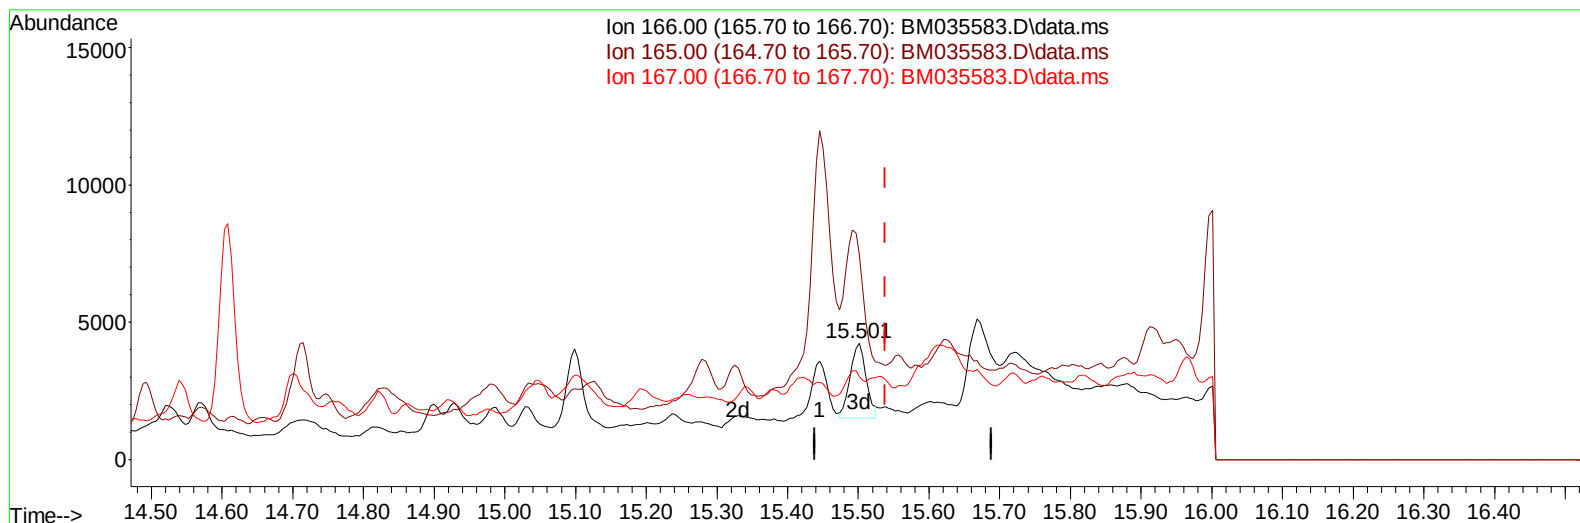

TIC: BM035583.D\data.ms

(12) Fluorene

15.501min (-0.037) 0.08 ng/ul m

response 4253

Ion	Exp%	Act%
166.00	100.00	100.00
165.00	98.40	175.44#
167.00	14.50	71.15#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
 Data File : BM035583.D
 Acq On : 21 Jun 2022 22:13
 Operator : CG/JU
 Sample : N3285-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4P5

Manual IntegrationsAPPROVED

Quant Time: Jun 22 01:33:28 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :Yogesh Patel 06/25/2022

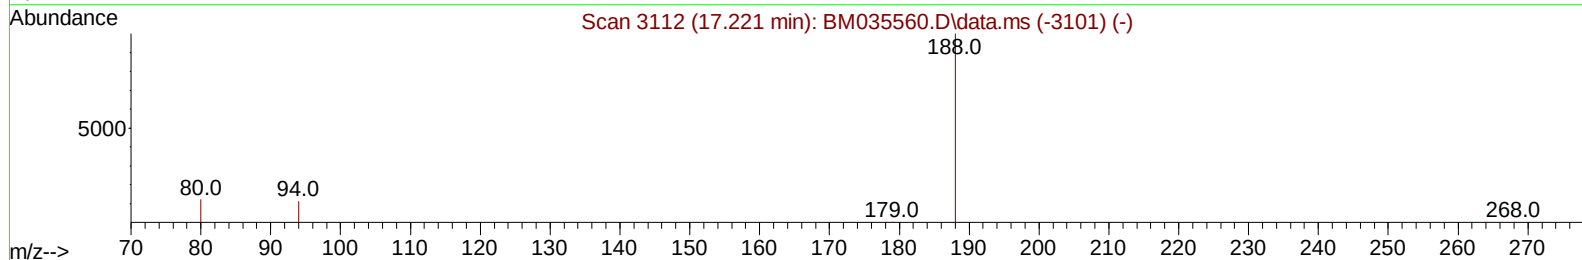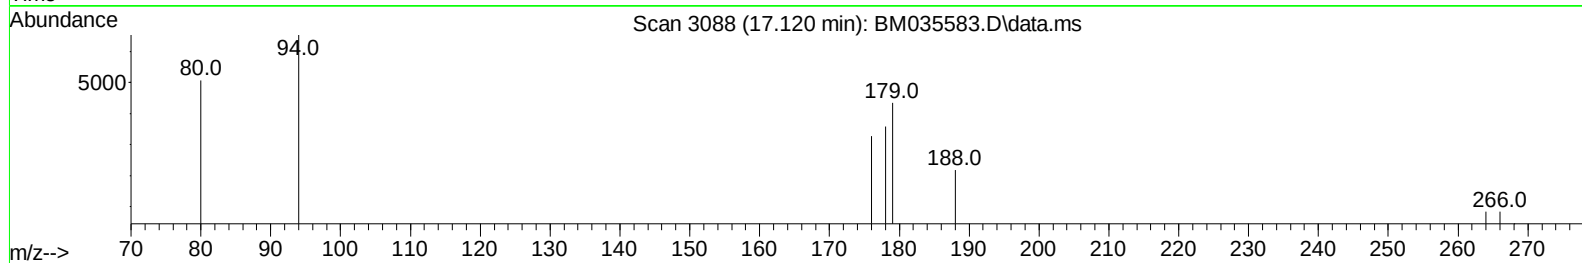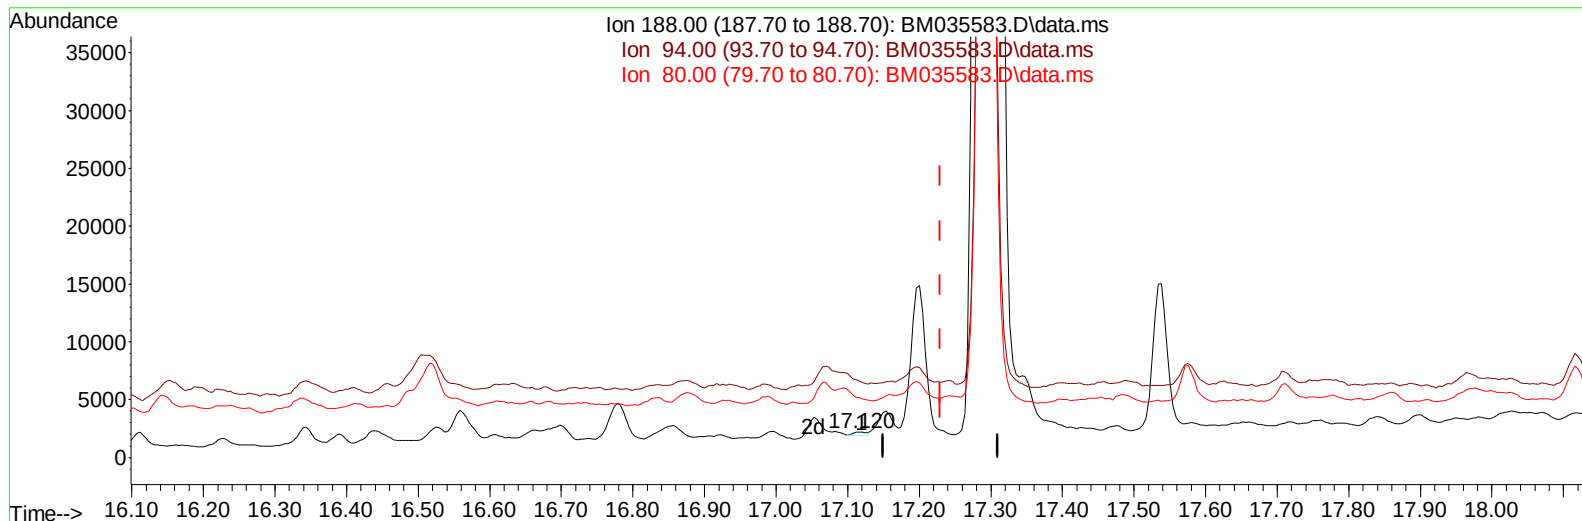

TIC: BM035583.D\data.ms

(13) Phenanthrene-d10 (I)

17.120min (-0.110) 0.40 ng/u1

response 329

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.00	298.08#
80.00	13.50	231.77#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
 Data File : BM035583.D
 Acq On : 21 Jun 2022 22:13
 Operator : CG/JU
 Sample : N3285-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4P5

Manual IntegrationsAPPROVED

Quant Time: Jun 22 01:33:28 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :Yogesh Patel 06/25/2022

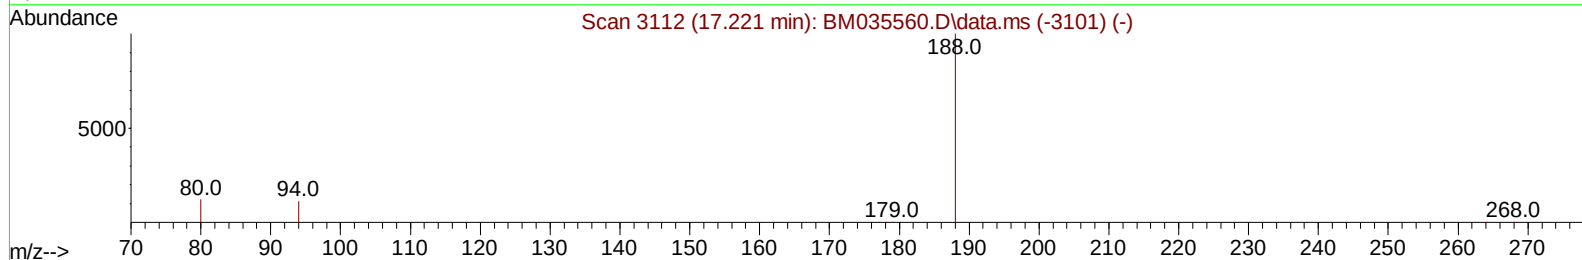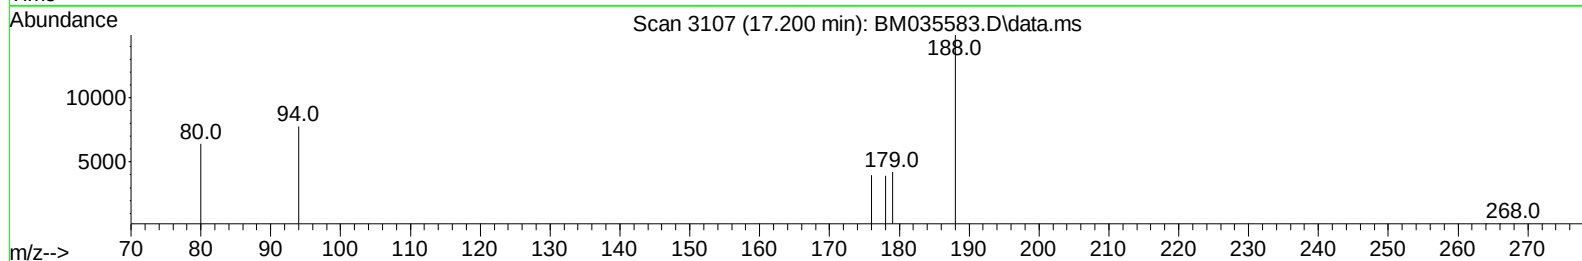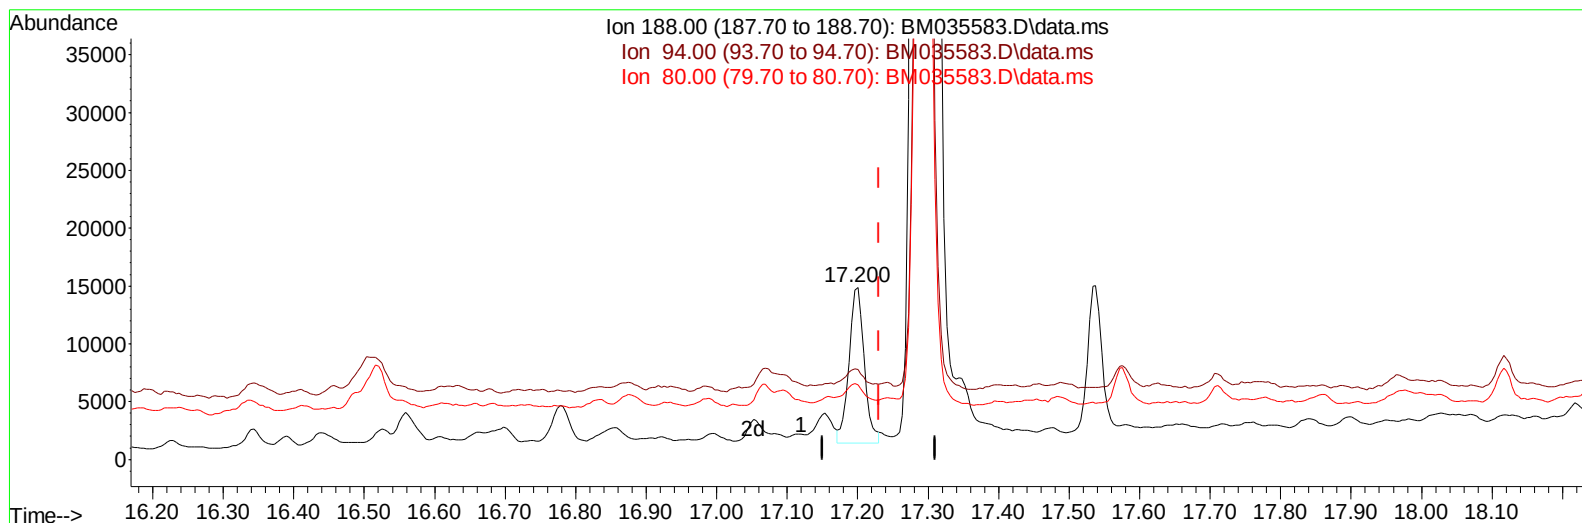

TIC: BM035583.D\data.ms

(13) Phenanthrene-d10 (I)

17.200min (-0.030) 0.40 ng/ul m

response 20361

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.00	52.14#
80.00	13.50	43.26#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
 Data File : BM035583.D
 Acq On : 21 Jun 2022 22:13
 Operator : CG/JU
 Sample : N3285-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4P5

Manual IntegrationsAPPROVED

Quant Time: Jun 22 01:33:28 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :Yogesh Patel 06/25/2022

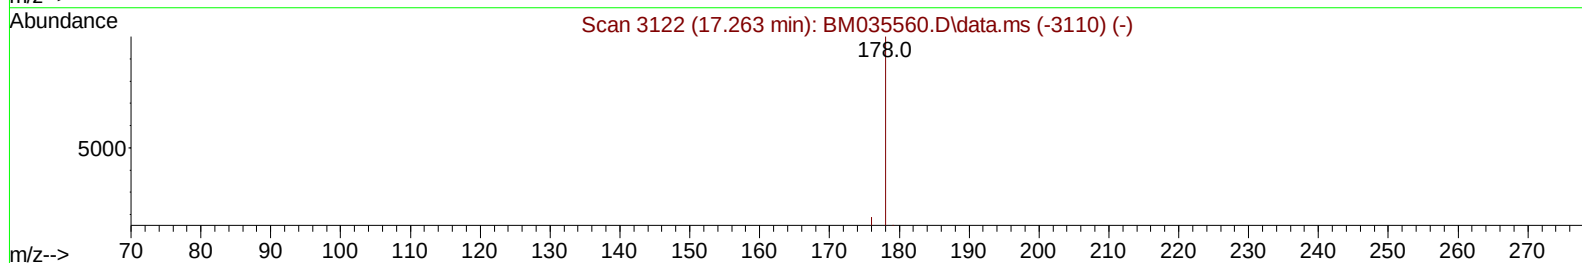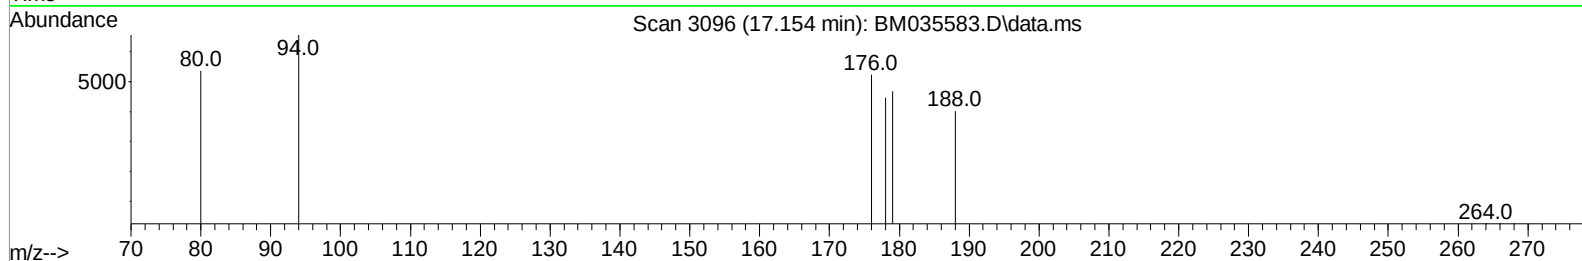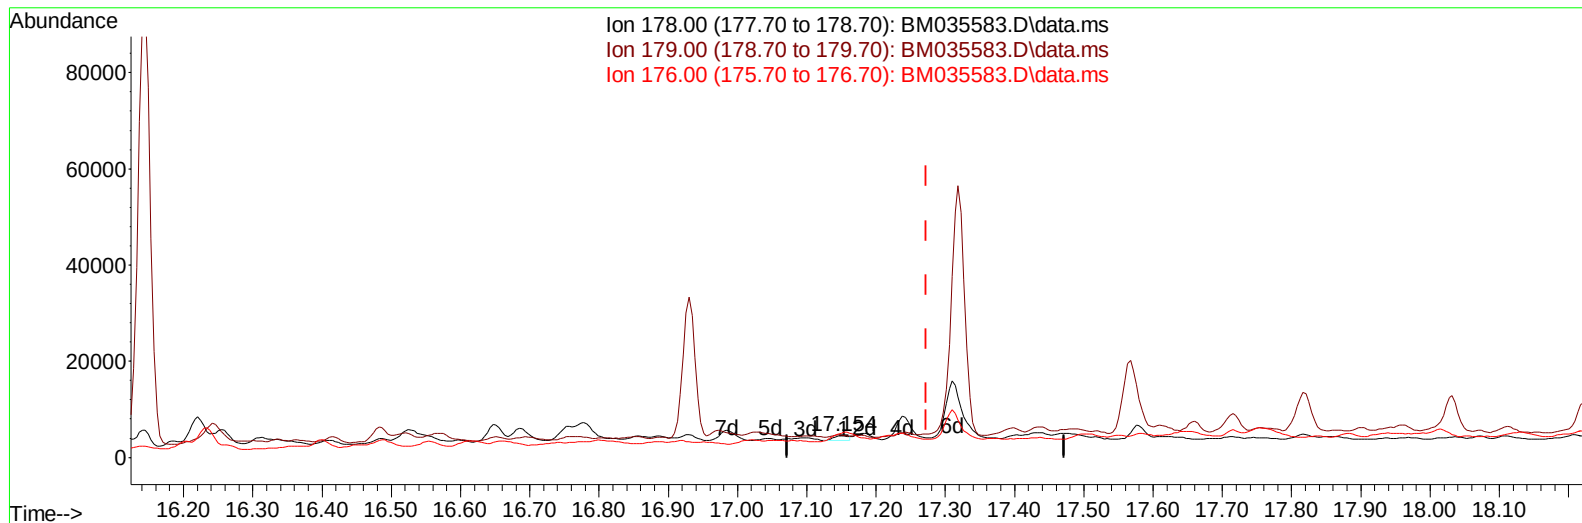

TIC: BM035583.D\data.ms

(15) Phenanthrene

17.154min (-0.118) 0.02 ng/u1

response 1475

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	16.50	104.66#
176.00	20.30	117.39#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
 Data File : BM035583.D
 Acq On : 21 Jun 2022 22:13
 Operator : CG/JU
 Sample : N3285-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4P5

Manual IntegrationsAPPROVED

Quant Time: Jun 22 01:33:28 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :Yogesh Patel 06/25/2022

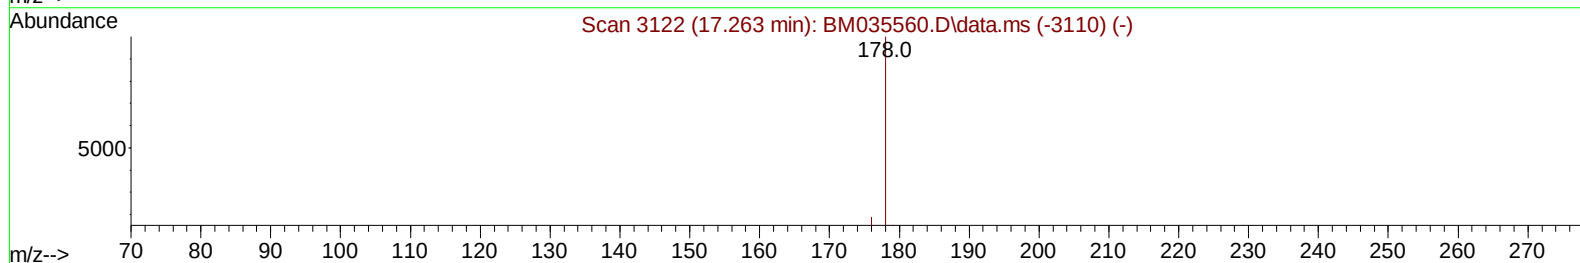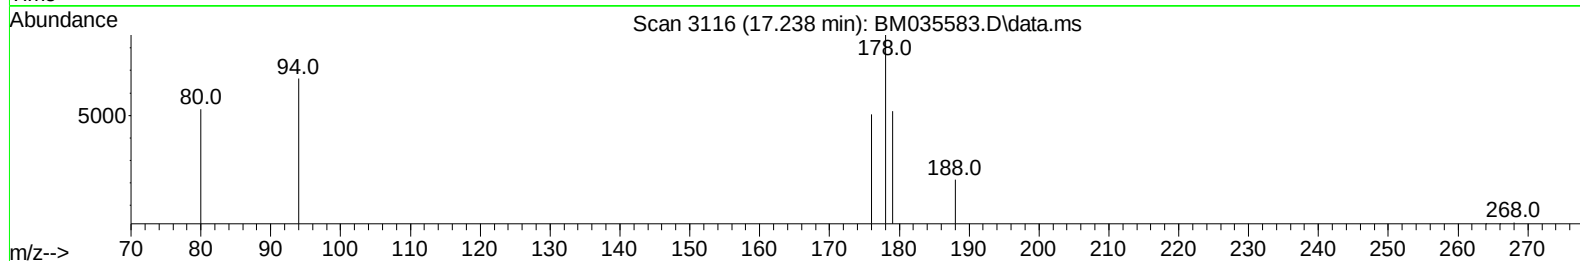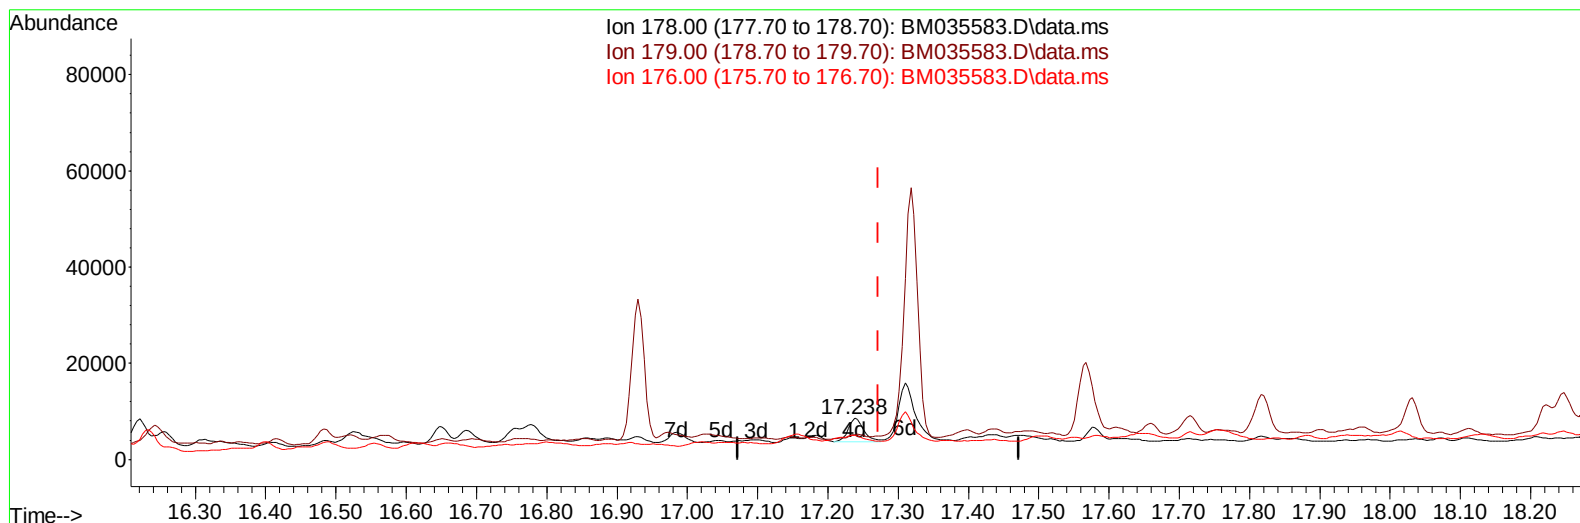

TIC: BM035583.D\data.ms

(15) Phenanthrene

17.238min (-0.034) 0.10 ng/ul m

response 7304

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	16.50	60.46#
176.00	20.30	58.91#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
 Data File : BM035583.D
 Acq On : 21 Jun 2022 22:13
 Operator : CG/JU
 Sample : N3285-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4P5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :Yogesh Patel 06/25/2022

Quant Time: Jun 22 01:33:28 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.812	152		4925	0.400	ng/ul	#-0.05
4) Naphthalene-d8	10.600	136		18075m	0.400	ng/ul	-0.04
9) Acenaphthene-d10	14.451	164		11539m	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.200	188		20361m	0.400	ng/ul	-0.03
17) Chrysene-d12	21.391	240		20137	0.400	ng/ul	#-0.02
23) Perylene-d12	23.726	264		19137	0.400	ng/ul	#-0.04
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.264	96		31281	4.514	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.200	152		9614	0.358	ng/ul	-0.04
18) Fluoranthene-d10	19.230	212		15186	0.224	ng/ul	-0.02
Target Compounds							
							Qvalue
2) 1,4-Dioxane	3.297	88		56965	8.257	ng/ul#	64
5) Naphthalene	10.649	128		18632m	0.304	ng/ul	
7) 2-Methylnaphthalene	12.272	142		7577m	0.217	ng/ul	
8) 1-Methylnaphthalene	12.492	142		7491m	0.233	ng/ul	
11) Acenaphthene	14.511	153		4460m	0.093	ng/ul	
12) Fluorene	15.501	166		4253m	0.078	ng/ul	
14) Pentachlorophenol	16.867	266		2639	0.676	ng/ul	98
15) Phenanthrene	17.238	178		7304m	0.098	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
Data File : BM035583.D
Acq On : 21 Jun 2022 22:13
Operator : CG/JU
Sample : N3285-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4P5

Manual IntegrationsAPPROVED

Quant Time: Jun 22 01:33:28 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/22/2022
Supervised By :Yogesh Patel 06/25/2022

