




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
Data File : BM035596.D
Acq On : 22 Jun 2022 06:40
Operator : CG/JU
Sample : PB145517BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK517

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/22/2022
Supervised By :Yogesh Patel 06/25/2022

Quant Time: Jun 22 07:18:35 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

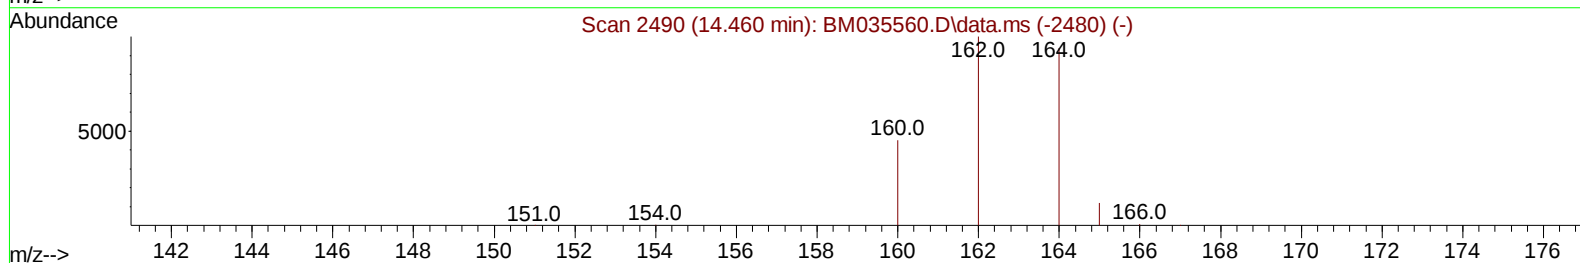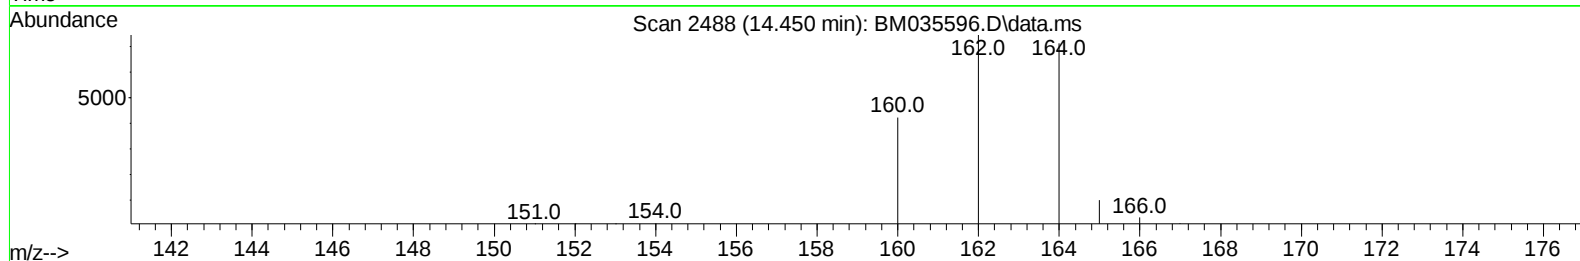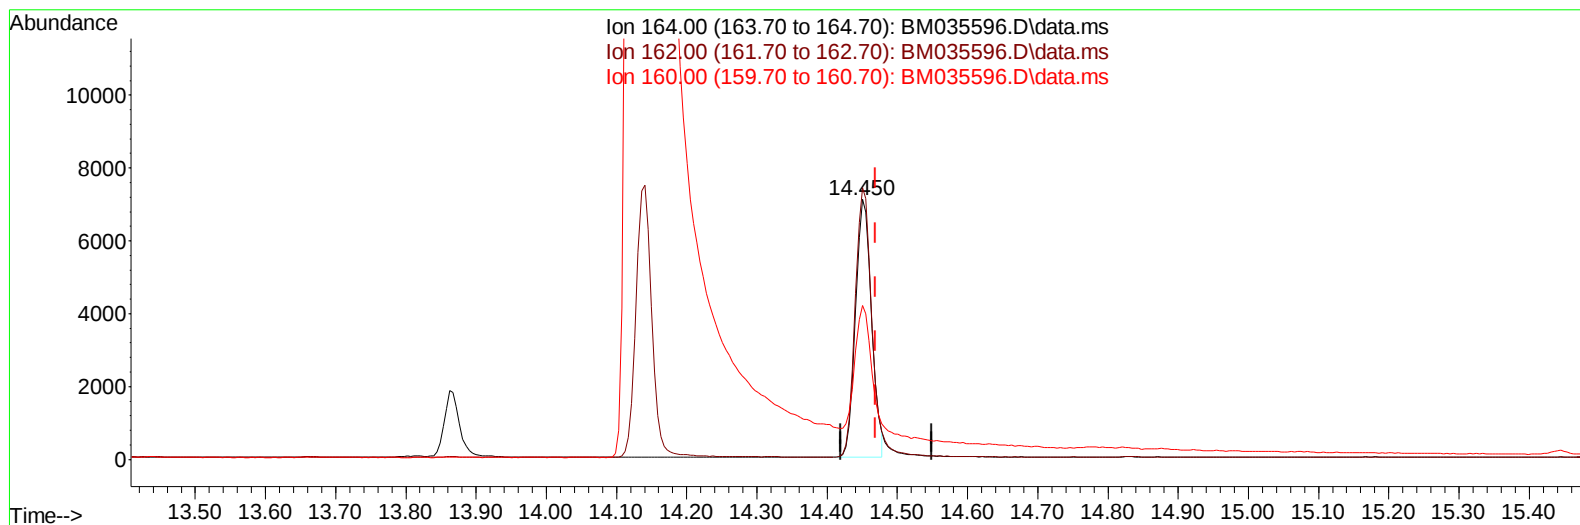

TIC: BM035596.D\data.ms

(9) Acenaphthene-d10 (I)

14.450min (-0.019) 0.40 ng/u1

response 11080

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	106.40	104.41
160.00	49.90	59.20
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
Data File : BM035596.D
Acq On : 22 Jun 2022 06:40
Operator : CG/JU
Sample : PB145517BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK517

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/22/2022
Supervised By :Yogesh Patel 06/25/2022

Quant Time: Jun 22 07:18:35 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

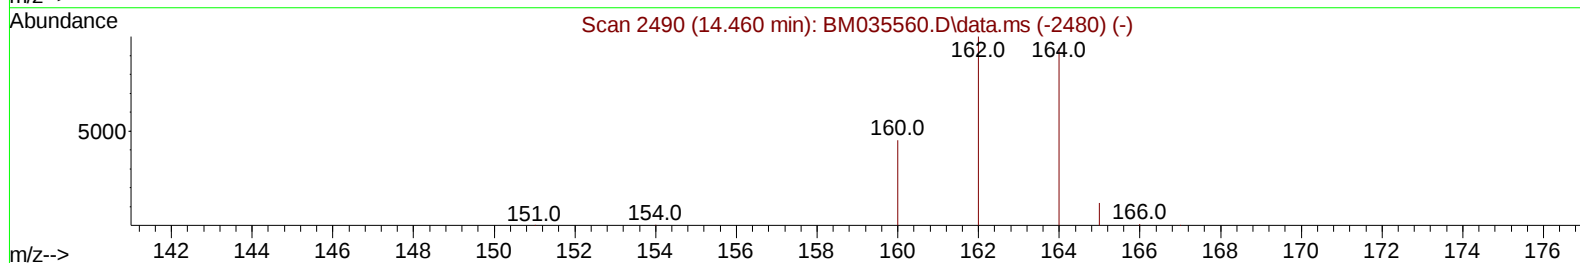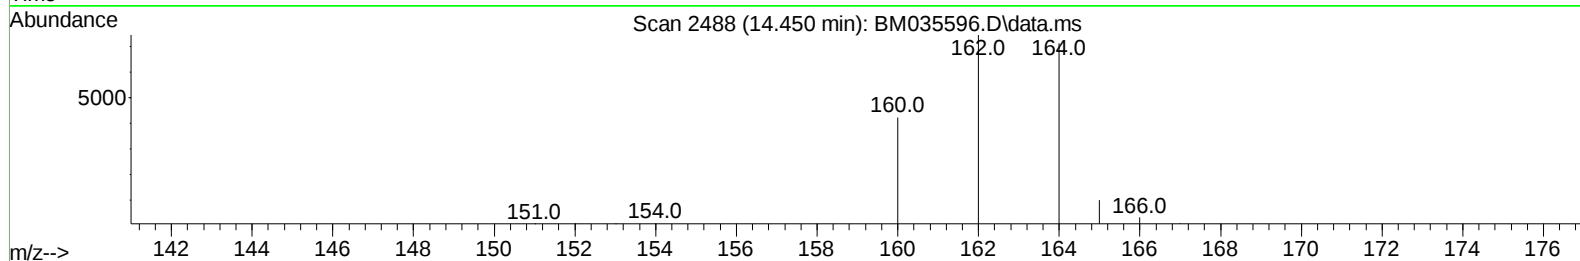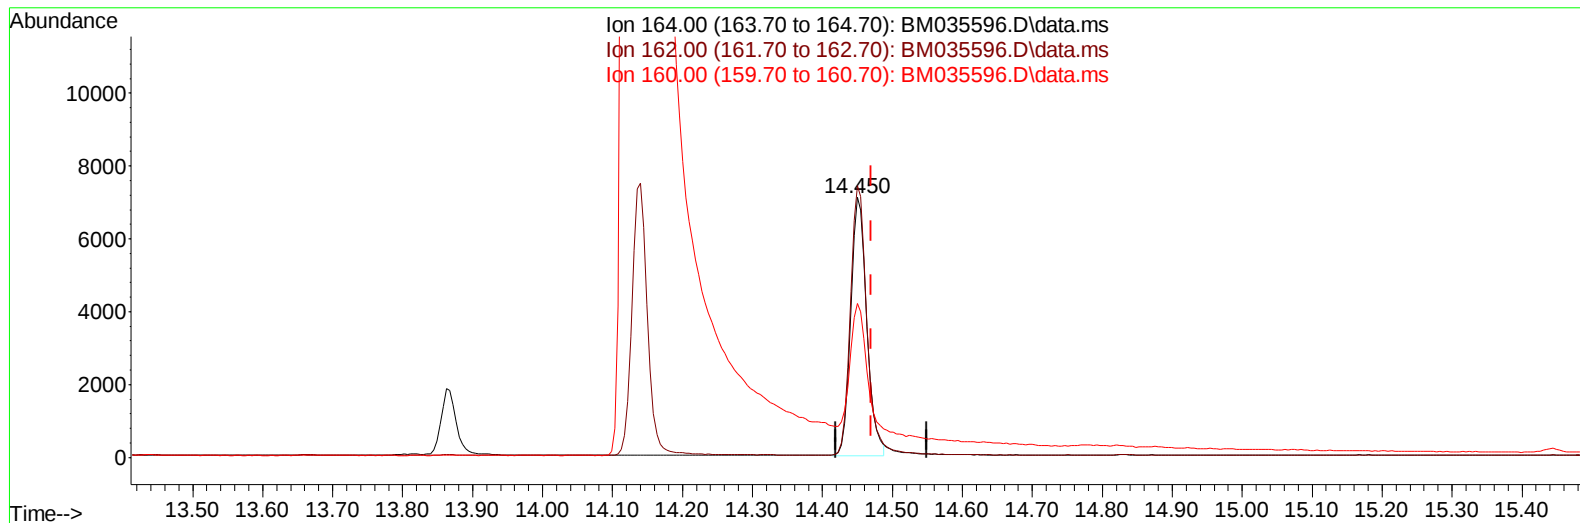

TIC: BM035596.D\data.ms

(9) Acenaphthene-d10 (I)

14.450min (-0.019) 0.40 ng/u1 m

response 11368

Ion	Exp%	Act%
164.00	100.00	100.00
162.00	106.40	104.41
160.00	49.90	59.20
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
 Data File : BM035596.D
 Acq On : 22 Jun 2022 06:40
 Operator : CG/JU
 Sample : PB145517BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK517

Manual IntegrationsAPPROVED

Quant Time: Jun 22 07:18:35 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :Yogesh Patel 06/25/2022

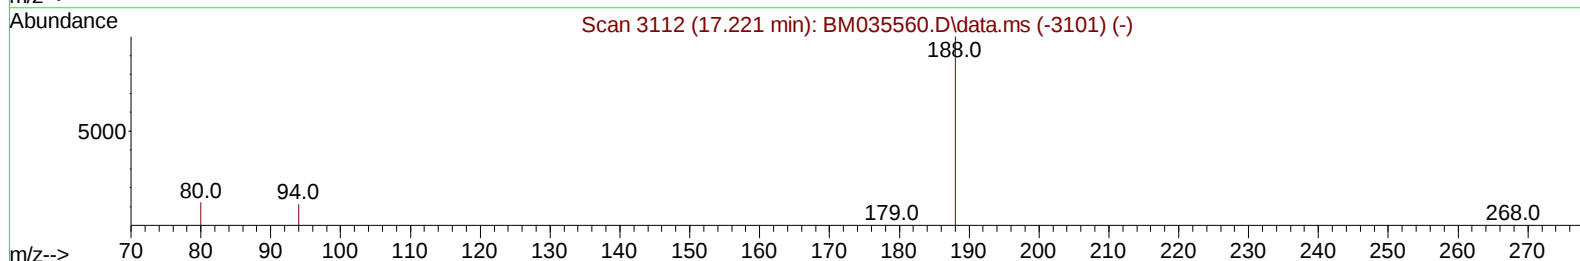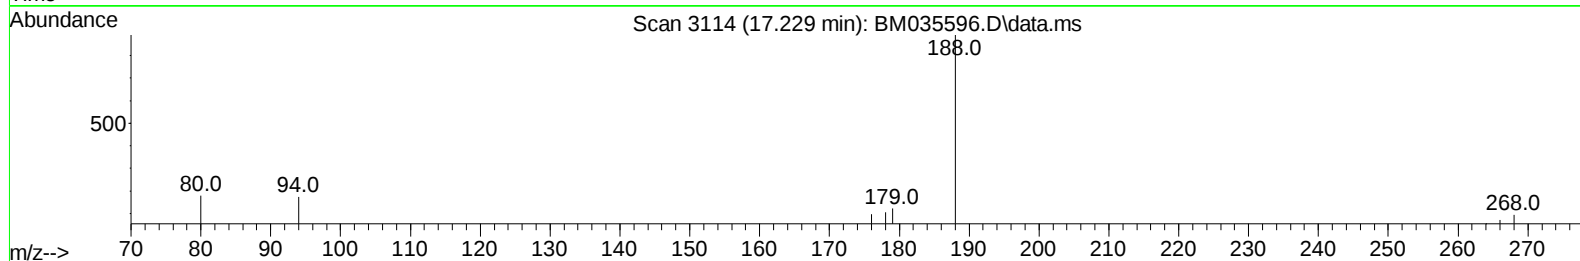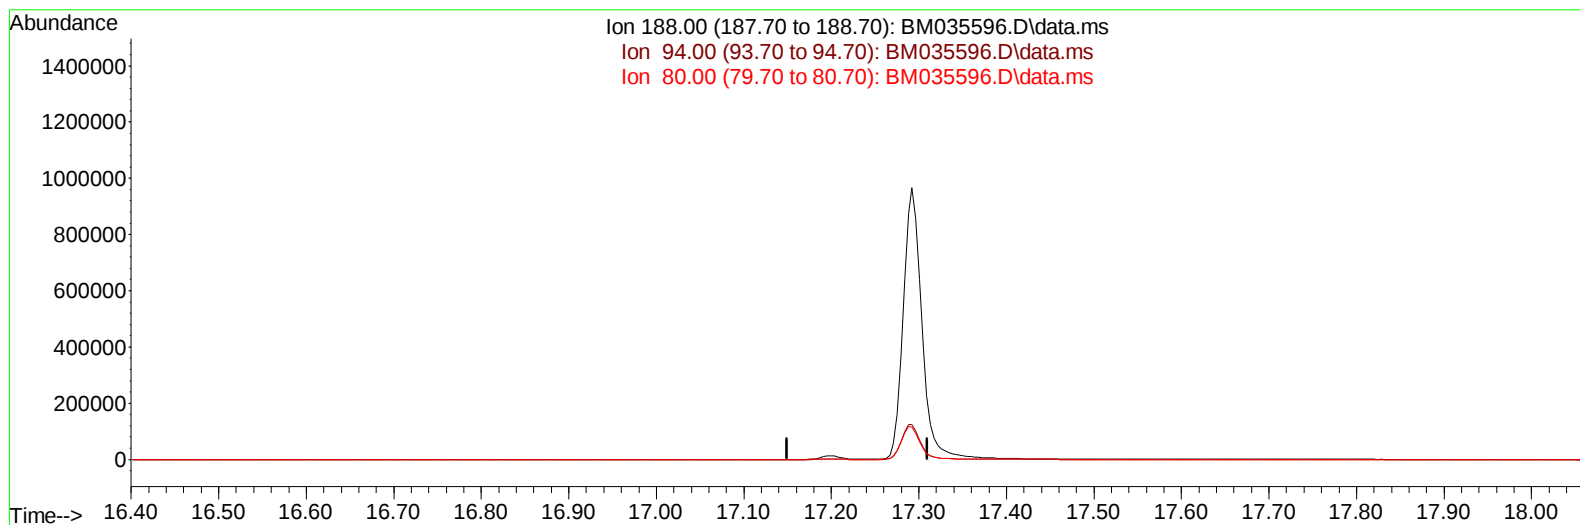

TIC: BM035596.D\data.ms

(13) Phenanthrene-d10 (I)

17.230min (-17.230) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	12.00	0.00#
80.00	13.50	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
 Data File : BM035596.D
 Acq On : 22 Jun 2022 06:40
 Operator : CG/JU
 Sample : PB145517BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK517

Manual IntegrationsAPPROVED

Quant Time: Jun 22 07:18:35 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :Yogesh Patel 06/25/2022

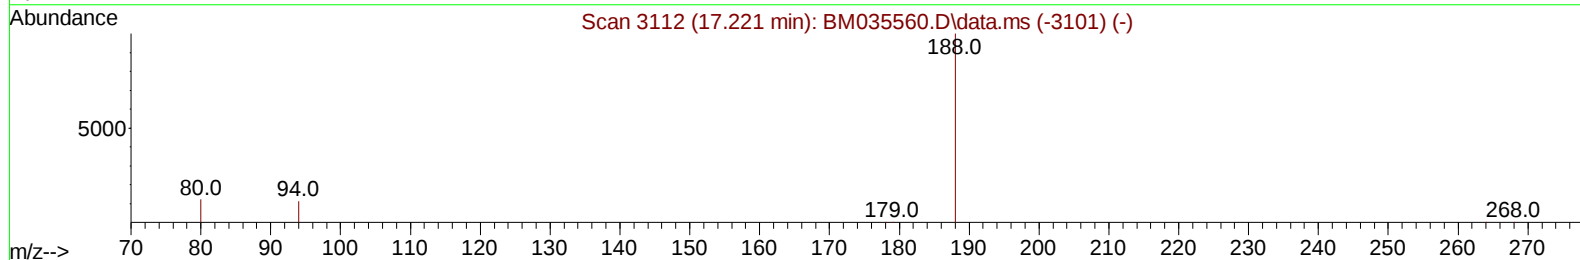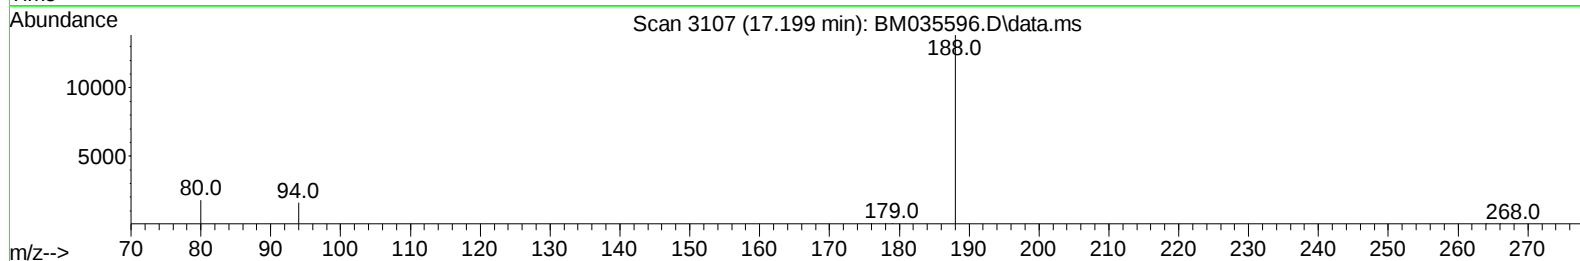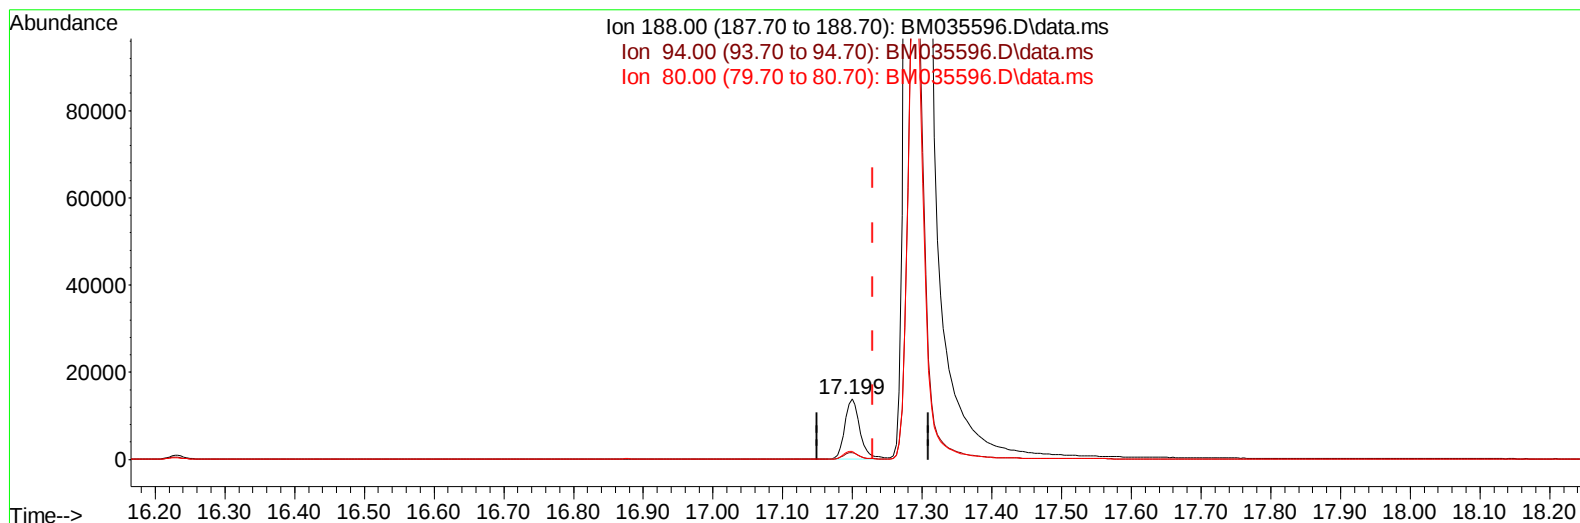

TIC: BM035596.D\data.ms

(13) Phenanthrene-d10 (I)

17.199min (-0.030) 0.40 ng/ul m

response 20856

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.00	11.52
80.00	13.50	12.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
 Data File : BM035596.D
 Acq On : 22 Jun 2022 06:40
 Operator : CG/JU
 Sample : PB145517BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK517

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :Yogesh Patel 06/25/2022

Quant Time: Jun 22 07:18:35 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.820	152		5958	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.605	136		19893	0.400	ng/ul	-0.04
9) Acenaphthene-d10	14.450	164		11368m	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.199	188		20856m	0.400	ng/ul	-0.03
17) Chrysene-d12	21.412	240		13834	0.400	ng/ul	0.00
23) Perylene-d12	23.733	264		16845	0.400	ng/ul	#-0.03
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.264	96		42977	5.127	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.244	152		8620	0.292	ng/ul	0.00
18) Fluoranthene-d10	19.233	212		14596	0.314	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
Data File : BM035596.D
Acq On : 22 Jun 2022 06:40
Operator : CG/JU
Sample : PB145517BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK517

Manual IntegrationsAPPROVED

Quant Time: Jun 22 07:18:35 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/22/2022
Supervised By :Yogesh Patel 06/25/2022

