

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
 Data File : BM035565.D
 Acq On : 21 Jun 2022 10:42
 Operator : CG/JU
 Sample : N3285-06
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4P9

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :Yogesh Patel 06/25/2022

Quant Time: Jun 22 01:32:11 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 20 01:56:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.821	152	5857	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.606	136	20697	0.400	ng/ul	-0.04
9) Acenaphthene-d10	14.455	164	11750m	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.199	188	22768m	0.400	ng/ul	-0.03
17) Chrysene-d12	21.401	240	17827	0.400	ng/ul	-0.01
23) Perylene-d12	23.736	264	19842	0.400	ng/ul	#-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	34721	4.213	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.222	152	9909	0.322	ng/ul	-0.02
18) Fluoranthene-d10	19.233	212	22696	0.379	ng/ul	-0.02
Target Compounds						
5) Naphthalene	10.661	128	2706	0.039	ng/ul#	Qvalue 90

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
Data File : BM035565.D
Acq On : 21 Jun 2022 10:42
Operator : CG/JU
Sample : N3285-06
Misc :
ALS Vial : 44 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
EW4P9

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 06/22/2022
Supervised By :Yogesh Patel 06/25/2022


Quant Time: Jun 22 01:32:11 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

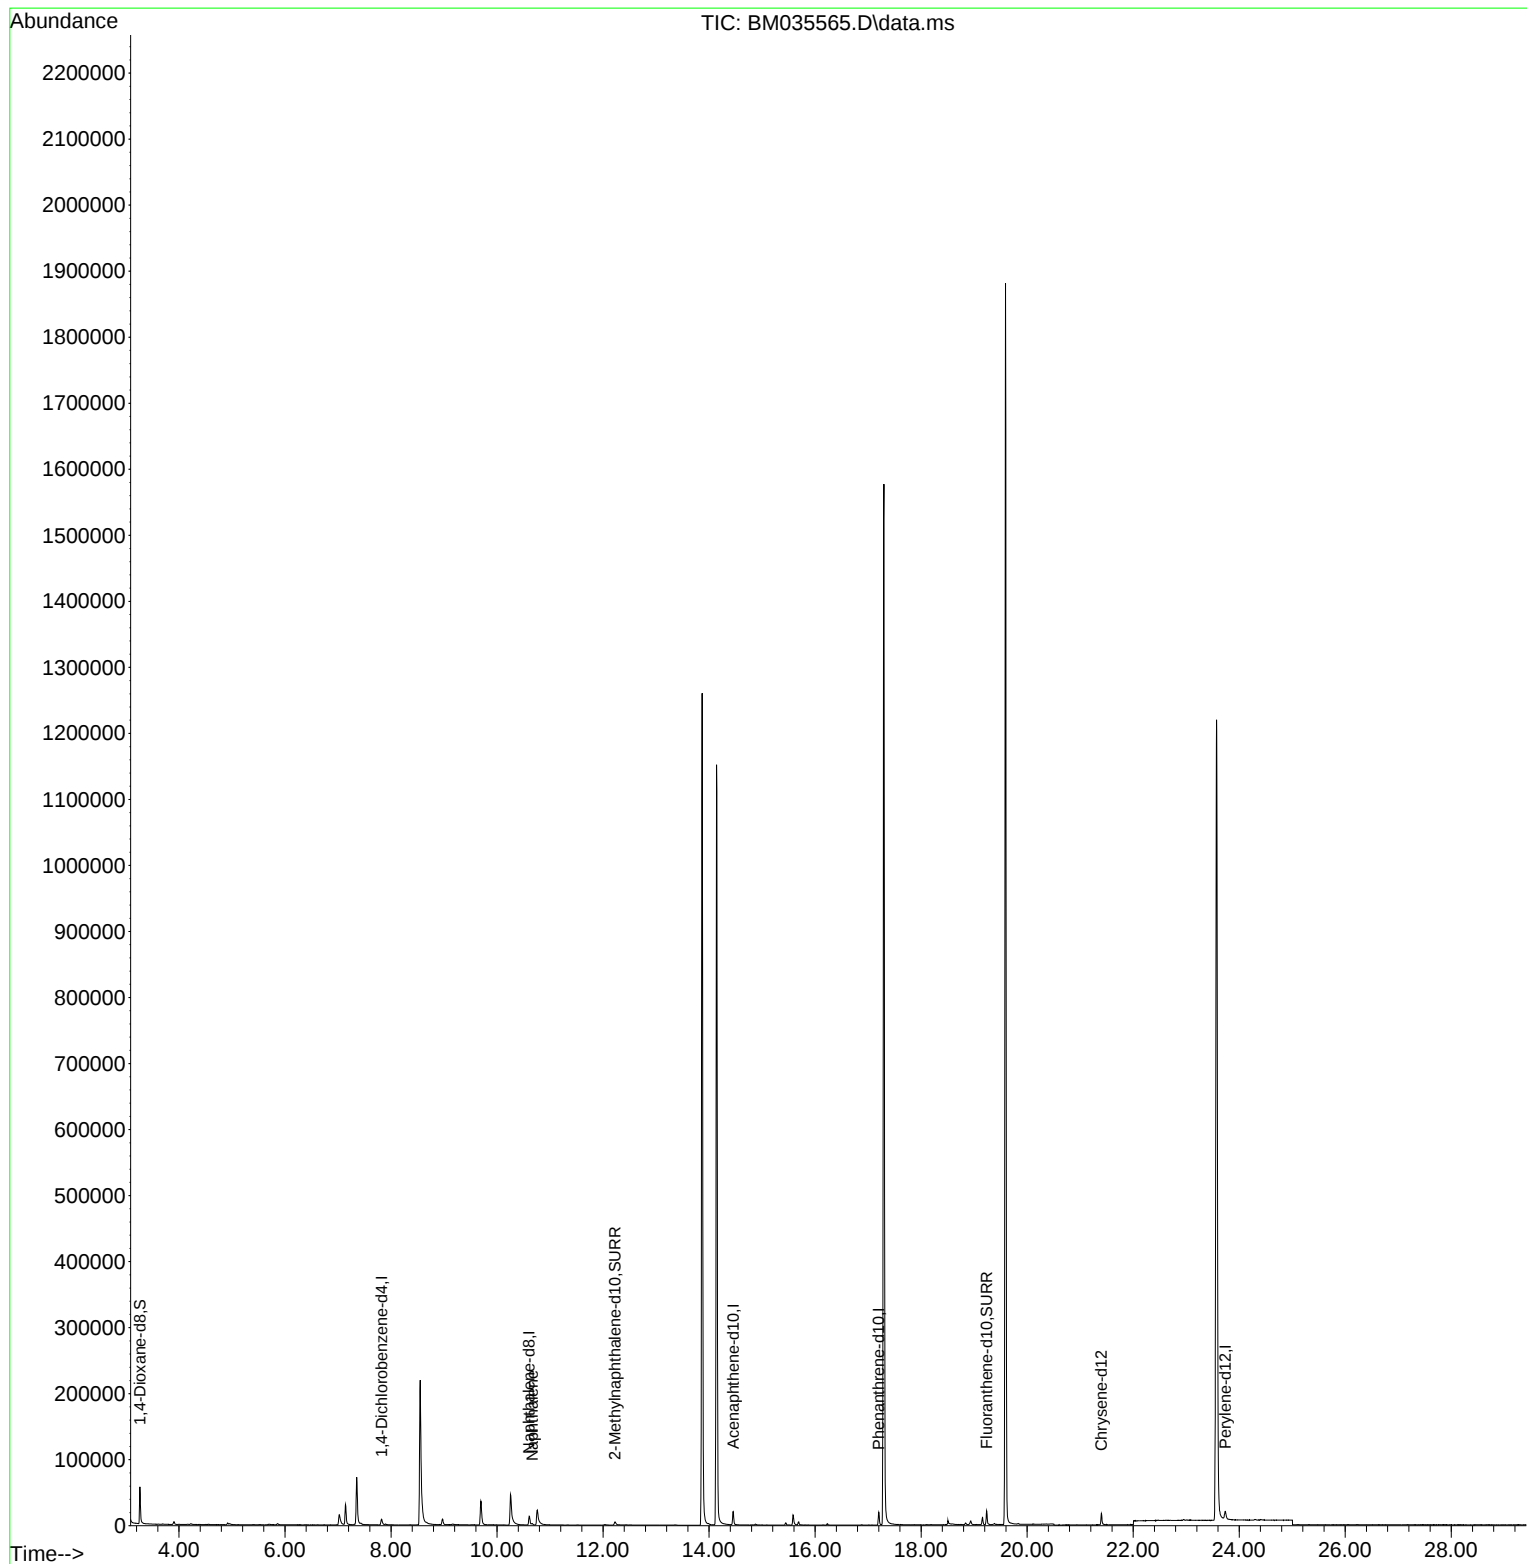

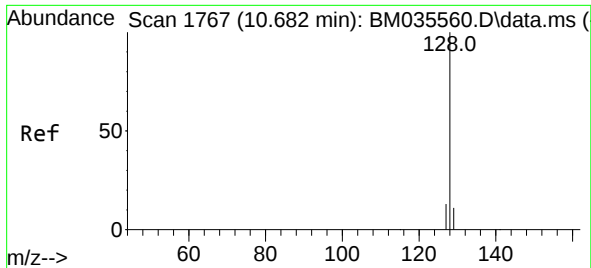

#5
Naphthalene
Concen: 0.039 ng/ul
RT: 10.661 min Scan# 11
Delta R.T. -0.033 min
Lab File: BM035565.D
Acq: 21 Jun 2022 10:42

Instrument :
BNA_M
ClientSampleId :
EW4P9

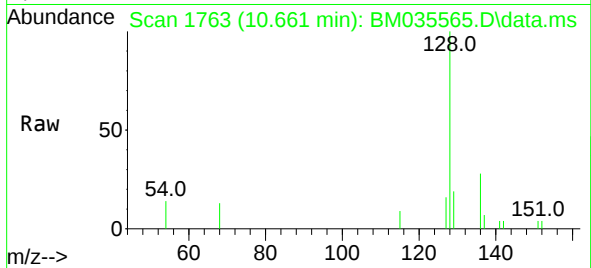

Tgt Ion:128 Resp: 2700
Ion Ratio Lower Upper
128 100
129 19.0 10.1 15.1
127 16.3 11.4 17.2

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 06/22/2022
Supervised By :Yogesh Patel 06/25/2022

