

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
 Data File : BM035566.D
 Acq On : 21 Jun 2022 11:19
 Operator : CG/JU
 Sample : N3298-01
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AA0

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 06/22/2022
 Supervised By :Yogesh Patel 06/25/2022

Quant Time: Jun 22 01:32:15 2022

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Jun 20 01:56:13 2022

Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.820	152	5094	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.605	136	16637	0.400	ng/ul	-0.04
9) Acenaphthene-d10	14.451	164	10609	0.400	ng/ul	#-0.02
13) Phenanthrene-d10	17.196	188	19306m	0.400	ng/ul	-0.03
17) Chrysene-d12	21.388	240	15897	0.400	ng/ul	-0.02
23) Perylene-d12	23.726	264	16406	0.400	ng/ul	#-0.04
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	30418	4.244	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.206	152	9668	0.391	ng/ul	-0.04
18) Fluoranthene-d10	19.225	212	21562	0.404	ng/ul	-0.03
Target Compounds						
					Qvalue	
5) Naphthalene	10.655	128	31592	0.561	ng/ul	98
7) 2-Methylnaphthalene	12.277	142	825	0.026	ng/ul#	60
8) 1-Methylnaphthalene	12.492	142	20836	0.705	ng/ul	99
10) Acenaphthylene	14.169	152	153640	2.571	ng/ul#	95
11) Acenaphthene	14.516	153	5202032	117.554	ng/ul	97
12) Fluorene	15.501	166	2093120	41.826	ng/ul	98
15) Phenanthrene	17.238	178	46084m	0.651	ng/ul	
16) Anthracene	17.327	178	266603	4.303	ng/ul	98
19) Fluoranthene	19.257	202	914092	11.248	ng/ul	100
20) Pyrene	19.620	202	355963	4.178	ng/ul	100
21) Benzo(a)anthracene	21.373	228	15510	0.258	ng/ul#	89
22) Chrysene	21.400	228	9833m	0.137	ng/ul	
24) Benzo(b)fluoranthene	23.019	252	1871	0.026	ng/ul#	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062022\
Data File : BM035566.D
Acq On : 21 Jun 2022 11:19
Operator : CG/JU
Sample : N3298-01
Misc :
ALS Vial : 45 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0AA0

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 06/22/2022
Supervised By :Yogesh Patel 06/25/2022


Quant Time: Jun 22 01:32:15 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM061822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 20 01:56:13 2022
Response via : Initial Calibration

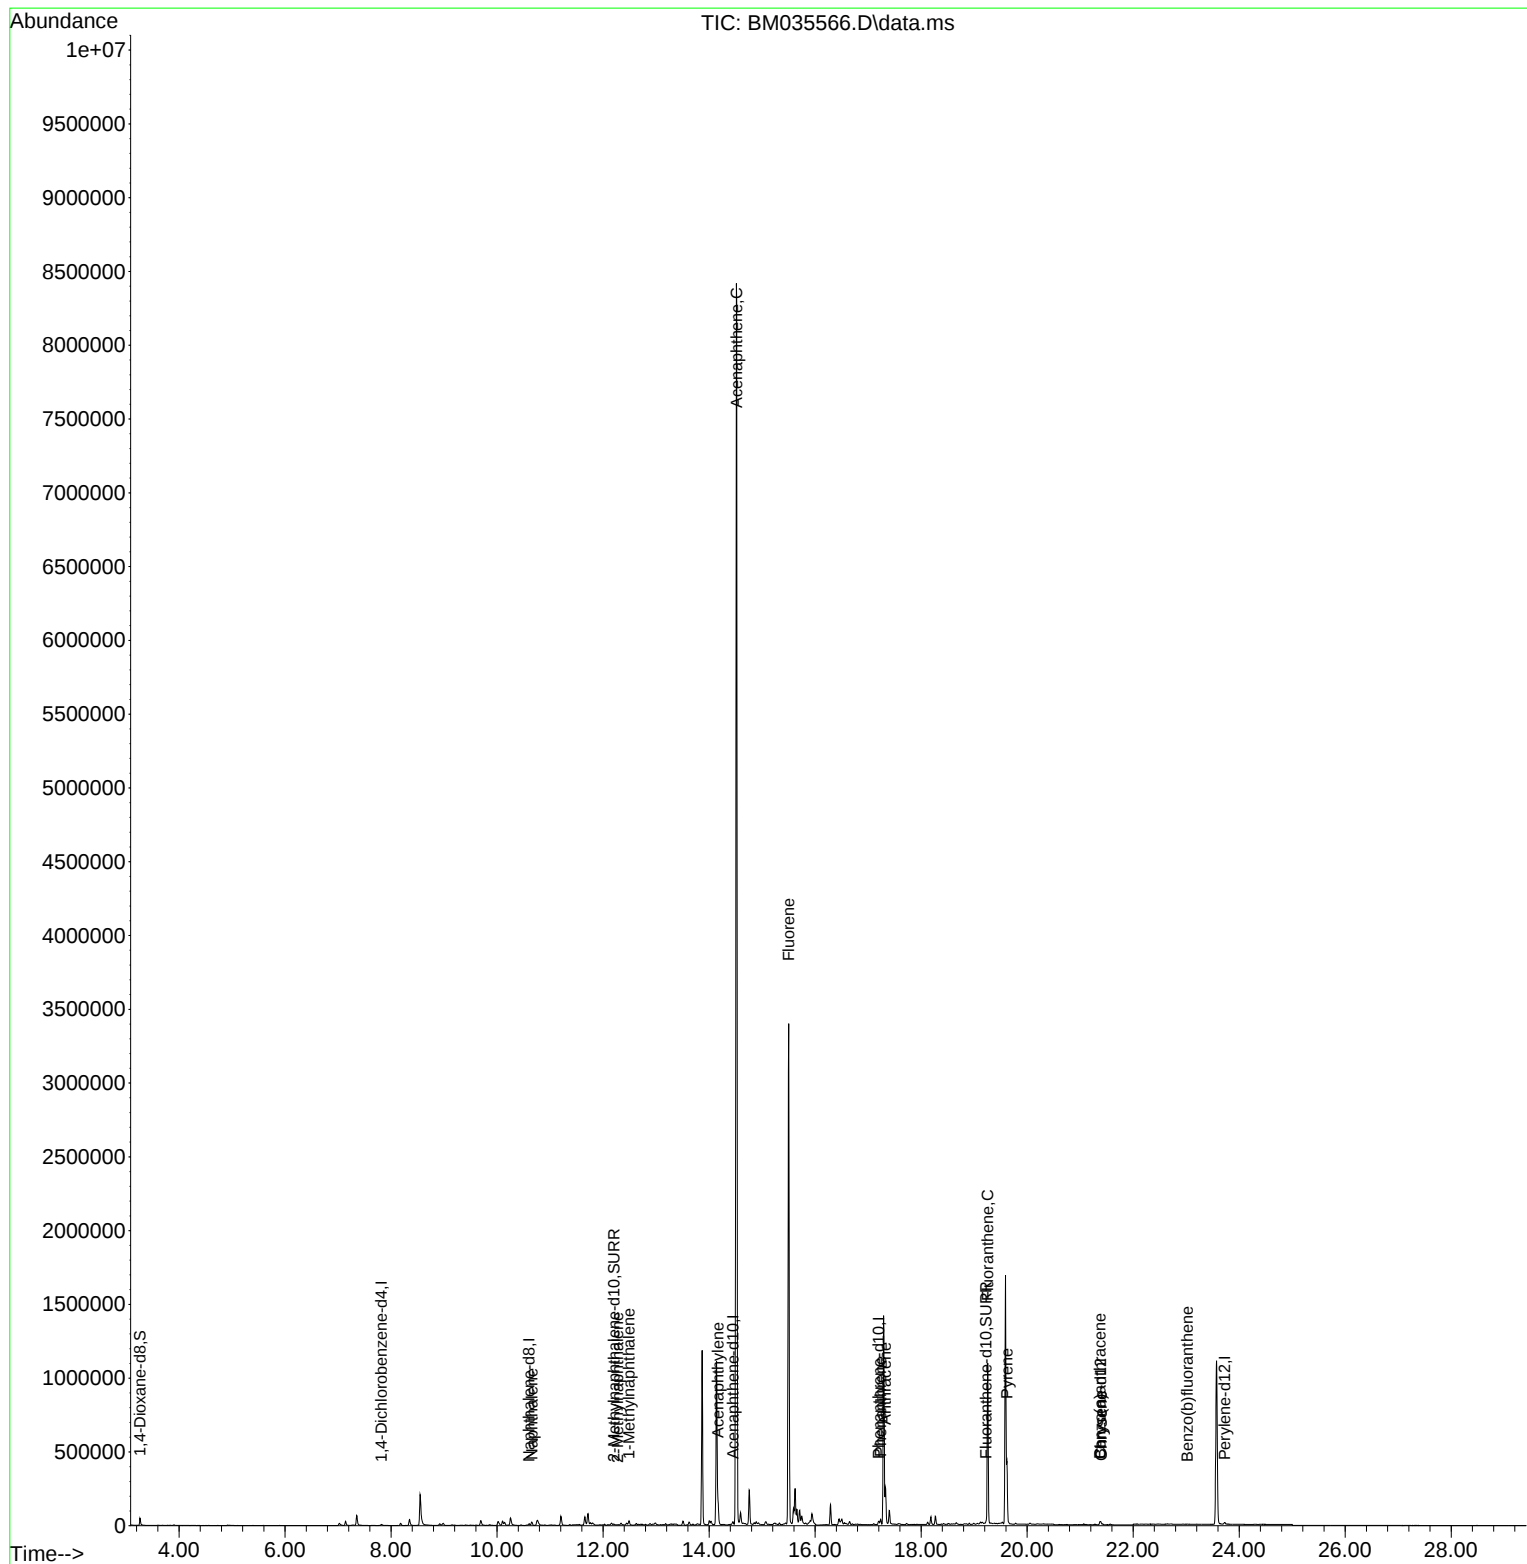



#5
Naphthalene
Concen: 0.561 ng/ul
RT: 10.655 min Scan# 1762
Delta R.T. -0.039 min
Lab File: BM035566.D
Acq: 21 Jun 2022 11:19




Instrument :
BNA_M
ClientSampleId :
C0AA0

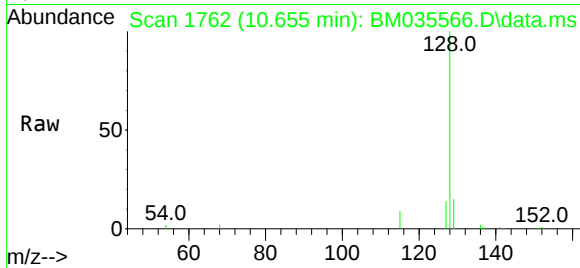

Tgt Ion:128 Resp: 31592
Ion Ratio Lower Upper
128 100
129 14.6 10.1 15.1
127 14.3 11.4 17.2




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 06/22/2022
Supervised By :Yogesh Patel 06/25/2022

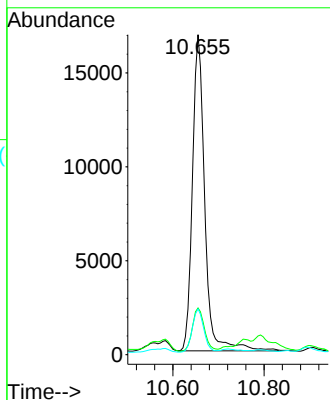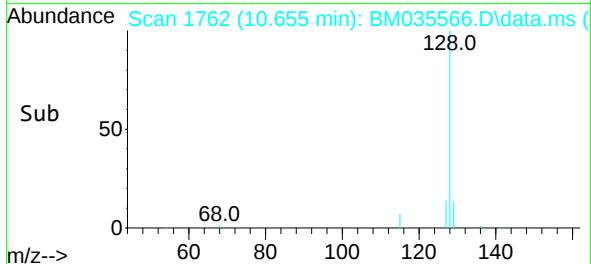

#7
2-Methylnaphthalene
Concen: 0.026 ng/ul
RT: 12.277 min Scan# 2057
Delta R.T. -0.044 min
Lab File: BM035566.D
Acq: 21 Jun 2022 11:19


Tgt Ion:142 Resp: 825
Ion Ratio Lower Upper
142 100
141 130.2 73.8 110.8#

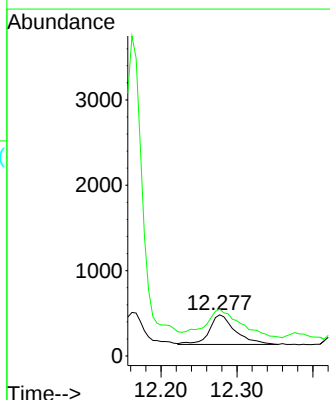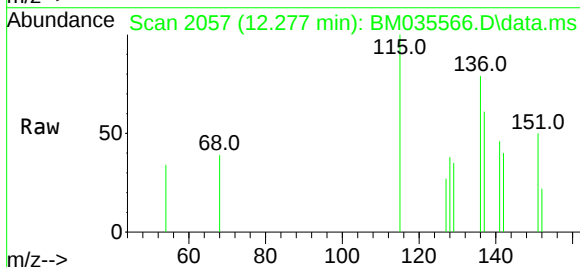



#8
1-Methylnaphthalene
Concen: 0.705 ng/ul
RT: 12.492 min Scan# 2096
Delta R.T. -0.033 min
Lab File: BM035566.D
Acq: 21 Jun 2022 11:19




Instrument :
BNA_M
ClientSampleId :
C0AA0

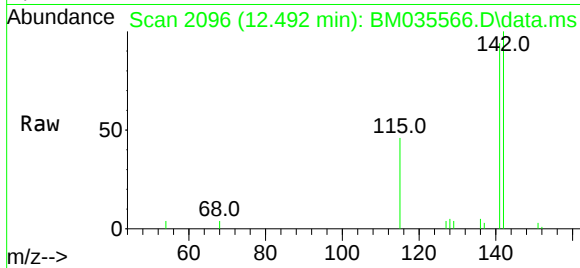

Tgt Ion:142 Resp: 20830
Ion Ratio Lower Upper
142 100
141 91.9 74.6 111.8




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 06/22/2022
Supervised By :Yogesh Patel 06/25/2022

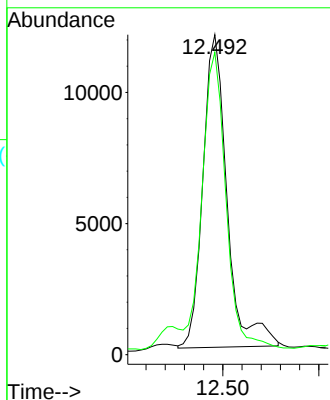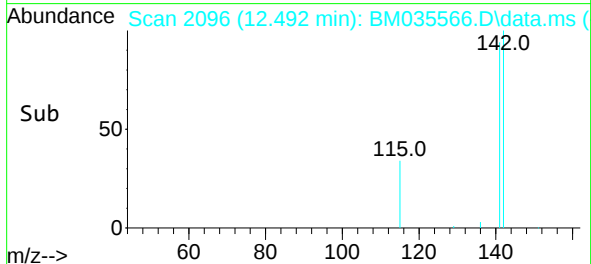

#10
Acenaphthylene
Concen: 2.571 ng/ul
RT: 14.169 min Scan# 2427
Delta R.T. -0.032 min
Lab File: BM035566.D
Acq: 21 Jun 2022 11:19


Tgt Ion:152 Resp: 153640
Ion Ratio Lower Upper
152 100
151 20.7 16.8 25.2
153 18.6 11.1 16.7#

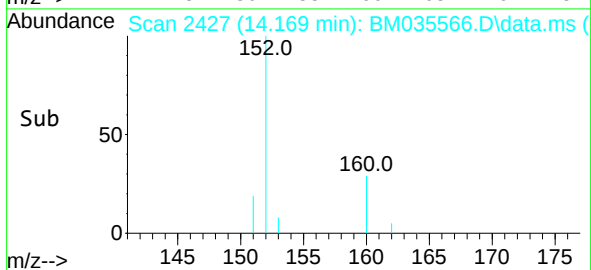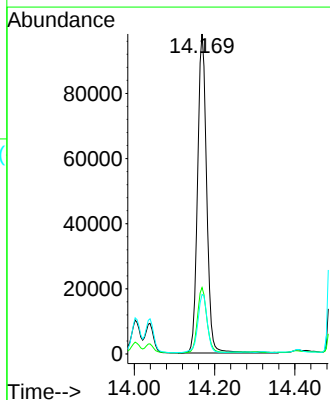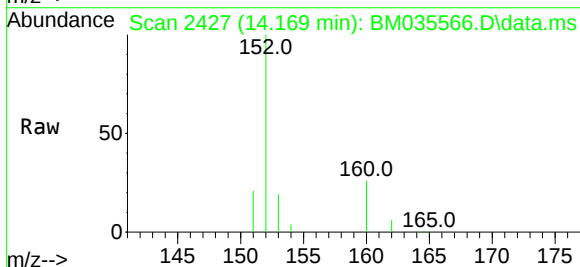

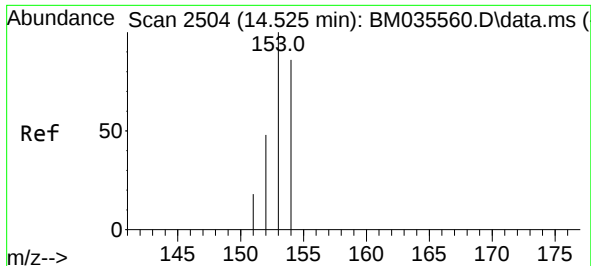

#11
Acenaphthene
Concen: 117.554 ng/u1
RT: 14.516 min Scan# 21
Delta R.T. -0.019 min
Lab File: BM035566.D
Acq: 21 Jun 2022 11:19




Instrument :
BNA_M
ClientSampleId :
C0AA0

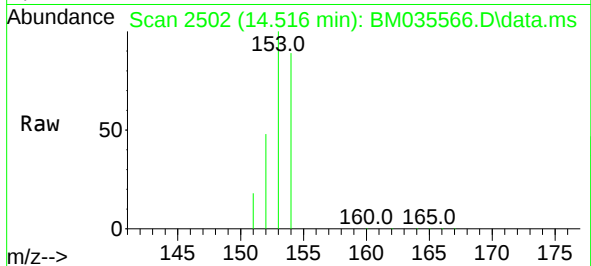

Tgt Ion:153 Resp: 520203
Ion Ratio Lower Upper
153 100
152 47.8 40.0 60.0
154 88.9 69.1 103.7




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 06/22/2022
Supervised By :Yogesh Patel 06/25/2022

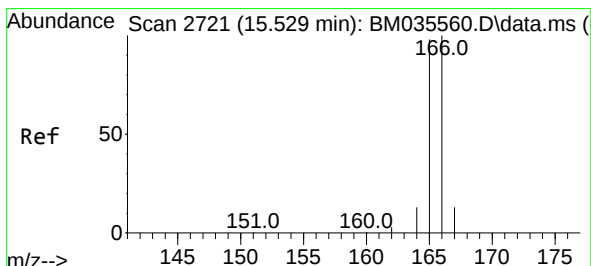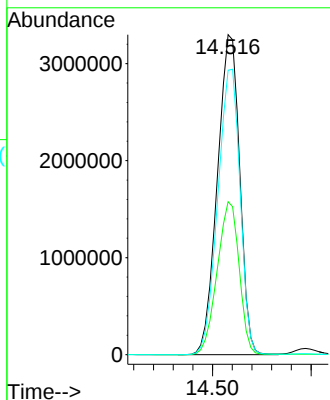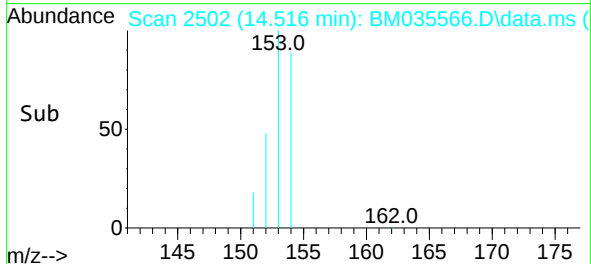

#12
Fluorene
Concen: 41.826 ng/u1
RT: 15.501 min Scan# 2715
Delta R.T. -0.037 min
Lab File: BM035566.D
Acq: 21 Jun 2022 11:19


Tgt Ion:166 Resp: 2093120
Ion Ratio Lower Upper
166 100
165 96.5 78.7 118.1
167 14.5 11.6 17.4

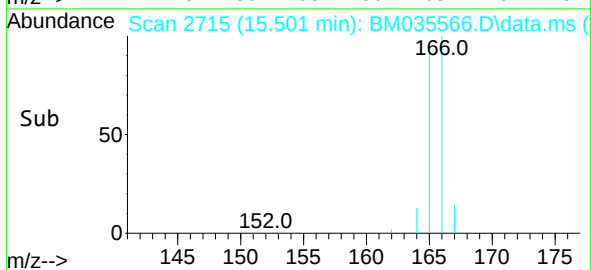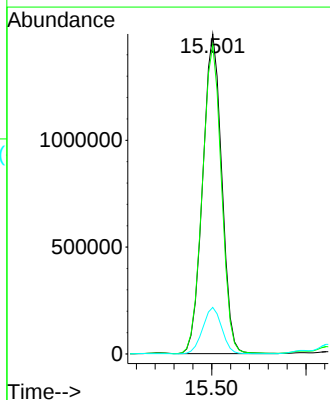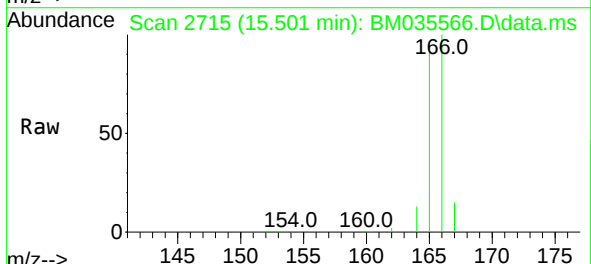

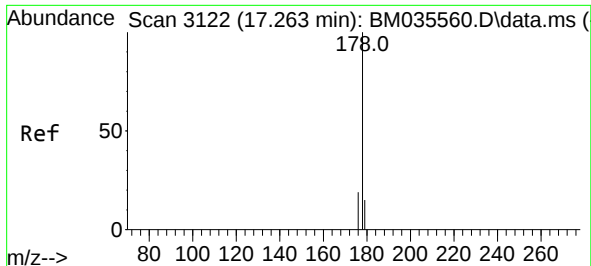

#15
Phenanthrene
Concen: 0.651 ng/ul m
RT: 17.238 min Scan# 3116
Delta R.T. -0.034 min
Lab File: BM035566.D
Acq: 21 Jun 2022 11:19




Instrument :
BNA_M
ClientSampleId :
C0AA0

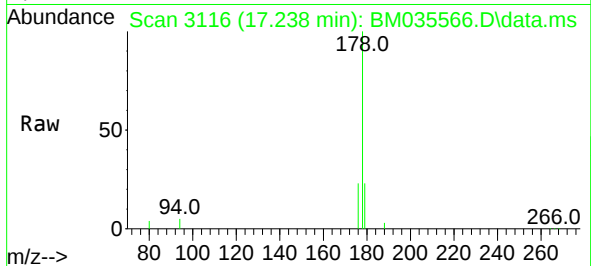


Tgt Ion:178 Resp: 46084
Ion Ratio Lower Upper
178 100
179 22.9 13.2 19.8
176 22.7 16.2 24.4

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 06/22/2022
Supervised By :Yogesh Patel 06/25/2022

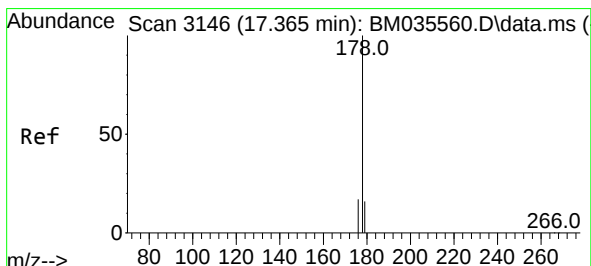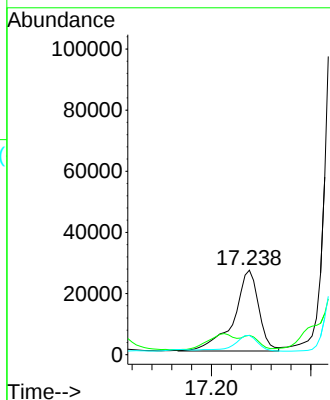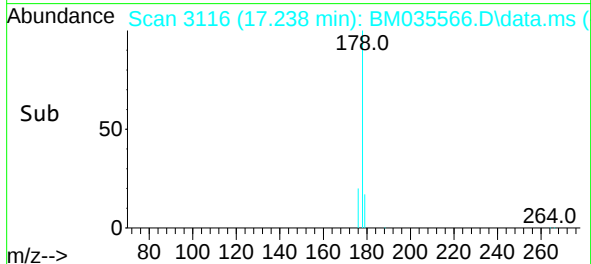


#16
Anthracene
Concen: 4.303 ng/ul
RT: 17.327 min Scan# 3137
Delta R.T. -0.046 min
Lab File: BM035566.D
Acq: 21 Jun 2022 11:19

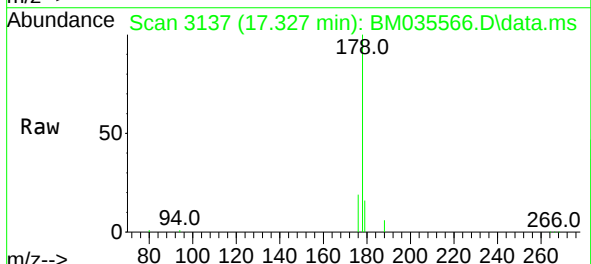


Tgt Ion:178 Resp: 266603
Ion Ratio Lower Upper
178 100
179 16.1 13.4 20.0
176 18.9 15.9 23.9

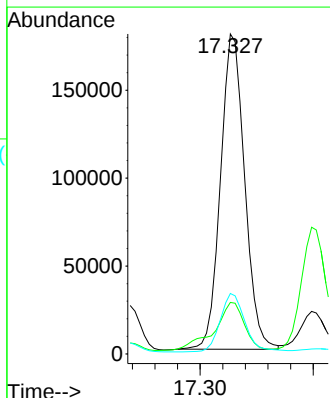

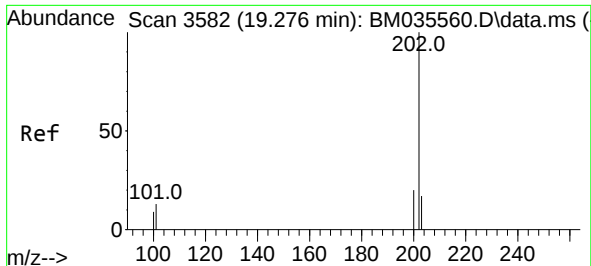

#19
Fluoranthene
Concen: 11.248 ng/ul
RT: 19.257 min Scan# 3578
Delta R.T. -0.028 min
Lab File: BM035566.D
Acq: 21 Jun 2022 11:19




Instrument :
BNA_M
ClientSampleId :
C0AA0




Tgt Ion:202 Resp: 914092
Ion Ratio Lower Upper
202 100
101 12.6 10.0 15.0
100 9.6 7.5 11.3

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 06/22/2022
Supervised By :Yogesh Patel 06/25/2022

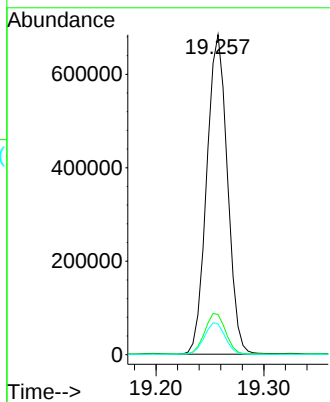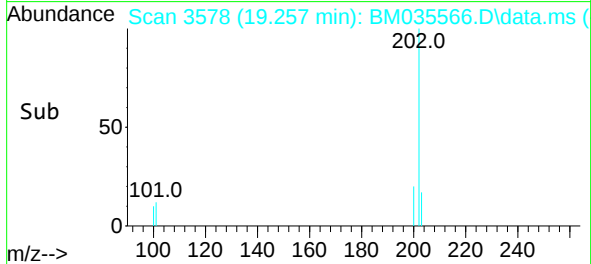


#20
Pyrene
Concen: 4.178 ng/ul
RT: 19.620 min Scan# 3656
Delta R.T. -0.028 min
Lab File: BM035566.D
Acq: 21 Jun 2022 11:19

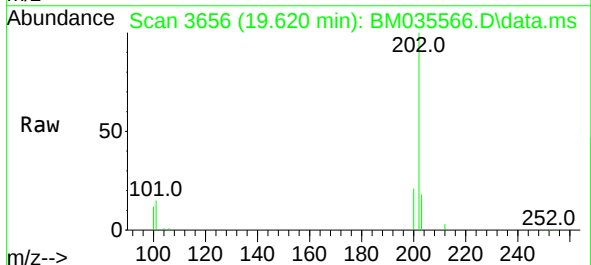


Tgt Ion:202 Resp: 355963
Ion Ratio Lower Upper
202 100
101 14.6 11.6 17.4
100 11.7 9.3 13.9

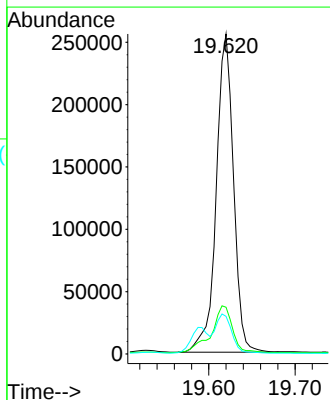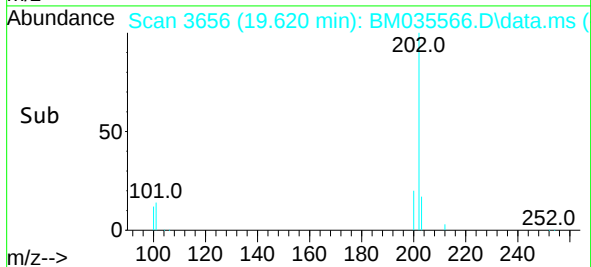

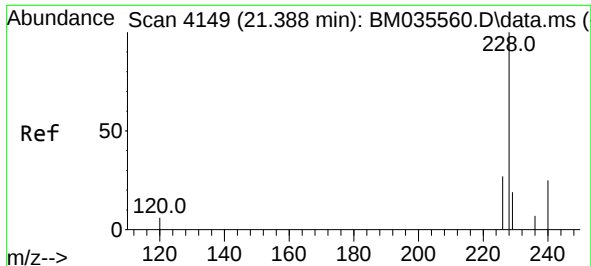

#21
Benzo(a)anthracene
Concen: 0.258 ng/ul
RT: 21.373 min Scan# 4149
Delta R.T. -0.026 min
Lab File: BM035566.D
Acq: 21 Jun 2022 11:19




Instrument :
BNA_M
ClientSampleId :
C0AA0




Tgt Ion:228 Resp: 15510
Ion Ratio Lower Upper
228 100
229 26.8 16.2 24.2#
226 32.1 22.3 33.5#

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 06/22/2022
Supervised By :Yogesh Patel 06/25/2022

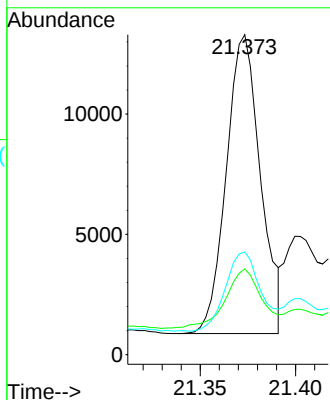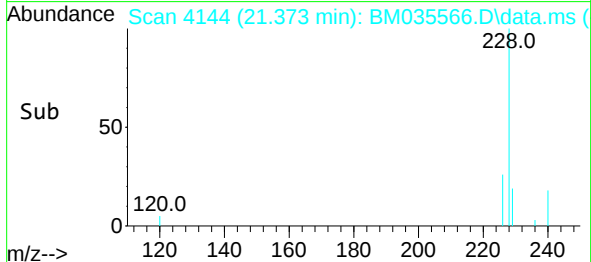


#22
Chrysene
Concen: 0.137 ng/ul m
RT: 21.400 min Scan# 4153
Delta R.T. -0.050 min
Lab File: BM035566.D
Acq: 21 Jun 2022 11:19

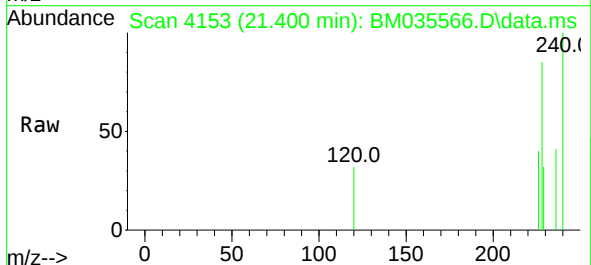


Tgt Ion:228 Resp: 9833
Ion Ratio Lower Upper
228 100
226 47.3 24.5 36.7#
229 38.2 15.8 23.8#

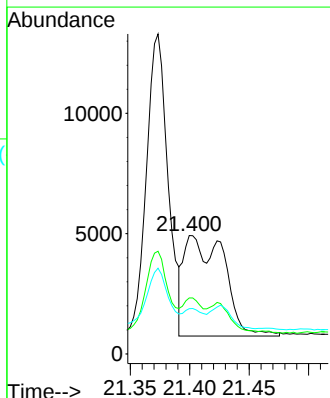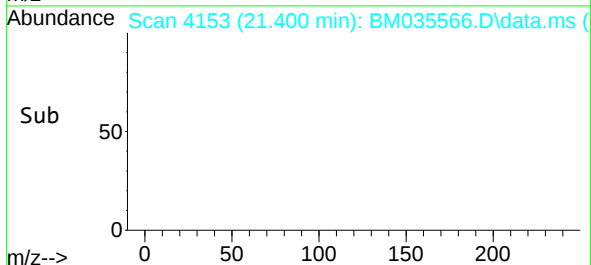



#24
Benzo(b)fluoranthene
Concen: 0.026 ng/ul
RT: 23.019 min Scan# 4712
Delta R.T. -0.032 min
Lab File: BM035566.D
Acq: 21 Jun 2022 11:19

Instrument :
BNA_M
ClientSampleId :
C0AA0



Tgt Ion:252 Resp: 187
Ion Ratio Lower Upper
252 100
253 92.2 0.0 60.6
125 104.4 0.0 44.8

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 06/22/2022
Supervised By :Yogesh Patel 06/25/2022

