

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062116\
 Data File : BM005896.D
 Acq On : 21 Jun 2016 18:11
 Operator : UM/SJ
 Sample : H3612-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9Z20

Quant Time: Jun 22 03:14:16 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 21 08:19:39 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	120620	20.00	ng/ul	0.00
18) Naphthalene-d8	10.46	136	640121	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	431837	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.07	188	1092865	20.00	ng/ul	0.00
75) Chrysene-d12	21.26	240	1467880	20.00	ng/ul	0.00
83) Perylene-d12	23.49	264	1620204	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.20	96	6125	1.99	ng/uL	0.00
5) Phenol-d5	6.85	99	278132	20.89	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.02	67	176105	22.86	ng/ul	0.00
9) 2-Chlorophenol-d4	7.21	132	203109	20.70	ng/ul	0.00
13) 4-Methylphenol-d8	8.37	113	245037	22.02	ng/ul	0.00
19) Nitrobenzene-d5	8.83	128	99089	21.36	ng/ul	0.00
22) 2-Nitrophenol-d4	9.55	143	102187	21.98	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.07	165	233342	21.17	ng/ul	0.00
29) 4-Chloroaniline-d4	10.60	131	326629	31.65	ng/ul	0.00
43) Dimethylphthalate-d6	13.74	166	906913	22.16	ng/ul	0.00
46) Acenaphthylene-d8	14.02	160	1083215	22.42	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	141100	19.99	ng/ul	0.00
57) Fluorene-d10	15.32	176	810678	23.96	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	92528	21.01	ng/ul	0.00
70) Anthracene-d10	17.17	188	1339702	24.18	ng/ul	0.00
76) Pyrene-d10	19.47	212	1678566	21.41	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.35	264	1970585	23.87	ng/ul	0.00


Target Compounds						Qvalue
44) Dimethylphthalate	13.79	163	283605	7.12	ng/ul	99
81) Bis(2-ethylhexyl)phthalate	21.20	149	70142	1.08	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062116\
Data File : BM005896.D
Acq On : 21 Jun 2016 18:11
Operator : UM/SJ
Sample : H3612-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9Z20

Quant Time: Jun 22 03:14:16 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062116.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 21 08:19:39 2016
Response via : Initial Calibration




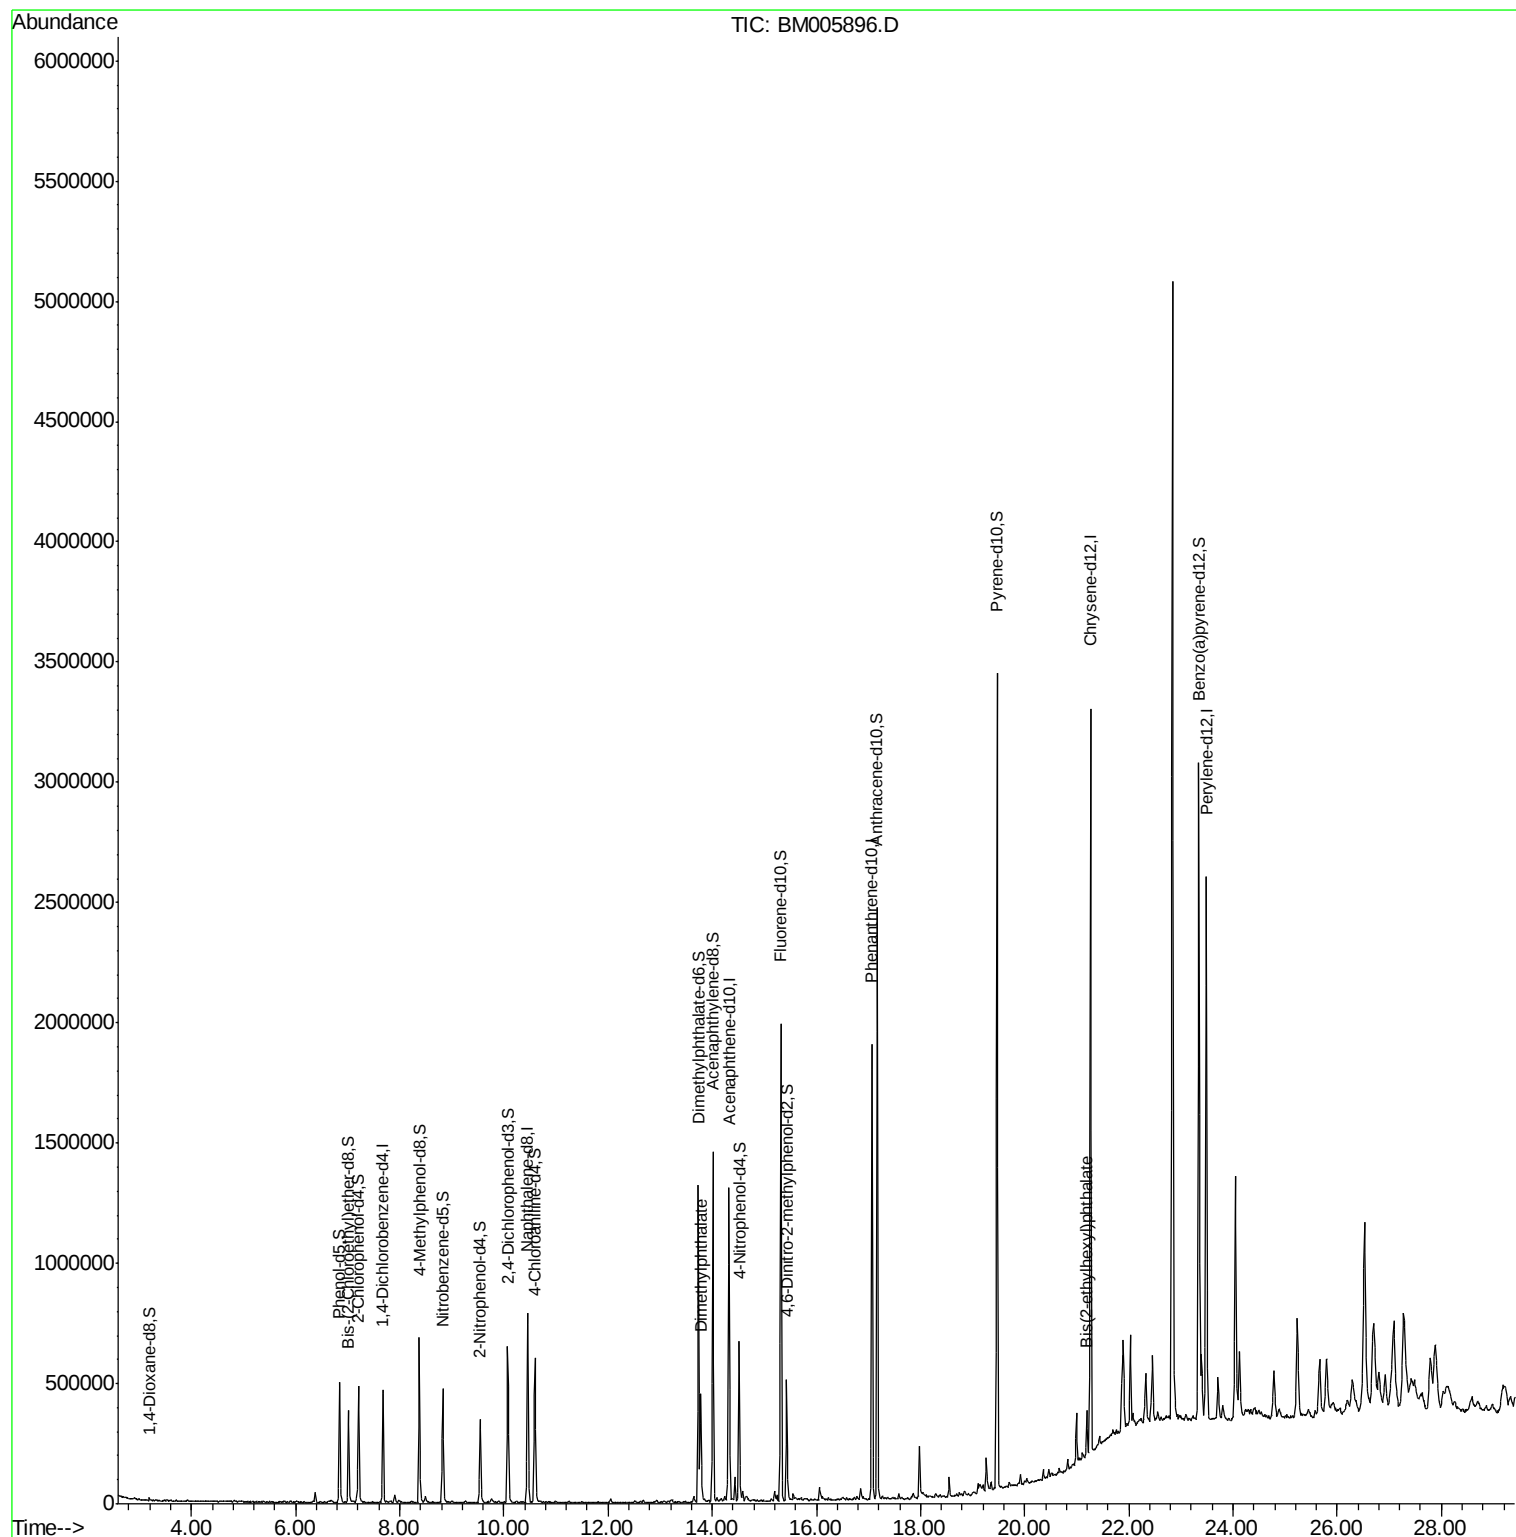


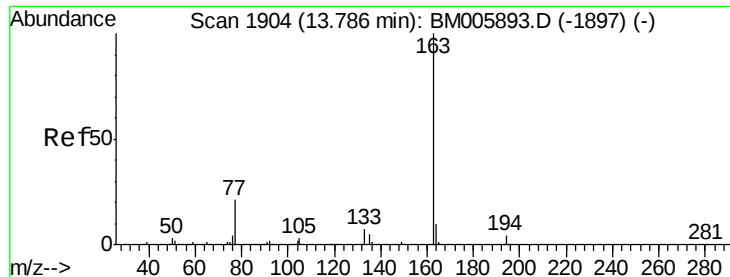

#44
 Dimethylphthalate
 Concen: 7.12 ng/ul
 RT: 13.79 min Scan# 1904
 Delta R.T. -0.01 min
 Lab File: BM005896.D
 Acq: 21 Jun 2016 18:11

Instrument :
 BNA_M
 ClientSampleId :
 D9Z20

Tgt Ion:163 Resp: 283605
 Ion Ratio Lower Upper
 163 100
 194 4.1 3.2 4.8
 164 9.3 7.6 11.4

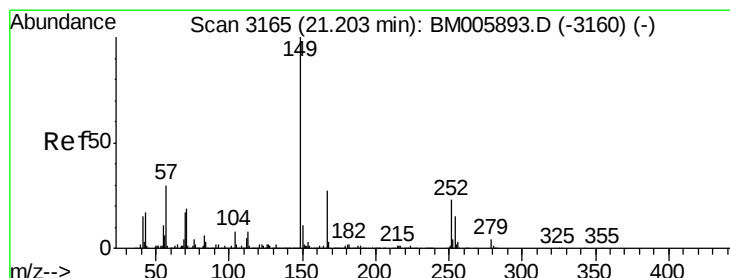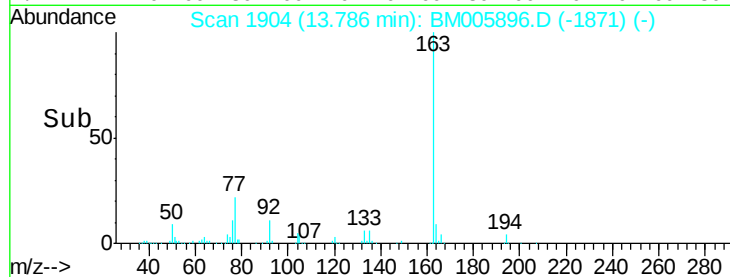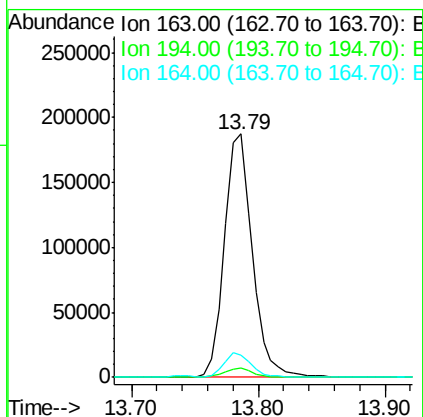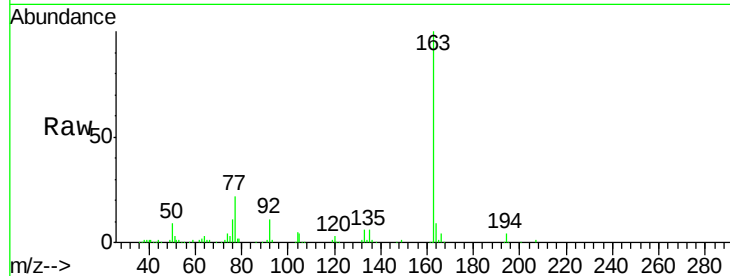

#81
 Bis(2-ethylhexyl)phthalate
 Concen: 1.08 ng/ul
 RT: 21.20 min Scan# 3164
 Delta R.T. 0.00 min
 Lab File: BM005896.D
 Acq: 21 Jun 2016 18:11

Tgt Ion:149 Resp: 70142
 Ion Ratio Lower Upper
 149 100
 167 28.5 22.2 33.2
 279 4.0 3.0 4.4

