

Data Path : Z:\HPCHEM1\BNA M\DATA\BM062116\
 Data File : BM005897.D
 Acq On : 21 Jun 2016 18:48
 Operator : UM/SJ
 Sample : H3612-10
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9Z27

Quant Time: Jun 22 03:14:24 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM062116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 21 08:19:39 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	206276	20.00	ng/ul	0.00
18) Naphthalene-d8	10.46	136	1084193	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	726041	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.07	188	1771244	20.00	ng/ul	0.00
75) Chrysene-d12	21.26	240	2029437	20.00	ng/ul	0.00
83) Perylene-d12	23.49	264	1998640	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.20	96	11544	2.19	ng/uL	0.00
5) Phenol-d5	6.85	99	484094	21.26	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.02	67	321654	24.41	ng/ul	0.00
9) 2-Chlorophenol-d4	7.21	132	377908	22.53	ng/ul	0.00
13) 4-Methylphenol-d8	8.37	113	431344	22.67	ng/ul	0.00
19) Nitrobenzene-d5	8.83	128	196849	25.05	ng/ul	0.00
22) 2-Nitrophenol-d4	9.55	143	204304	25.95	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.08	165	414831	22.22	ng/ul	0.00
29) 4-Chloroaniline-d4	10.60	131	639489	36.58	ng/ul	0.00
43) Dimethylphthalate-d6	13.74	166	1646624	23.93	ng/ul	0.00
46) Acenaphthylene-d8	14.02	160	1927443	23.73	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	197637	16.65	ng/ul	0.00
57) Fluorene-d10	15.32	176	1407678	24.74	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	140298	19.66	ng/ul	0.00
70) Anthracene-d10	17.17	188	2246358	25.02	ng/ul	0.00
76) Pyrene-d10	19.47	212	2593532	23.93	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.35	264	2573416	25.27	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.79	163	519623	7.76	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM062116\
Data File : BM005897.D
Acq On : 21 Jun 2016 18:48
Operator : UM/SJ
Sample : H3612-10
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9Z27

Quant Time: Jun 22 03:14:24 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM062116.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 21 08:19:39 2016
Response via : Initial Calibration

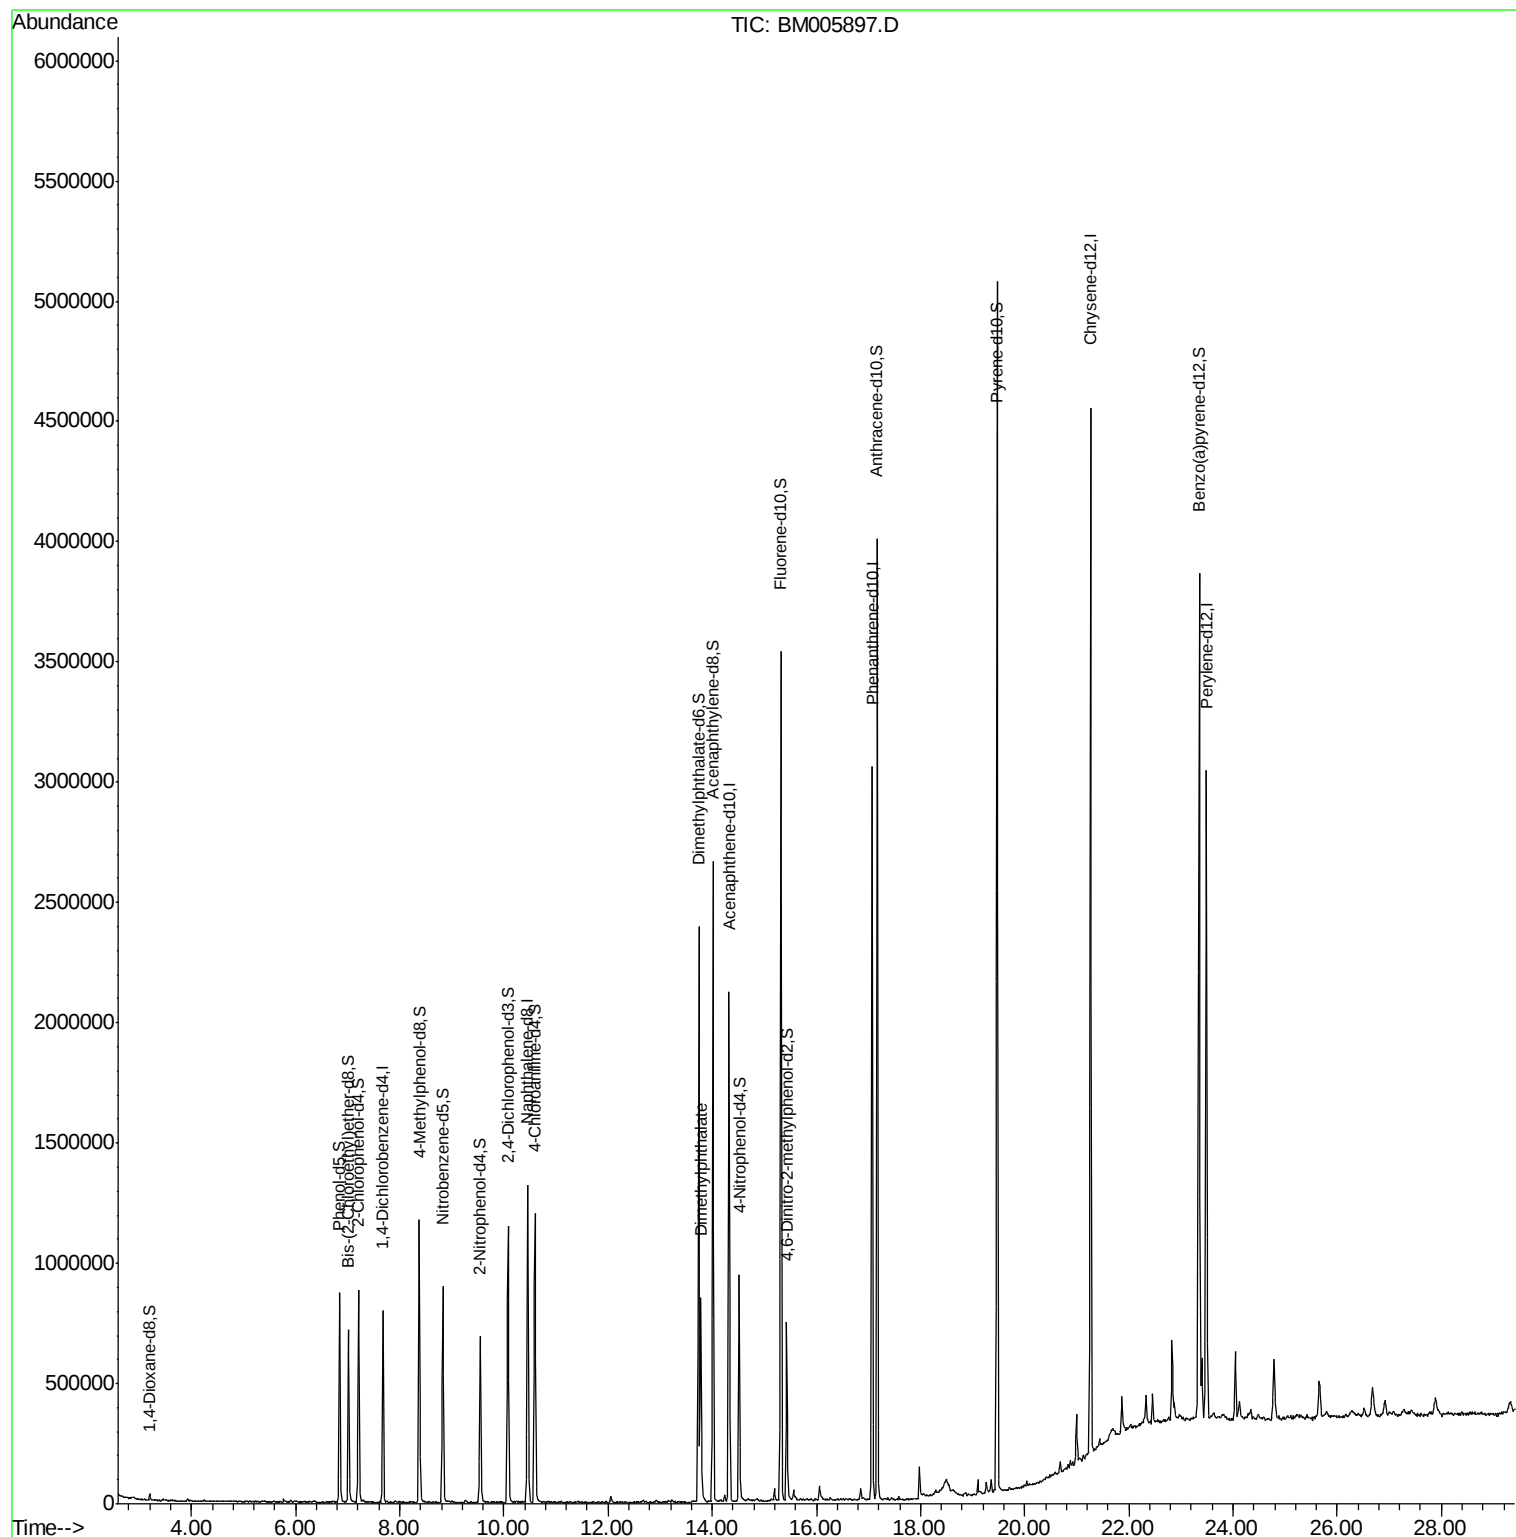

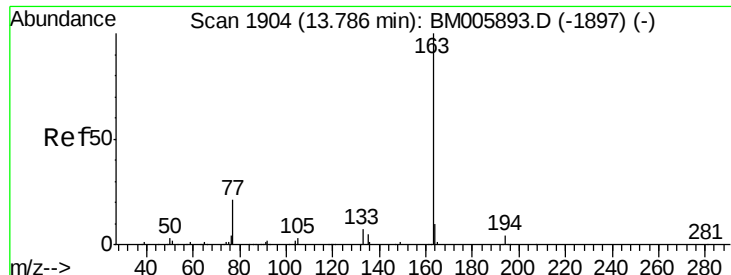

#44
 Dimethylphthalate
 Concen: 7.76 ng/ul
 RT: 13.79 min Scan# 1904
 Delta R.T. -0.01 min
 Lab File: BM005897.D
 Acq: 21 Jun 2016 18:48

Instrument :
 BNA_M
 ClientSampleId :
 D9Z27

Tot Ion	Ratio	Lower	Upper
163	100		
194	3.7	3.2	4.8
164	9.9	7.6	11.4

