

Data Path : Z:\HPCHEM1\BNA M\DATA\BM062116\
 Data File : BM005898.D
 Acq On : 21 Jun 2016 19:24
 Operator : UM/SJ
 Sample : H3612-17
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9Z35

Quant Time: Jun 22 03:14:32 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM062116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 21 08:19:39 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	194487	20.00	ng/ul	0.00
18) Naphthalene-d8	10.46	136	1011460	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	677493	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.07	188	1631532	20.00	ng/ul	0.00
75) Chrysene-d12	21.26	240	1953653	20.00	ng/ul	0.00
83) Perylene-d12	23.49	264	1954251	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.20	96	12027	2.42	ng/uL	0.00
5) Phenol-d5	6.85	99	483754	22.54	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.02	67	321646	25.89	ng/ul	0.00
9) 2-Chlorophenol-d4	7.21	132	368779	23.31	ng/ul	0.00
13) 4-Methylphenol-d8	8.37	113	427434	23.83	ng/ul	0.00
19) Nitrobenzene-d5	8.83	128	188565	25.72	ng/ul	0.00
22) 2-Nitrophenol-d4	9.55	143	198129	26.97	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.08	165	405725	23.29	ng/ul	0.00
29) 4-Chloroaniline-d4	10.60	131	614607	37.69	ng/ul	0.00
43) Dimethylphthalate-d6	13.74	166	1601521	24.94	ng/ul	0.00
46) Acenaphthylene-d8	14.02	160	1899508	25.06	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	238077	21.50	ng/ul	0.00
57) Fluorene-d10	15.32	176	1377471	25.95	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	165238	25.14	ng/ul	0.00
70) Anthracene-d10	17.17	188	2200369	26.60	ng/ul	0.00
76) Pyrene-d10	19.47	212	2582336	24.75	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.35	264	2686018	26.98	ng/ul	0.00


Target Compounds					Ovalue
44) Dimethylphthalate	13.79	163	475355	7.61	ng/ul 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM062116\
Data File : BM005898.D
Acq On : 21 Jun 2016 19:24
Operator : UM/SJ
Sample : H3612-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9Z35

Quant Time: Jun 22 03:14:32 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM062116.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 21 08:19:39 2016
Response via : Initial Calibration

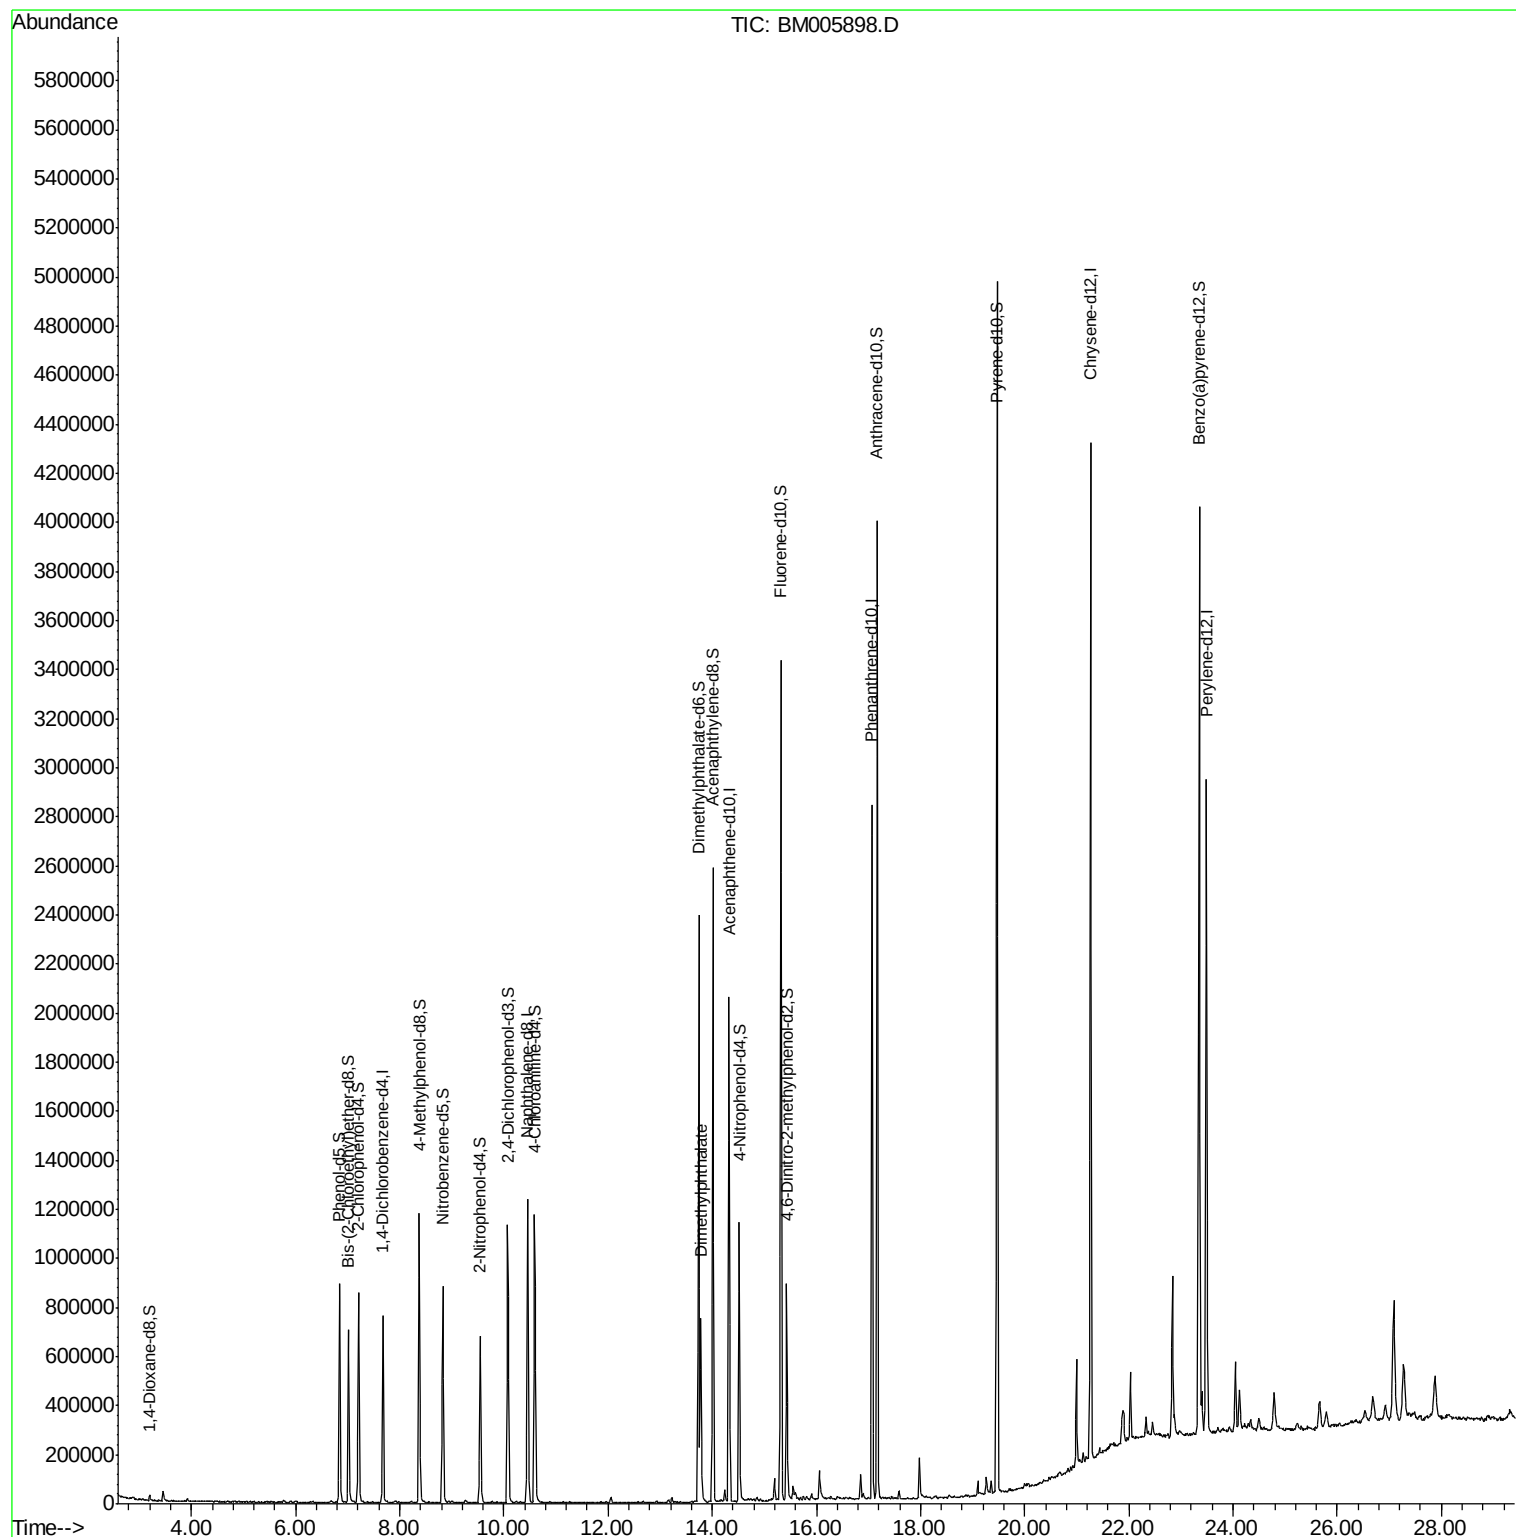

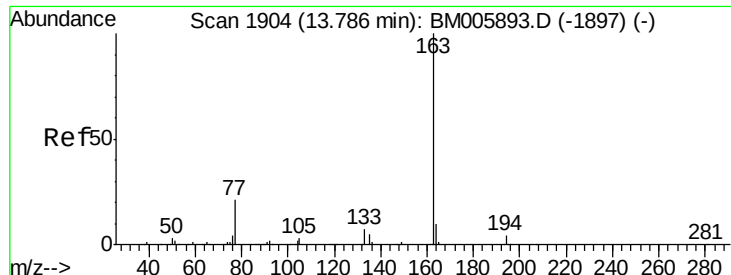

#44

Dimethylphthalate

Concen: 7.61 ng/ul

RT: 13.79 min Scan# 1904

Delta R.T. -0.01 min

Lab File: BM005898.D

Acq: 21 Jun 2016 19:24

Instrument :

BNA_M

ClientSampleId :

D9Z35


Tot Ion:163 Resp: 475355

Ion Ratio Lower Upper

163 100

194 3.8 3.2 4.8

164 9.6 7.6 11.4

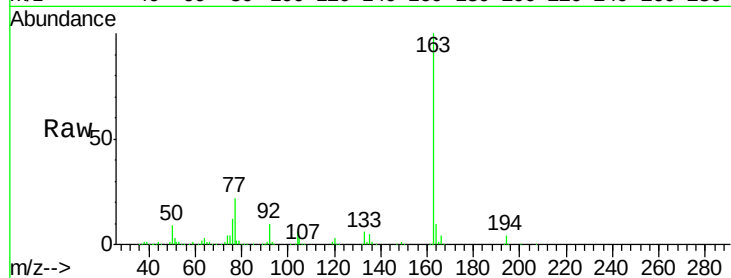

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

