

Data Path : Z:\HPCHEM1\BNA M\DATA\BM062116\
 Data File : BM005899.D
 Acq On : 21 Jun 2016 20:00
 Operator : UM/SJ
 Sample : H3612-18
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9Z36

Quant Time: Jun 22 03:24:26 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM062116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 21 08:19:39 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	189083	20.00	ng/ul	0.00
18) Naphthalene-d8	10.46	136	1045755	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	698431	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.07	188	1689593	20.00	ng/ul	0.00
75) Chrysene-d12	21.26	240	2008347	20.00	ng/ul	0.00
83) Perylene-d12	23.49	264	2013377	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.20	96	9240	1.91	ng/uL	0.00
5) Phenol-d5	6.85	99	412563	19.77	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.02	67	272017	22.52	ng/ul	0.00
9) 2-Chlorophenol-d4	7.21	132	313472	20.38	ng/ul	0.00
13) 4-Methylphenol-d8	8.37	113	357014	20.47	ng/ul	0.00
19) Nitrobenzene-d5	8.83	128	160032	21.11	ng/ul	0.00
22) 2-Nitrophenol-d4	9.55	143	165654	21.81	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.07	165	344361	19.12	ng/ul	0.00
29) 4-Chloroaniline-d4	10.59	131	319597	18.96	ng/ul	0.00
43) Dimethylphthalate-d6	13.74	166	1315937	19.88	ng/ul	0.00
46) Acenaphthylene-d8	14.02	160	1572837	20.13	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	160521	14.06	ng/ul	0.00
57) Fluorene-d10	15.32	176	1133608	20.71	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	137866	20.25	ng/ul	0.00
70) Anthracene-d10	17.17	188	1787030	20.86	ng/ul	0.00
76) Pyrene-d10	19.47	212	2128920	19.85	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.35	264	2187736	21.33	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.79	163	402481	6.25	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM062116\
Data File : BM005899.D
Acq On : 21 Jun 2016 20:00
Operator : UM/SJ
Sample : H3612-18
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9Z36

Quant Time: Jun 22 03:24:26 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM062116.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 21 08:19:39 2016
Response via : Initial Calibration

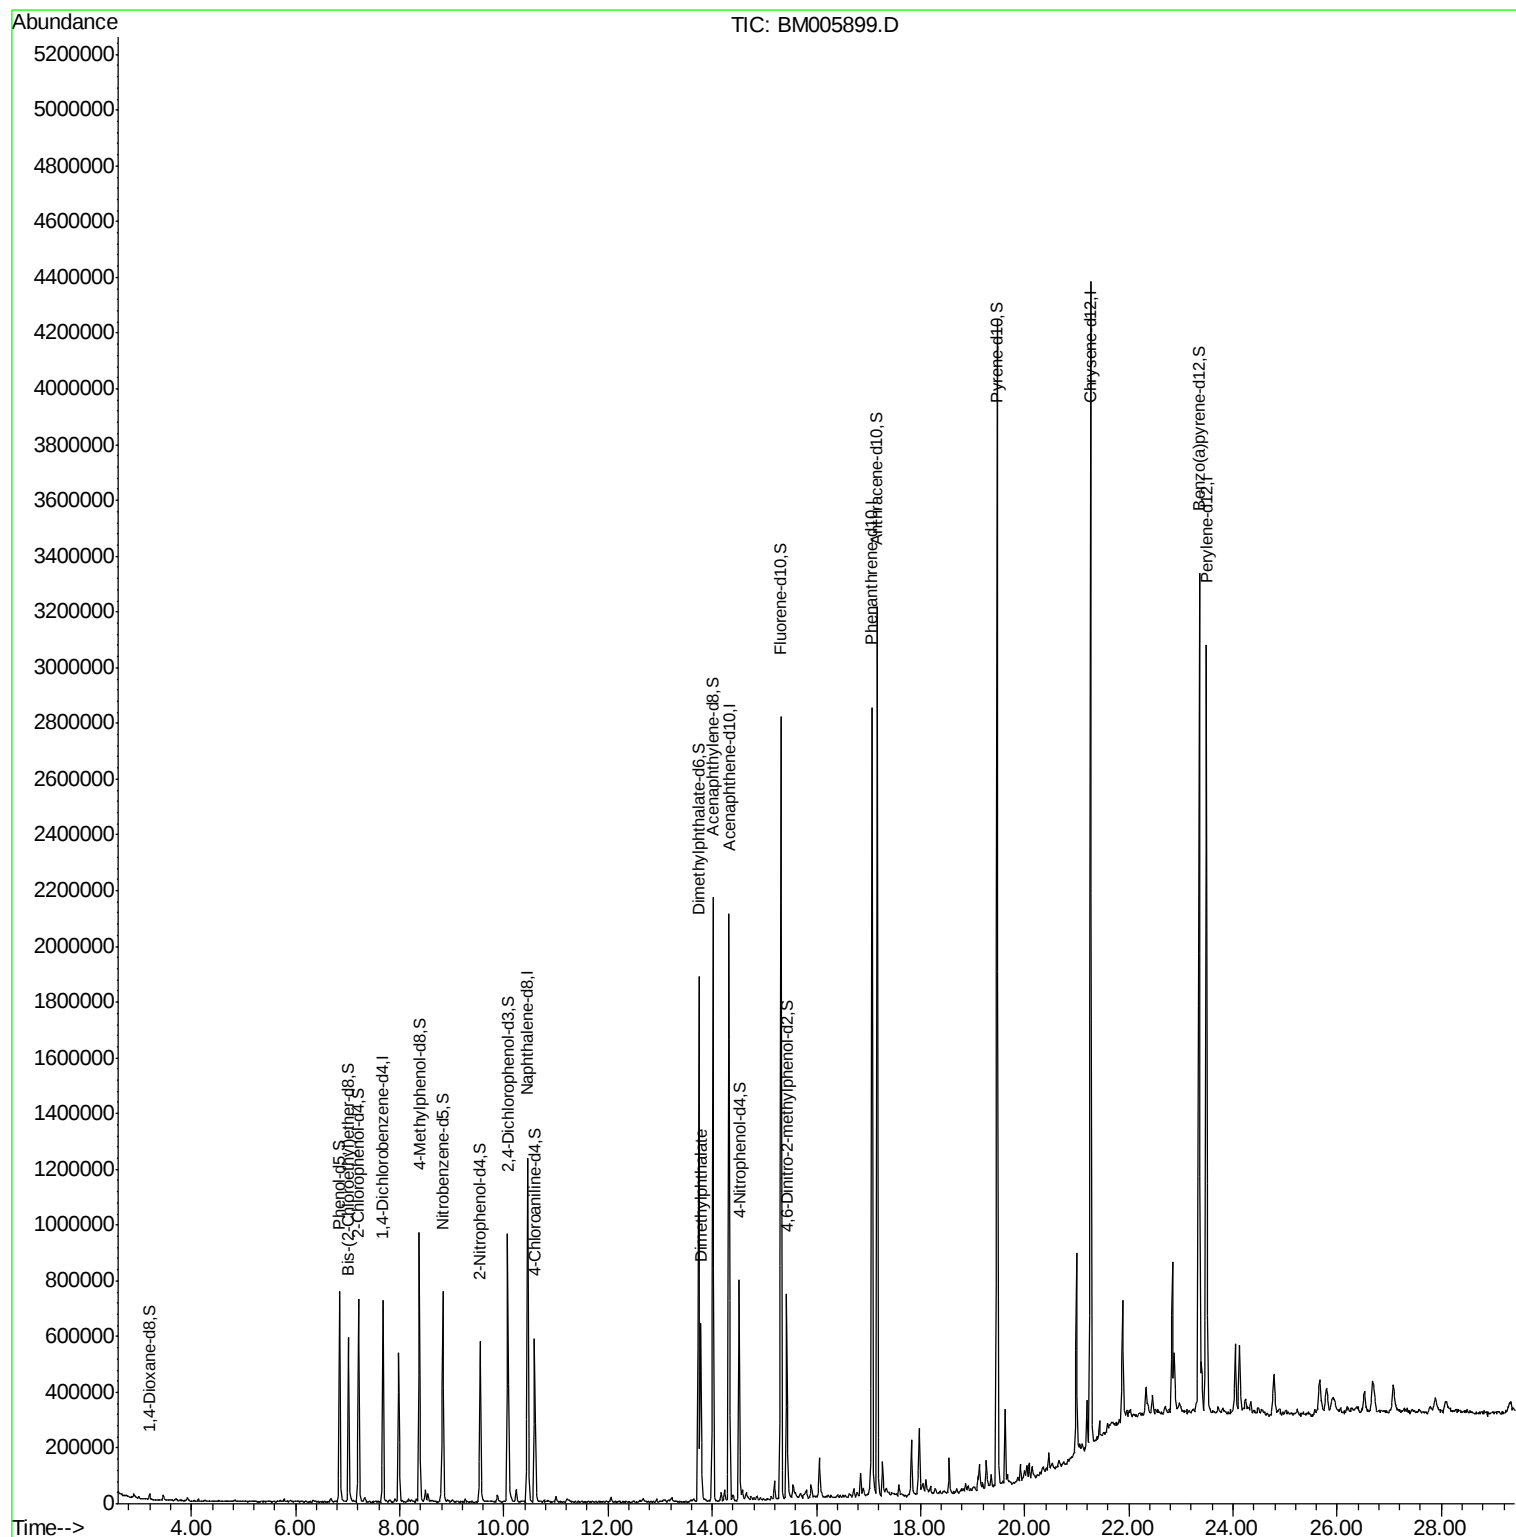

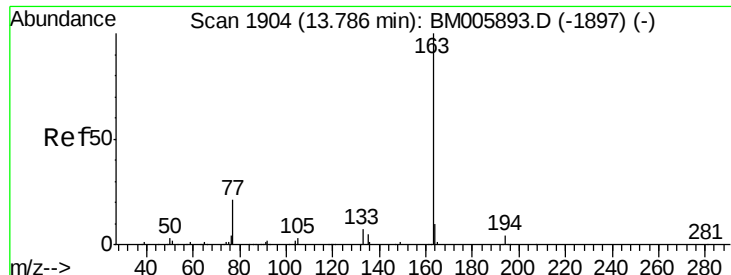

#44
 Dimethylphthalate
 Concen: 6.25 ng/ul
 RT: 13.79 min Scan# 1904
 Delta R.T. -0.01 min
 Lab File: BM005899.D
 Acq: 21 Jun 2016 20:00

Instrument :
 BNA_M
 ClientSampleId :
 D9Z36

Tot Ion:	163	Resp:	402481
Ion	Ratio	Lower	Upper
163	100		
194	3.8	3.2	4.8
164	9.5	7.6	11.4

