

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062116\
 Data File : BM005881.D
 Acq On : 21 Jun 2016 05:44
 Operator : UM/SJ
 Sample : PB91207BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK07

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062116.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.846	716	724	736	rBV	1152677	1860333	19.68%	2.039%
2	7.016	747	753	766	rVB	889189	1454106	15.38%	1.594%
3	7.210	779	786	797	rBV	1107126	1824730	19.30%	2.000%
4	7.681	859	866	875	rVB	792259	1309893	13.86%	1.436%
5	8.381	976	985	994	rBV	1467605	2493375	26.38%	2.733%
6	8.834	1054	1062	1072	rBV	1123206	1939967	20.52%	2.126%
7	9.545	1176	1183	1192	rBV	836778	1500785	15.88%	1.645%
8	10.081	1266	1274	1288	rBV	1427503	2537744	26.85%	2.781%
9	10.463	1330	1339	1351	rBV	1303856	2263757	23.95%	2.481%
10	10.598	1353	1362	1376	rBV	2929365	5260839	55.66%	5.765%
11	13.739	1889	1896	1912	rBV	3356403	4963296	52.51%	5.439%
12	14.016	1935	1943	1955	rBV	3414647	5308344	56.16%	5.818%
13	14.327	1989	1996	2003	rBV2	2170119	3457468	36.58%	3.789%
14	14.522	2022	2029	2042	rBV	1749110	2693351	28.49%	2.952%
15	15.322	2158	2165	2172	rBV	4532008	6808940	72.03%	7.462%
16	15.433	2178	2184	2200	rBV	988758	1529282	16.18%	1.676%
17	15.563	2200	2206	2215	rVB2	65144	118828	1.26%	0.130%
18	17.074	2456	2463	2469	rBV	3124851	4650744	49.20%	5.097%
19	17.168	2473	2479	2490	rVB2	5096908	7834327	82.88%	8.586%
20	19.104	2803	2808	2812	rBV	77581	115371	1.22%	0.126%
21	19.474	2864	2871	2882	rBV	6297442	9341327	98.82%	10.237%
22	21.268	3170	3176	3181	rBV	4878683	6440630	68.14%	7.058%
23	23.356	3523	3531	3538	rBV2	4798581	9452421	100.00%	10.359%
24	23.492	3548	3554	3565	rVB2	3109128	6087449	64.40%	6.671%


Sum of corrected areas: 91247307

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062116\
Data File : BM005881.D
Acq On : 21 Jun 2016 05:44
Operator : UM/SJ
Sample : PB91207BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK07

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

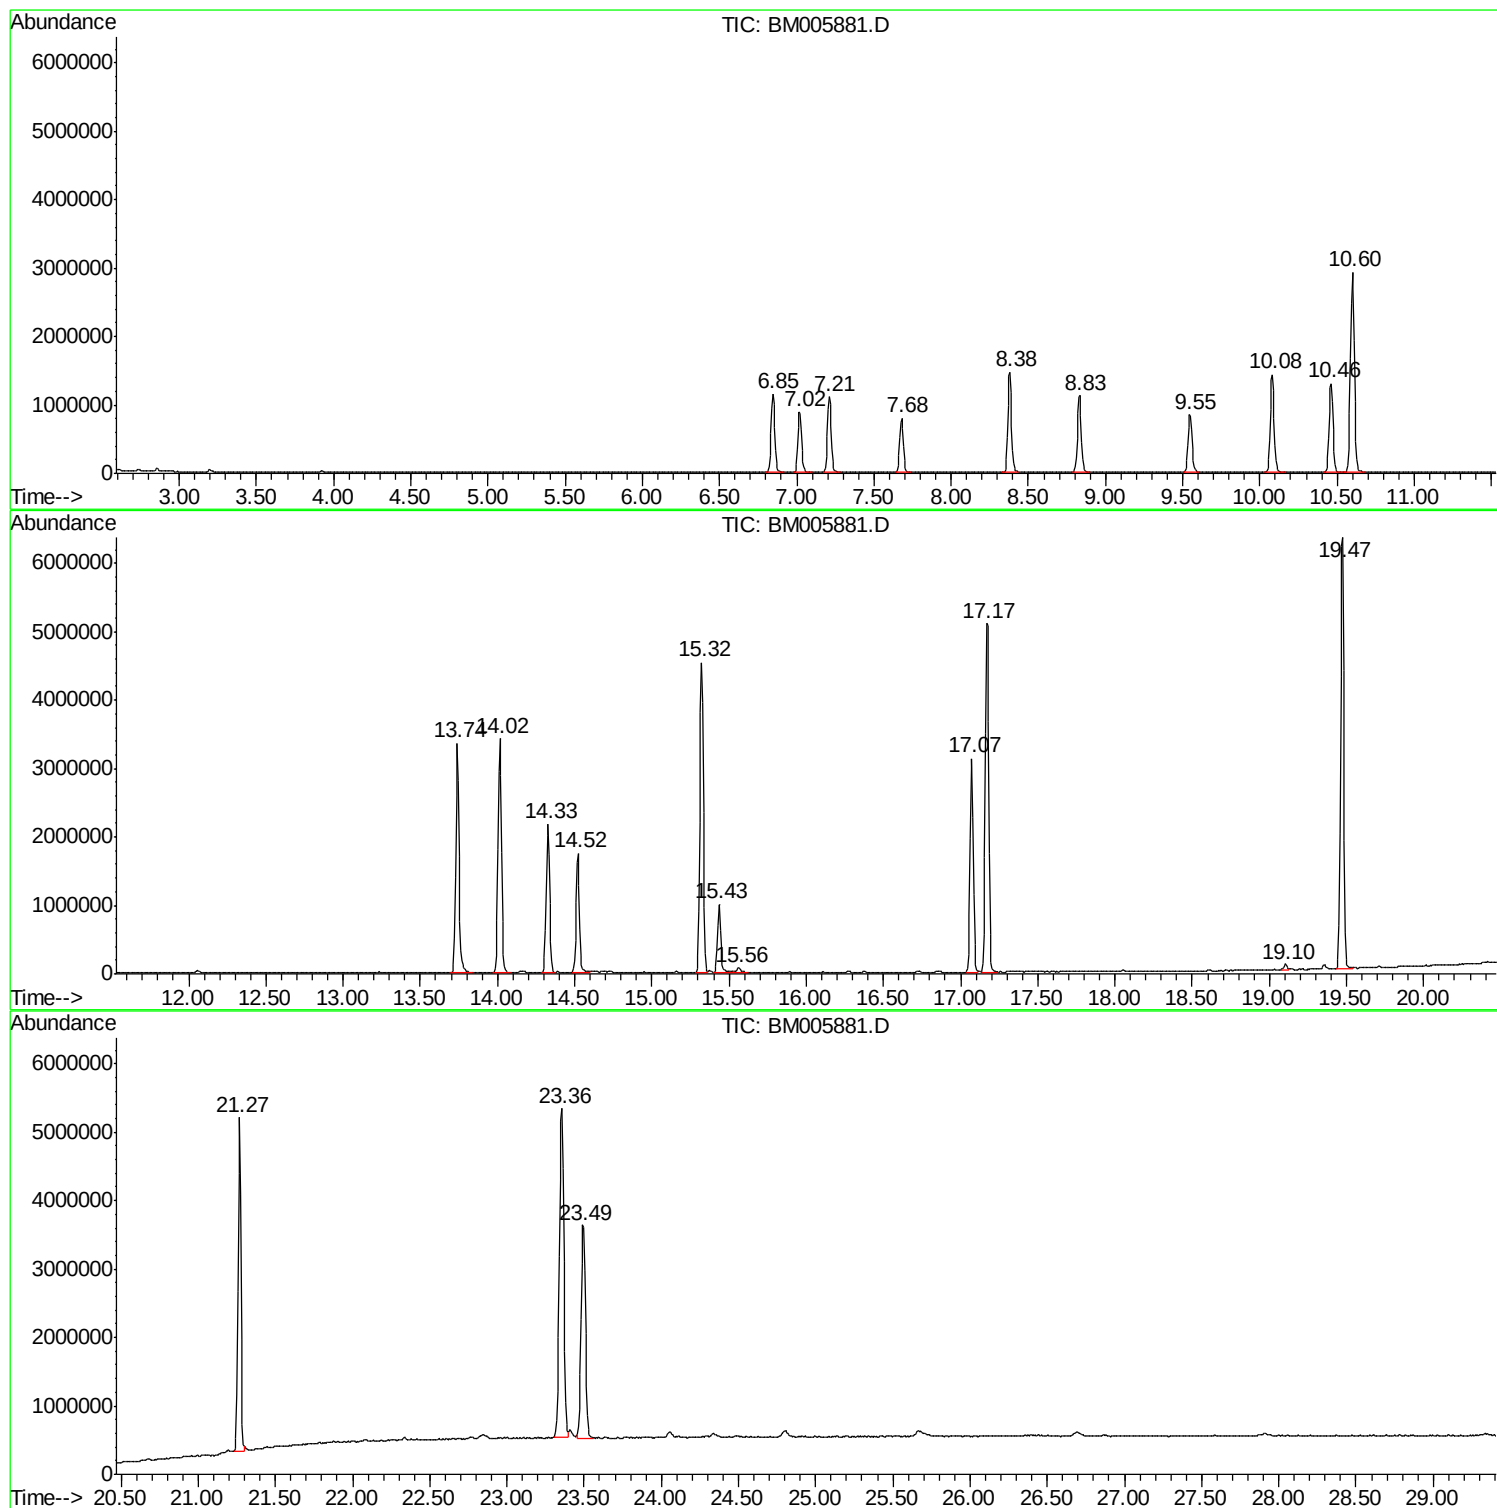

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062116\
Data File : BM005881.D
Acq On : 21 Jun 2016 05:44
Operator : UM/SJ
Sample : PB91207BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK07

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062116\
Data File : BM005881.D
Acq On : 21 Jun 2016 05:44
Operator : UM/SJ
Sample : PB91207BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK07

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc