

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062117\
Quantitation Report (Qedit)




Data File : BM010632.D
Acq On : 21 Jun 2017 20:40
Operator : SJ/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Jun 22 00:46:25 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 22 00:43:46 2017
Response via : Initial Calibration

Instrument :
BNA_M
LabSampleId :
SSTD02041

Manual Integrations
APPROVED

mohammad
6/22/2017 5:32:49 PM

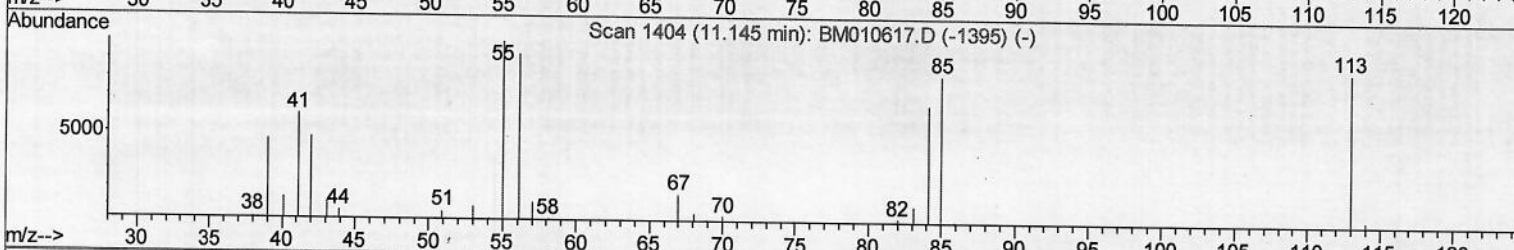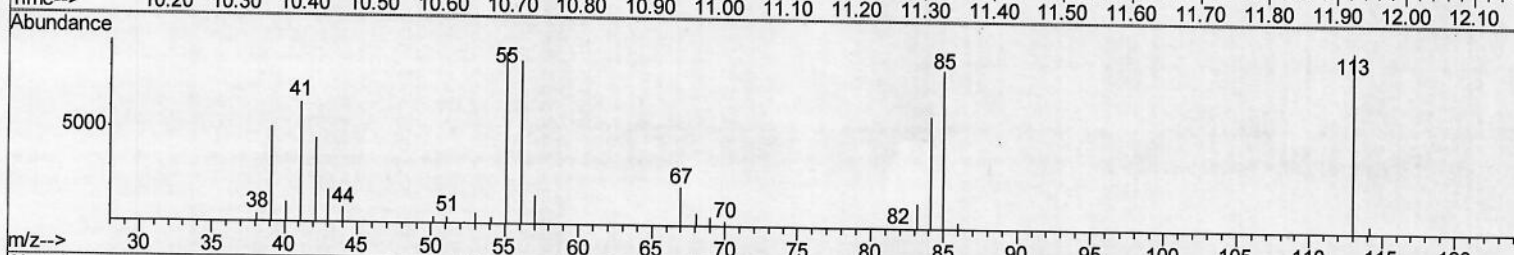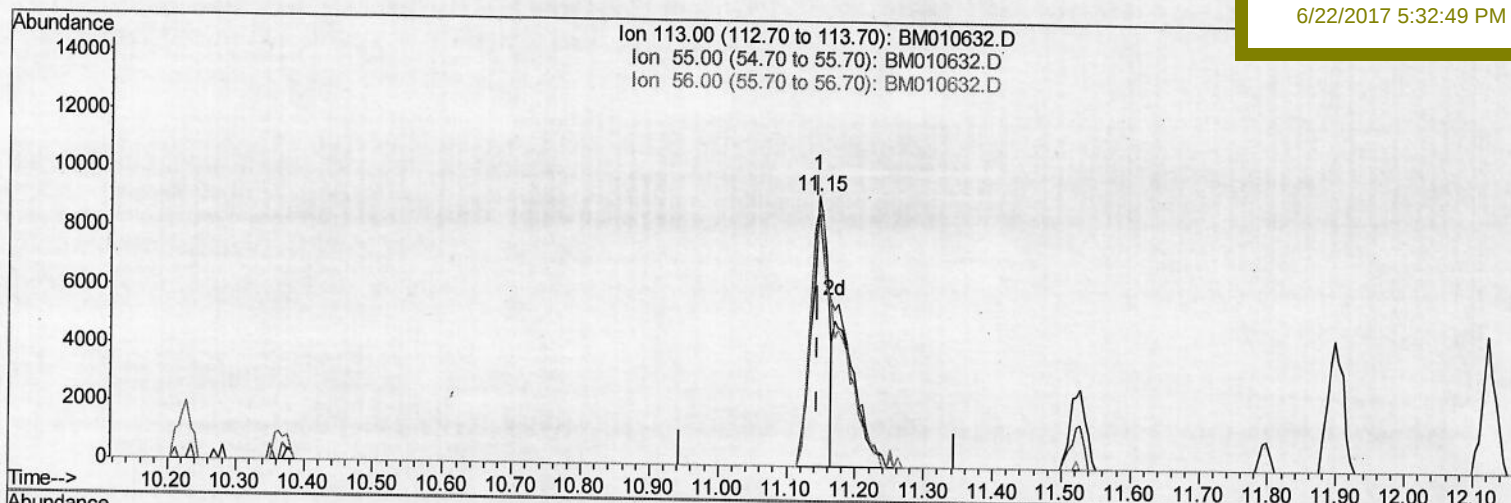

TIC: BM010632.D

(32) Caprolactam

11.145min (+0.000) 10.99ng/ul

response 15280

Ion	Exp%	Act%
113.00	100	100
55.00	118.50	95.09
56.00	107.50	91.07
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062117\
Quantitation Report (Qedit)




Data File : BM010632.D
Acq On : 21 Jun 2017 20:40
Operator : SJ/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Jun 22 00:46:25 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 22 00:43:46 2017
Response via : Initial Calibration

Instrument :
BNA_M
LabSampleId :
SSTD02041

Manual Integrations
APPROVED

mohammad
6/22/2017 5:32:49 PM

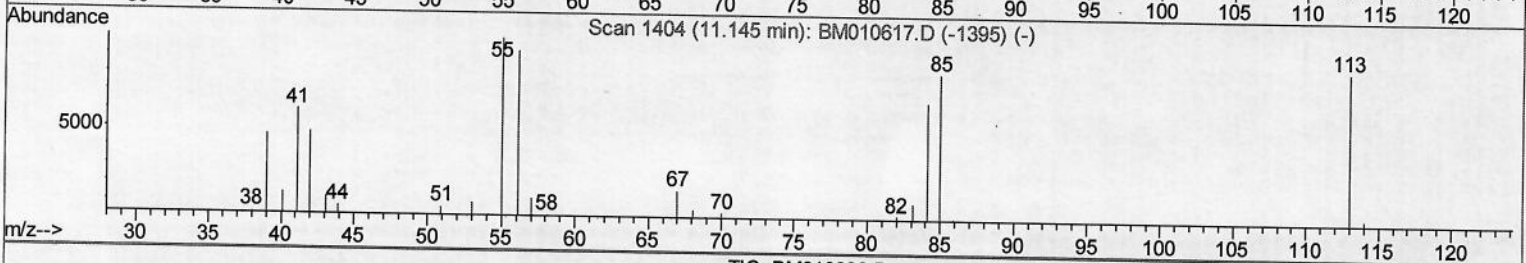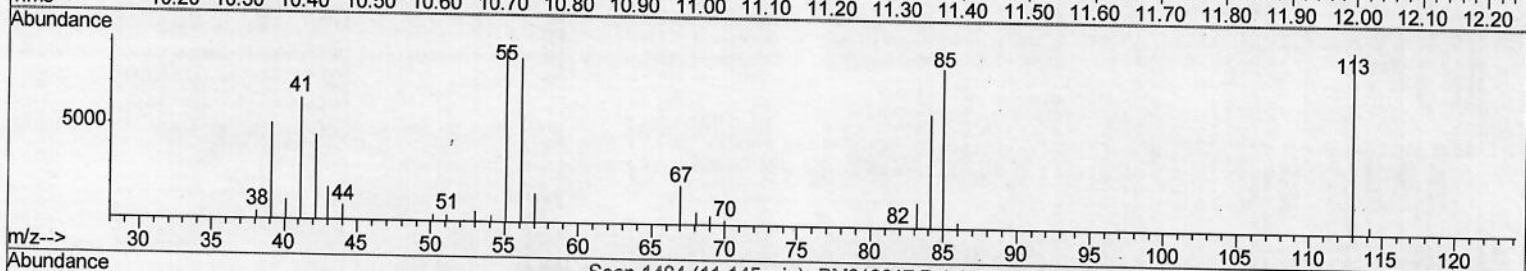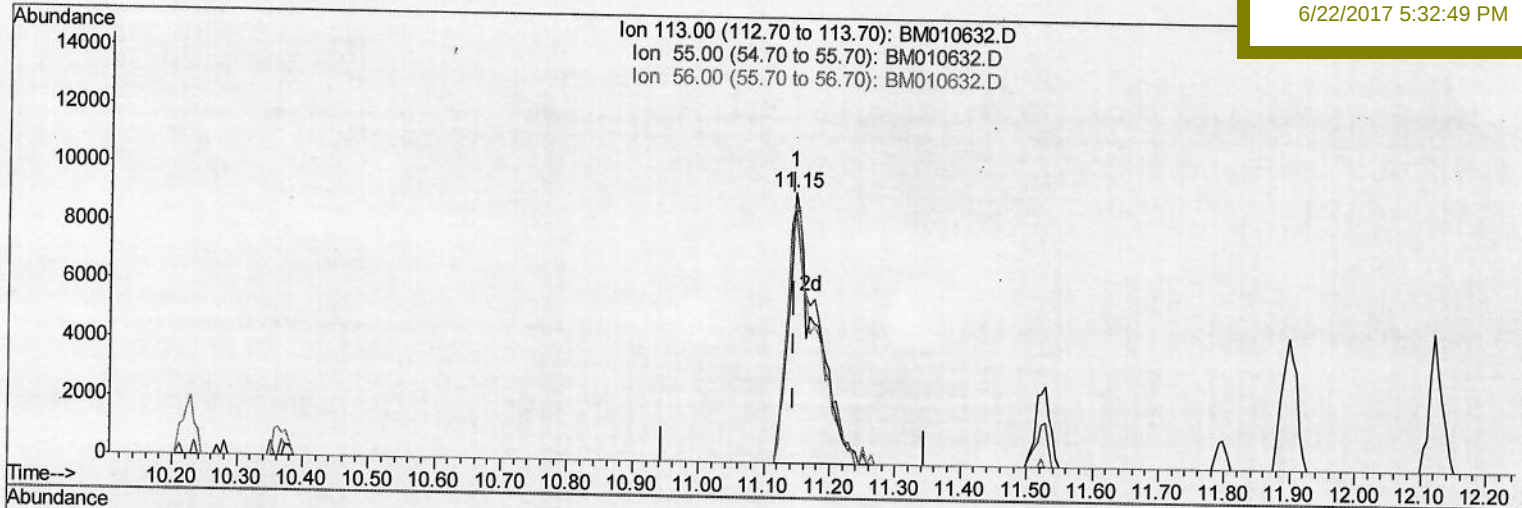

TIC: BM010632.D

(32) Caprolactam

11.145min (+0.000) 19.14ng/ul m

response 26616

Ion	Exp%	Act%
113.00	100	100
55.00	118.50	95.09
56.00	107.50	91.07
0.00	0.00	0.00

S.J
06/26/17

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062117\
Quantitation Report (Qedit)




Data File : BM010632.D
Acq On : 21 Jun 2017 20:40
Operator : SJ/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Jun 22 00:46:25 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 22 00:43:46 2017
Response via : Initial Calibration

Instrument :
BNA_M
LabSampleId :
SSTD02041

Manual Integrations
APPROVED

mohammad
6/22/2017 5:32:49 PM

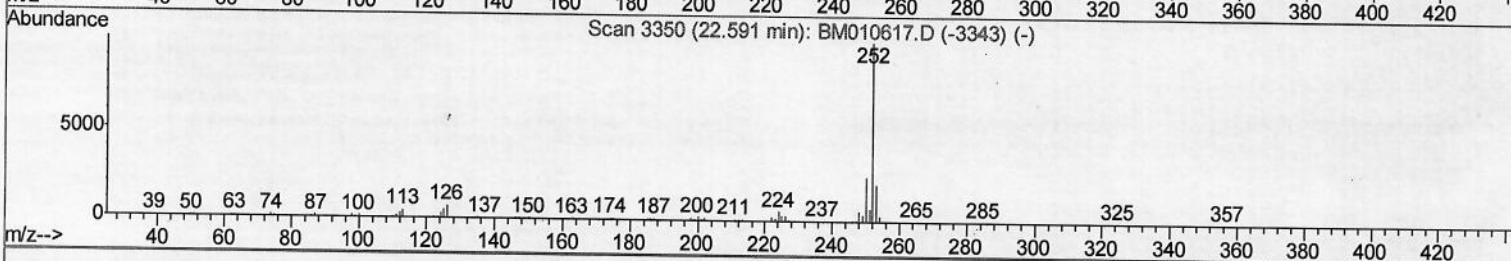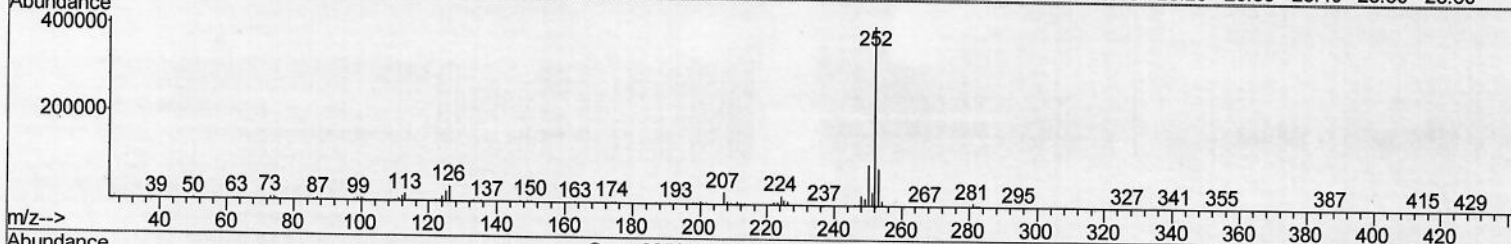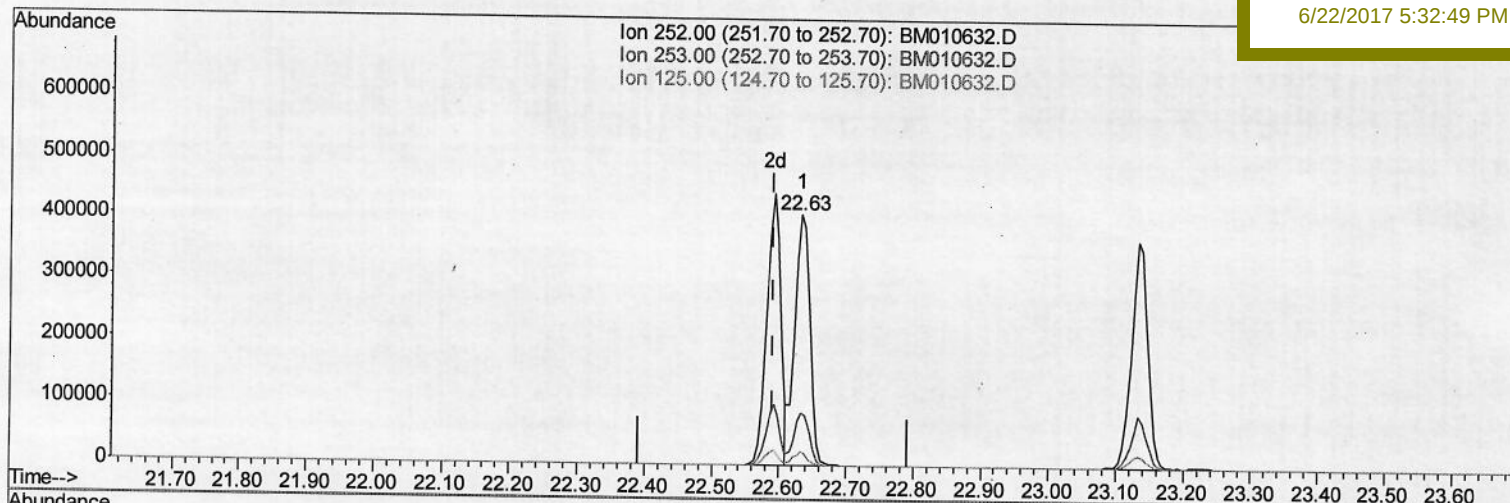

TIC: BM010632.D

(85) Benzo(b)fluoranthene

22.633min (+0.041) 18.93ng/ul

response 640259

Ion	Exp%	Act%
252.00	100	100
253.00	22.40	20.78
125.00	4.50	5.30
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062117\
Quantitation Report (Qedit)




Data File : BM010632.D
Acq On : 21 Jun 2017 20:40
Operator : SJ/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Jun 22 00:46:25 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 22 00:43:46 2017
Response via : Initial Calibration

Instrument :
BNA_M
LabSampleId :
SSTD02041

Manual Integrations
APPROVED

mohammad
6/22/2017 5:32:49 PM

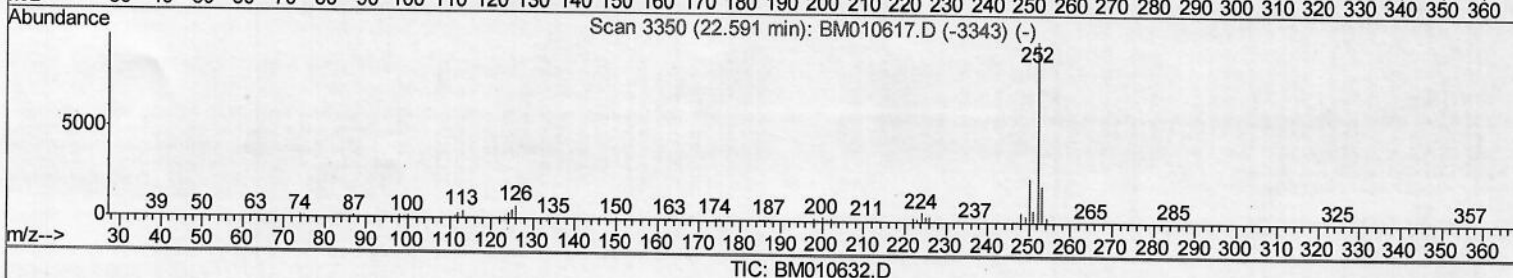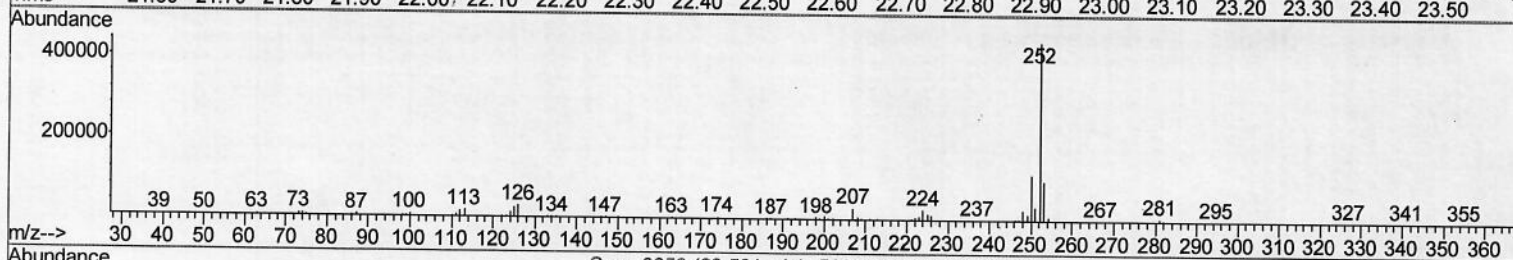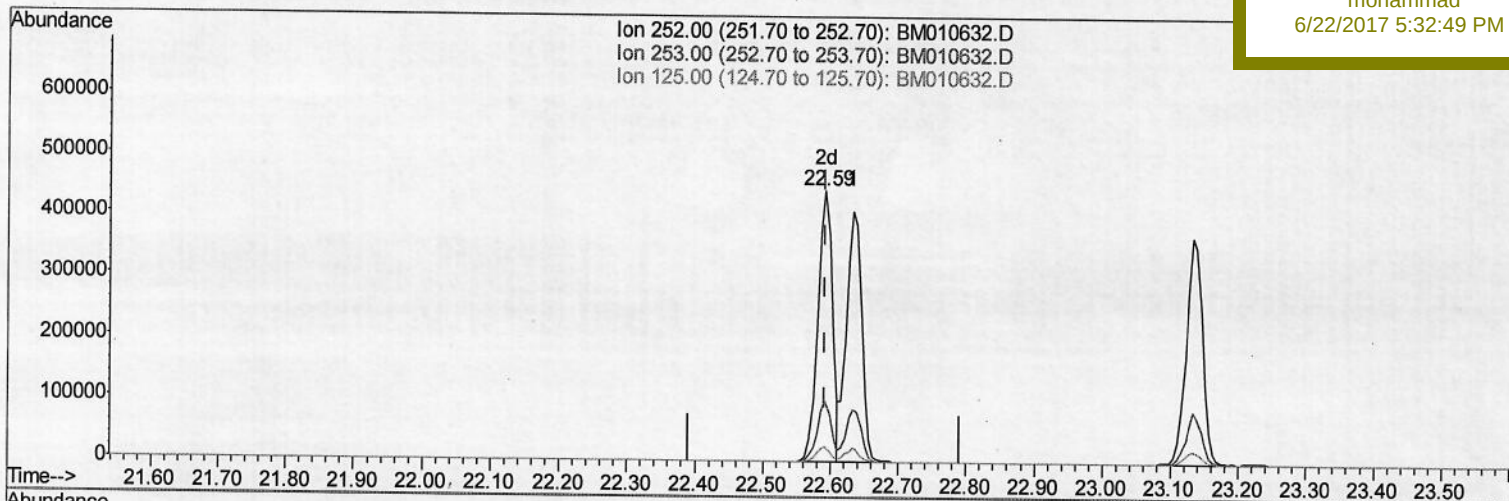

(85) Benzo(b)fluoranthene

22.592min (+0.000) 19.31ng/ul m

response 653176

Ion	Exp%	Act%
252.00	100	100
253.00	22.40	22.12
125.00	4.50	5.48#
0.00	0.00	0.00

> 5.9
06/26/17

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062117\
Quantitation Report (QT Reviewed)

Data File : BM010632.D
Acq On : 21 Jun 2017 20:40
Operator : SJ/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_M
LabSampleId :
SSTD02041

Quant Time: Jun 22 01:36:51 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 22 00:43:46 2017
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
6/22/2017 5:32:49 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	50970	20.00	ng/ul	0.00
18) Naphthalene-d8	10.23	136	235242	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.12	164	173531	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.87	188	454165	20.00	ng/ul	0.00
75) Chrysene-d12	21.09	240	557020	20.00	ng/ul	0.00
83) Perylene-d12	23.23	264	521026	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.08	96	7697	8.65	ng/uL	0.00
5) Phenol-d5	6.65	99	88899	18.31	ng/ul	0.00
7) Bis-(2-Chloroethyl) ether-d	6.82	67	47600	17.17	ng/ul	0.00
9) 2-Chlorophenol-d4	7.00	132	67270	19.75	ng/ul	0.00
13) 4-Methylphenol-d8	8.17	113	76509	19.01	ng/ul	0.00
19) Nitrobenzene-d5	8.61	128	32732	19.51	ng/ul	0.00
22) 2-Nitrophenol-d4	9.32	143	40422	20.91	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.85	165	81792	20.09	ng/ul	0.00
29) 4-Chloroaniline-d4	10.37	131	99614	23.22	ng/ul	0.00
43) Dimethylphthalate-d6	13.54	166	303862	19.95	ng/ul	0.00
46) Acenaphthylene-d8	13.80	160	336940	19.02	ng/ul	0.00
51) 4-Nitrophenol-d4	14.33	143	52219	19.48	ng/ul	0.00
57) Fluorene-d10	15.12	176	259737	19.73	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.25	200	56560	20.28	ng/ul	0.00
70) Anthracene-d10	16.97	188	435292	19.85	ng/ul	0.00
76) Pyrene-d10	19.28	212	522069	20.18	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.09	264	494823	19.65	ng/ul	0.00

Target Compounds

					Qvalue
2) 1,4-Dioxane	3.10	88	7986	8.04 ng/uL#	24
4) Benzaldehyde	6.62	77	63644	22.27 ng/ul	88
6) Phenol	6.67	94	89869	17.97 ng/ul	90
8) Bis(2-Chloroethyl) ether	6.90	93	65501	17.99 ng/ul	95
10) 2-Chlorophenol	7.03	128	66881	19.64 ng/ul	95
11) 2-Methylphenol	7.90	108	71597	18.78 ng/ul	99
12) 2,2'-oxybis(1-Chloropropan	8.00	45	43405	17.08 ng/ul#	88
14) Acetophenone	8.28	105	122172	18.59 ng/ul	93
15) N-Nitroso-di-n-propylamine	8.27	70	64130	18.11 ng/ul	93
16) 4-Methylphenol	8.23	108	78319	18.67 ng/ul	96
17) Hexachloroethane	8.53	117	30365	20.06 ng/ul	88
20) Nitrobenzene	8.65	77	96251	19.66 ng/ul	93
21) Isophorone	9.17	82	177965	18.28 ng/ul	99
23) 2-Nitrophenol	9.35	139	42708	20.82 ng/ul	89
24) 2,4-Dimethylphenol	9.42	107	102409	19.63 ng/ul	98
25) Bis(2-Chloroethoxy)methane	9.66	93	97912	18.14 ng/ul	95
27) 2,4-Dichlorophenol	9.88	162	79281	20.01 ng/ul#	88
28) Naphthalene	10.27	128	230525	19.69 ng/ul	99
30) 4-Chloroaniline	10.39	127	93682	21.72 ng/ul	95
31) Hexachlorobutadiene	10.57	225	65376	21.88 ng/ul	96
32) Caprolactam	11.15	113	26616m	19.14 ng/ul	
33) 4-Chloro-3-methylphenol	11.52	107	98683	19.53 ng/ul	94
34) 2-Methylnaphthalene	11.90	142	189151	20.10 ng/ul	96

SJ
06/26/17

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062117\
Quantitation Report (QT Reviewed)

Data File : BM010632.D
Acq On : 21 Jun 2017 20:40
Operator : SJ/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_M
LabSampleId :
SSTD02041

Quant Time: Jun 22 01:36:51 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 22 00:43:46 2017
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
6/22/2017 5:32:49 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
36) 1,2,4,5-Tetrachlorobenzene	12.28	216	119689	19.54	ng/ul#	93
37) Hexachlorocyclopentadiene	12.26	237	72043	20.46	ng/ul	96
38) 2,4,6-Trichlorophenol	12.53	196	81887	19.58	ng/ul	98
39) 2,4,5-Trichlorophenol	12.59	196	86233	19.97	ng/ul	100
40) 1,1'-Biphenyl	12.94	154	263675	19.44	ng/ul	98
41) 2-Chloronaphthalene	12.97	162	204151	19.12	ng/ul	96
42) 2-Nitroaniline	13.19	65	63412	20.31	ng/ul	99
44) Dimethylphthalate	13.59	163	292476	19.59	ng/ul	99
45) 2,6-Dinitrotoluene	13.70	165	54465	21.06	ng/ul#	87
47) Acenaphthylene	13.83	152	324630	19.24	ng/ul	98
48) 3-Nitroaniline	14.03	138	52396	20.09	ng/ul	97
49) Acenaphthene	14.18	153	217044	19.06	ng/ul	98
50) 2,4-Dinitrophenol	14.23	184	39038	20.84	ng/ul#	86
52) 4-Nitrophenol	14.34	109	75354	22.15	ng/ul	87
53) Dibenzofuran	14.52	168	337935	19.60	ng/ul	93
54) 2,4-Dinitrotoluene	14.49	165	84005	20.94	ng/ul	96
55) 2,3,4,6-Tetrachlorophenol	14.75	232	86688	19.84	ng/ul	92
56) Diethylphthalate	14.97	149	306719	19.52	ng/ul	96
58) Fluorene	15.17	166	278246	19.28	ng/ul	99
59) 4-Chlorophenyl-phenylether	15.17	204	160789	20.50	ng/ul	93
60) 4-Nitroaniline	15.20	138	57875	18.78	ng/ul	92
63) 4,6-Dinitro-2-methylphenol	15.26	198	59673	20.08	ng/ul#	96
64) N-Nitrosodiphenylamine	15.39	169	245793	19.51	ng/ul	99
65) 4-Bromophenyl-phenylether	16.07	248	99987	19.23	ng/ul#	89
66) Hexachlorobenzene	16.18	284	108442	19.80	ng/ul#	83
67) Atrazine	16.36	200	111992	21.11	ng/ul	94
68) Pentachlorophenol	16.52	266	75583	19.58	ng/ul	95
69) Phenanthrene	16.92	178	474113	19.64	ng/ul	97
71) Anthracene	17.00	178	488367	19.63	ng/ul	97
72) Carbazole	17.28	167	420302	19.37	ng/ul	99
73) Di-n-butylphthalate	17.86	149	526362	19.07	ng/ul	99
74) Fluoranthene	18.94	202	620701	19.95	ng/ul#	96
77) Pyrene	19.31	202	639611	19.88	ng/ul	99
78) Butylbenzylphthalate	20.24	149	249395	20.62	ng/ul	97
79) 3,3'-Dichlorobenzidine	21.02	252	226967	20.37	ng/ul#	97
80) Benzo(a)anthracene	21.07	228	665086	20.50	ng/ul	99
81) Bis(2-ethylhexyl)phthalate	21.03	149	360159	19.52	ng/ul#	98
82) Chrysene	21.12	228	589043	20.37	ng/ul	99
84) Di-n-octyl phthalate	21.89	149	622655	17.10	ng/ul	96
85) Benzo(b)fluoranthene	22.59	252	653176m	19.31	ng/ul	
86) Benzo(k)fluoranthene	22.63	252	640259	19.97	ng/ul#	98
88) Benzo(a)pyrene	23.13	252	616819	19.81	ng/ul	99
89) Indeno(1,2,3-cd)pyrene	25.34	276	660645	20.46	ng/ul	97
90) Dibenzo(a,h)anthracene	25.36	278	542075	20.14	ng/ul	97
91) Benzo(g,h,i)perylene	25.99	276	530079	20.62	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

> 5.1
06/26/17

```

Data File   : BM010632.D
Acq On      : 21 Jun 2017   20:40
Operator    : SJ/JU
Sample      : SSTDCCC020
Misc        :
ALS Vial    : 2      Sample Multiplier: 1

```

Instrument :
BNA_M
LabSampleId :
SSTD02041

Manual Integrations
APPROVED

mohammad
6/22/2017 5:32:49 PM

