

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062117\
 Data File : BM010643.D
 Acq On : 22 Jun 2017 03:14
 Operator : SJ/JU
 Sample : I3522-11ME 5X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F5C31ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.645	635	639	651	rVB	43021	63408	3.02%	0.413%
2	6.816	663	668	675	rBB2	28364	44485	2.12%	0.290%
3	6.998	694	699	706	rBB2	42487	64173	3.06%	0.418%
4	7.463	772	778	786	rVB	315212	476959	22.75%	3.109%
5	8.169	891	898	903	rBB2	58525	87115	4.16%	0.568%
6	8.604	965	972	979	rBB	43032	67255	3.21%	0.438%
7	9.322	1089	1094	1098	rBV2	38468	57958	2.76%	0.378%
8	9.851	1177	1184	1190	rBB2	61470	97098	4.63%	0.633%
9	10.228	1241	1248	1254	rBV	460018	749851	35.77%	4.888%
10	10.369	1265	1272	1279	rBB	54727	83914	4.00%	0.547%
11	13.533	1805	1810	1815	rBV	141189	181872	8.68%	1.186%
12	13.580	1815	1818	1823	rVB	27177	33462	1.60%	0.218%
13	13.798	1850	1855	1866	rVB2	134510	213225	10.17%	1.390%
14	14.116	1903	1909	1916	rVB2	780033	1164376	55.54%	7.590%
15	14.321	1938	1944	1951	rVB	38980	53458	2.55%	0.348%
16	15.115	2073	2079	2084	rBV	184283	262243	12.51%	1.709%
17	15.168	2084	2088	2095	rVB2	54160	74449	3.55%	0.485%
18	15.233	2095	2099	2105	rVB	36794	49538	2.36%	0.323%
19	16.868	2371	2377	2381	rBV	1143383	1523166	72.65%	9.929%
20	16.909	2381	2384	2389	rVV	163908	211159	10.07%	1.376%
21	16.962	2389	2393	2396	rVV	201028	314919	15.02%	2.053%
22	16.998	2396	2399	2406	rVV	886247	1196958	57.09%	7.802%
23	17.274	2440	2446	2452	rBV	296585	395030	18.84%	2.575%
24	17.792	2529	2534	2538	rBV4	36631	44970	2.15%	0.293%
25	17.874	2542	2548	2553	rBV2	35973	52976	2.53%	0.345%
26	17.939	2553	2559	2563	rBV2	62703	90913	4.34%	0.593%
27	18.674	2679	2684	2689	rBV3	16778	26600	1.27%	0.173%
28	18.727	2689	2693	2699	rBV5	31036	52103	2.49%	0.340%
29	18.939	2721	2729	2738	rVB	441088	585735	27.94%	3.818%
30	19.086	2749	2754	2760	rVB5	26457	35889	1.71%	0.234%
31	19.274	2782	2786	2789	rBV2	329075	489448	23.35%	3.190%
32	19.303	2789	2791	2800	rVB	381742	423339	20.19%	2.759%
33	19.386	2800	2805	2811	rVB3	15460	25530	1.22%	0.166%
34	19.486	2819	2822	2828	rBV2	24303	34898	1.66%	0.227%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062117\
 Data File : BM010643.D
 Acq On : 22 Jun 2017 03:14
 Operator : SJ/JU
 Sample : I3522-11ME 5X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F5C31ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
 Title : SVOA CALIBRATION

35	19.639	2842	2848	2854	rBV5	29870	71149	3.39%	0.464%
36	19.780	2865	2872	2873	rBV4	34923	57314	2.73%	0.374%
37	19.809	2873	2877	2882	rVB	87724	127575	6.09%	0.832%
38	19.909	2889	2894	2898	rBV	88950	114645	5.47%	0.747%
39	19.962	2898	2903	2908	rVB3	44081	66701	3.18%	0.435%
40	20.103	2923	2927	2932	rBV	30301	45605	2.18%	0.297%
41	20.150	2932	2935	2937	rBV2	19115	23164	1.10%	0.151%
42	20.521	2994	2998	3002	rBV6	24882	41432	1.98%	0.270%
43	20.562	3002	3005	3011	rVB6	17565	36363	1.73%	0.237%
44	20.727	3030	3033	3037	rBV2	48128	60007	2.86%	0.391%
45	20.762	3037	3039	3042	rBV3	28305	32880	1.57%	0.214%
46	20.803	3042	3046	3047	rBV	41736	49259	2.35%	0.321%
47	21.086	3087	3094	3097	rBV	1477319	2096461	100.00%	13.665%
48	21.115	3097	3099	3107	rVB	194128	261634	12.48%	1.705%
49	21.344	3133	3138	3142	rBV	66062	97603	4.66%	0.636%
50	21.380	3142	3144	3149	rBV3	29948	54434	2.60%	0.355%
51	22.586	3344	3349	3362	rVB	215969	623958	29.76%	4.067%
52	22.744	3373	3376	3380	rBV2	38225	53065	2.53%	0.346%
53	23.038	3421	3426	3430	rBV	105565	177721	8.48%	1.158%
54	23.086	3430	3434	3438	rVV2	144654	260959	12.45%	1.701%
55	23.127	3438	3441	3450	rVB2	133768	270074	12.88%	1.760%
56	23.221	3450	3457	3464	rBV	756619	1390814	66.34%	9.066%


Sum of corrected areas: 15341289

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062117\
Data File : BM010643.D
Acq On : 22 Jun 2017 03:14
Operator : SJ/JU
Sample : I3522-11ME 5X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F5C31ME

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

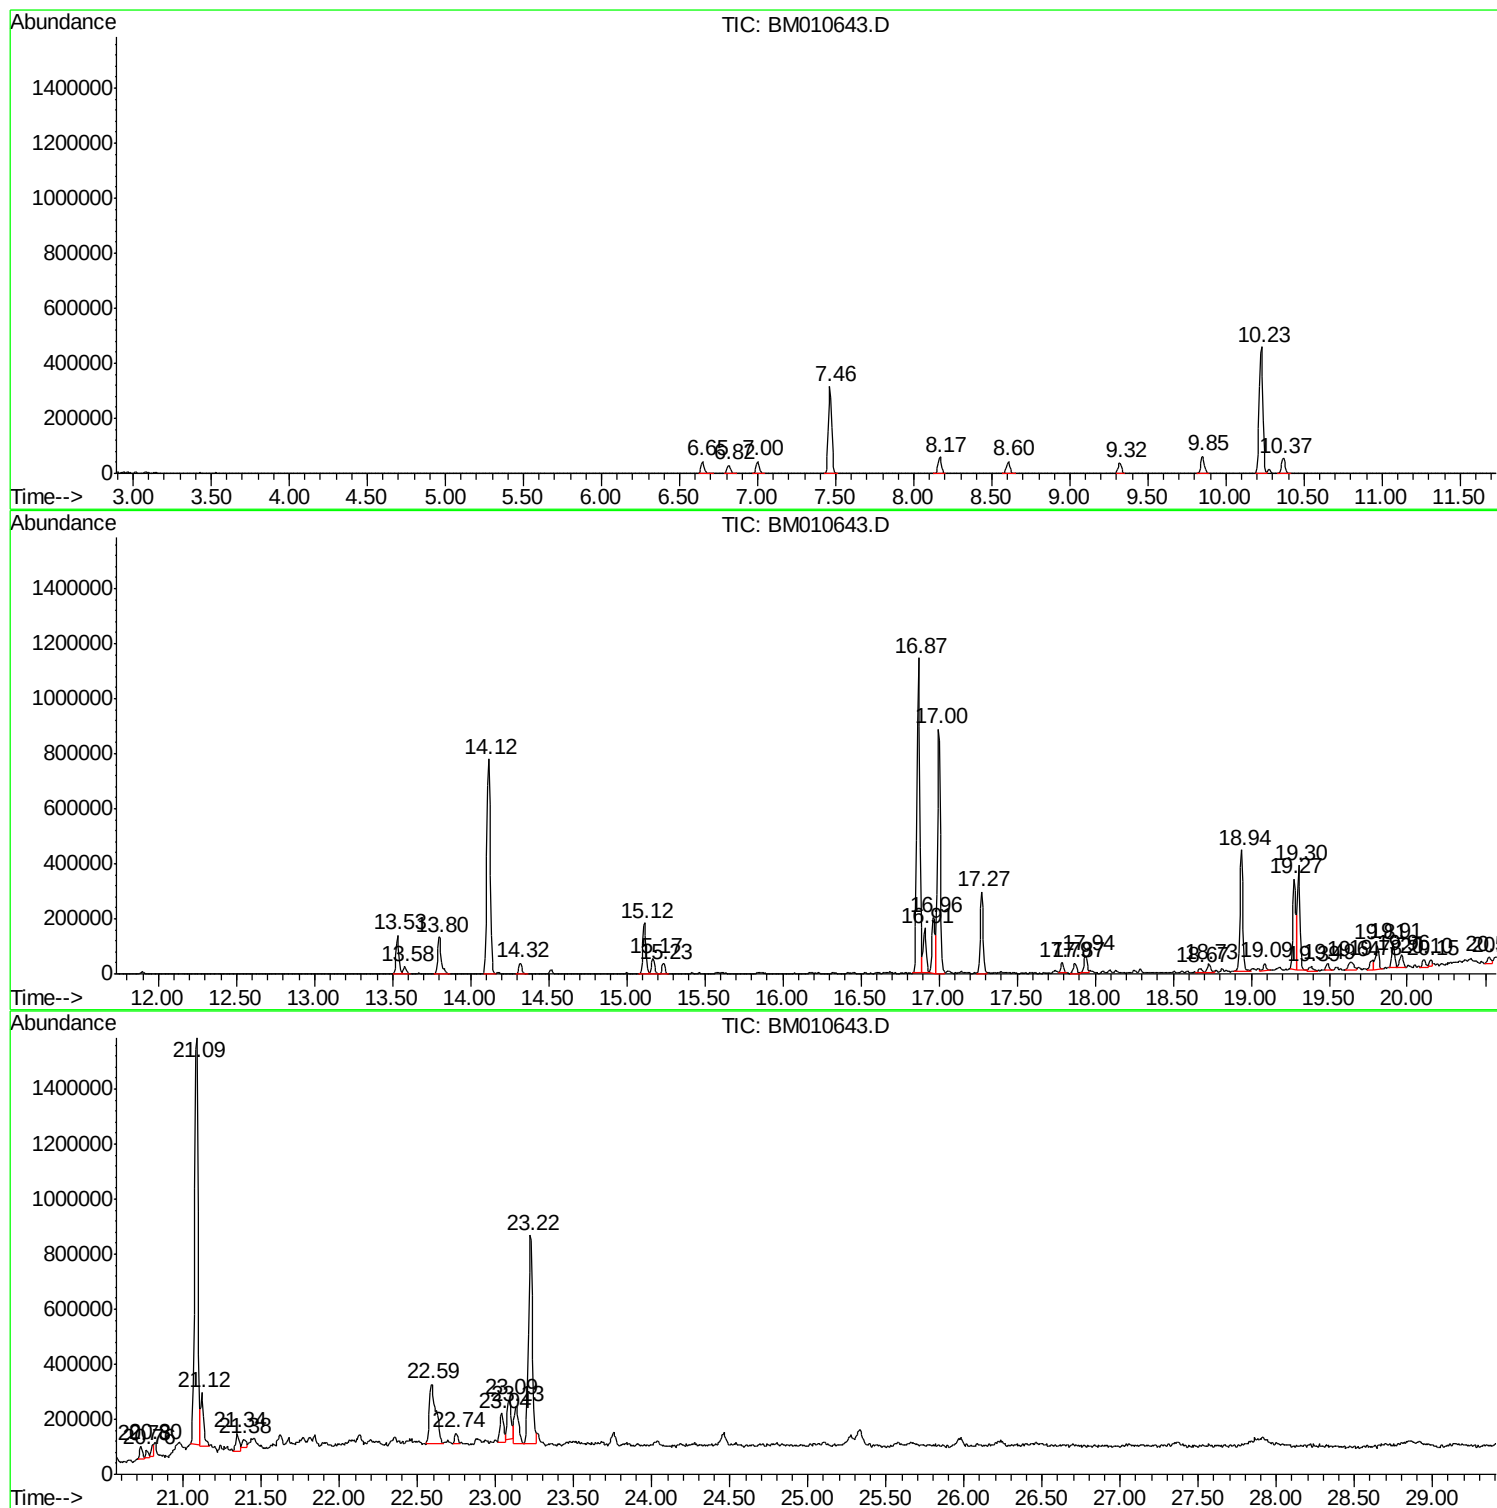

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062117\
Data File : BM010643.D
Acq On : 22 Jun 2017 03:14
Operator : SJ/JU
Sample : I3522-11ME 5X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F5C31ME

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062117\
Data File : BM010643.D
Acq On : 22 Jun 2017 03:14
Operator : SJ/JU
Sample : I3522-11ME 5X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F5C31ME

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc